
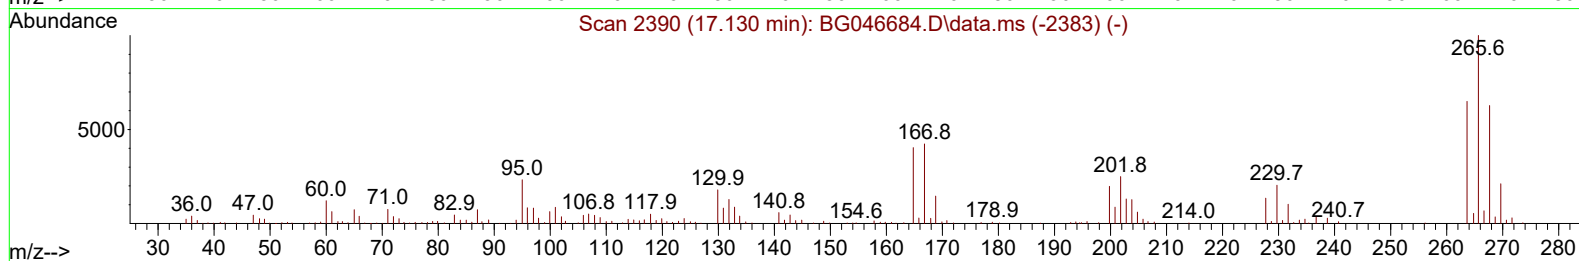
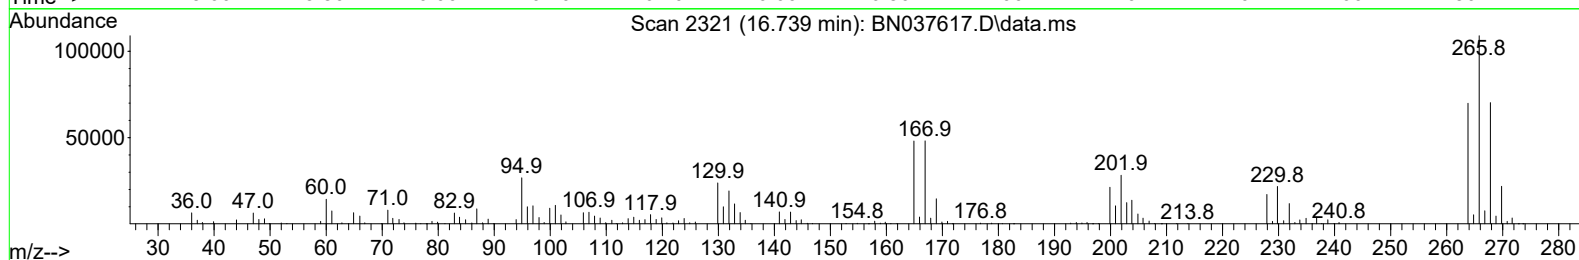


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081925\
Data File : BN037617.D
Acq On : 20 Aug 2025 03:35
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 20 07:01:46 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 06 01:49:15 2025
Response via : Initial Calibration

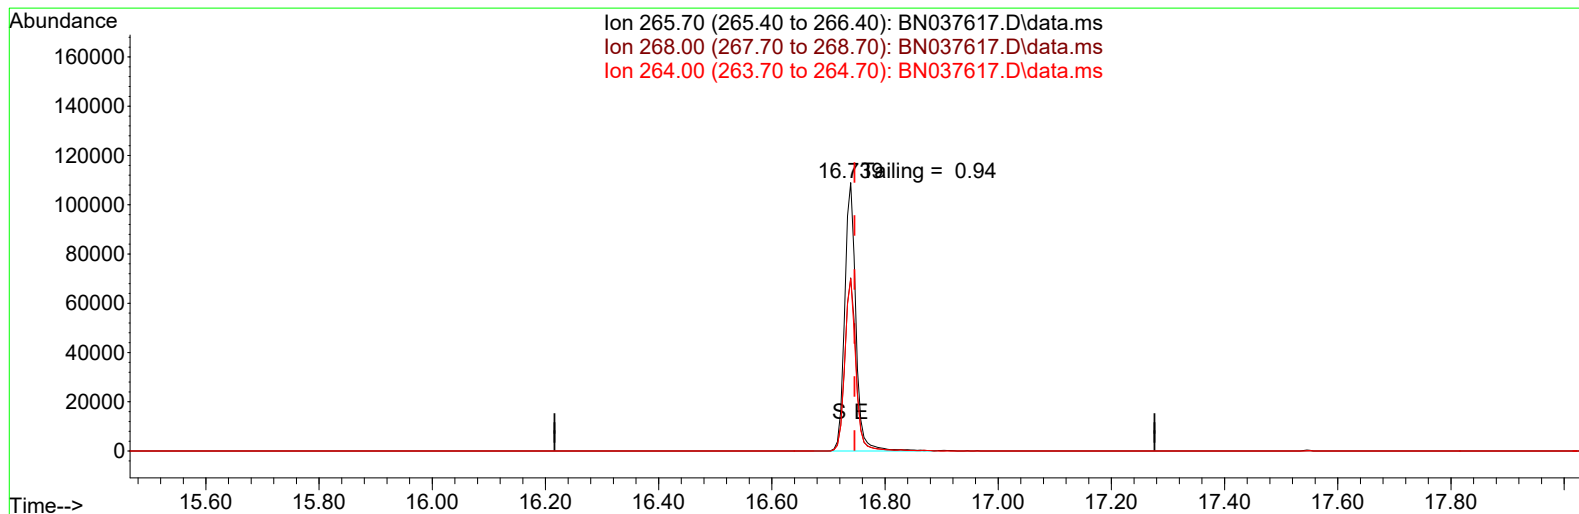

TIC: BN037617.D\data.ms

(70) Pentachlorophenol (C)




16.739min (-0.006) 24577.65 ng

response 150060

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.52
264.00	61.60	64.16
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081925\
Data File : BN037617.D
Acq On : 20 Aug 2025 03:35
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 20 07:01:46 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 06 01:49:15 2025
Response via : Initial Calibration

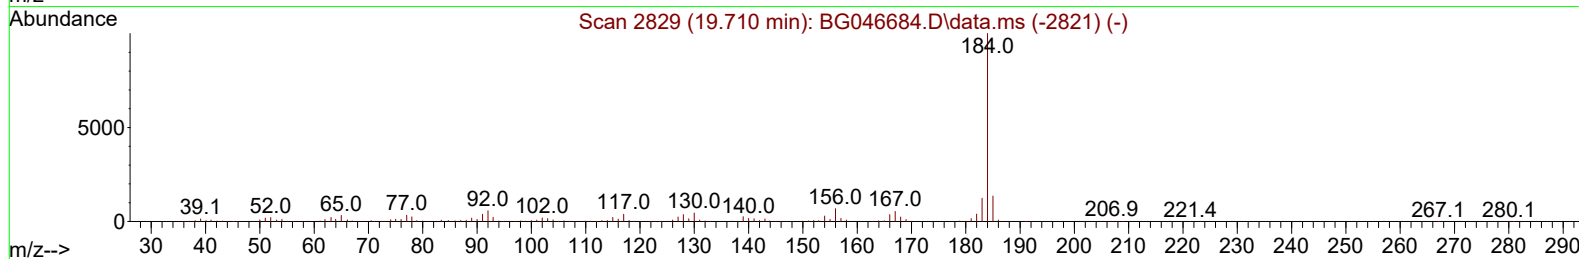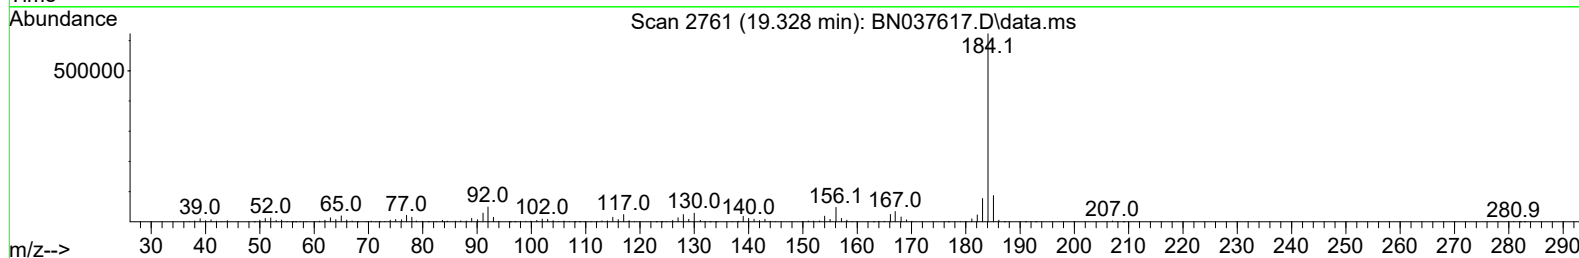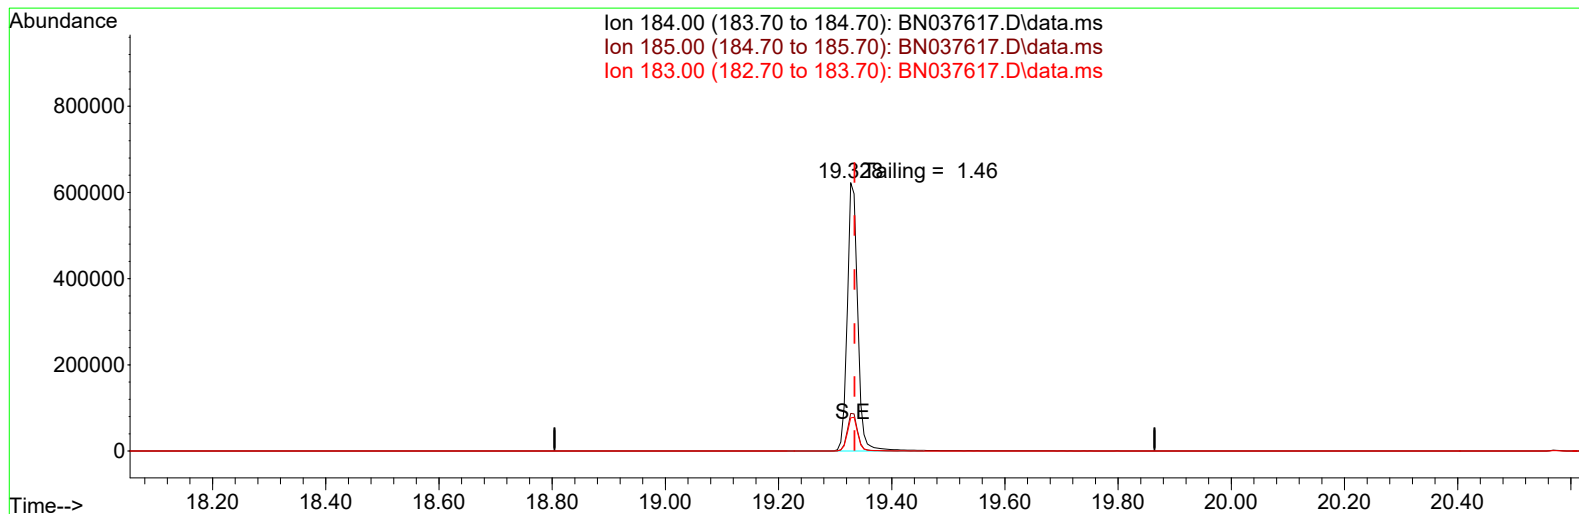

TIC: BN037617.D\data.ms

(77) Benzidine

19.328min (-0.006) 0.00 ng

response 801660

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.02
183.00	13.20	12.34
0.00	0.00	0.00