
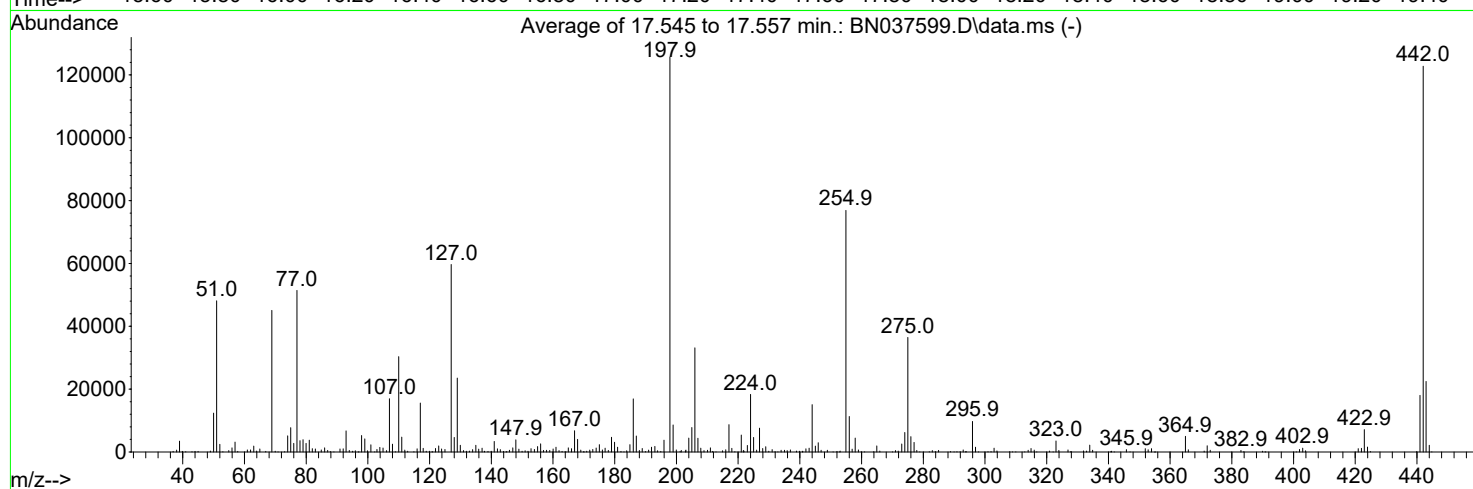


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081925\
Data File : BN037599.D
Acq On : 19 Aug 2025 10:00
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN081225.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Aug 13 05:00:58 2025

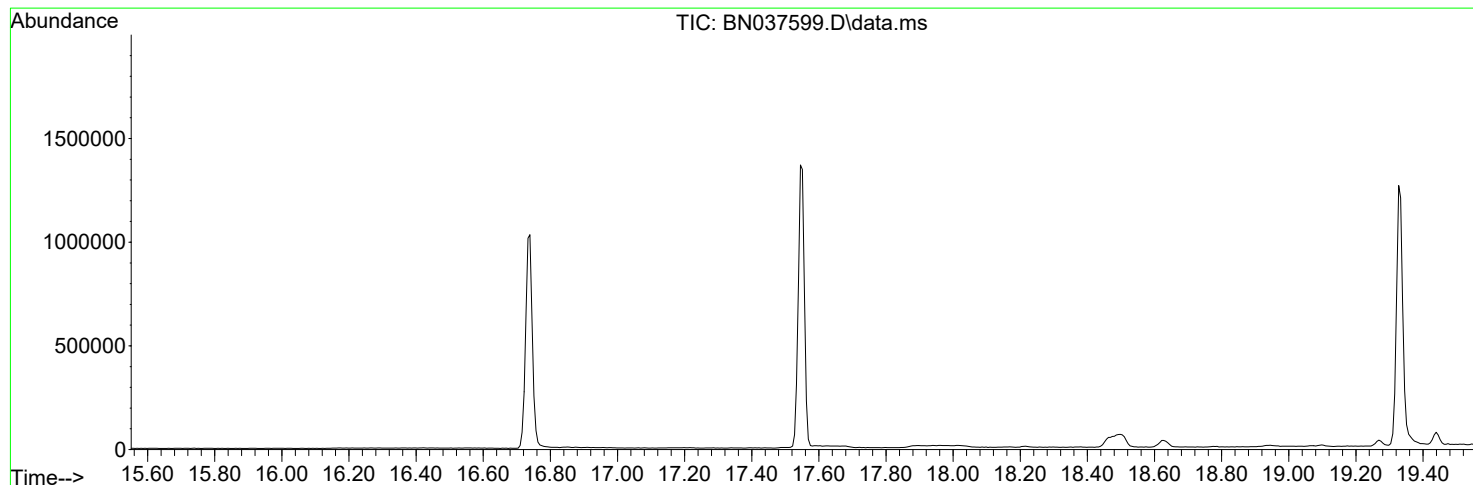

AutoFind: Scans 2458, 2459, 2460; Background Corrected with Scan 2451

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	0.0	0	PASS
69	69	100	100	100.0	45078	PASS
70	69	0.00	2	0.5	240	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	125645	PASS
199	198	5	9	6.9	8618	PASS
365	198	1	100	4.0	4986	PASS
441	443	0.01	150	80.4	18037	PASS
442	442	100	100	100.0	122741	PASS
443	442	15	24	18.3	22437	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/19/2025	BNA_N	<u>BN037599.D</u>
Compound Name	Response	Retention Time
DDT	413417	20.574
DDD	3425	20.133
DDE	498	19.627
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3923	417340	0.94

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081925\
Data File : BN037599.D
Acq On : 19 Aug 2025 10:00
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 20 06:58:42 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 06 01:49:15 2025
Response via : Initial Calibration

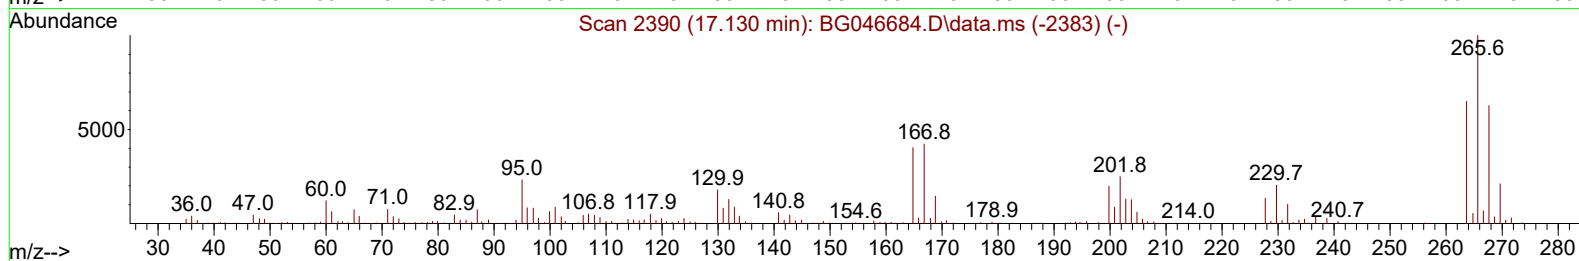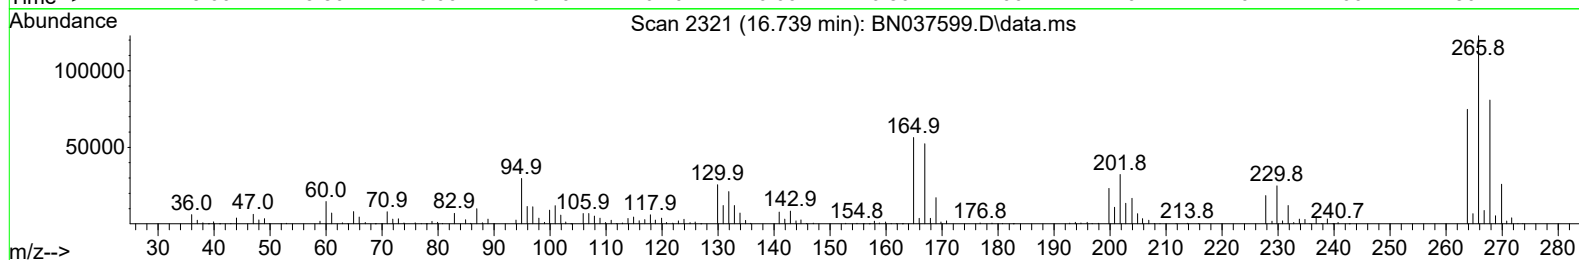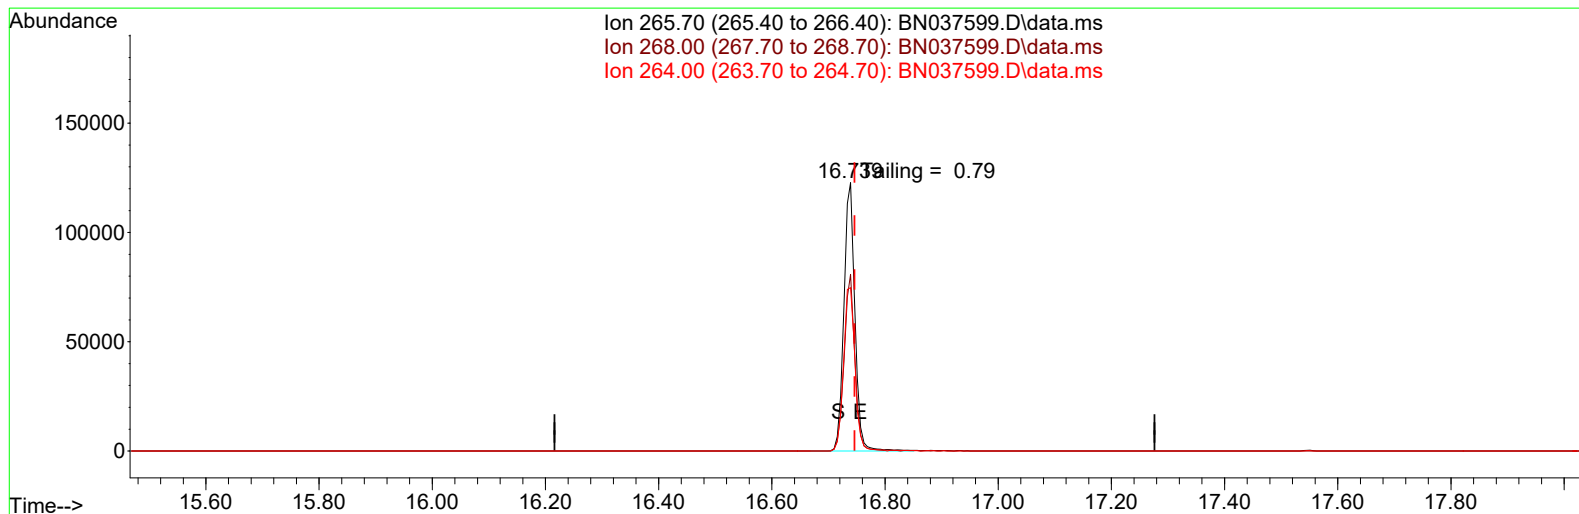

TIC: BN037599.D\data.ms

(70) Pentachlorophenol (C)

16.739min (-0.007) 26205.47 ng




response 166374

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.84
264.00	61.60	60.88
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081925\
Data File : BN037599.D
Acq On : 19 Aug 2025 10:00
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 20 06:58:42 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 06 01:49:15 2025
Response via : Initial Calibration

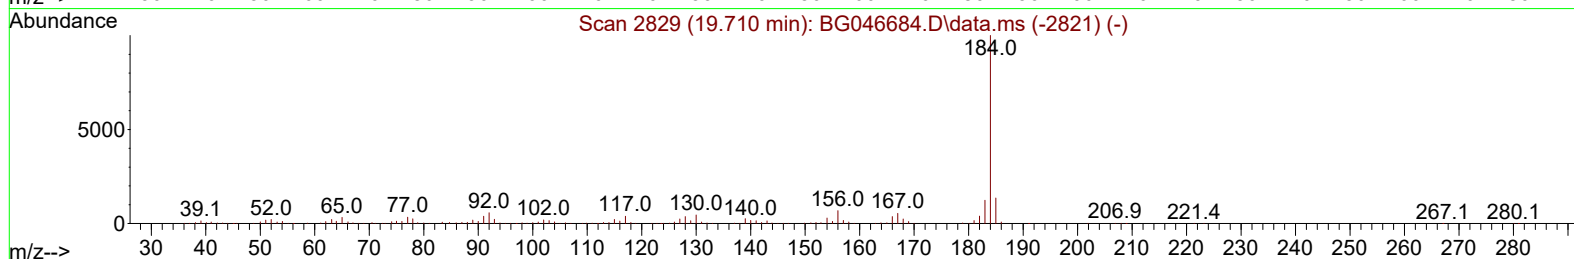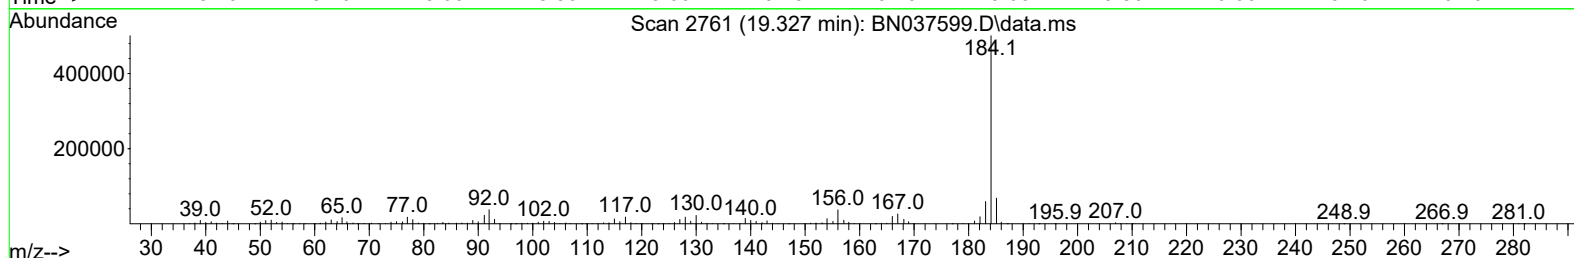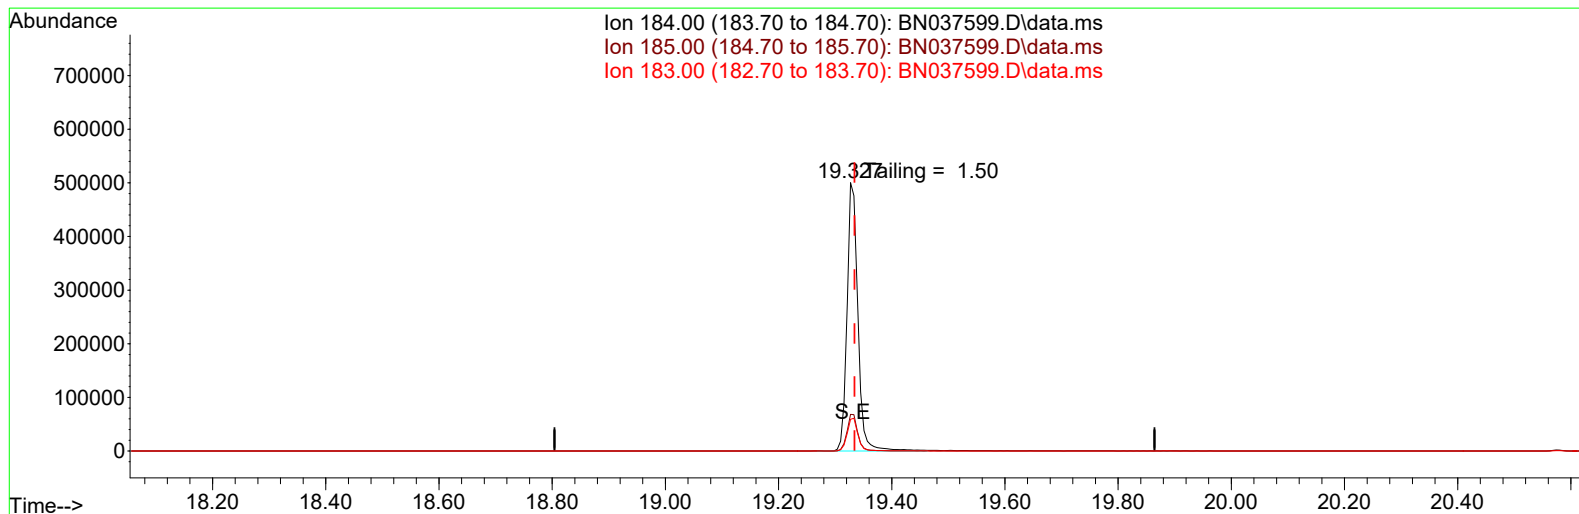

TIC: BN037599.D\data.ms

(77) Benzidine

19.327min (-0.007) 0.00 ng

response 670806

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.65
183.00	13.20	11.83
0.00	0.00	0.00