

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN082019\
 Data File : BN007273.D
 Acq On : 20 Aug 2019 20:15
 Operator : HP/JU
 Sample : K4409-14
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 S301-J-1.5-2.0-081919-FD

Quant Time: Aug 20 20:46:32 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN082019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Aug 20 18:52:43 2019

Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.41	152	5109	0.40	ng	0.00
7) Naphthalene-d8	10.16	136	19541	0.40	ng	0.00
13) Acenaphthene-d10	14.05	164	11369	0.40	ng	0.00
19) Phenanthrene-d10	16.81	188	26712	0.40	ng	0.00
27) Chrysene-d12	21.03	240	27931	0.40	ng	0.00
34) Perylene-d12	23.13	264	30736	0.40	ng	0.00

System Monitoring Compounds

4) 2-Fluorophenol	5.04	112	4082	0.26	ng	0.00
5) Phenol-d6	6.60	99	5618	0.31	ng	0.00
8) Nitrobenzene-d5	8.54	82	4190	0.28	ng	0.00
11) 2-Methylnaphthalene-d10	11.77	152	8947	0.26	ng	0.00
14) 2,4,6-Tribromophenol	15.56	330	1761	0.28	ng	0.00
15) 2-Fluorobiphenyl	12.67	172	11516	0.24	ng	0.00
25) Fluoranthene-d10	18.85	212	19688	0.23	ng	0.00
29) Terphenyl-d14	19.47	244	14352	0.21	ng	0.00

Target Compounds


						Qvalue
9) Naphthalene	10.22	128	11057	0.200	ng	97
12) 2-Methylnaphthalene	11.84	142	3568	0.093	ng	96
16) Acenaphthylene	13.77	152	8980	0.149	ng	99
17) Acenaphthene	14.12	154	7061	0.184	ng	97
18) Fluorene	15.11	166	7308	0.146	ng	98
23) Phenanthrene	16.84	178	147286	1.759	ng	100
24) Anthracene	16.94	178	38861	0.515	ng	97
26) Fluoranthene	18.88	202	615357	6.068	ng	100
28) Pyrene	19.24	202	546302	5.230	ng	# 95
30) Benzo(a)anthracene	21.01	228	380642	3.665	ng	96
31) Chrysene	21.06	228	293734	2.771	ng	97
32) Bis(2-ethylhexyl)phthalate	20.97	149	39063	0.941	ng	98
33) Indeno(1,2,3-cd)pyrene	25.20	276	235423	1.846	ng	96
35) Benzo(b)fluoranthene	22.52	252	493381	4.306	ng	99
36) Benzo(k)fluoranthene	22.52	252	493381	4.395	ng	99
37) Benzo(a)pyrene	23.05	252	349427	3.384	ng	99
38) Dibenzo(a,h)anthracene	25.21	278	59595	0.549	ng	# 93
39) Benzo(g,h,i)perylene	25.83	276	226506	2.065	ng	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN082019\
Data File : BN007273.D
Acq On : 20 Aug 2019 20:15
Operator : HP/JU
Sample : K4409-14
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
S301-J-1.5-2.0-081919-FD

Quant Time: Aug 20 20:46:32 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN082019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 20 18:52:43 2019
Response via : Initial Calibration

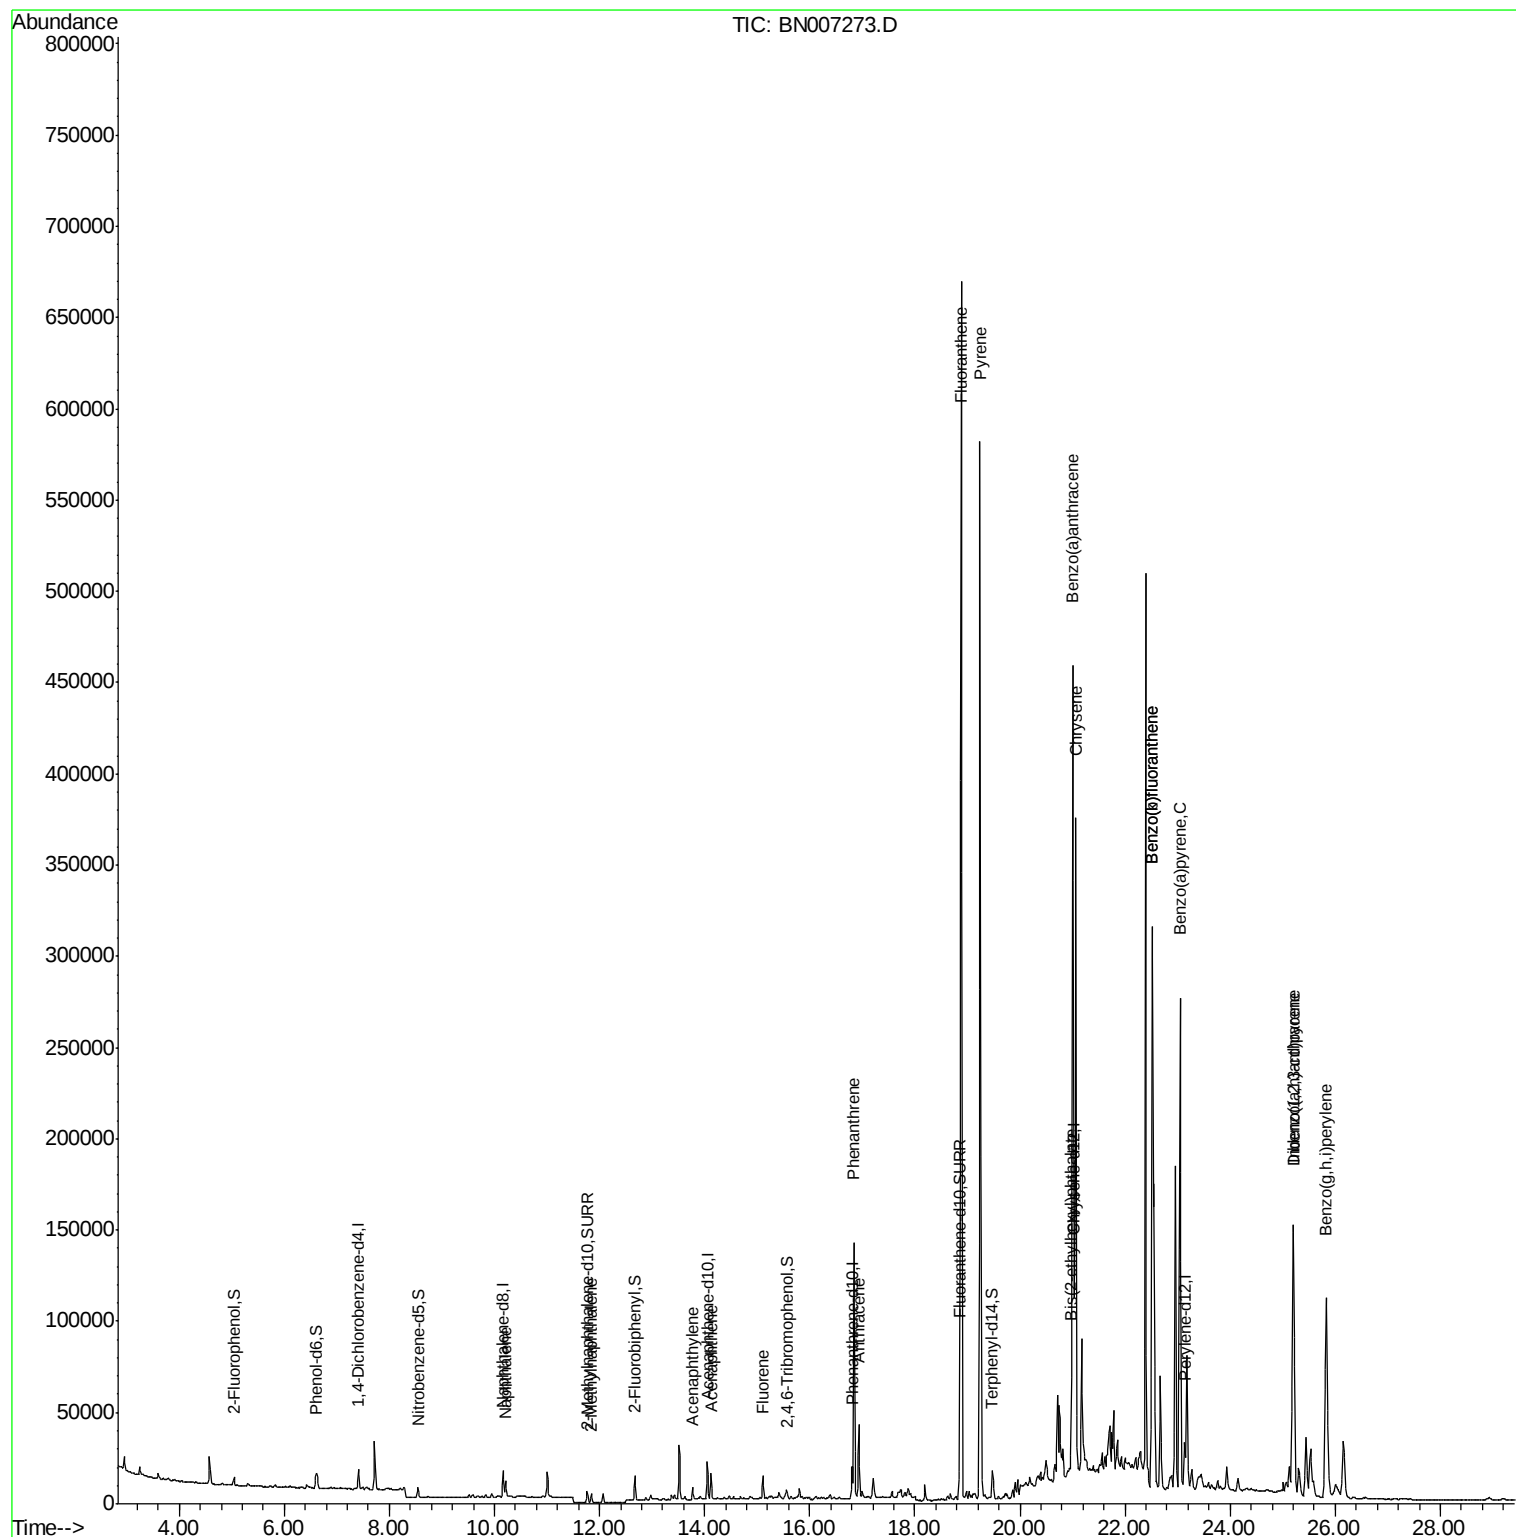







#1

1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.41 min Scan# 569
Delta R.T. 0.00 min
Lab File: BN007273.D
Acq: 20 Aug 2019 20:15

Instrument :
BNA_N
ClientSampleId :
S301-J-1.5-2.0-081919-FD




Tgt Ion:152 Resp: 5109
Ion Ratio Lower Upper
152 100
150 151.1 123.8 185.8
115 59.4 47.3 70.9

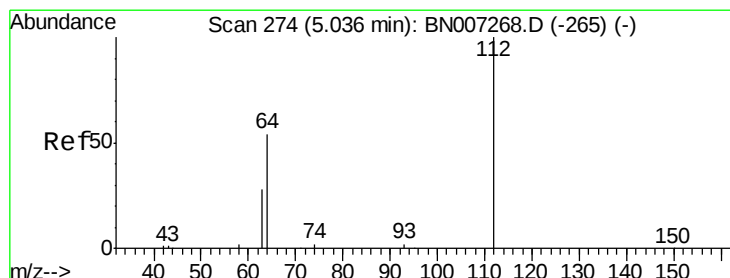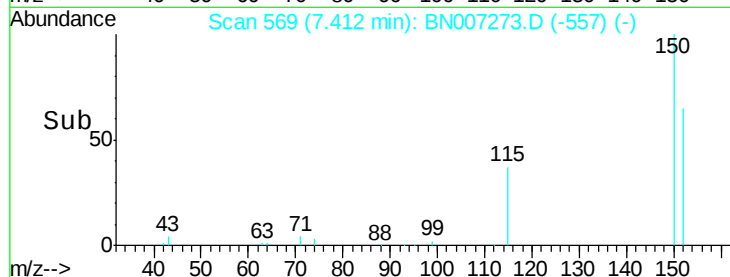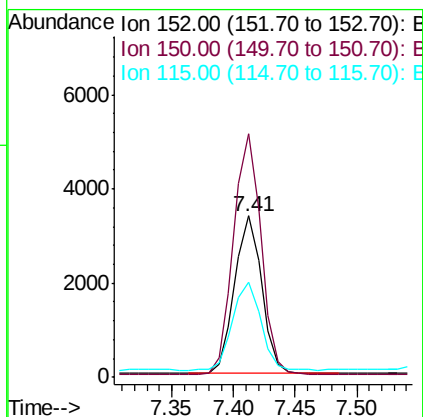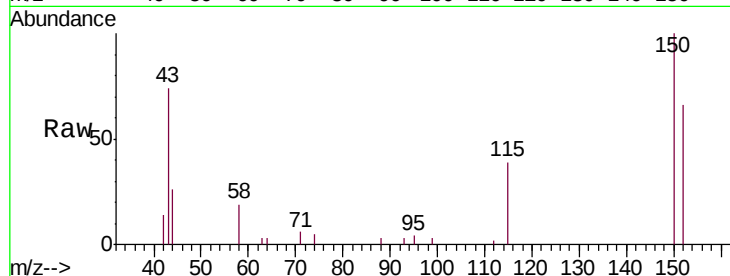


#4

2-Fluorophenol
Concen: 0.262 ng
RT: 5.04 min Scan# 275
Delta R.T. 0.01 min
Lab File: BN007273.D
Acq: 20 Aug 2019 20:15

Tgt Ion:112 Resp: 4082
Ion Ratio Lower Upper
112 100
64 52.1 41.8 62.8
63 27.1 22.6 34.0

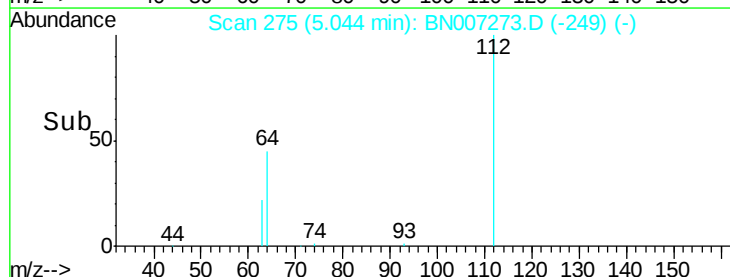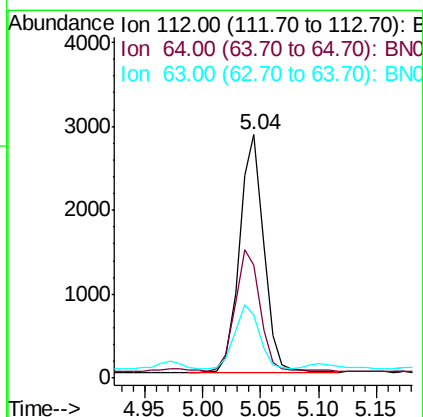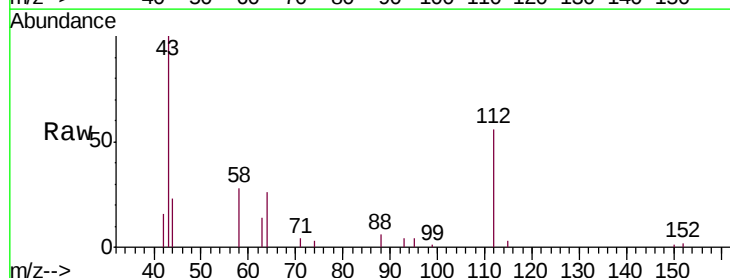

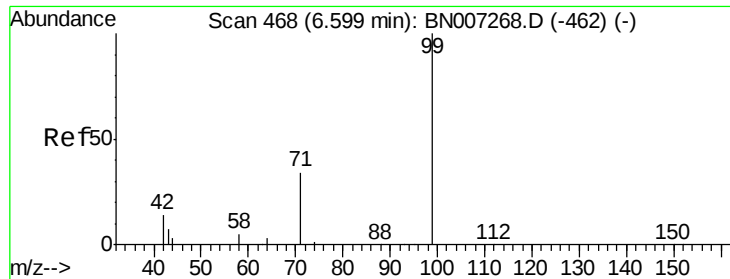

#5

Phenol-d6

Concen: 0.310 ng

RT: 6.60 min Scan# 468

Delta R.T. 0.00 min

Lab File: BN007273.D

Acq: 20 Aug 2019 20:15

Instrument :

BNA_N

ClientSampleId :

S301-J-1.5-2.0-081919-FD


Tgt Ion: 99 Resp: 5618

Ion Ratio Lower Upper

99 100

42 26.1 14.3 21.5#




71 34.4 27.3 40.9

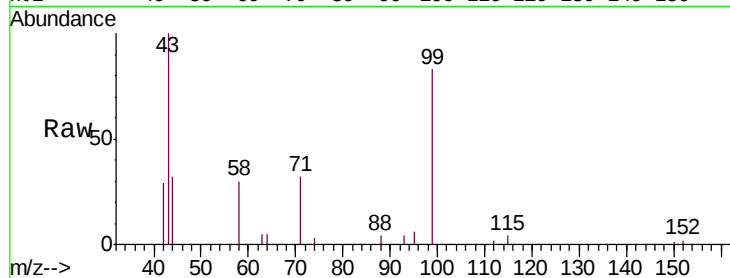

Abundance Ion 99.00 (98.70 to 99.70): BN007268.D (-462) (-)

Ion 42.00 (41.70 to 42.70): BN007268.D (-462) (-)

Ion 71.00 (70.70 to 71.70): BN007268.D (-462) (-)

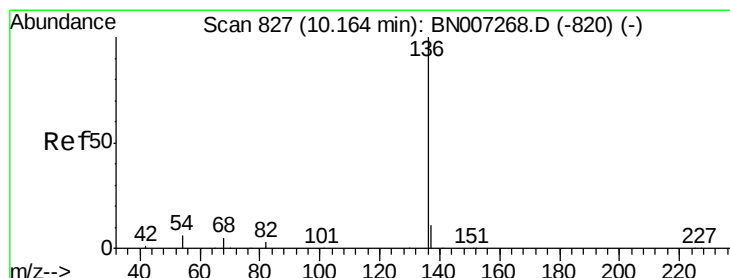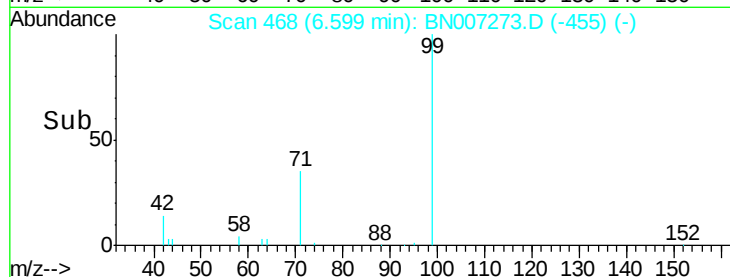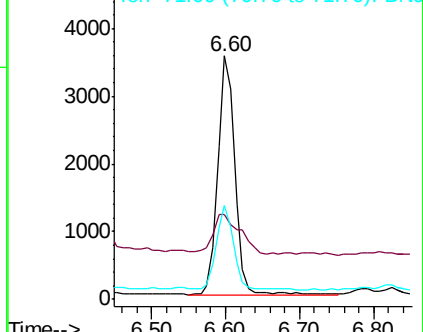

#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.16 min Scan# 827

Delta R.T. 0.00 min

Lab File: BN007273.D

Acq: 20 Aug 2019 20:15

Tgt Ion: 136 Resp: 19541


Ion Ratio Lower Upper

136 100

137 11.3 9.1 13.7

54 7.4 5.9 8.9

68 7.2 5.6 8.4


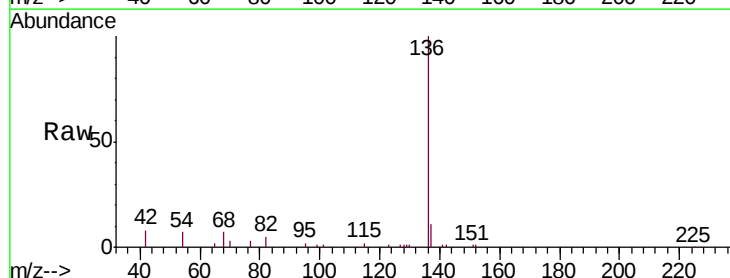



Abundance Ion 136.00 (135.70 to 136.70): BN007268.D (-820) (-)

Ion 137.00 (136.70 to 137.70): BN007268.D (-820) (-)

Ion 54.00 (53.70 to 54.70): BN007268.D (-820) (-)

Ion 68.00 (67.70 to 68.70): BN007268.D (-820) (-)

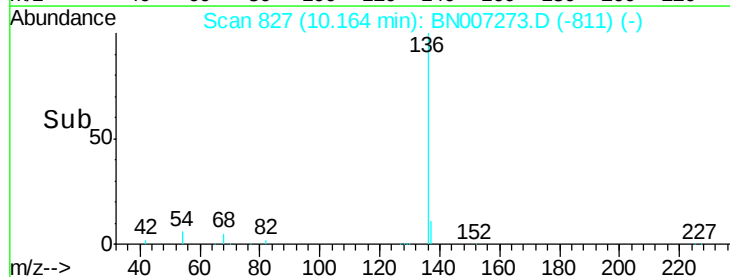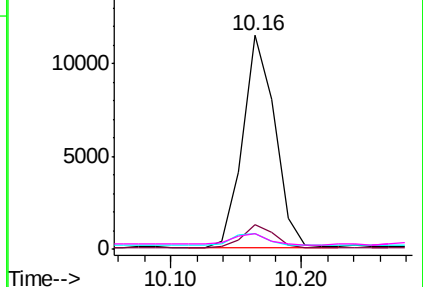



#8

Nitrobenzene-d5

Concen: 0.279 ng

RT: 8.54 min Scan# 699

Delta R.T. 0.00 min

Lab File: BN007273.D

Acq: 20 Aug 2019 20:15

Instrument :

BNA_N

ClientSampleId :

S301-J-1.5-2.0-081919-FD


Tgt Ion: 82 Resp: 4190

Ion Ratio Lower Upper

82 100

128 44.2 35.8 53.6




54 46.2 34.7 52.1

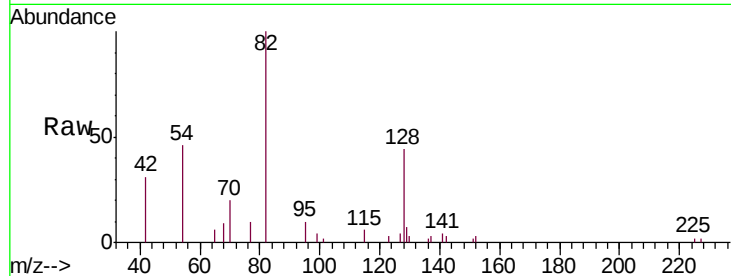

Abundance Ion 82.00 (81.70 to 82.70): BN007268.D (-696) (-)

Ion 128.00 (127.70 to 128.70): BN007268.D (-696) (-)

Ion 54.00 (53.70 to 54.70): BN007268.D (-696) (-)

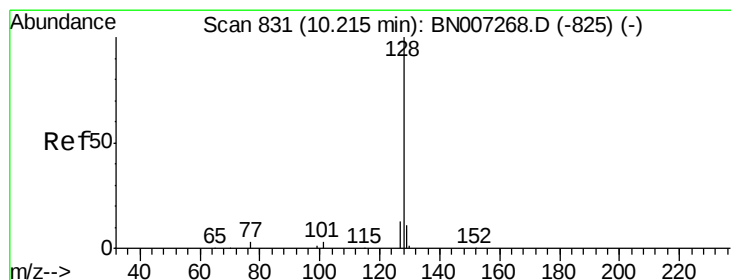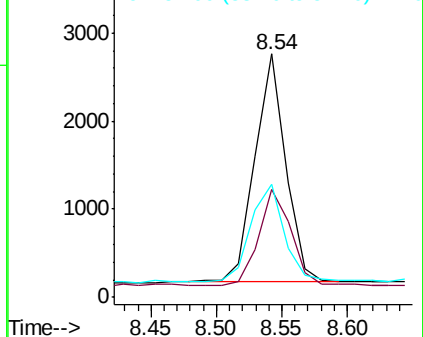

#9

Naphthalene

Concen: 0.200 ng

RT: 10.22 min Scan# 831

Delta R.T. 0.00 min

Lab File: BN007273.D

Acq: 20 Aug 2019 20:15


Tgt Ion: 128 Resp: 11057

Ion Ratio Lower Upper

128 100

129 12.4 9.1 13.7



127 14.7 10.6 16.0




Abundance Ion 128.00 (127.70 to 128.70): BN007268.D (-825) (-)

Ion 129.00 (128.70 to 129.70): BN007268.D (-825) (-)

Ion 127.00 (126.70 to 127.70): BN007268.D (-825) (-)

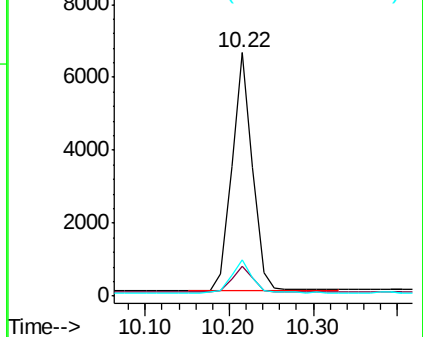

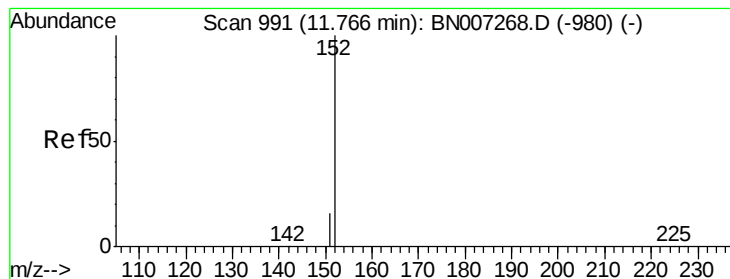

#11

2-Methylnaphthalene-d10

Concen: 0.265 ng

RT: 11.77 min Scan# 991

Delta R.T. 0.00 min

Lab File: BN007273.D

Acq: 20 Aug 2019 20:15

Instrument :

BNA_N

ClientSampleId :


S301-J-1.5-2.0-081919-FD

Tgt Ion:152 Resp: 8947

Ion Ratio Lower Upper




152 100

151 19.1 15.2 22.8

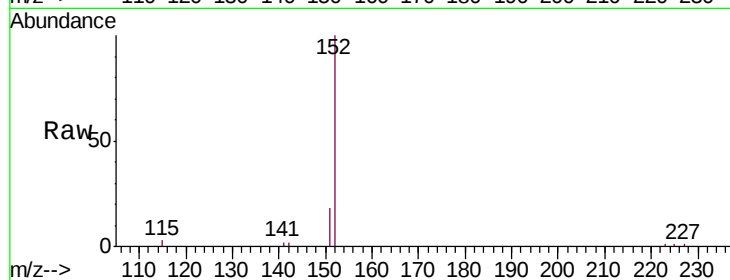

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

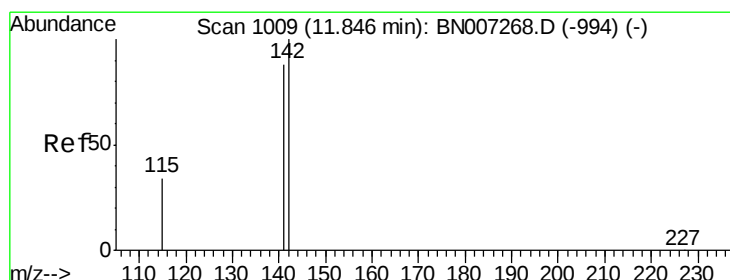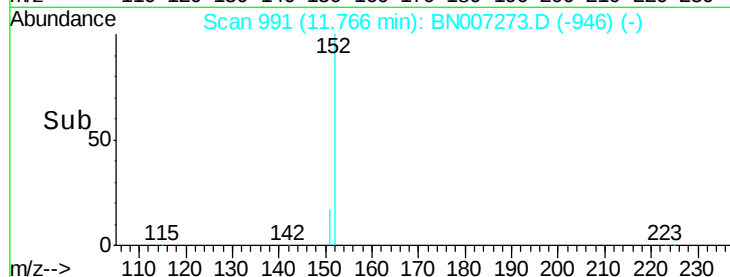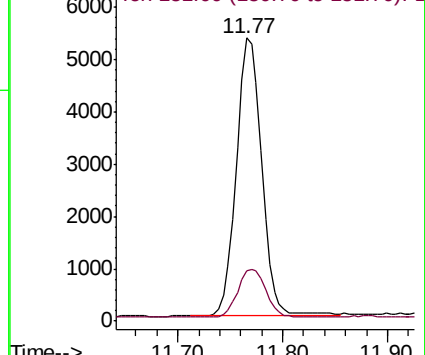

#12

2-Methylnaphthalene

Concen: 0.093 ng

RT: 11.84 min Scan# 1008

Delta R.T. -0.00 min

Lab File: BN007273.D

Acq: 20 Aug 2019 20:15


Tgt Ion:142 Resp: 3568

Ion Ratio Lower Upper

142 100

141 88.7 70.7 106.1



115 42.0 28.1 42.1

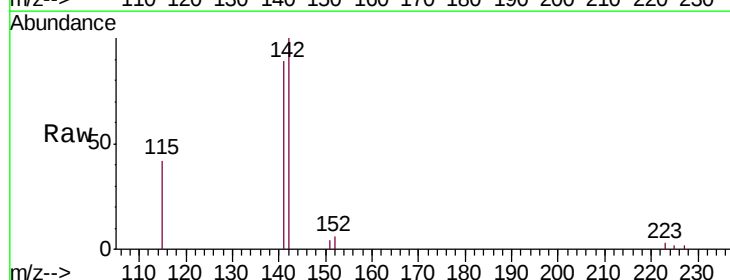


Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

Ion 115.00 (114.70 to 115.70): E

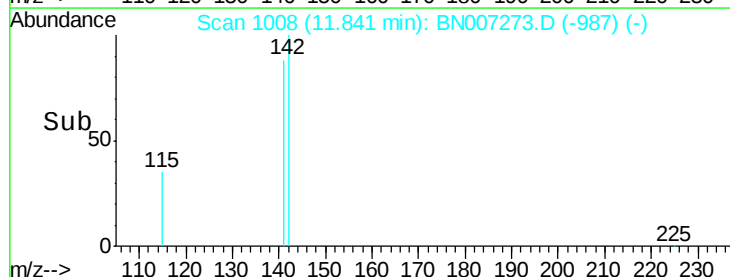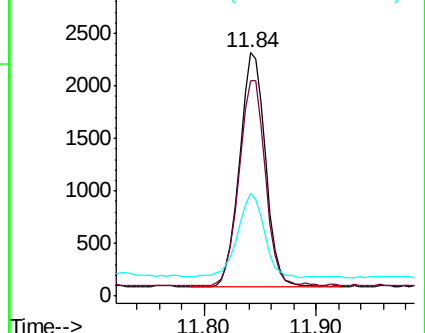



#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.05 min Scan# 1296

Delta R.T. 0.00 min

Lab File: BN007273.D

Acq: 20 Aug 2019 20:15

Instrument :

BNA_N

ClientSampleId :

S301-J-1.5-2.0-081919-FD





Tgt Ion:164 Resp: 11369

Ion Ratio Lower Upper

164 100

162 103.6 82.0 123.0

160 47.7 38.2 57.4

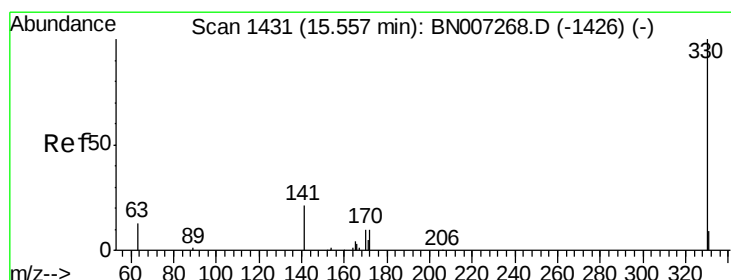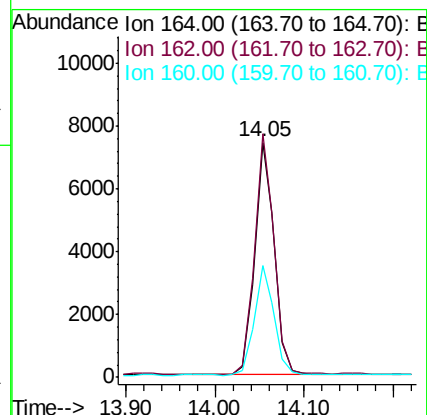

#14

2,4,6-Tribromophenol

Concen: 0.276 ng

RT: 15.56 min Scan# 1431

Delta R.T. 0.00 min

Lab File: BN007273.D

Acq: 20 Aug 2019 20:15




Tgt Ion:330 Resp: 1761


Ion Ratio Lower Upper

330 100

332 0.0 0.0 0.0

141 47.9 30.3 45.5#

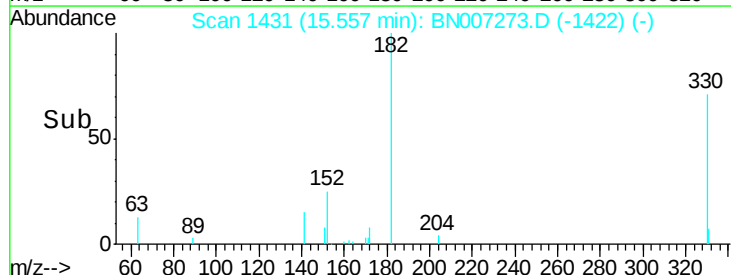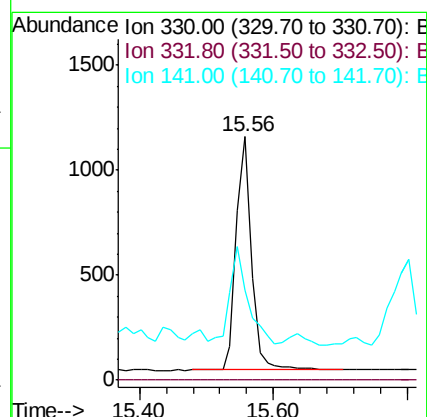



#15

2-Fluorobiphenyl

Concen: 0.236 ng

RT: 12.67 min Scan# 1172

Delta R.T. 0.00 min

Lab File: BN007273.D

Acq: 20 Aug 2019 20:15

Instrument :

BNA_N

ClientSampleId :

S301-J-1.5-2.0-081919-FD


Tgt Ion:172 Resp: 11516

Ion Ratio Lower Upper

172 100

171 35.8 28.6 43.0




170 23.1 18.7 28.1



Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

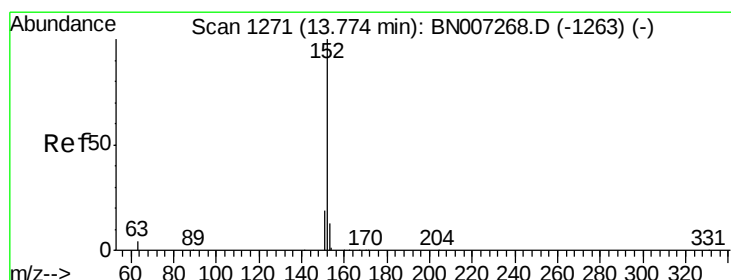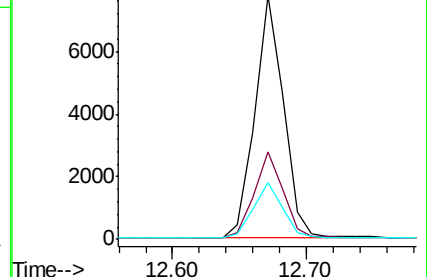

#16

Acenaphthylene

Concen: 0.149 ng

RT: 13.77 min Scan# 1271

Delta R.T. 0.00 min

Lab File: BN007273.D

Acq: 20 Aug 2019 20:15


Tgt Ion:152 Resp: 8980

Ion Ratio Lower Upper

152 100

151 19.4 15.4 23.2



153 13.4 10.1 15.1




Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

Ion 153.00 (152.70 to 153.70): E

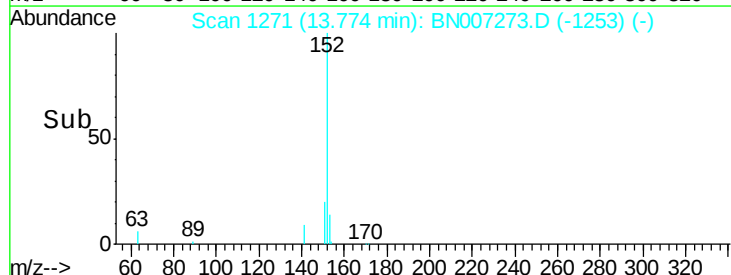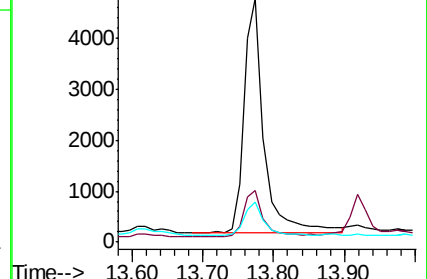



#17

Acenaphthene

Concen: 0.184 ng

RT: 14.12 min Scan# 1302

Delta R.T. 0.00 min

Lab File: BN007273.D

Acq: 20 Aug 2019 20:15

Instrument :

BNA_N

ClientSampleId :

S301-J-1.5-2.0-081919-FD


Tgt Ion:154 Resp: 7061

Ion Ratio Lower Upper




154 100

153 113.6 89.9 134.9

152 59.1 43.9 65.9



Abundance Ion 154.00 (153.70 to 154.70): E
Ion 153.00 (152.70 to 153.70): E
Ion 152.00 (151.70 to 152.70): E

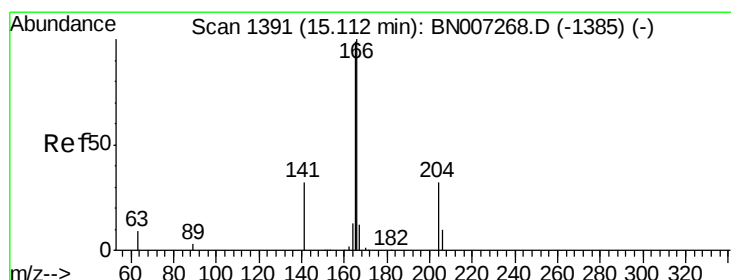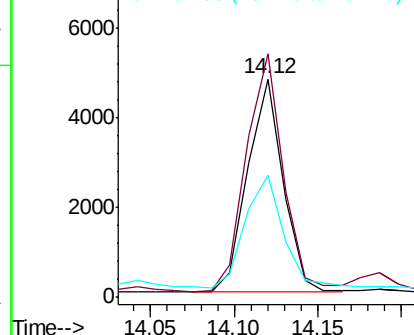

#18

Fluorene

Concen: 0.146 ng

RT: 15.11 min Scan# 1391

Delta R.T. 0.00 min

Lab File: BN007273.D

Acq: 20 Aug 2019 20:15


Tgt Ion:166 Resp: 7308

Ion Ratio Lower Upper



166 100


165 99.5 78.3 117.5

167 14.5 11.1 16.7



Abundance Ion 166.00 (165.70 to 166.70): E
Ion 165.00 (164.70 to 165.70): E
Ion 167.00 (166.70 to 167.70): E

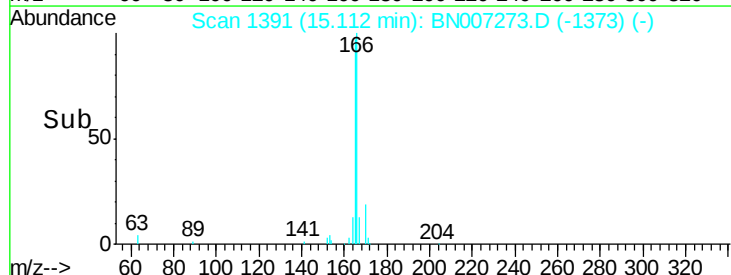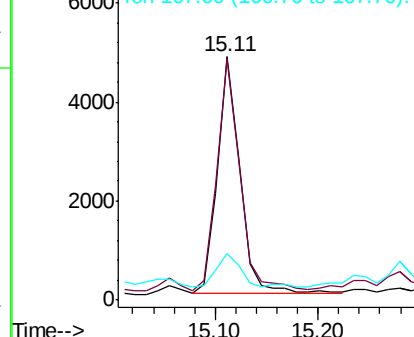



#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 16.81 min Scan# 1547

Delta R.T. 0.00 min

Lab File: BN007273.D

Acq: 20 Aug 2019 20:15

Instrument :

BNA_N

ClientSampleId :

S301-J-1.5-2.0-081919-FD


Tgt Ion:188 Resp: 26712

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0




80 6.8 5.2 7.8

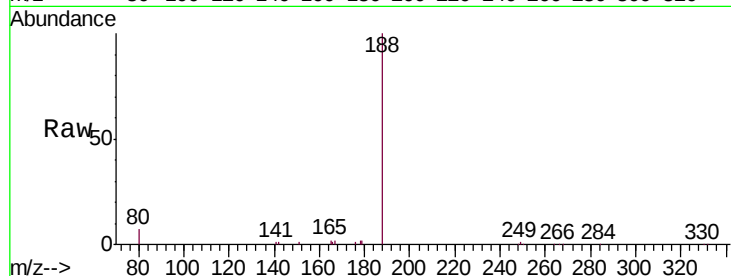

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BNC

Ion 80.00 (79.70 to 80.70): BNC

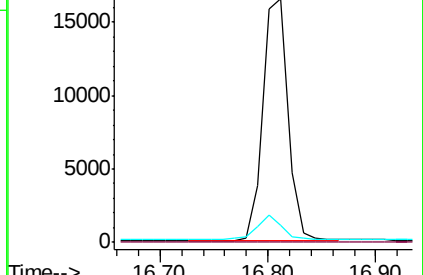

#23

Phenanthrene

Concen: 1.759 ng

RT: 16.84 min Scan# 1550

Delta R.T. 0.00 min

Lab File: BN007273.D

Acq: 20 Aug 2019 20:15


Tgt Ion:178 Resp: 147286

Ion Ratio Lower Upper

178 100

176 19.0 15.2 22.8



179 15.2 12.3 18.5




Abundance Ion 178.00 (177.70 to 178.70): E

Ion 176.00 (175.70 to 176.70): E

Ion 179.00 (178.70 to 179.70): E

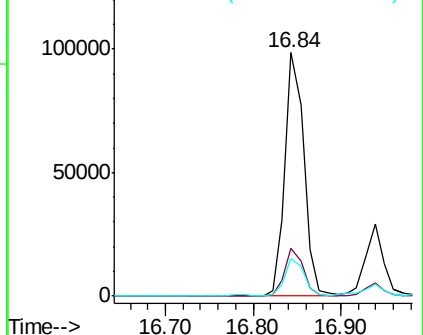



#24

Anthracene

Concen: 0.515 ng

RT: 16.94 min Scan# 1559

Delta R.T. 0.00 min

Lab File: BN007273.D

Acq: 20 Aug 2019 20:15

Instrument :

BNA_N

ClientSampleId :

S301-J-1.5-2.0-081919-FD


Tgt Ion:178 Resp: 38861

Ion Ratio Lower Upper

178 100

176 18.3 14.3 21.5




179 18.0 12.3 18.5



Abundance Ion 178.00 (177.70 to 178.70): E

Ion 176.00 (175.70 to 176.70): E

Ion 179.00 (178.70 to 179.70): E

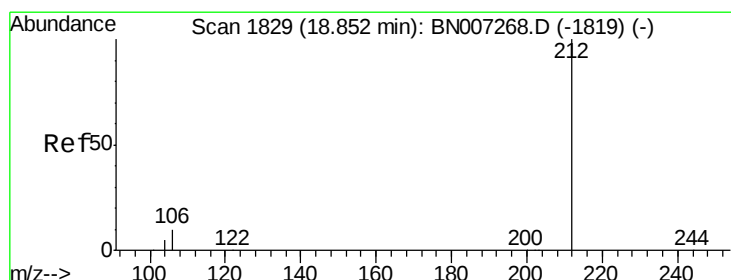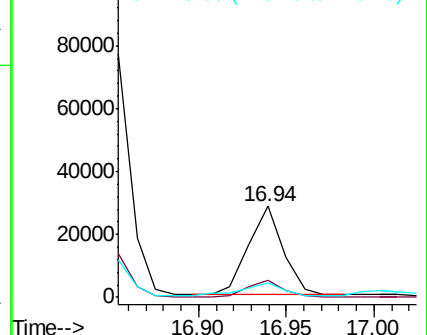

#25

Fluoranthene-d10

Concen: 0.232 ng

RT: 18.85 min Scan# 1829

Delta R.T. 0.00 min

Lab File: BN007273.D

Acq: 20 Aug 2019 20:15


Tgt Ion:212 Resp: 19688

Ion Ratio Lower Upper

212 100

106 10.5 8.2 12.4



104 6.7 4.7 7.1




Abundance Ion 212.00 (211.70 to 212.70): E

Ion 106.00 (105.70 to 106.70): E

Ion 104.00 (103.70 to 104.70): E

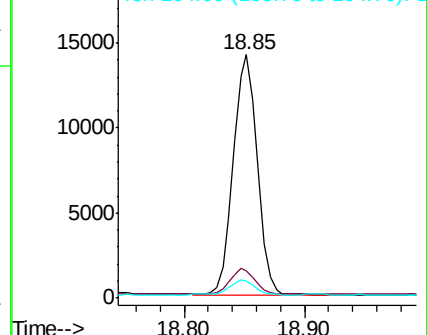

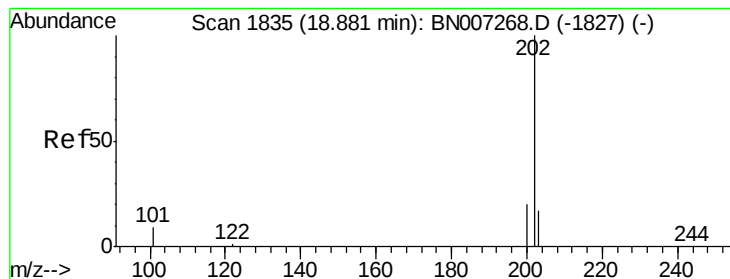

#26

Fluoranthene

Concen: 6.068 ng

RT: 18.88 min Scan# 1835

Delta R.T. 0.00 min

Lab File: BN007273.D

Acq: 20 Aug 2019 20:15


Instrument :

BNA_N




ClientSampleId :

S301-J-1.5-2.0-081919-FD

Tgt Ion:	202	Resp:	615357
Ion	Ratio	Lower	Upper
202	100		
101	9.0	7.2	10.8
203	17.4	13.8	20.6

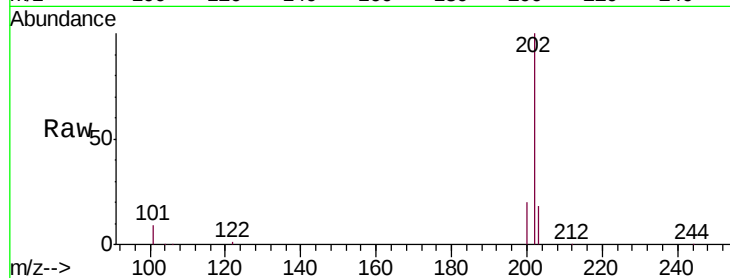

Abundance Ion 202.00 (201.70 to 202.70): E
Ion 101.00 (100.70 to 101.70): E
Ion 203.00 (202.70 to 203.70): E

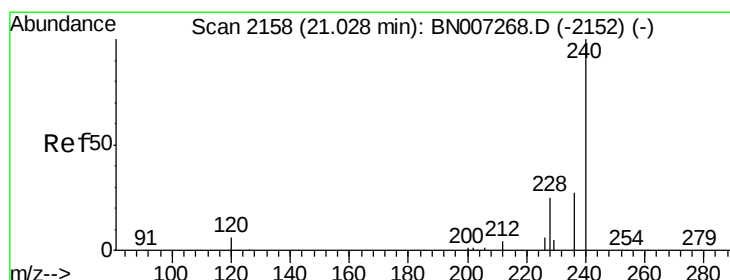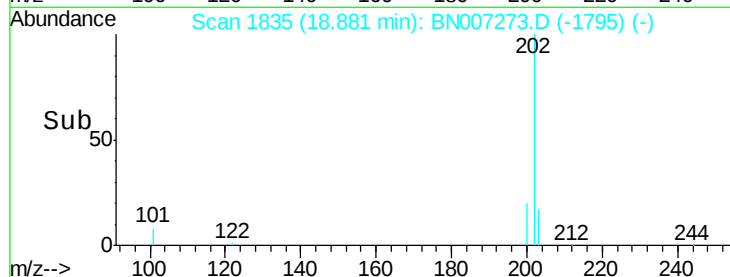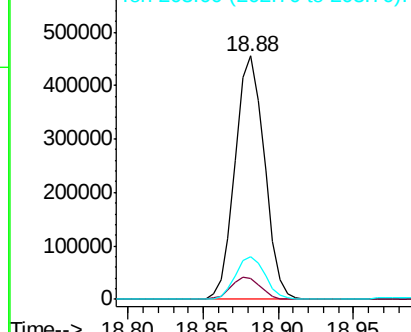

#27

Chrysene-d12

Concen: 0.400 ng


RT: 21.03 min Scan# 2158

Delta R.T. 0.00 min



Lab File: BN007273.D


Acq: 20 Aug 2019 20:15

Tgt Ion:	240	Resp:	27931
Ion	Ratio	Lower	Upper
240	100		
120	8.3	5.6	8.4
236	27.8	21.6	32.4

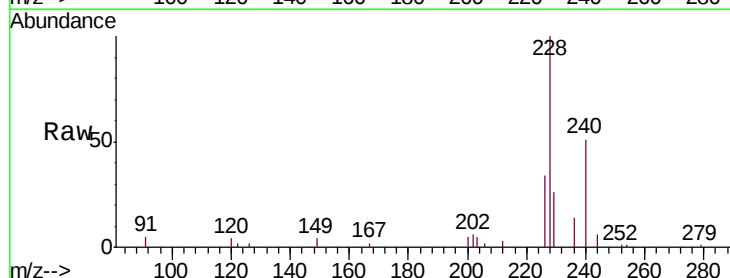

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E



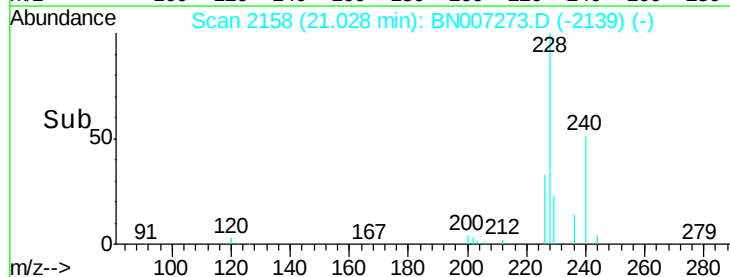
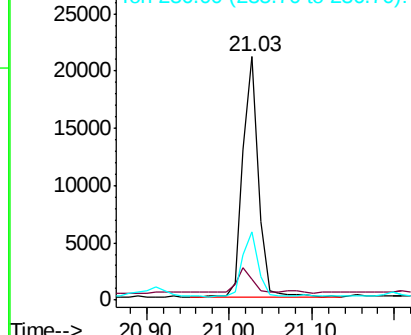




#28
 Pyrene
 Concen: 5.230 ng
 RT: 19.24 min Scan# 1908
 Delta R.T. 0.00 min
 Lab File: BN007273.D
 Acq: 20 Aug 2019 20:15




Instrument :
 BNA_N
 ClientSampleId :
 S301-J-1.5-2.0-081919-FD


Tgt Ion: 202 Resp: 546302
 Ion Ratio Lower Upper
 202 100
 200 21.0 16.7 25.1
 203 22.4 13.9 20.9#

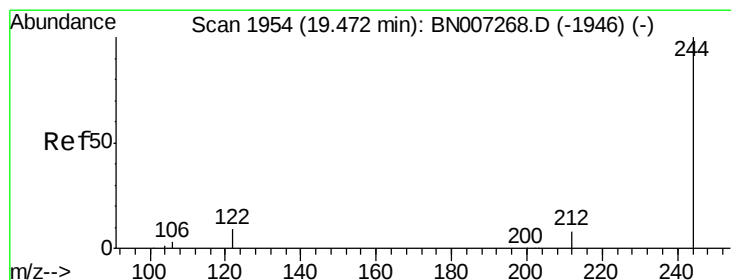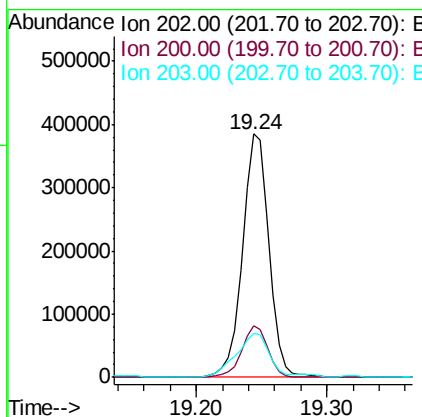

#29
 Terphenyl-d14
 Concen: 0.205 ng
 RT: 19.47 min Scan# 1954
 Delta R.T. 0.00 min
 Lab File: BN007273.D
 Acq: 20 Aug 2019 20:15

Tgt Ion: 244 Resp: 14352
 Ion Ratio Lower Upper
 244 100
 212 9.0 6.5 9.7
 122 12.0 7.9 11.9#

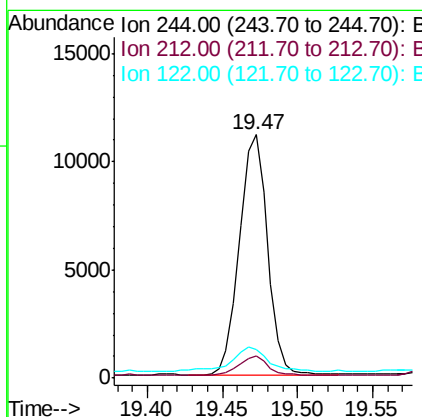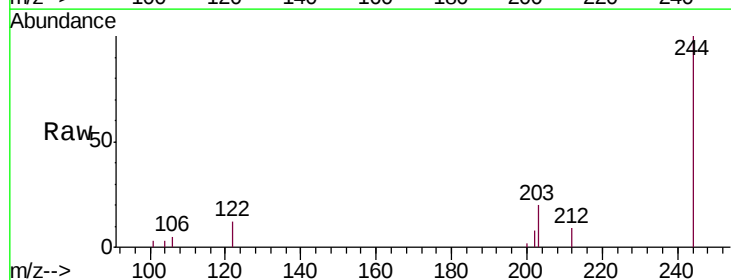



#30

Benzo(a)anthracene

Concen: 3.665 ng

RT: 21.01 min Scan# 2156

Delta R.T. -0.01 min

Lab File: BN007273.D

Acq: 20 Aug 2019 20:15

Instrument :

BNA_N

ClientSampleId :

S301-J-1.5-2.0-081919-FD


Tgt Ion:228 Resp: 380642

Ion Ratio Lower Upper

228 100

226 28.4 20.6 30.8




229 20.3 16.9 25.3



Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

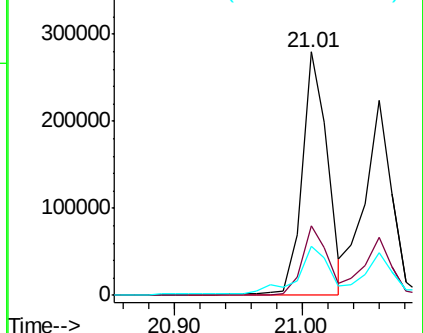

#31

Chrysene

Concen: 2.771 ng

RT: 21.06 min Scan# 2161

Delta R.T. 0.00 min

Lab File: BN007273.D

Acq: 20 Aug 2019 20:15


Tgt Ion:228 Resp: 293734

Ion Ratio Lower Upper

228 100

226 29.9 24.6 36.8



229 22.1 15.6 23.4




Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

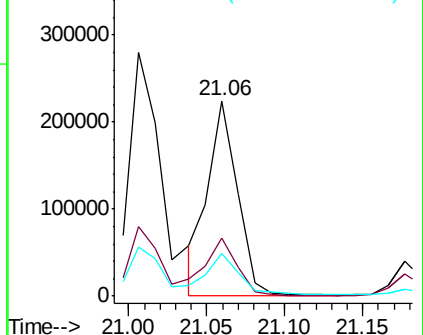



#32

Bis(2-ethylhexyl)phthalate

Concen: 0.941 ng

RT: 20.97 min Scan# 2153

Delta R.T. -0.01 min

Lab File: BN007273.D

Acq: 20 Aug 2019 20:15

Instrument :

BNA_N

ClientSampleId :

S301-J-1.5-2.0-081919-FD


Tgt Ion:149 Resp: 39063

Ion Ratio Lower Upper

149 100

167 28.6 23.8 35.6




279 4.6 3.8 5.8



Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

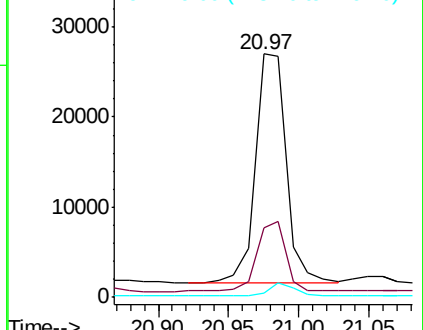

#33

Indeno(1,2,3-cd)pyrene

Concen: 1.846 ng

RT: 25.20 min Scan# 3104

Delta R.T. -0.01 min

Lab File: BN007273.D

Acq: 20 Aug 2019 20:15


Tgt Ion:276 Resp: 235423

Ion Ratio Lower Upper

276 100

138 18.0 17.1 25.7



277 24.4 20.1 30.1




Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E




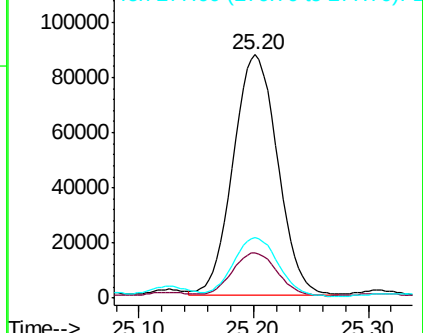


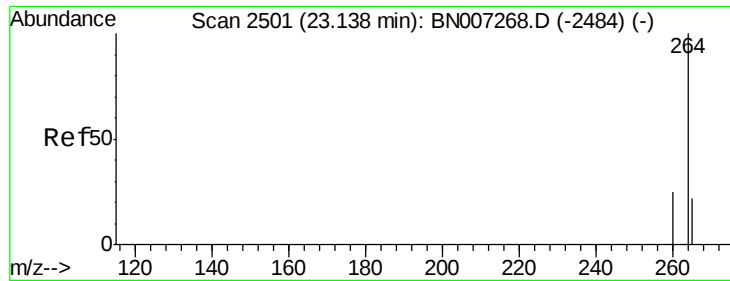

#34
Perylene-d12
Concen: 0.400 ng
RT: 23.13 min Scan# 2500
Delta R.T. -0.00 min
Lab File: BN007273.D
Acq: 20 Aug 2019 20:15




Instrument :
BNA_N
ClientSampleId :
S301-J-1.5-2.0-081919-FD


Tgt Ion: 264 Resp: 30736
Ion Ratio Lower Upper
264 100
260 26.2 20.1 30.1
265 41.6 29.0 43.6

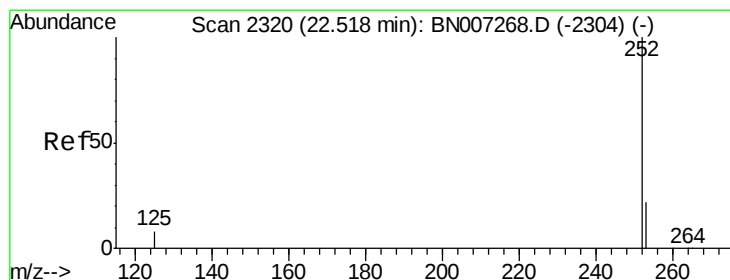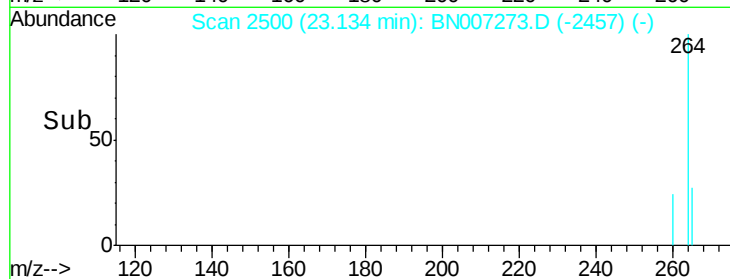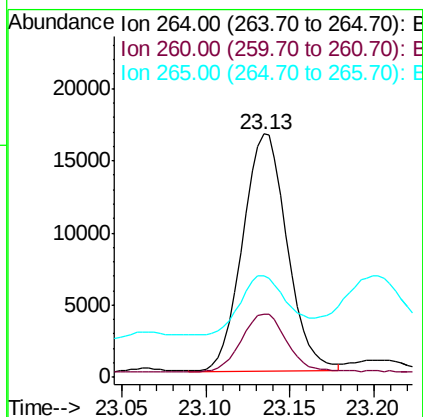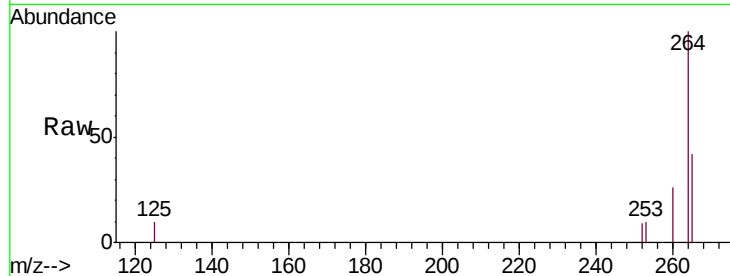

#35
Benzo(b)fluoranthene
Concen: 4.306 ng
RT: 22.52 min Scan# 2320
Delta R.T. 0.00 min
Lab File: BN007273.D
Acq: 20 Aug 2019 20:15

Tgt Ion: 252 Resp: 493381
Ion Ratio Lower Upper
252 100
253 22.7 18.5 27.7
125 9.6 7.8 11.6

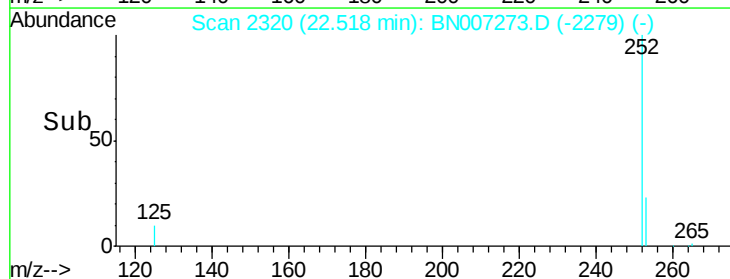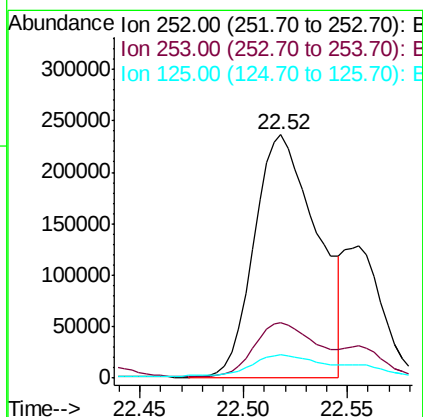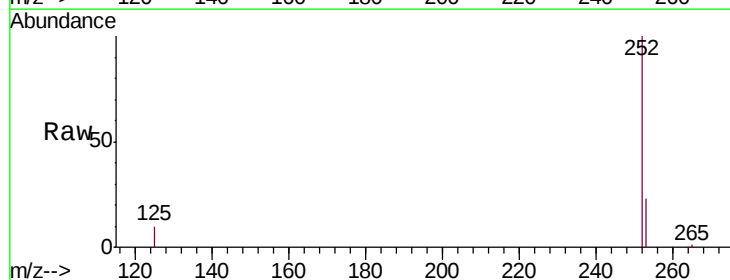

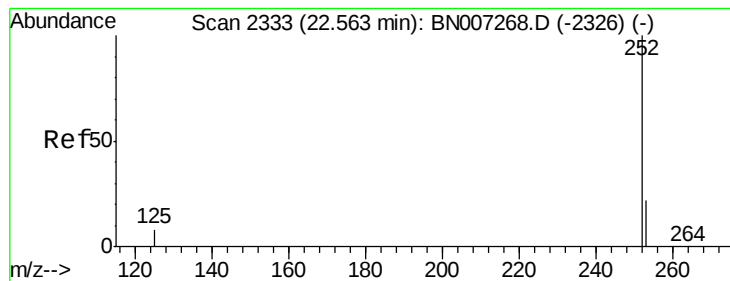

#36

Benzo(k)fluoranthene

Concen: 4.395 ng

RT: 22.52 min Scan# 2320

Delta R.T. -0.04 min

Lab File: BN007273.D

Acq: 20 Aug 2019 20:15

Instrument :

BNA_N

ClientSampleId :

S301-J-1.5-2.0-081919-FD


Tgt Ion:252 Resp: 493381

Ion Ratio Lower Upper




252 100

253 22.7 18.4 27.6

125 9.6 8.0 12.0

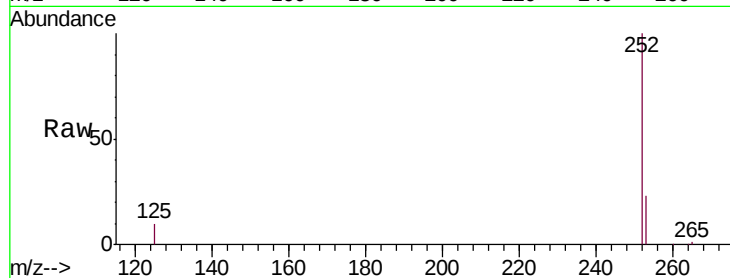

Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

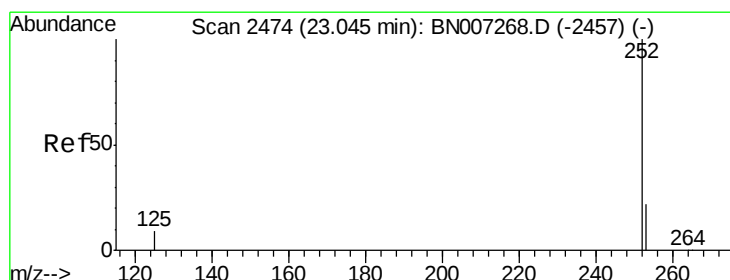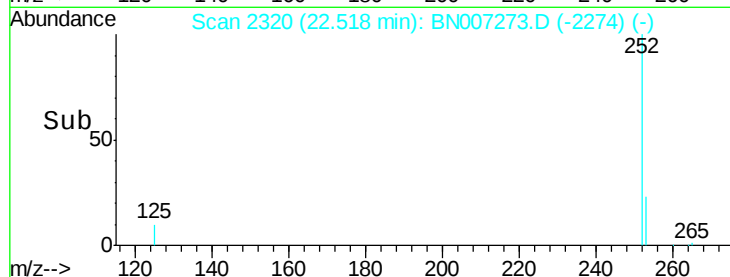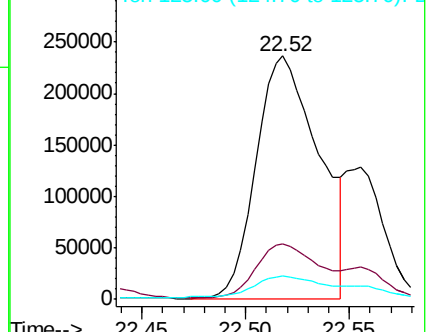

#37

Benzo(a)pyrene

Concen: 3.384 ng

RT: 23.05 min Scan# 2474

Delta R.T. 0.00 min

Lab File: BN007273.D

Acq: 20 Aug 2019 20:15


Tgt Ion:252 Resp: 349427

Ion Ratio Lower Upper



252 100


253 23.1 18.7 28.1

125 9.7 8.7 13.1

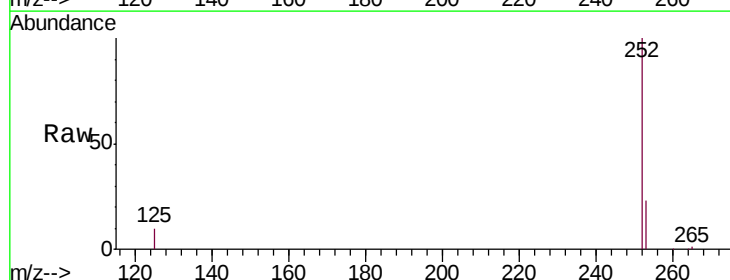

Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

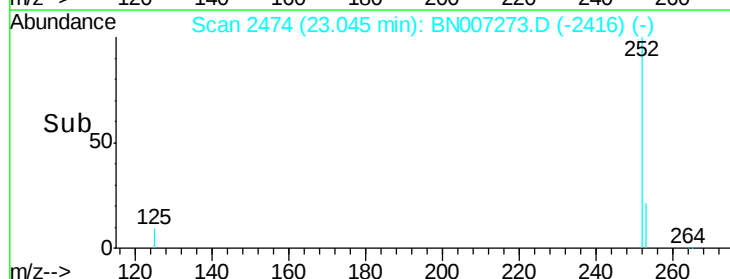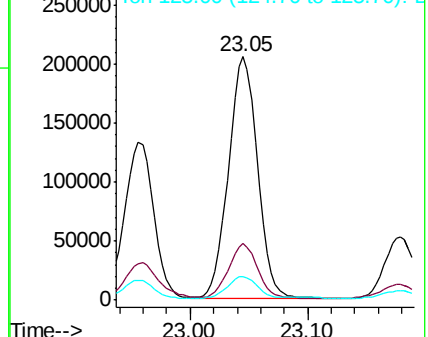



#38

Dibenzo(a,h)anthracene

Concen: 0.549 ng

RT: 25.21 min Scan# 3107

Delta R.T. -0.01 min

Lab File: BN007273.D

Acq: 20 Aug 2019 20:15

Instrument :

BNA_N

ClientSampleId :

S301-J-1.5-2.0-081919-FD


Tgt Ion: 278 Resp: 59595

Ion Ratio Lower Upper

278 100

139 18.0 11.8 17.8#

279 27.6 19.8 29.6






Abundance

Ion 278.00 (277.70 to 278.70): E

Ion 139.00 (138.70 to 139.70): E

Ion 279.00 (278.70 to 279.70): E

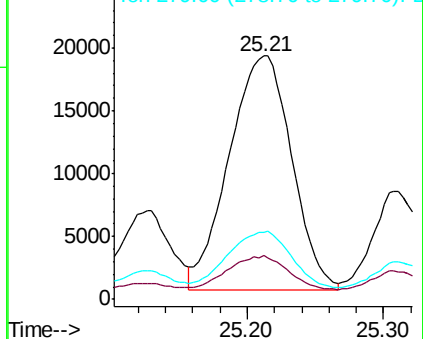

#39

Benzo(g,h,i)perylene

Concen: 2.065 ng

RT: 25.83 min Scan# 3287

Delta R.T. -0.00 min

Lab File: BN007273.D

Acq: 20 Aug 2019 20:15


Tgt Ion: 276 Resp: 226506

Ion Ratio Lower Upper

276 100

277 24.5 19.5 29.3

138 18.9 15.3 22.9



Abundance

Ion 276.00 (275.70 to 276.70): E

Ion 277.00 (276.70 to 277.70): E

Ion 138.00 (137.70 to 138.70): E

