


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN082019\
 Data File : BN007260.D
 Acq On : 20 Aug 2019 11:20
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN082019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Aug 20 18:52:43 2019

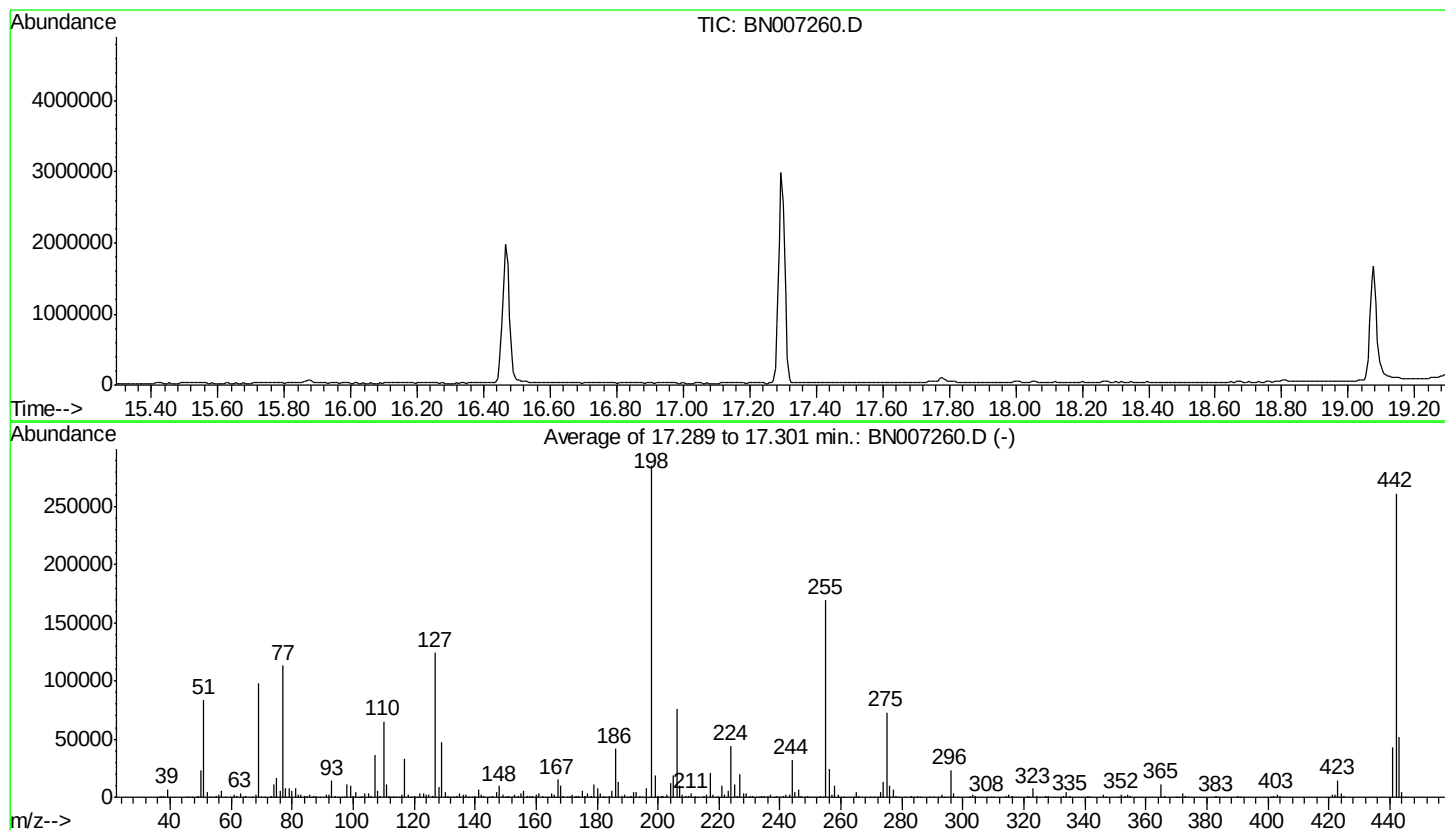

AutoFind: Scans 2457, 2458, 2459; Background Corrected with Scan 2450

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.4	83802	PASS
68	69	0.00	2	1.9	1873	PASS
69	198	0.00	100	34.4	98102	PASS
70	69	0.00	2	0.4	393	PASS
127	198	10	80	43.5	123968	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	285269	PASS
199	198	5	9	6.6	18715	PASS
275	198	10	60	25.6	72968	PASS
365	198	1	100	3.9	11110	PASS
441	198	0.01	100	15.2	43341	PASS
442	198	50	100	91.6	261418	PASS
443	442	15	24	19.8	51826	PASS