


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN082019\
 Data File : BN007275.D
 Acq On : 21 Aug 2019 02:25
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN082019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Aug 20 18:52:43 2019

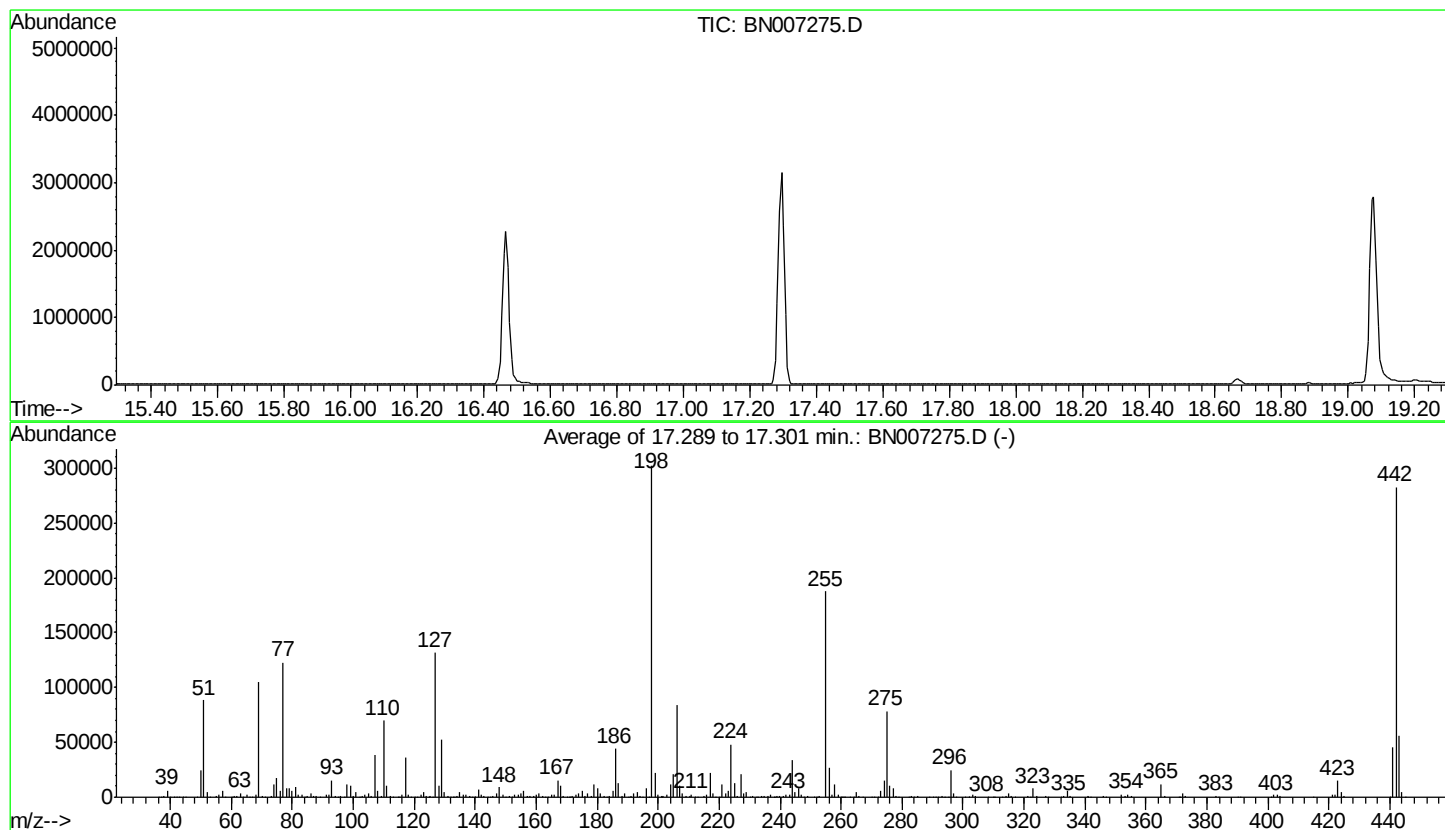

AutoFind: Scans 2457, 2458, 2459; Background Corrected with Scan 2450

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.3	88464	PASS
68	69	0.00	2	2.0	2058	PASS
69	198	0.00	100	34.8	105265	PASS
70	69	0.00	2	0.8	799	PASS
127	198	10	80	43.5	131554	PASS
197	198	0.00	2	0.2	524	PASS
198	198	100	100	100.0	302144	PASS
199	198	5	9	7.2	21778	PASS
275	198	10	60	26.0	78418	PASS
365	198	1	100	3.9	11843	PASS
441	198	0.01	100	15.0	45181	PASS
442	198	50	100	93.6	282666	PASS
443	442	15	24	19.9	56237	PASS