

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN082020\
 Data File : BN011532.D
 Acq On : 20 Aug 2020 20:17
 Operator : CG/JU
 Sample : PB131082BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK82

Quant Time: Aug 21 03:15:29 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081420MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Aug 21 03:13:08 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.42	152	168222	20.00	ng/ul	0.00
18) Naphthalene-d8	10.16	136	617435	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.06	164	382139	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.82	188	817420	20.00	ng/ul	0.00
78) Chrysene-d12	21.03	240	843024	20.00	ng/ul	0.00
86) Perylene-d12	23.14	264	791502	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.10	96	22657	6.46	ng/uL	0.00
5) Phenol-d5	6.63	99	405483	34.09	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.78	67	217388	35.85	ng/ul	0.00
9) 2-Chlorophenol-d4	6.97	132	367337	34.45	ng/ul	0.00
13) 4-Methylphenol-d8	8.13	113	326441	33.80	ng/ul	0.00
19) Nitrobenzene-d5	8.56	128	171241	35.78	ng/ul	0.00
22) 2-Nitrophenol-d4	9.27	143	191333	35.55	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.80	165	343256	33.76	ng/ul	0.00
29) 4-Chloroaniline-d4	10.32	131	450875	37.08	ng/ul	0.00
44) Dimethylphthalate-d6	13.48	166	1030750	34.64	ng/ul	0.00
47) Acenaphthylene-d8	13.75	160	1271102	35.50	ng/ul	0.00
52) 4-Nitrophenol-d4	14.29	143	150569	29.87	ng/ul	0.00
58) Fluorene-d10	15.06	176	876242	33.64	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.20	200	140082	25.84	ng/ul	0.00
71) Anthracene-d10	16.91	188	1354528	34.69	ng/ul	0.00
79) Pyrene-d10	19.22	212	1553488	35.87	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.00	264	1433109	32.60	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
15) N-Nitroso-di-n-propylamine	8.13	70	8435	1.247	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN082020\
Data File : BN011532.D
Acq On : 20 Aug 2020 20:17
Operator : CG/JU
Sample : PB131082BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK82

Quant Time: Aug 21 03:15:29 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081420MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Aug 21 03:13:08 2020
Response via : Initial Calibration

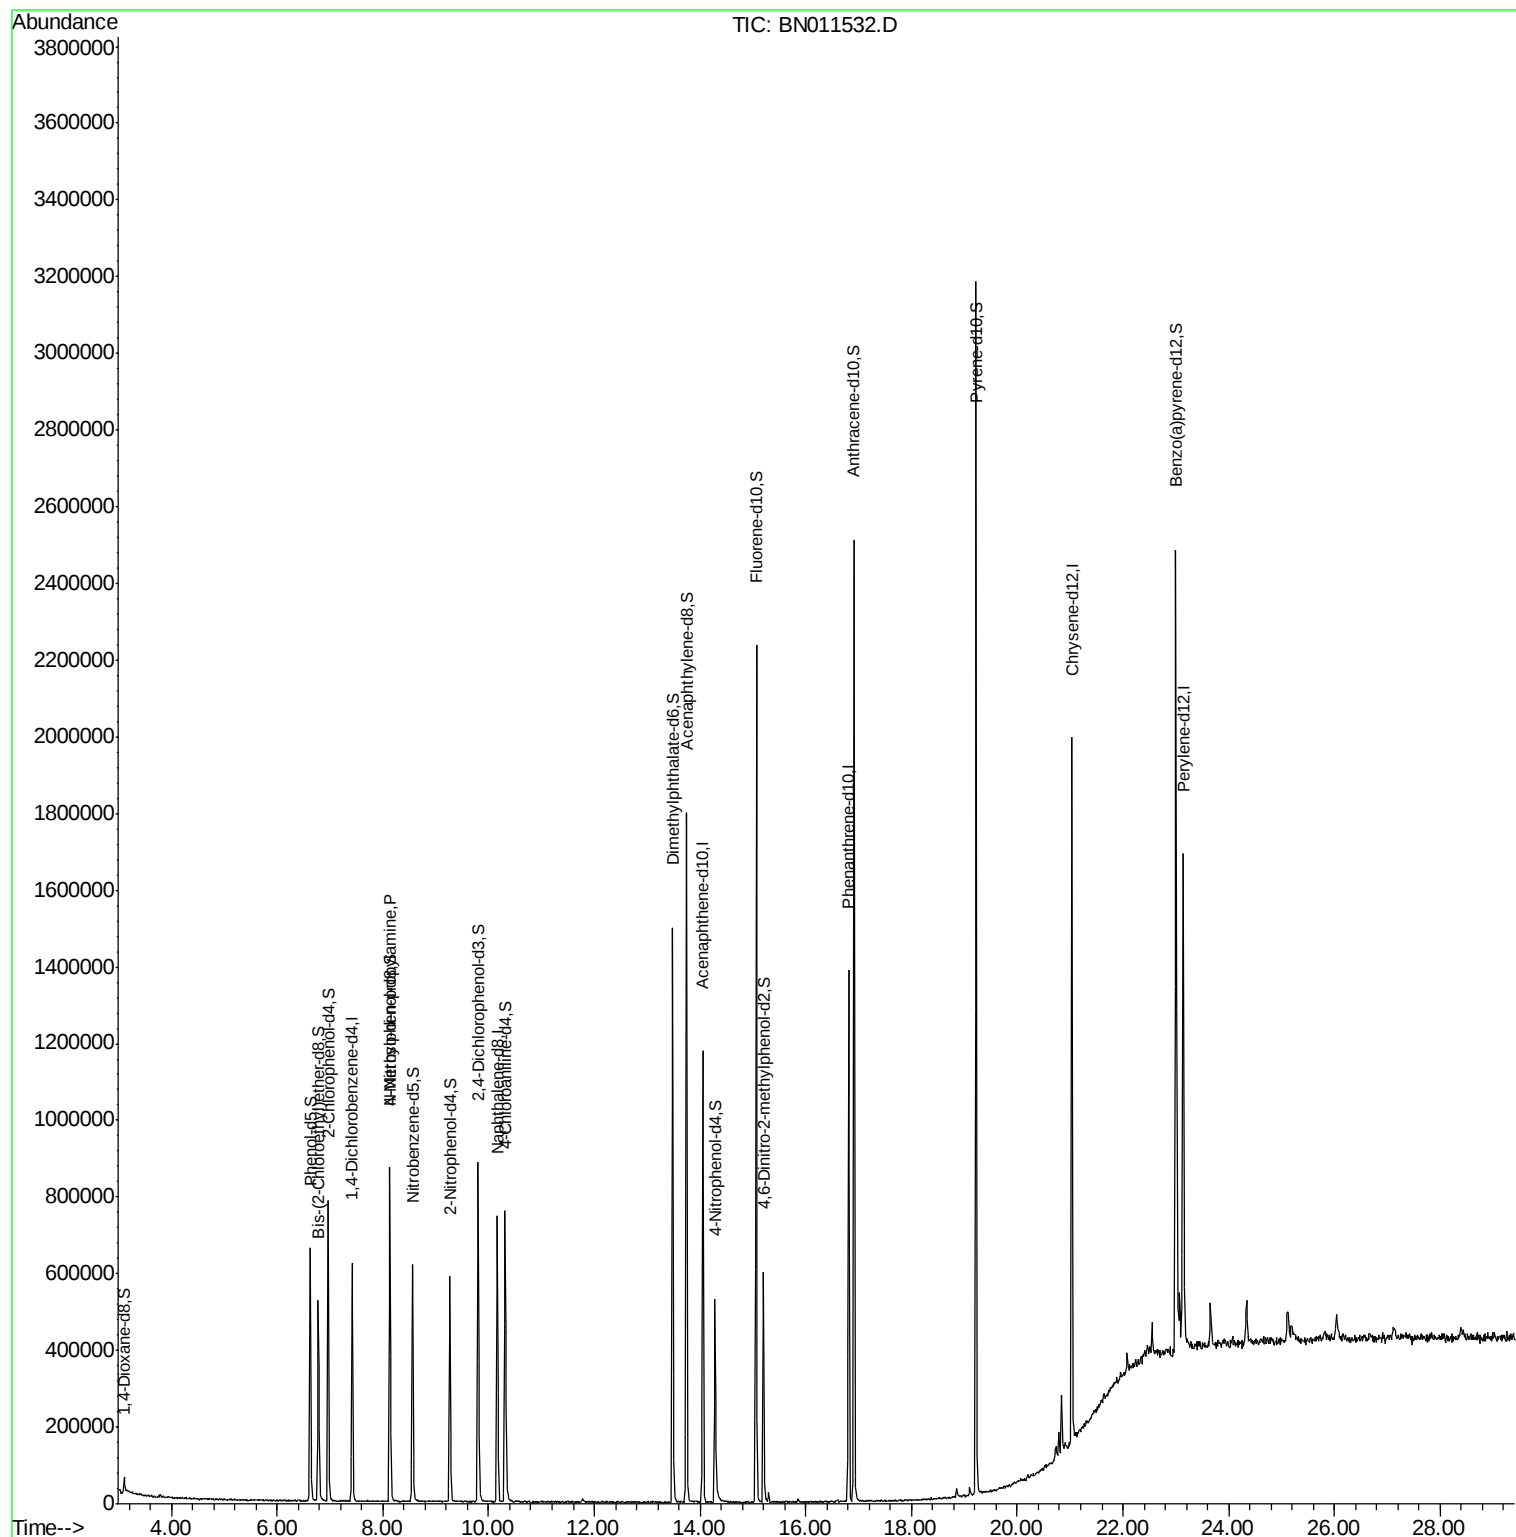

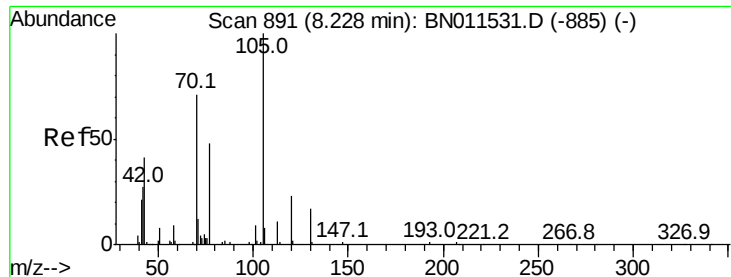

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.247 ng/ul
 RT: 8.13 min Scan# 875
 Delta R.T. -0.09 min
 Lab File: BN011532.D
 Acq: 20 Aug 2020 20:17

Instrument :
 BNA_N
 ClientSampleId :
 SBLK82

Tot Ion	Ion	Ratio	Lower	Upper
70	100			
42	230.2	27.2	40.8#	
101	0.0	8.3	12.5#	
130	0.0	19.4	29.0#	

