

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN082020\
 Data File : BN011535.D
 Acq On : 20 Aug 2020 22:04
 Operator : CG/JU
 Sample : L3668-21
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBFX2

Quant Time: Aug 21 03:15:47 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081420MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Aug 21 03:13:08 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.42	152	112921	20.00	ng/ul	0.00
18) Naphthalene-d8	10.16	136	436761	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.06	164	290480	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.81	188	597822	20.00	ng/ul	0.00
78) Chrysene-d12	21.03	240	642029	20.00	ng/ul	0.00
86) Perylene-d12	23.14	264	600237	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.11	96	12330	5.24	ng/uL	0.00
5) Phenol-d5	6.63	99	45913	5.75	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.78	67	112609	27.67	ng/ul	0.00
9) 2-Chlorophenol-d4	6.97	132	174466	24.38	ng/ul	0.00
13) 4-Methylphenol-d8	8.13	113	86164	13.29	ng/ul	0.00
19) Nitrobenzene-d5	8.56	128	107708	31.82	ng/ul	0.00
22) 2-Nitrophenol-d4	9.28	143	98701	25.93	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.80	165	169454	23.56	ng/ul	0.00
29) 4-Chloroaniline-d4	10.33	131	13361	1.55	ng/ul	0.02
44) Dimethylphthalate-d6	13.48	166	709753	31.38	ng/ul	0.00
47) Acenaphthylene-d8	13.74	160	804623	29.56	ng/ul	0.00
52) 4-Nitrophenol-d4	14.30	143	14362	3.75	ng/ul	0.01
58) Fluorene-d10	15.06	176	544495	27.50	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.20	200	88572	22.34	ng/ul	0.00
71) Anthracene-d10	16.91	188	930824	32.59	ng/ul	0.00
79) Pyrene-d10	19.22	212	1294081	39.24	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.01	264	1019459	30.58	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.53	163	223276	9.617	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN082020\
Data File : BN011535.D
Acq On : 20 Aug 2020 22:04
Operator : CG/JU
Sample : L3668-21
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBFX2

Quant Time: Aug 21 03:15:47 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081420MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Aug 21 03:13:08 2020
Response via : Initial Calibration

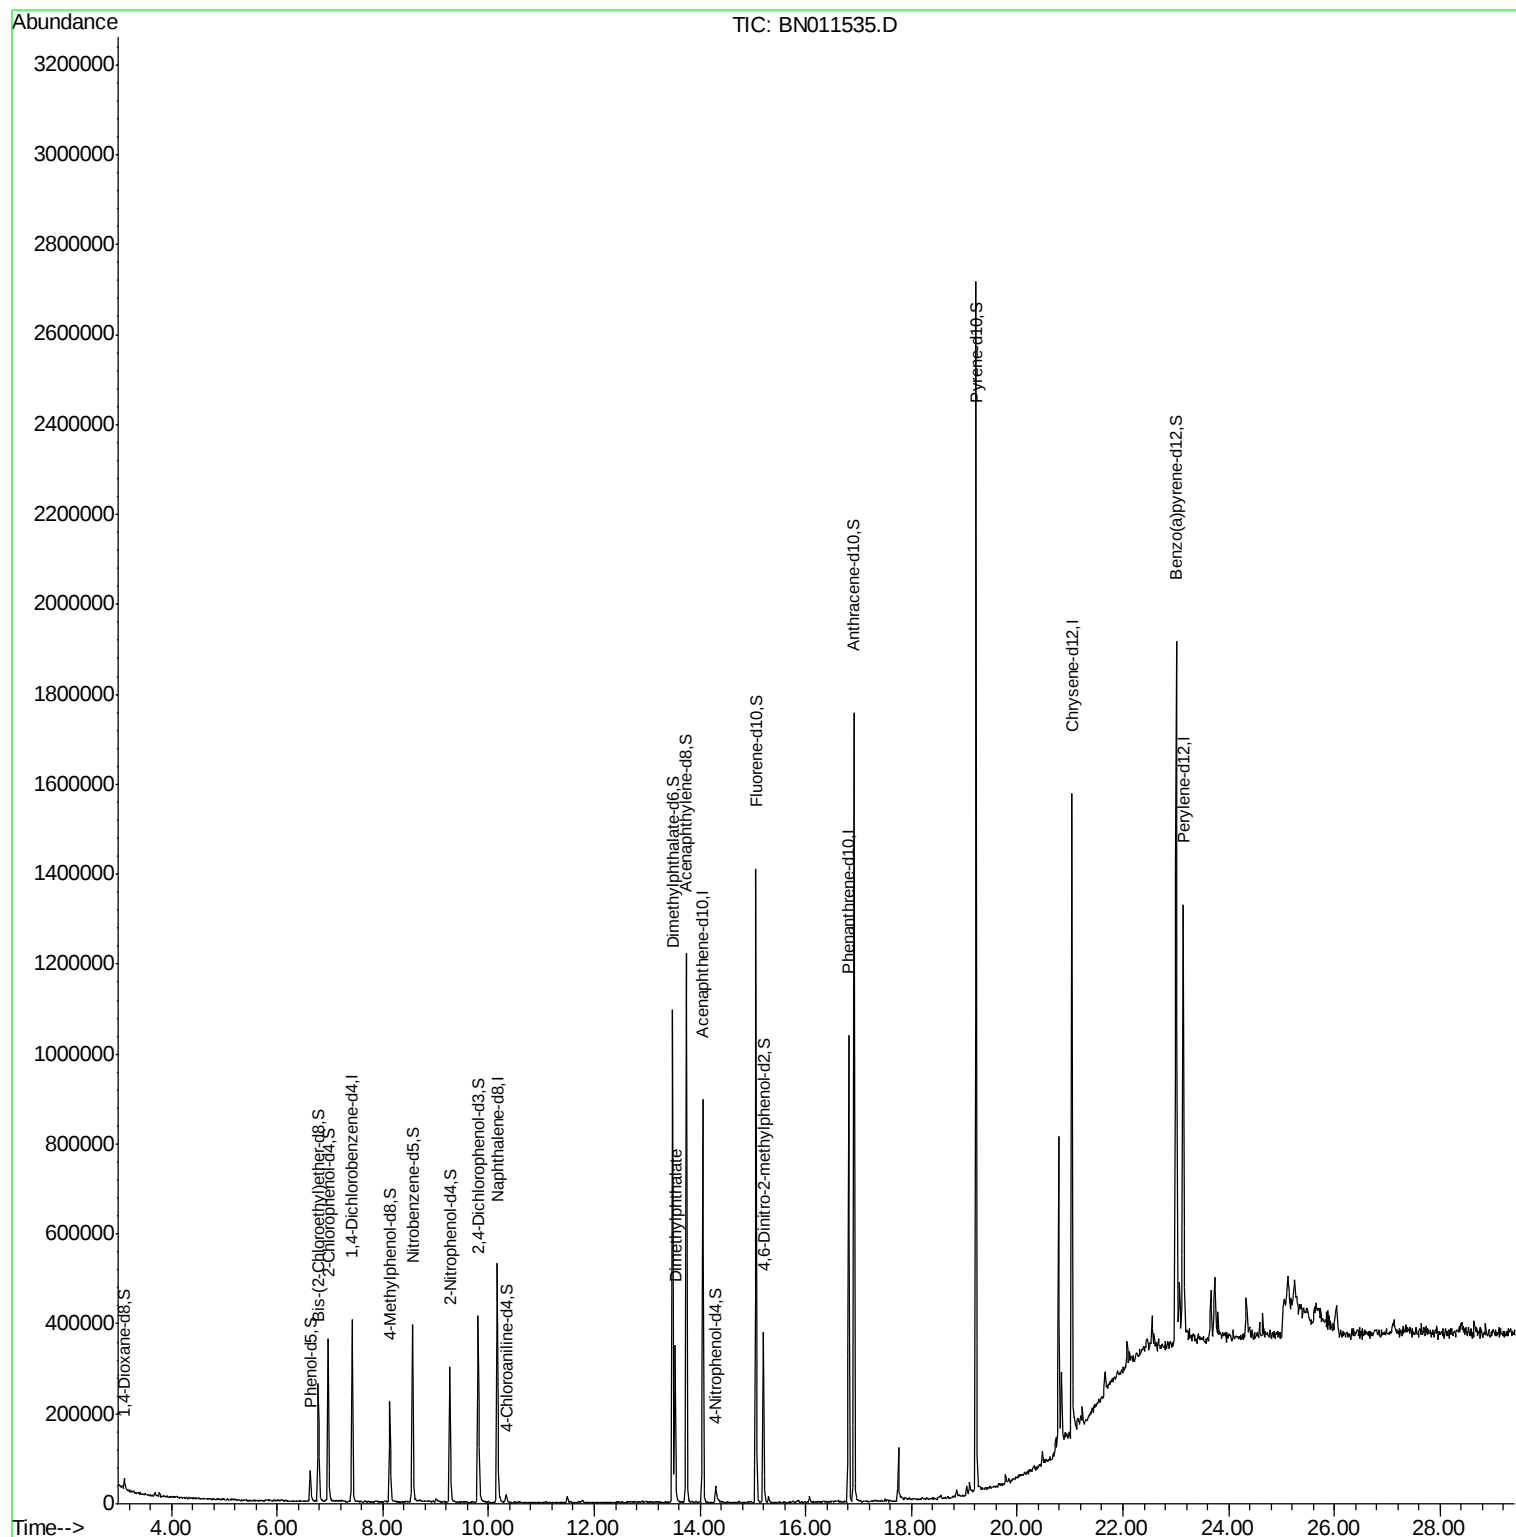


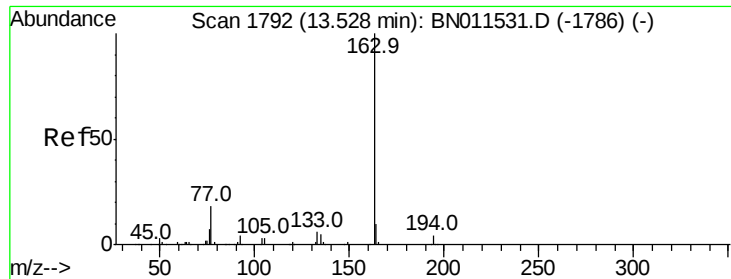

#45
 Dimethylphthalate
 Concen: 9.617 ng/ul
 RT: 13.53 min Scan# 1792
 Delta R.T. 0.00 min
 Lab File: BN011535.D
 Acq: 20 Aug 2020 22:04

Instrument :
 BNA_N
 ClientSampleId :
 DBFX2

Tot Ion	Ratio	Lower	Upper
163	100		
194	4.3	3.8	5.6
164	9.5	8.7	13.1

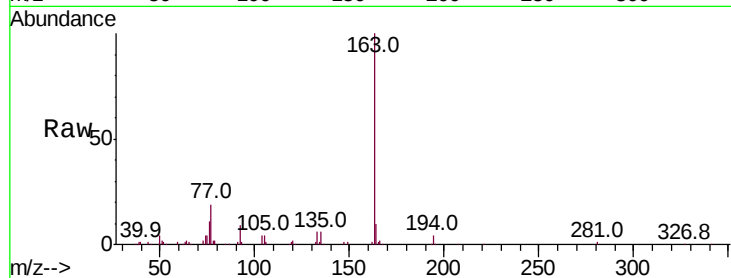

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

