

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN082020\
 Data File : BN011539.D
 Acq On : 21 Aug 2020 00:27
 Operator : CG/JU
 Sample : L3708-14
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBFW2

Quant Time: Aug 21 03:16:10 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081420MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Aug 21 03:13:08 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.42	152	178648	20.00	ng/ul	0.00
18) Naphthalene-d8	10.16	136	670259	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.06	164	409068	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.81	188	894557	20.00	ng/ul	0.00
78) Chrysene-d12	21.03	240	897592	20.00	ng/ul	0.00
86) Perylene-d12	23.13	264	886357	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.10	96	21043	5.65	ng/uL	0.00
5) Phenol-d5	6.63	99	76164	6.03	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.78	67	170802	26.52	ng/ul	0.00
9) 2-Chlorophenol-d4	6.96	132	232591	20.54	ng/ul	0.00
13) 4-Methylphenol-d8	8.13	113	137945	13.45	ng/ul	0.00
19) Nitrobenzene-d5	8.56	128	137349	26.44	ng/ul	0.00
22) 2-Nitrophenol-d4	9.27	143	149948	25.66	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.80	165	253830	22.99	ng/ul	0.00
29) 4-Chloroaniline-d4	10.32	131	24285	1.84	ng/ul	0.00
44) Dimethylphthalate-d6	13.48	166	861796	27.06	ng/ul	0.00
47) Acenaphthylene-d8	13.74	160	997020	26.01	ng/ul	0.00
52) 4-Nitrophenol-d4	14.29	143	16791	3.11	ng/ul	0.00
58) Fluorene-d10	15.06	176	777699	27.89	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.20	200	127867	21.55	ng/ul	0.00
71) Anthracene-d10	16.91	188	1280603	29.97	ng/ul	0.00
79) Pyrene-d10	19.22	212	1455807	31.57	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.00	264	1336115	27.14	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.53	163	122687	3.753	ng/ul	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN082020\
Data File : BN011539.D
Acq On : 21 Aug 2020 00:27
Operator : CG/JU
Sample : L3708-14
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBFW2

Quant Time: Aug 21 03:16:10 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081420MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Aug 21 03:13:08 2020
Response via : Initial Calibration

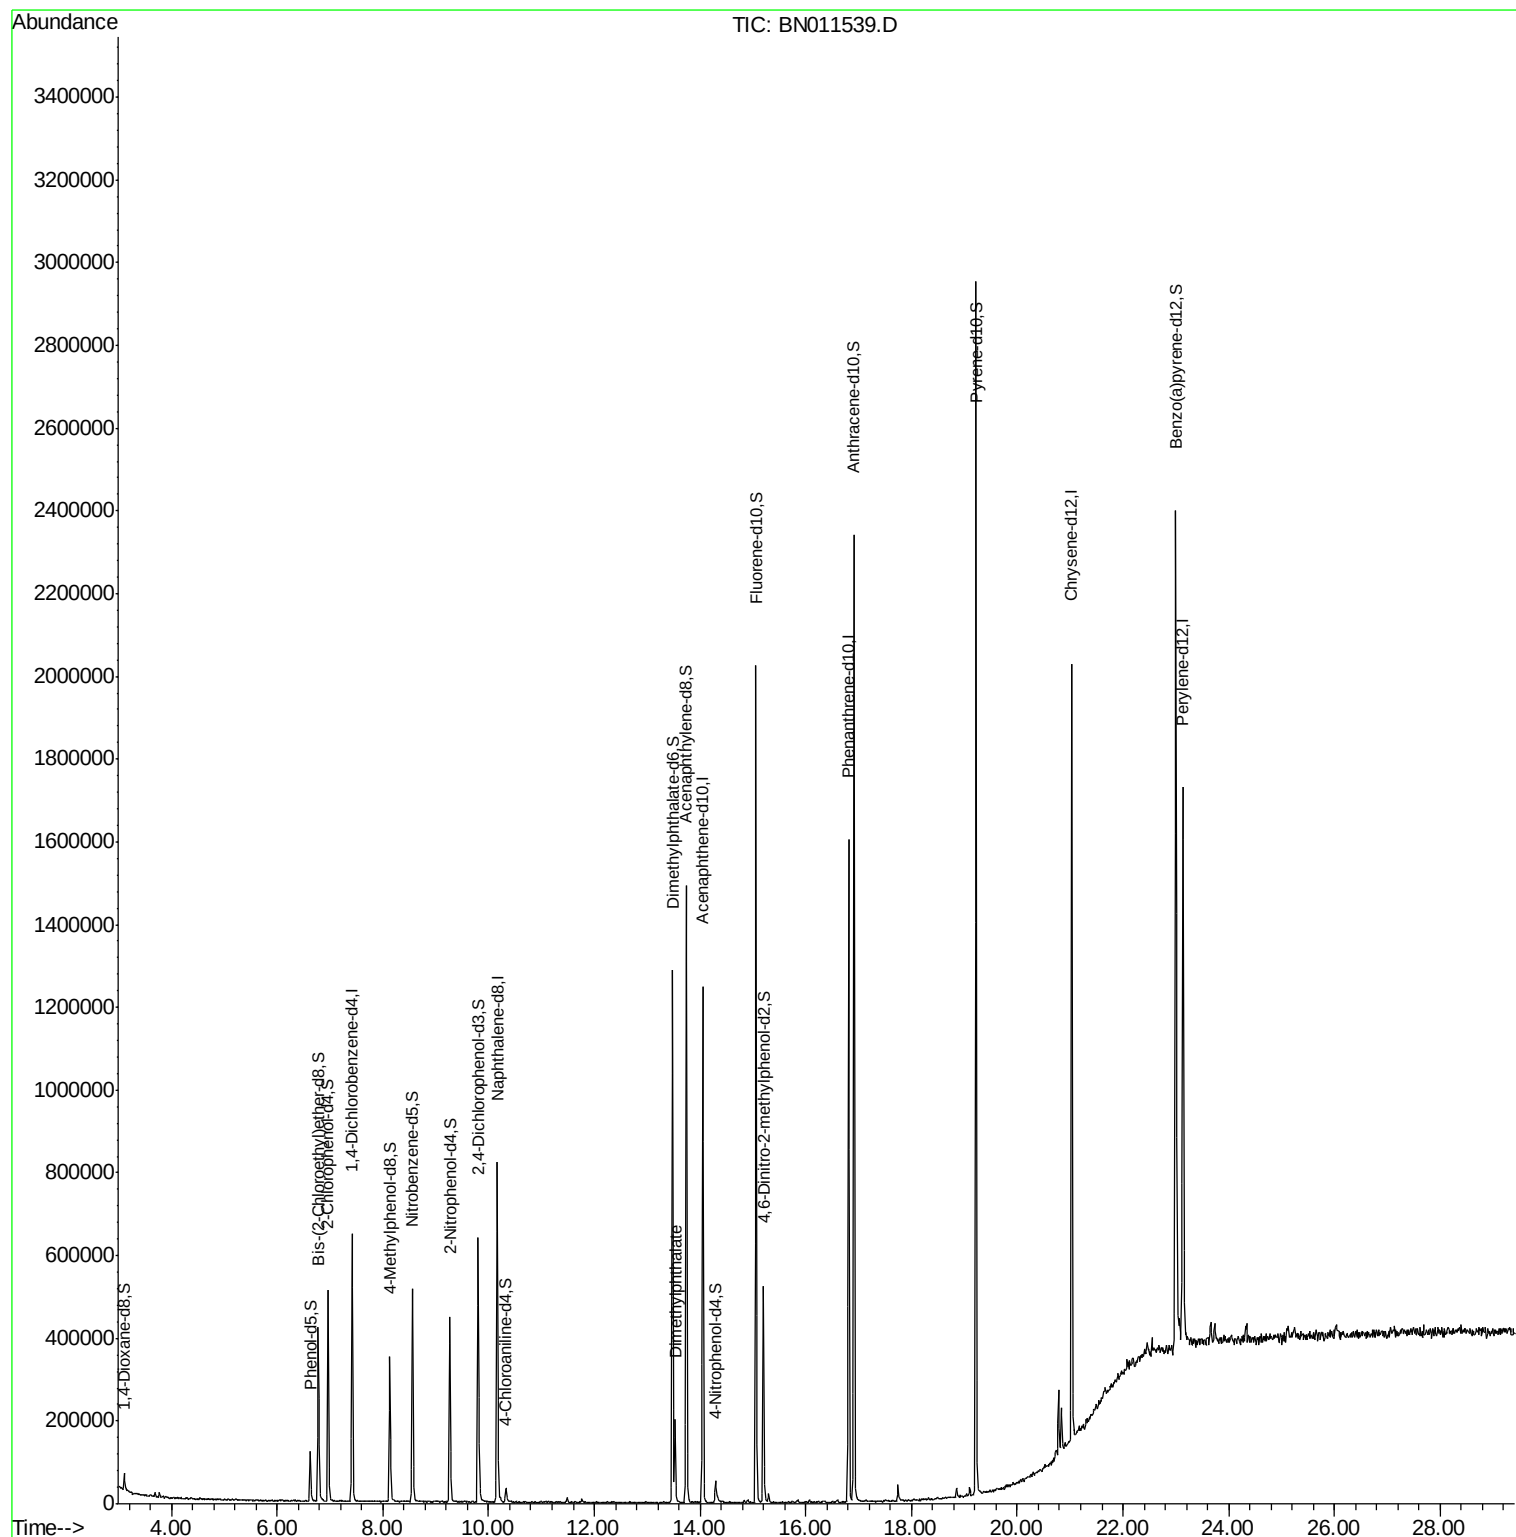

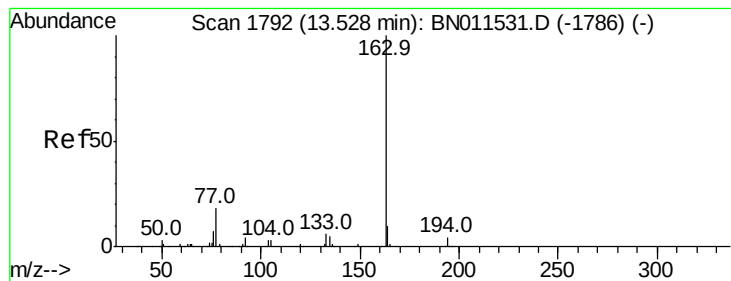

#45

Dimethylphthalate

Concen: 3.753 ng/ul

RT: 13.53 min Scan# 1792

Delta R.T. -0.00 min

Lab File: BN011539.D

Acq: 21 Aug 2020 00:27

Instrument :

BNA_N

ClientSampleId :

DBFW2


Tot Ion:163 Resp: 122687

Ion Ratio Lower Upper

163 100

194 4.7 3.8 5.6

164 8.9 8.7 13.1

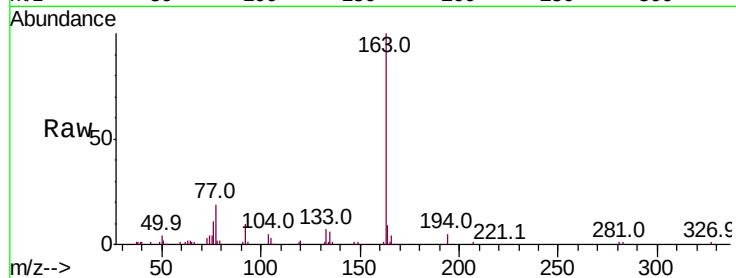

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

