

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN082020\
 Data File : BN011543.D
 Acq On : 21 Aug 2020 02:50
 Operator : CG/JU
 Sample : L3708-06
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBFS8

Quant Time: Aug 21 04:34:55 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081420MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Aug 21 03:13:08 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.42	152	172000	20.00	ng/ul	0.00
18) Naphthalene-d8	10.16	136	637089	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.06	164	348732	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.81	188	745091	20.00	ng/ul	0.00
78) Chrysene-d12	21.03	240	783987	20.00	ng/ul	0.00
86) Perylene-d12	23.13	264	763432	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.10	96	21529	6.01	ng/uL	0.00
5) Phenol-d5	6.62	99	69249	5.69	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.78	67	162582	26.22	ng/ul	0.00
9) 2-Chlorophenol-d4	6.96	132	223895	20.54	ng/ul	0.00
13) 4-Methylphenol-d8	8.13	113	128821	13.04	ng/ul	0.00
19) Nitrobenzene-d5	8.56	128	129162	26.16	ng/ul	0.00
22) 2-Nitrophenol-d4	9.27	143	140529	25.31	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.80	165	234405	22.34	ng/ul	0.00
29) 4-Chloroaniline-d4	10.33	131	21588	1.72	ng/ul	0.01
44) Dimethylphthalate-d6	13.48	166	693222	25.53	ng/ul	0.00
47) Acenaphthylene-d8	13.74	160	833498	25.51	ng/ul	0.00
52) 4-Nitrophenol-d4	14.29	143	15595	3.39	ng/ul	0.00
58) Fluorene-d10	15.06	176	626018	26.34	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.20	200	108114	21.88	ng/ul	0.00
71) Anthracene-d10	16.91	188	1083442	30.44	ng/ul	0.00
79) Pyrene-d10	19.22	212	1239354	30.77	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.00	264	1267812	29.90	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.53	163	127792	4.585	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN082020\
Data File : BN011543.D
Acq On : 21 Aug 2020 02:50
Operator : CG/JU
Sample : L3708-06
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBFS8

Quant Time: Aug 21 04:34:55 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081420MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Aug 21 03:13:08 2020
Response via : Initial Calibration

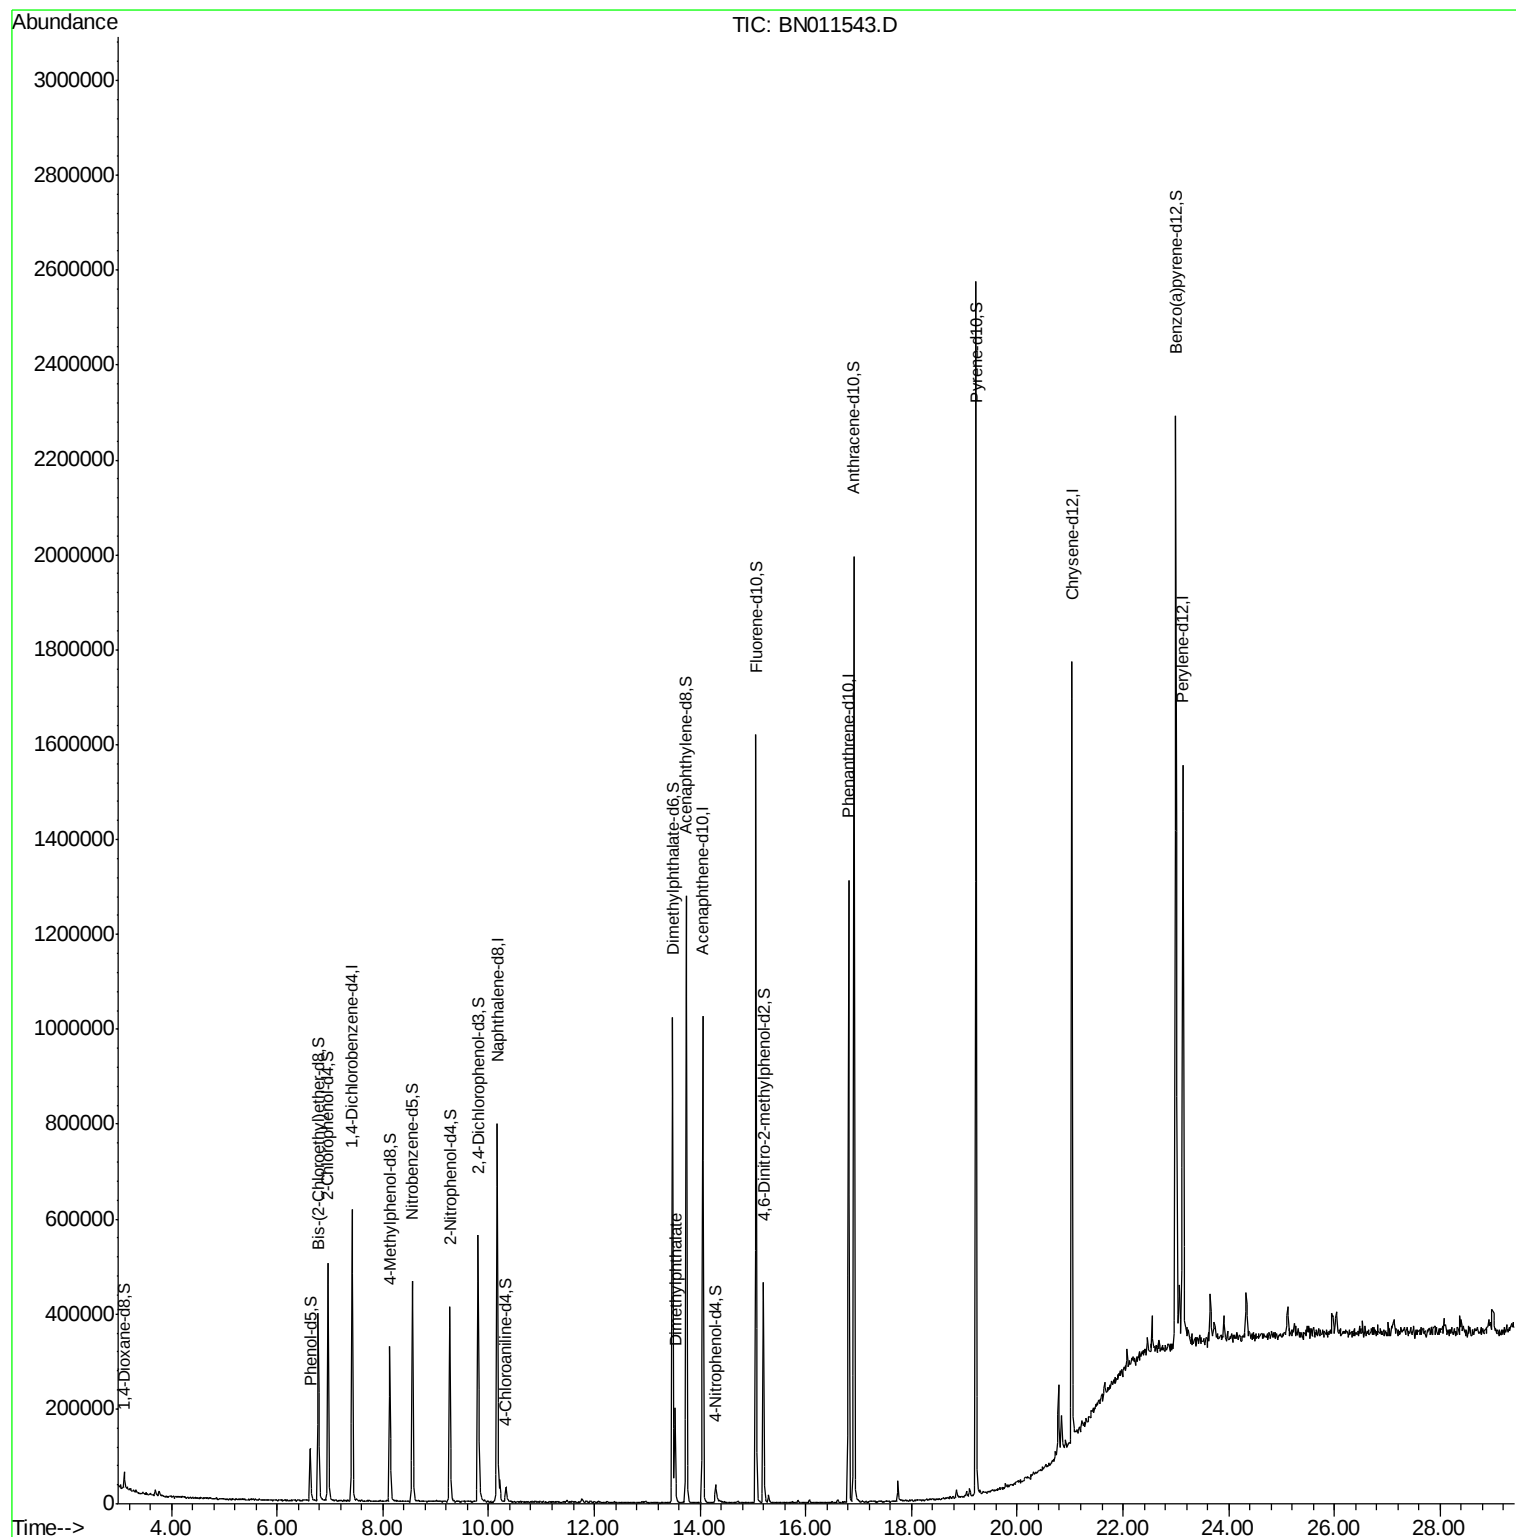

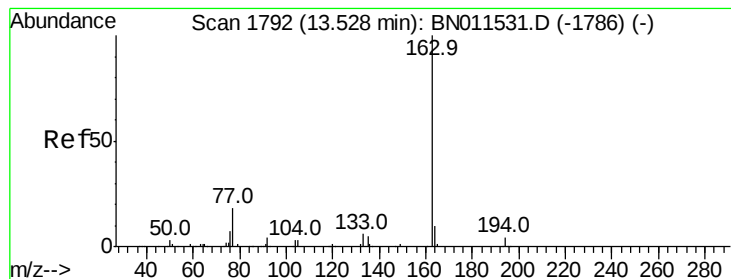

#45

Dimethylphthalate

Concen: 4.585 ng/ul

RT: 13.53 min Scan# 1792

Delta R.T. -0.00 min

Lab File: BN011543.D

Acq: 21 Aug 2020 02:50

Instrument :

BNA_N

ClientSampleId :

DBFS8


Tot Ion:163 Resp: 127792

Ion Ratio Lower Upper

163 100

194 4.6 3.8 5.6

164 9.7 8.7 13.1

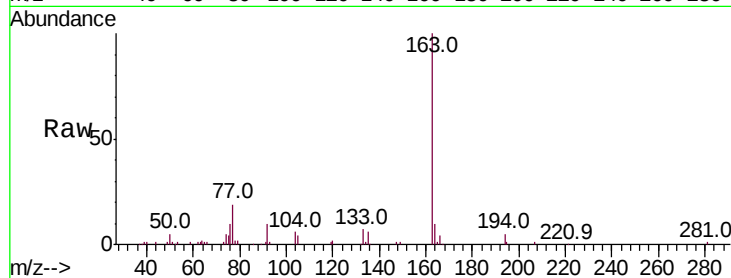

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

