

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN082020\
 Data File : BN011551.D
 Acq On : 21 Aug 2020 08:16
 Operator : CG/JU
 Sample : L3708-08
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBFT5

Quant Time: Aug 21 09:06:38 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081420MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Aug 21 07:37:59 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.42	152	200628	20.00	ng/ul	0.00
18) Naphthalene-d8	10.16	136	670699	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.05	164	411581	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.81	188	897121	20.00	ng/ul	0.00
78) Chrysene-d12	21.03	240	913532	20.00	ng/ul	0.00
86) Perylene-d12	23.14	264	912059	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.10	96	21419	5.12	ng/uL	0.00
5) Phenol-d5	6.62	99	74137	5.23	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.78	67	185285	25.62	ng/ul	0.00
9) 2-Chlorophenol-d4	6.96	132	251123	19.75	ng/ul	0.00
13) 4-Methylphenol-d8	8.13	113	121744	10.57	ng/ul	0.00
19) Nitrobenzene-d5	8.56	128	129254	24.87	ng/ul	0.00
22) 2-Nitrophenol-d4	9.27	143	146402	25.04	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.80	165	244824	22.16	ng/ul	0.00
29) 4-Chloroaniline-d4	10.33	131	22410	1.70	ng/ul	0.01
44) Dimethylphthalate-d6	13.48	166	811285	25.32	ng/ul	0.00
47) Acenaphthylene-d8	13.74	160	949894	24.63	ng/ul	0.00
52) 4-Nitrophenol-d4	14.29	143	19992	3.68	ng/ul	0.00
58) Fluorene-d10	15.06	176	730725	26.05	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.19	200	138008	23.20	ng/ul	0.00
71) Anthracene-d10	16.91	188	1269766	29.63	ng/ul	0.00
79) Pyrene-d10	19.22	212	1492598	31.81	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.01	264	1401458	27.67	ng/ul	0.00


Target Compounds				Ovalue
45) Dimethylphthalate	13.53	163	124776	3.793 ng/ul# 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN082020\
Data File : BN011551.D
Acq On : 21 Aug 2020 08:16
Operator : CG/JU
Sample : L3708-08
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBFT5

Quant Time: Aug 21 09:06:38 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081420MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Aug 21 07:37:59 2020
Response via : Initial Calibration

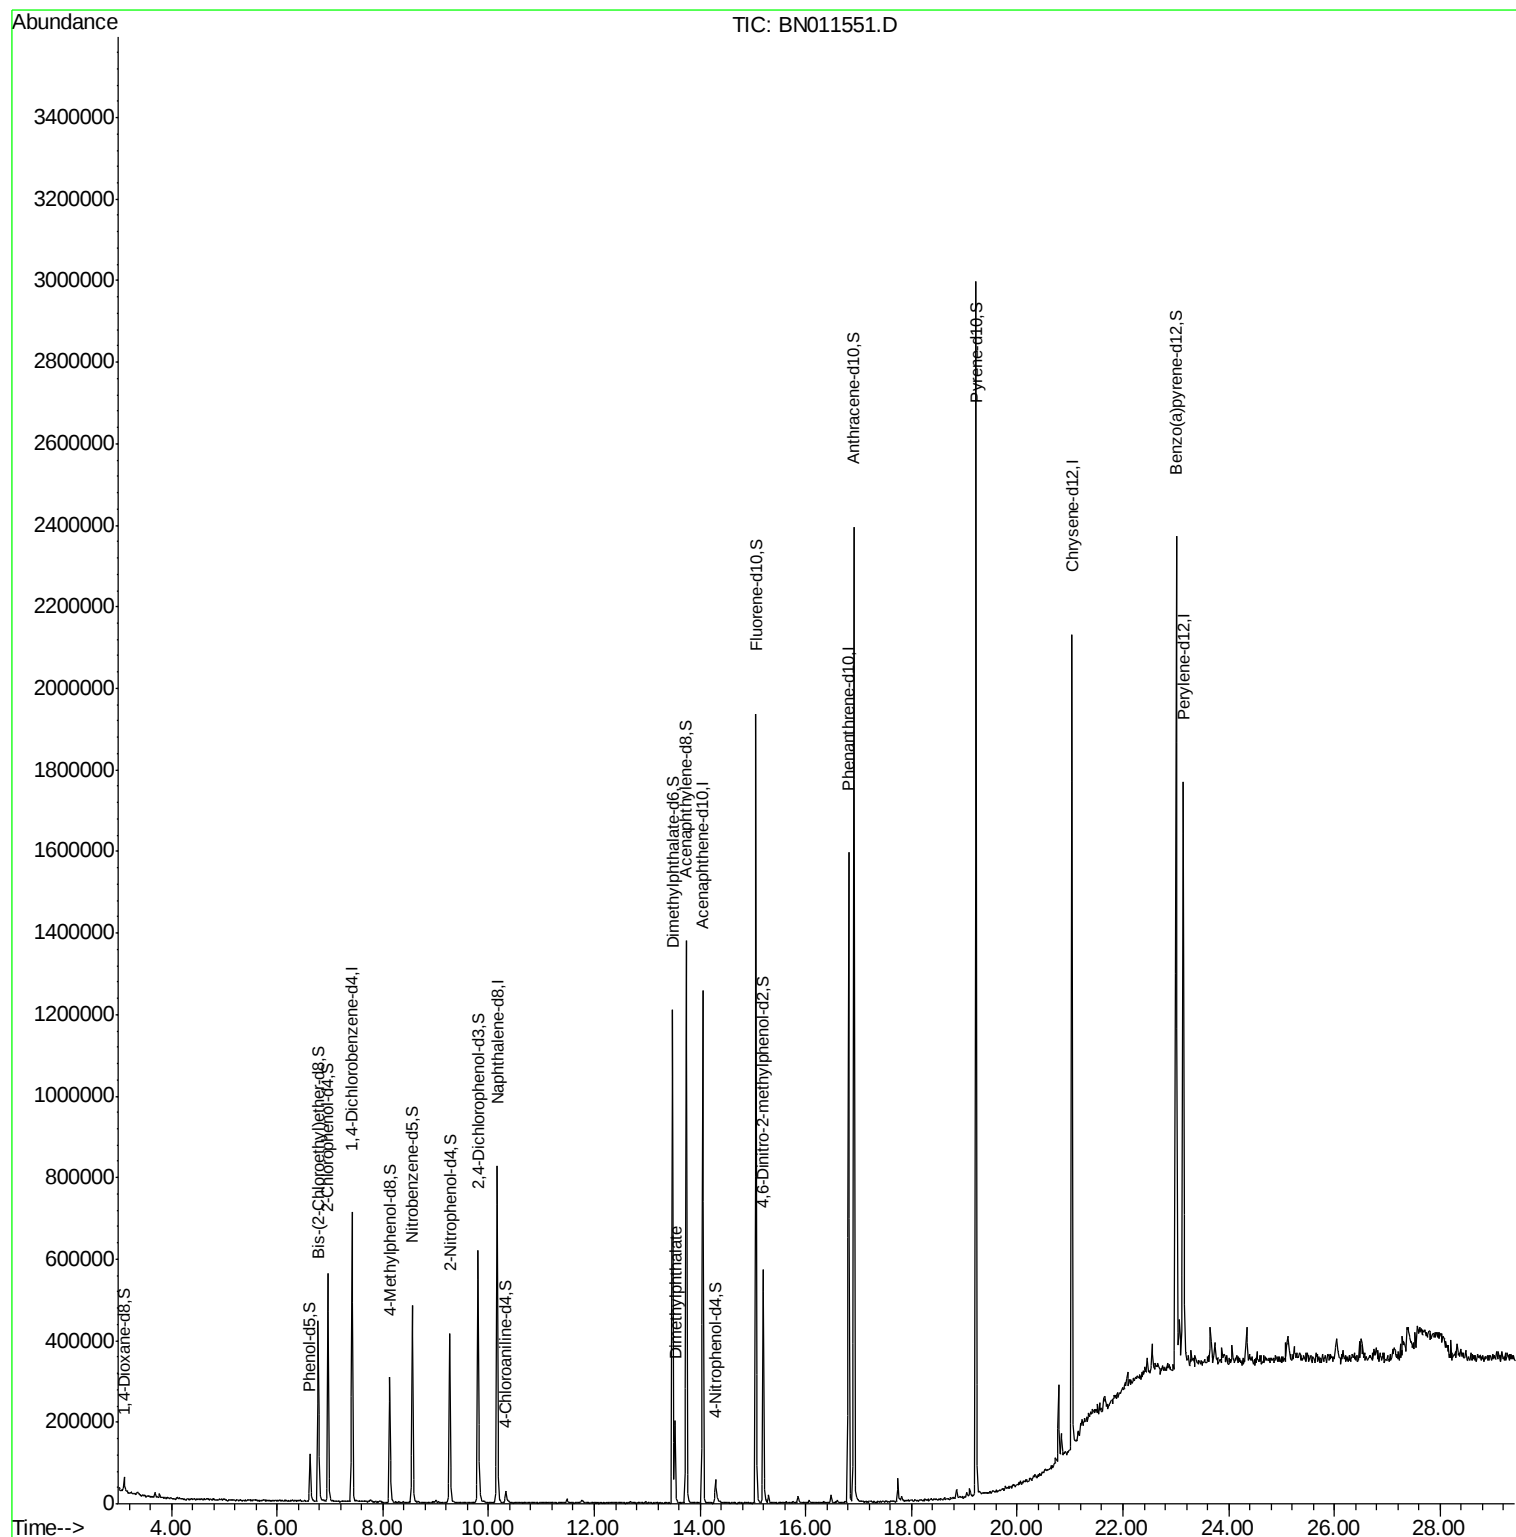

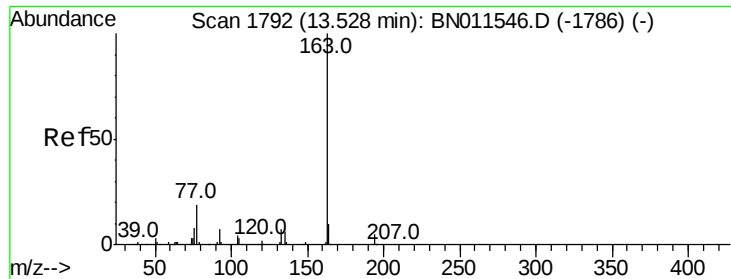

#45

Dimethylphthalate

Concen: 3.793 ng/ul

RT: 13.53 min Scan# 1792

Delta R.T. 0.00 min

Lab File: BN011551.D

Acq: 21 Aug 2020 08:16

Instrument :

BNA_N

ClientSampleId :

DBFT5


Tot Ion:163 Resp: 124776

Ion Ratio Lower Upper

163 100

194 3.5 3.8 5.6#

164 9.6 8.7 13.1

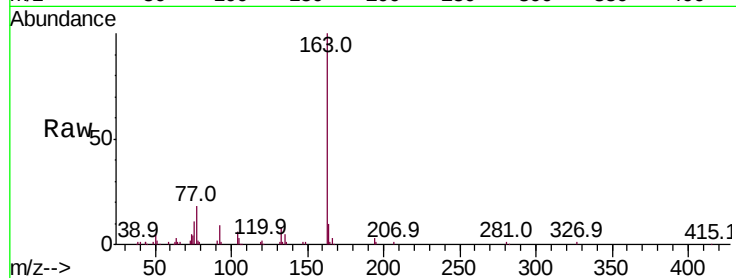

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

