

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN082020\
 Data File : BN011527.D
 Acq On : 20 Aug 2020 16:42
 Operator : CG/JU
 Sample : L3668-15
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBFW6

Quant Time: Aug 20 17:25:16 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081420MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 20 13:39:40 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.42	152	133432	20.00	ng/ul	0.00
18) Naphthalene-d8	10.17	136	492033	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.06	164	367182	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.82	188	709957	20.00	ng/ul	0.00
78) Chrysene-d12	21.03	240	743318	20.00	ng/ul	0.00
86) Perylene-d12	23.14	264	657981	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.11	96	15311	5.51	ng/uL	0.00
5) Phenol-d5	6.63	99	49765	5.27	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.78	67	132664	27.58	ng/ul	0.00
9) 2-Chlorophenol-d4	6.97	132	188366	22.27	ng/ul	0.00
13) 4-Methylphenol-d8	8.13	113	93848	12.25	ng/ul	0.00
19) Nitrobenzene-d5	8.56	128	116472	30.54	ng/ul	0.00
22) 2-Nitrophenol-d4	9.27	143	121222	28.26	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.80	165	191979	23.69	ng/ul	0.00
29) 4-Chloroaniline-d4	10.33	131	12260	1.27	ng/ul	0.02
44) Dimethylphthalate-d6	13.48	166	788001	27.56	ng/ul	0.00
47) Acenaphthylene-d8	13.75	160	928042	26.97	ng/ul	0.00
52) 4-Nitrophenol-d4	14.30	143	17609	3.64	ng/ul	0.00
58) Fluorene-d10	15.06	176	707351	28.26	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.20	200	115703	24.57	ng/ul	0.00
71) Anthracene-d10	16.92	188	1121859	33.08	ng/ul	0.00
79) Pyrene-d10	19.22	212	1273740	33.36	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.02	264	1150329	31.48	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.53	163	106128	3.616	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN082020\
Data File : BN011527.D
Acq On : 20 Aug 2020 16:42
Operator : CG/JU
Sample : L3668-15
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBFW6

Quant Time: Aug 20 17:25:16 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081420MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 20 13:39:40 2020
Response via : Initial Calibration

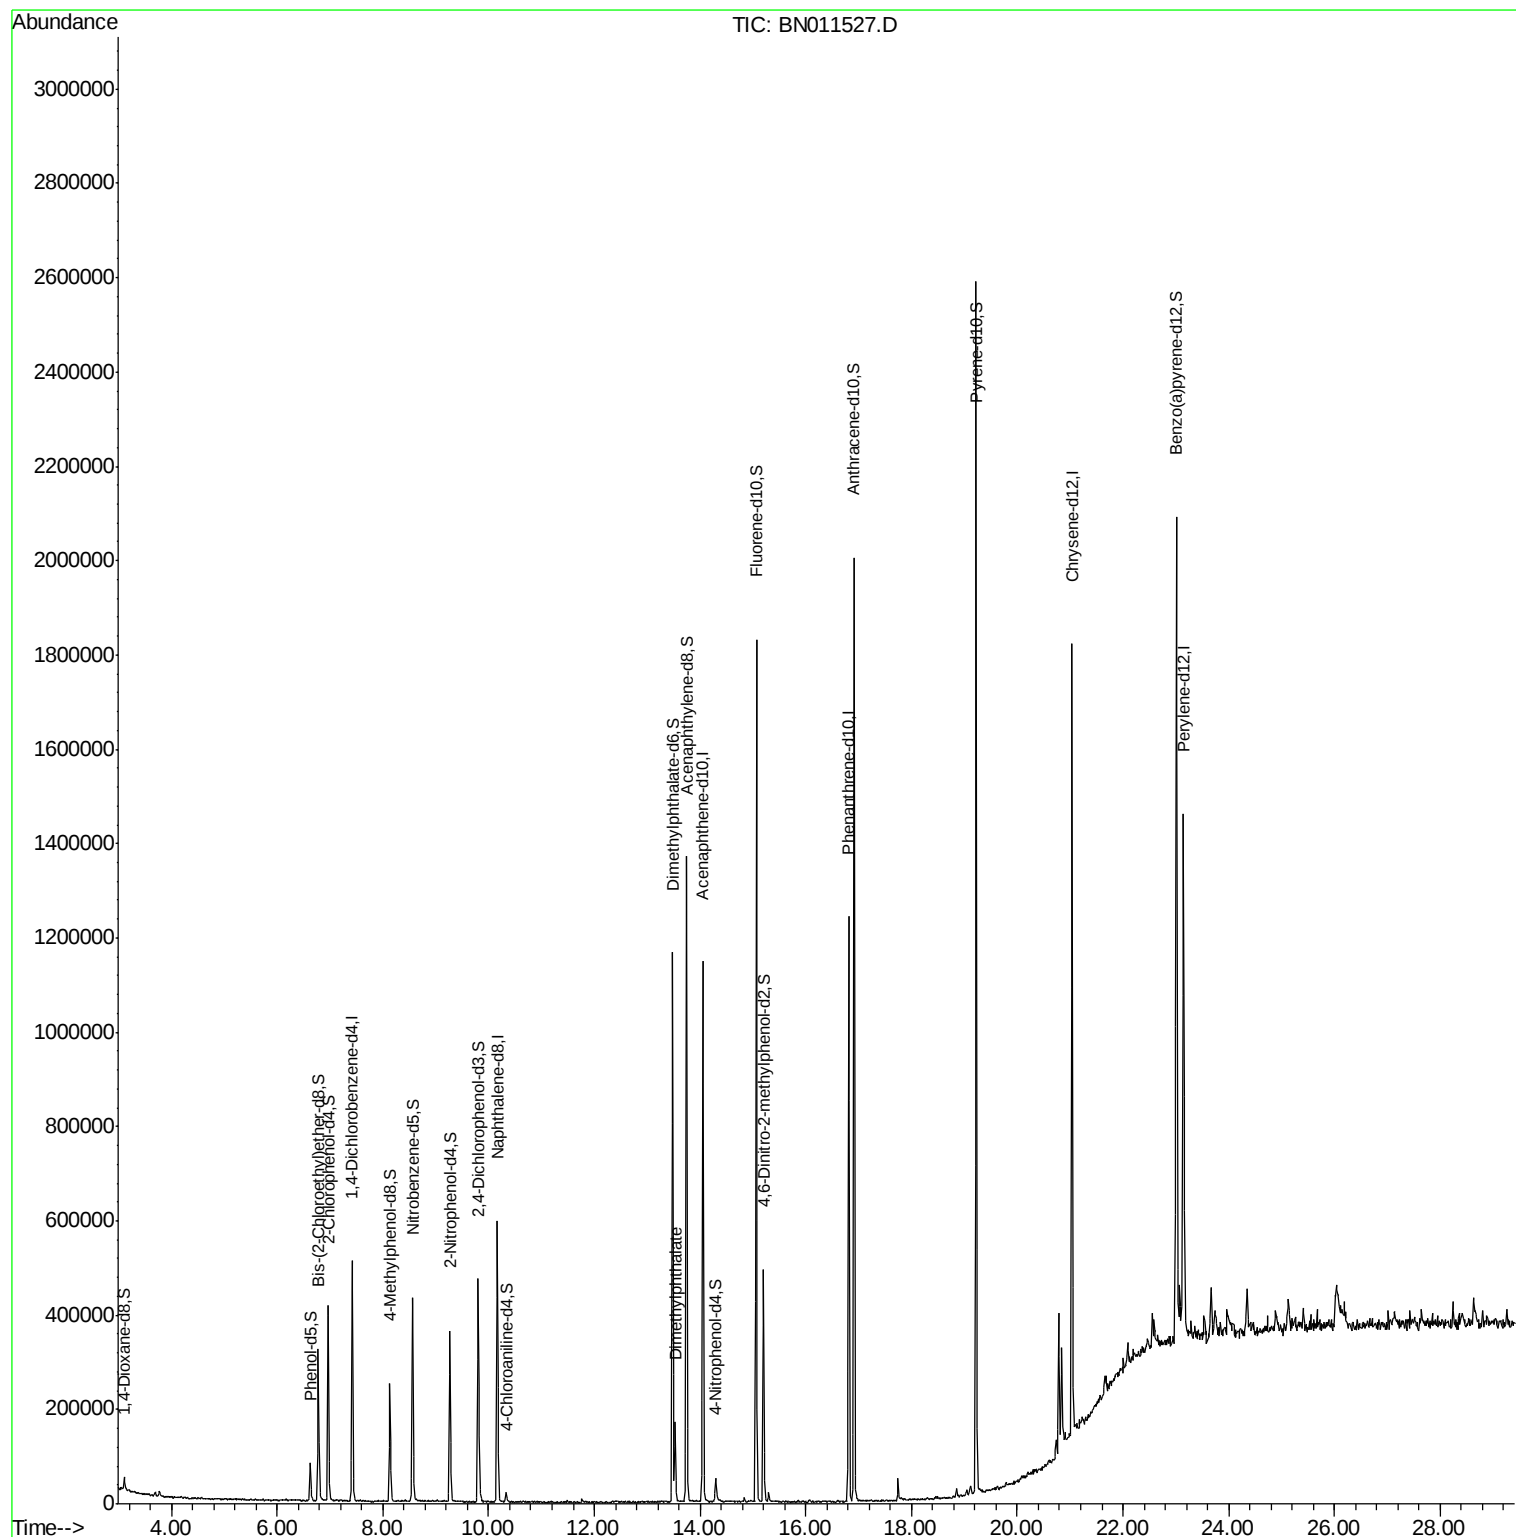

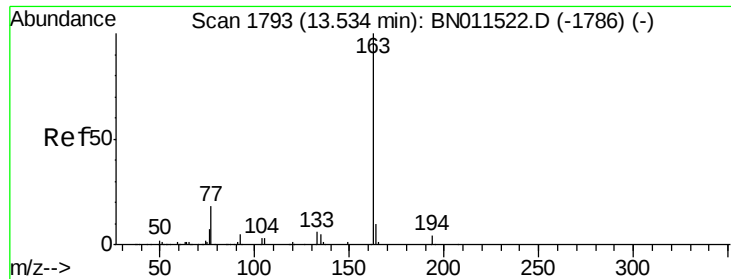

#45
 Dimethylphthalate
 Concen: 3.616 ng/ul
 RT: 13.53 min Scan# 1792
 Delta R.T. -0.01 min
 Lab File: BN011527.D
 Acq: 20 Aug 2020 16:42

Instrument :
 BNA_N
 ClientSampleId :
 DBFW6

Tot Ion	Ratio	Lower	Upper
163	100		
194	5.1	3.8	5.6
164	10.0	8.7	13.1

