

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN082020\
 Data File : BN011529.D
 Acq On : 20 Aug 2020 17:54
 Operator : CG/JU
 Sample : L3668-19
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBFX0

Quant Time: Aug 20 18:25:06 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081420MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 20 13:39:40 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.42	152	143457	20.00	ng/ul	0.00
18) Naphthalene-d8	10.17	136	552788	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.06	164	307734	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.81	188	695877	20.00	ng/ul	0.00
78) Chrysene-d12	21.03	240	710600	20.00	ng/ul	0.00
86) Perylene-d12	23.14	264	674128	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.10	96	21267	7.11	ng/uL	0.00
5) Phenol-d5	6.63	99	121268	11.95	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.78	67	150737	29.15	ng/ul	0.00
9) 2-Chlorophenol-d4	6.97	132	219781	24.17	ng/ul	0.00
13) 4-Methylphenol-d8	8.13	113	152927	18.57	ng/ul	0.00
19) Nitrobenzene-d5	8.56	128	120532	28.13	ng/ul	0.00
22) 2-Nitrophenol-d4	9.28	143	138179	28.68	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.80	165	244456	26.85	ng/ul	0.00
29) 4-Chloroaniline-d4	10.32	131	89839	8.25	ng/ul	0.00
44) Dimethylphthalate-d6	13.48	166	735125	30.68	ng/ul	0.00
47) Acenaphthylene-d8	13.74	160	837707	29.05	ng/ul	0.00
52) 4-Nitrophenol-d4	14.29	143	40469	9.97	ng/ul	0.00
58) Fluorene-d10	15.06	176	632027	30.13	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.20	200	107447	23.28	ng/ul	0.00
71) Anthracene-d10	16.91	188	1055464	31.75	ng/ul	0.00
79) Pyrene-d10	19.22	212	1246966	34.16	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.01	264	1174320	31.37	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.53	163	329598	13.401	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN082020\
Data File : BN011529.D
Acq On : 20 Aug 2020 17:54
Operator : CG/JU
Sample : L3668-19
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBFX0

Quant Time: Aug 20 18:25:06 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081420MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 20 13:39:40 2020
Response via : Initial Calibration

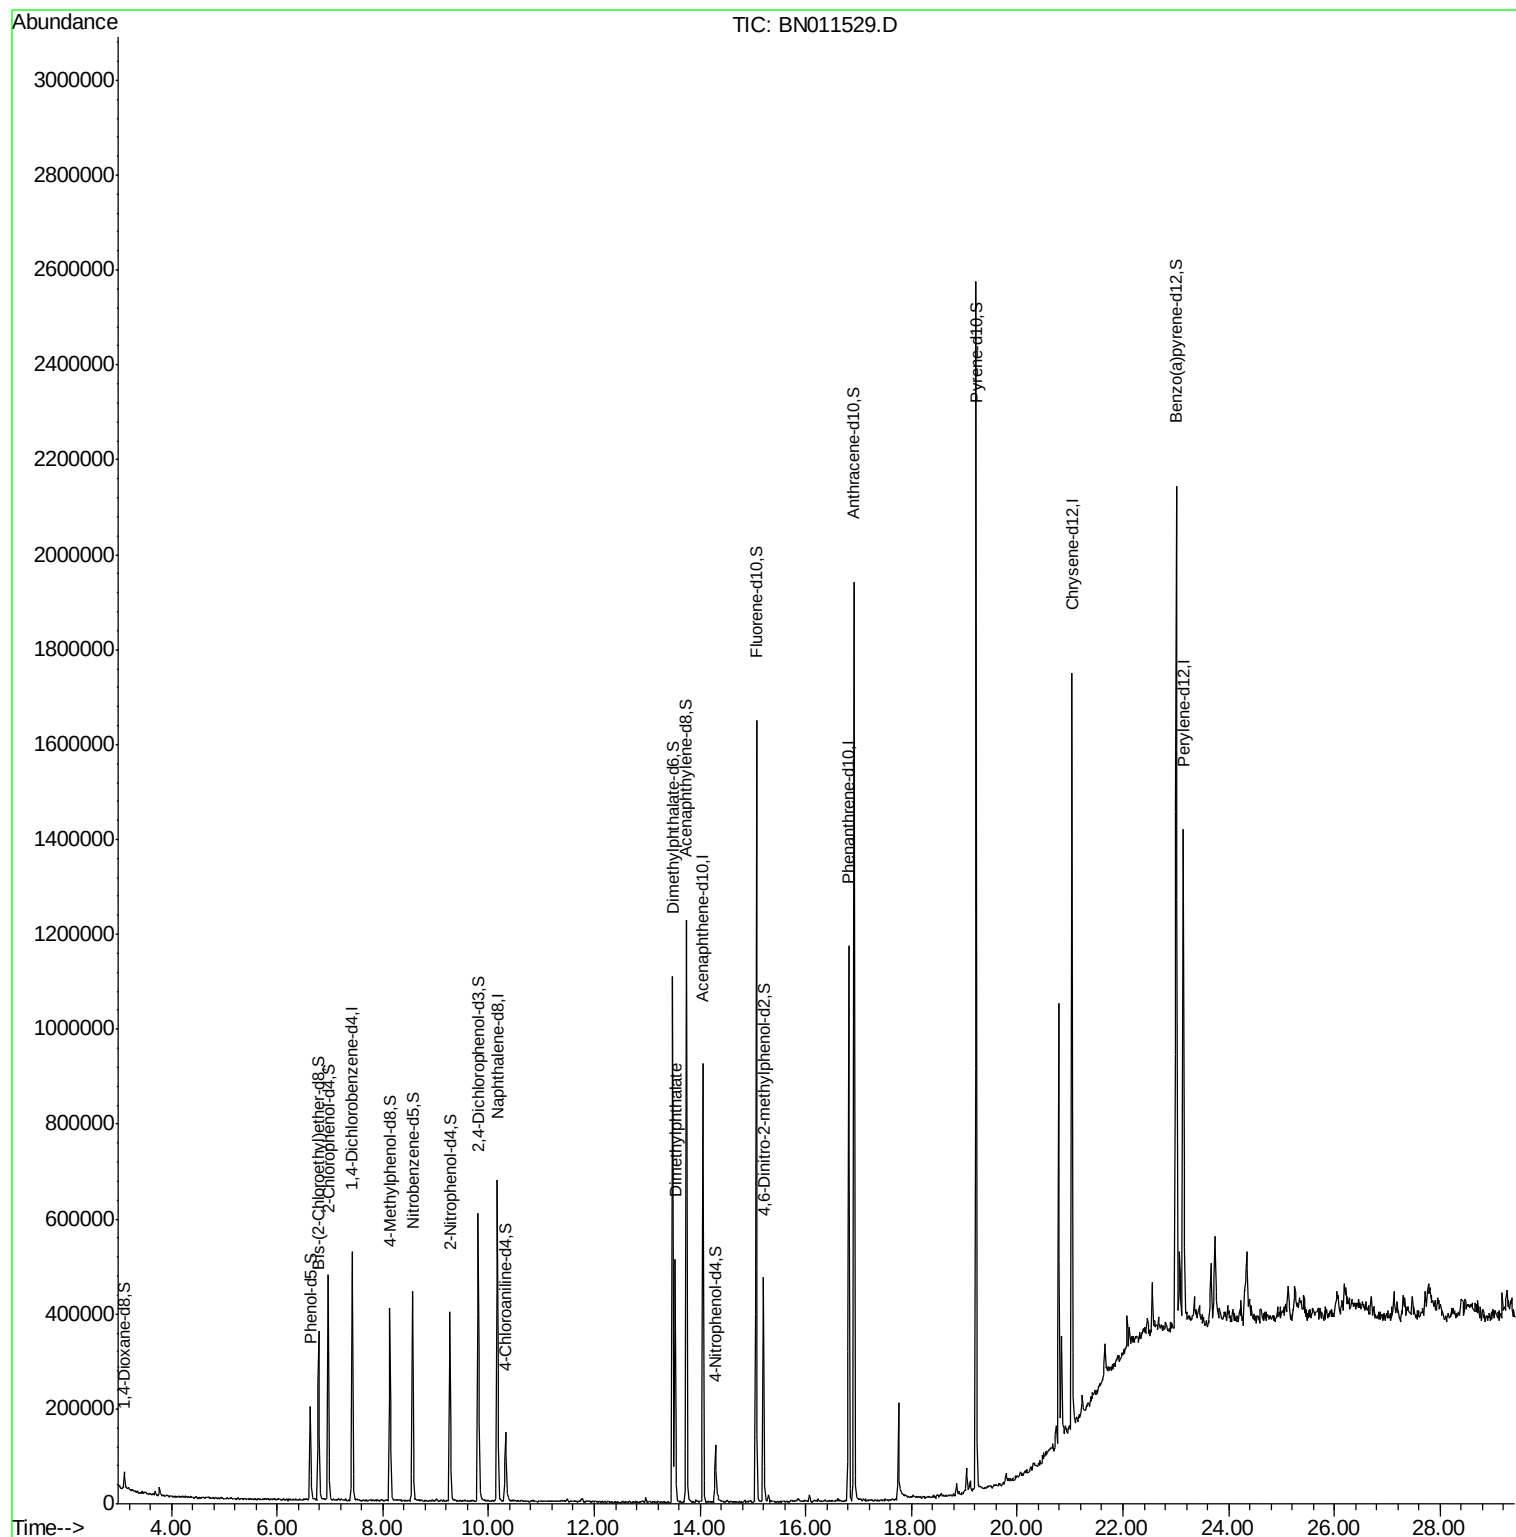

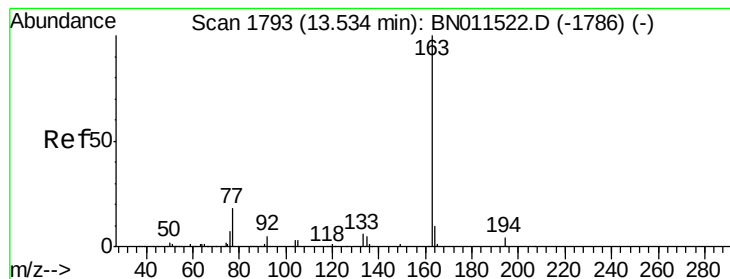

#45

Dimethylphthalate

Concen: 13.401 ng/ul

RT: 13.53 min Scan# 1792

Delta R.T. -0.01 min

Lab File: BN011529.D

Acq: 20 Aug 2020 17:54

Instrument :

BNA_N

ClientSampleId :

DBFX0



Tot Ion:163 Resp: 329598

Ion Ratio Lower Upper

163 100

194 4.4 3.8 5.6

164 10.5 8.7 13.1

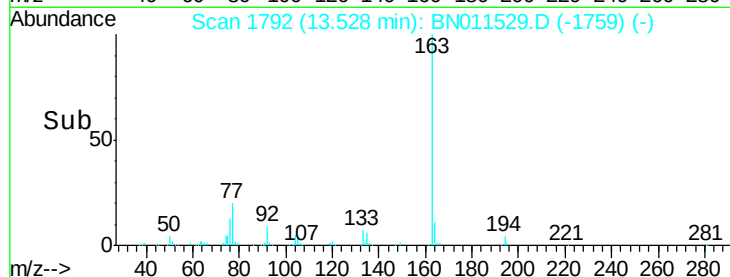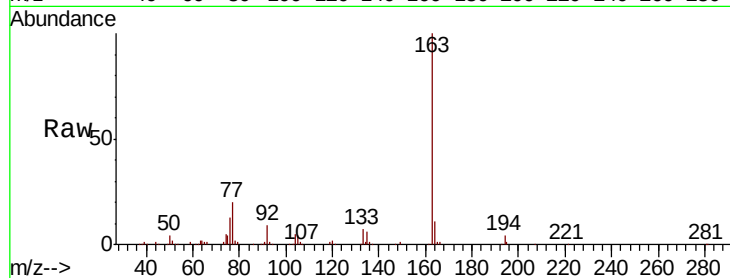

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

