

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN082020\
 Data File : BN011538.D
 Acq On : 20 Aug 2020 23:51
 Operator : CG/JU
 Sample : L3668-16
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBFW7

Quant Time: Aug 21 03:16:03 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081420MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Aug 21 03:13:08 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.42	152	93760	20.00	ng/ul	0.00
18) Naphthalene-d8	10.16	136	435042	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.06	164	272896	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.81	188	609455	20.00	ng/ul	0.00
78) Chrysene-d12	21.03	240	609633	20.00	ng/ul	0.00
86) Perylene-d12	23.13	264	552300	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.11	96	14399	7.37	ng/uL	0.00
5) Phenol-d5	6.63	99	64561	9.74	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.78	67	159488	47.19	ng/ul	0.00
9) 2-Chlorophenol-d4	6.96	132	214426	36.08	ng/ul	0.00
13) 4-Methylphenol-d8	8.13	113	109652	20.37	ng/ul	0.00
19) Nitrobenzene-d5	8.56	128	116643	34.59	ng/ul	0.00
22) 2-Nitrophenol-d4	9.27	143	129231	34.08	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.80	165	245751	34.30	ng/ul	0.00
29) 4-Chloroaniline-d4	10.33	131	18350	2.14	ng/ul	0.01
44) Dimethylphthalate-d6	13.48	166	886063	41.70	ng/ul	0.00
47) Acenaphthylene-d8	13.74	160	1020608	39.91	ng/ul	0.00
52) 4-Nitrophenol-d4	14.29	143	21934	6.09	ng/ul	0.00
58) Fluorene-d10	15.06	176	805790	43.32	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.20	200	146513	36.25	ng/ul	0.00
71) Anthracene-d10	16.91	188	1393384	47.86	ng/ul	0.00
79) Pyrene-d10	19.22	212	1625545	51.90	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.00	264	1540131	50.21	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.53	163	132699	6.084	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN082020\
Data File : BN011538.D
Acq On : 20 Aug 2020 23:51
Operator : CG/JU
Sample : L3668-16
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBFW7

Quant Time: Aug 21 03:16:03 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081420MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Aug 21 03:13:08 2020
Response via : Initial Calibration

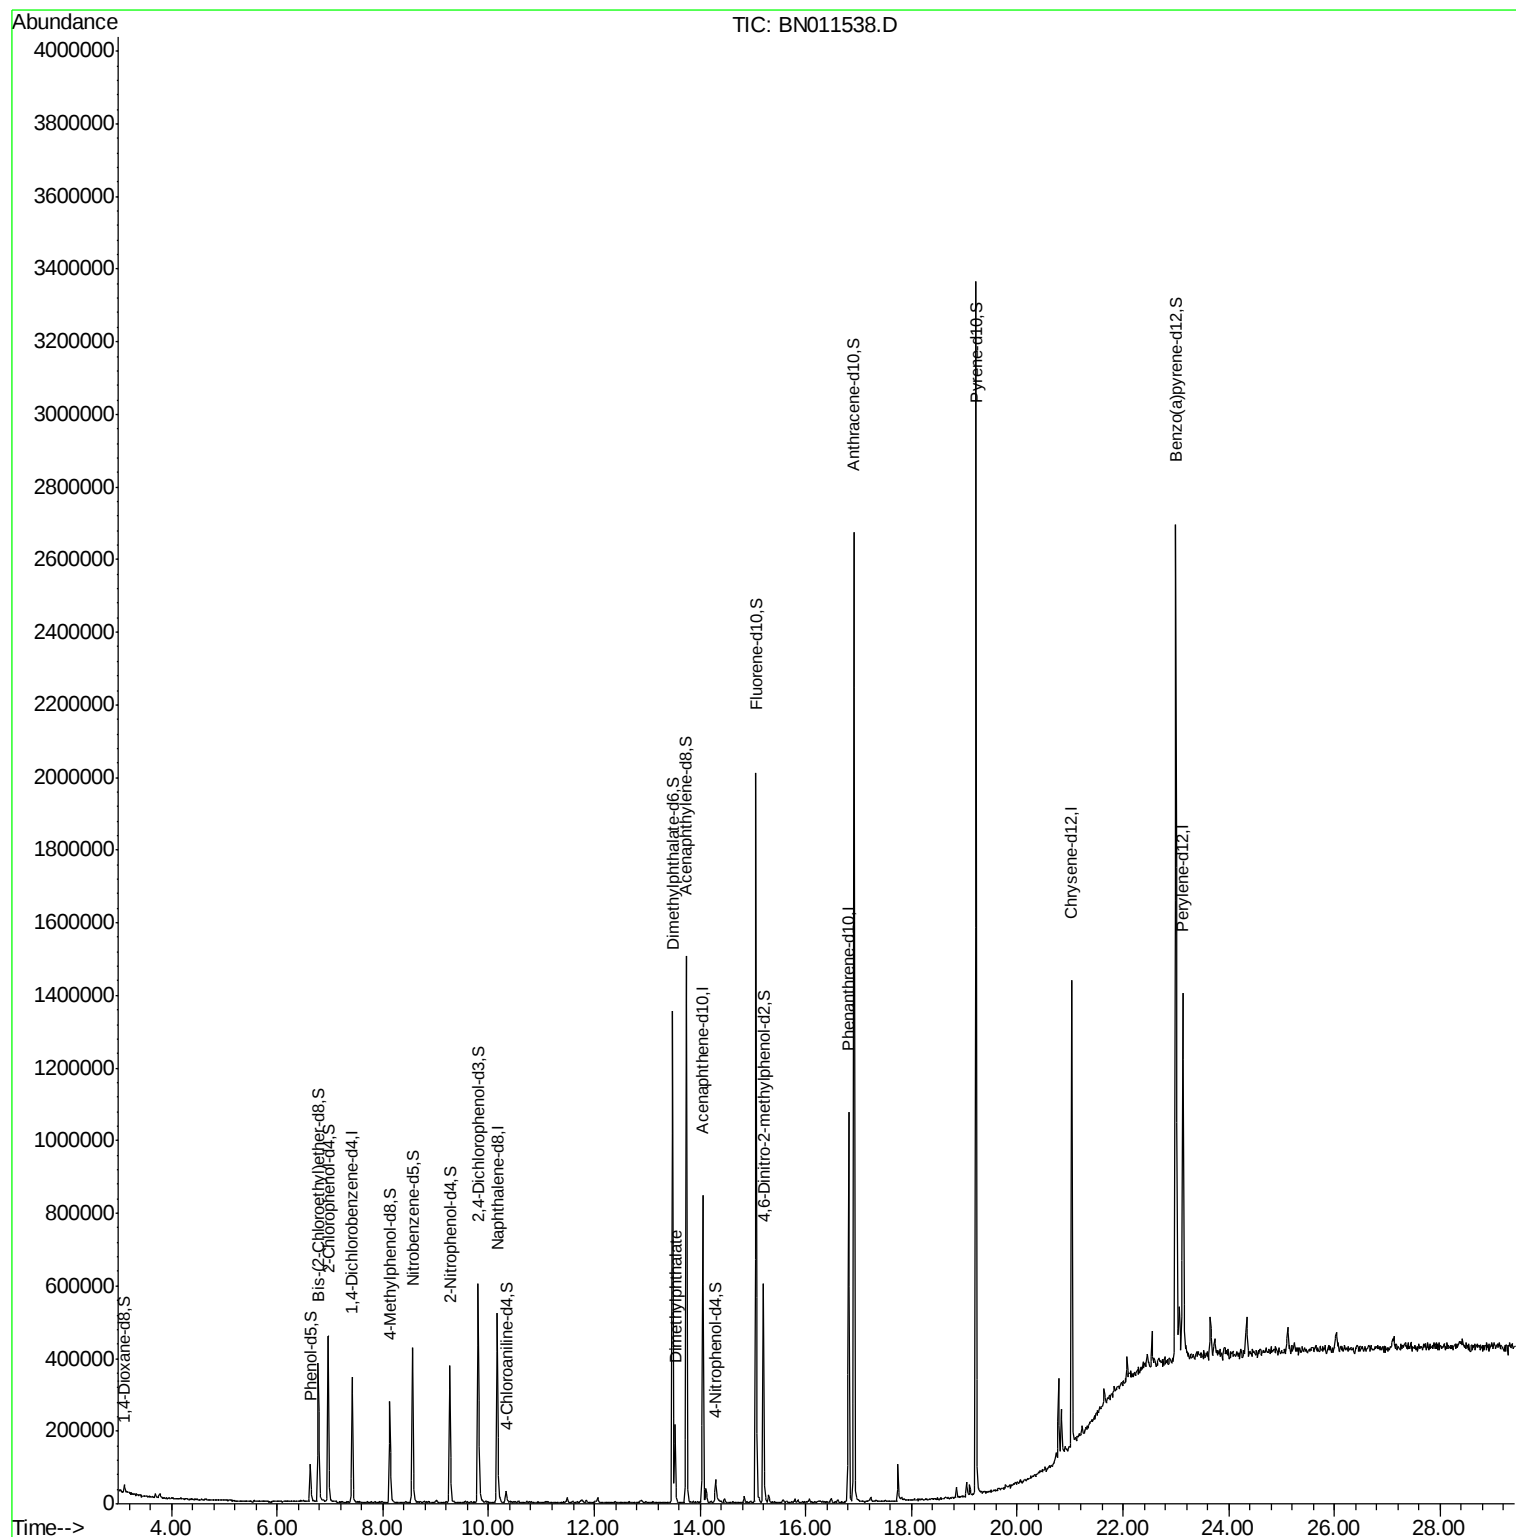

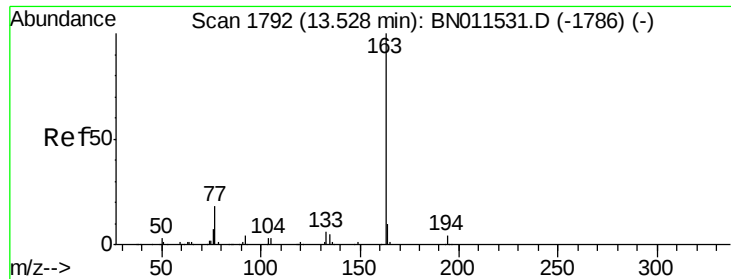

#45

Dimethylphthalate

Concen: 6.084 ng/ul

RT: 13.53 min Scan# 1792

Delta R.T. -0.00 min

Lab File: BN011538.D

Acq: 20 Aug 2020 23:51

Instrument :

BNA_N

ClientSampleId :

DBFW7



Tot Ion:163 Resp: 132699

Ion Ratio Lower Upper

163 100

194 4.3 3.8 5.6

164 10.8 8.7 13.1

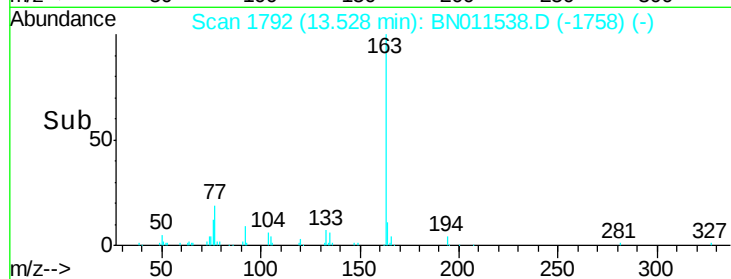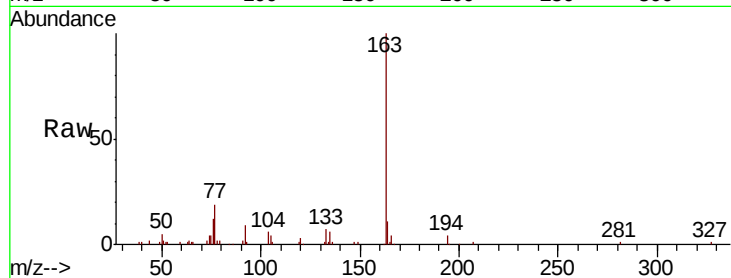

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

