

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN082020\
 Data File : BN011540.D
 Acq On : 21 Aug 2020 01:02
 Operator : CG/JU
 Sample : L3708-01
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBFW5

Quant Time: Aug 21 03:16:15 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081420MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Aug 21 03:13:08 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.42	152	171681	20.00	ng/ul	0.00
18) Naphthalene-d8	10.16	136	652729	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.06	164	407282	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.81	188	864029	20.00	ng/ul	0.00
78) Chrysene-d12	21.03	240	873356	20.00	ng/ul	0.00
86) Perylene-d12	23.13	264	806956	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.11	96	21598	6.04	ng/uL	0.00
5) Phenol-d5	6.63	99	58796	4.84	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.78	67	155345	25.10	ng/ul	0.00
9) 2-Chlorophenol-d4	6.97	132	210531	19.35	ng/ul	0.00
13) 4-Methylphenol-d8	8.13	113	117480	11.92	ng/ul	0.00
19) Nitrobenzene-d5	8.56	128	124249	24.56	ng/ul	0.00
22) 2-Nitrophenol-d4	9.27	143	137496	24.17	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.80	165	237868	22.13	ng/ul	0.00
29) 4-Chloroaniline-d4	10.33	131	19800	1.54	ng/ul	0.01
44) Dimethylphthalate-d6	13.48	166	856577	27.01	ng/ul	0.00
47) Acenaphthylene-d8	13.74	160	943646	24.73	ng/ul	0.00
52) 4-Nitrophenol-d4	14.30	143	17307	3.22	ng/ul	0.01
58) Fluorene-d10	15.06	176	729185	26.27	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.20	200	117709	20.54	ng/ul	0.00
71) Anthracene-d10	16.91	188	1171183	28.38	ng/ul	0.00
79) Pyrene-d10	19.22	212	1381945	30.80	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.00	264	1299897	29.01	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.53	163	141549	4.348	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN082020\
Data File : BN011540.D
Acq On : 21 Aug 2020 01:02
Operator : CG/JU
Sample : L3708-01
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBFW5

Quant Time: Aug 21 03:16:15 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081420MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Aug 21 03:13:08 2020
Response via : Initial Calibration

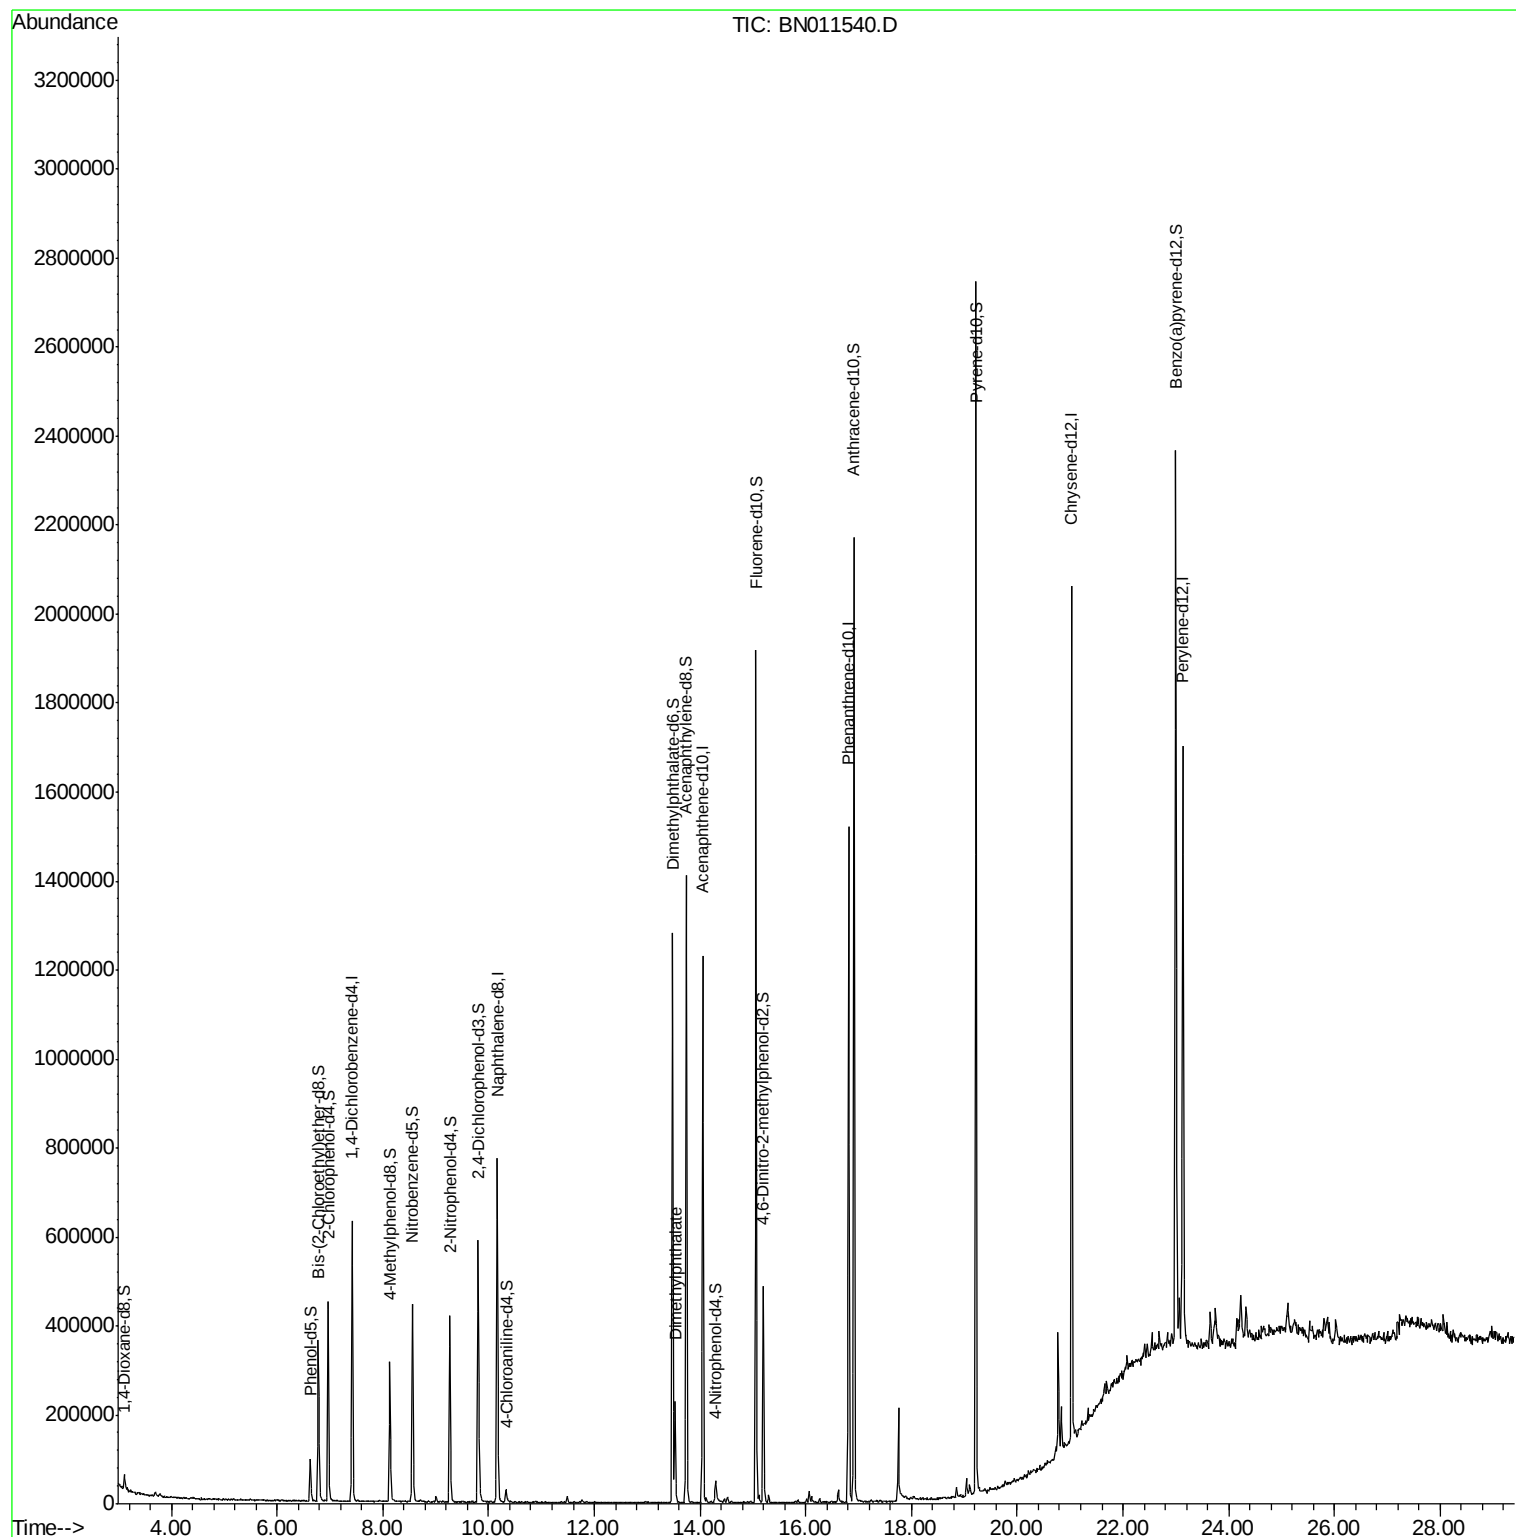

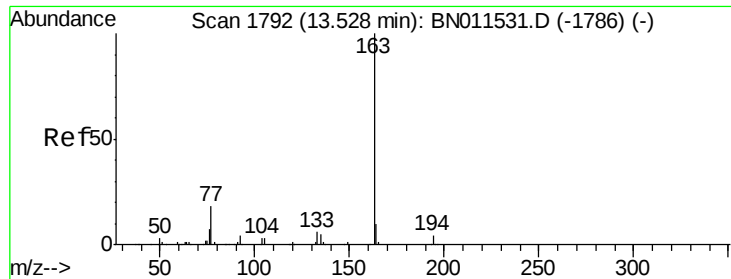

#45

Dimethylphthalate

Concen: 4.348 ng/ul

RT: 13.53 min Scan# 1792

Delta R.T. -0.00 min

Lab File: BN011540.D

Acq: 21 Aug 2020 01:02

Instrument :

BNA_N

ClientSampleId :

DBFW5


Tot Ion:163 Resp: 141549

Ion Ratio Lower Upper

163 100

194 4.1 3.8 5.6

164 9.6 8.7 13.1

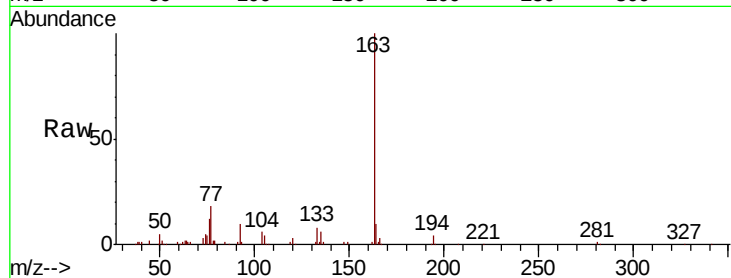

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

