

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN082020\
 Data File : BN011552.D
 Acq On : 21 Aug 2020 08:52
 Operator : CG/JU
 Sample : L3708-13
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBFW1

Quant Time: Aug 21 11:00:12 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081420MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Aug 21 04:54:28 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.42	152	170292	20.00	ng/ul	0.00
18) Naphthalene-d8	10.16	136	575844	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.05	164	360896	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.81	188	772651	20.00	ng/ul	0.00
78) Chrysene-d12	21.03	240	824683	20.00	ng/ul	0.00
86) Perylene-d12	23.14	264	798690	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.10	96	23599	6.65	ng/uL	0.00
5) Phenol-d5	6.62	99	82131	6.82	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.78	67	193504	31.52	ng/ul	0.00
9) 2-Chlorophenol-d4	6.96	132	261729	24.25	ng/ul	0.00
13) 4-Methylphenol-d8	8.13	113	135113	13.82	ng/ul	0.00
19) Nitrobenzene-d5	8.56	128	134769	30.20	ng/ul	0.00
22) 2-Nitrophenol-d4	9.27	143	148894	29.66	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.80	165	251086	26.48	ng/ul	0.00
29) 4-Chloroaniline-d4	10.32	131	23316	2.06	ng/ul	0.00
44) Dimethylphthalate-d6	13.48	166	851784	30.31	ng/ul	0.00
47) Acenaphthylene-d8	13.74	160	1010271	29.87	ng/ul	0.00
52) 4-Nitrophenol-d4	14.29	143	20968	4.40	ng/ul	0.00
58) Fluorene-d10	15.06	176	756441	30.75	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.19	200	131060	25.58	ng/ul	0.00
71) Anthracene-d10	16.91	188	1203415	32.60	ng/ul	0.00
79) Pyrene-d10	19.22	212	1392232	32.86	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.01	264	1396376	31.48	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.53	163	137274	4.759	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN082020\
Data File : BN011552.D
Acq On : 21 Aug 2020 08:52
Operator : CG/JU
Sample : L3708-13
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBFW1

Quant Time: Aug 21 11:00:12 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081420MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Aug 21 04:54:28 2020
Response via : Initial Calibration

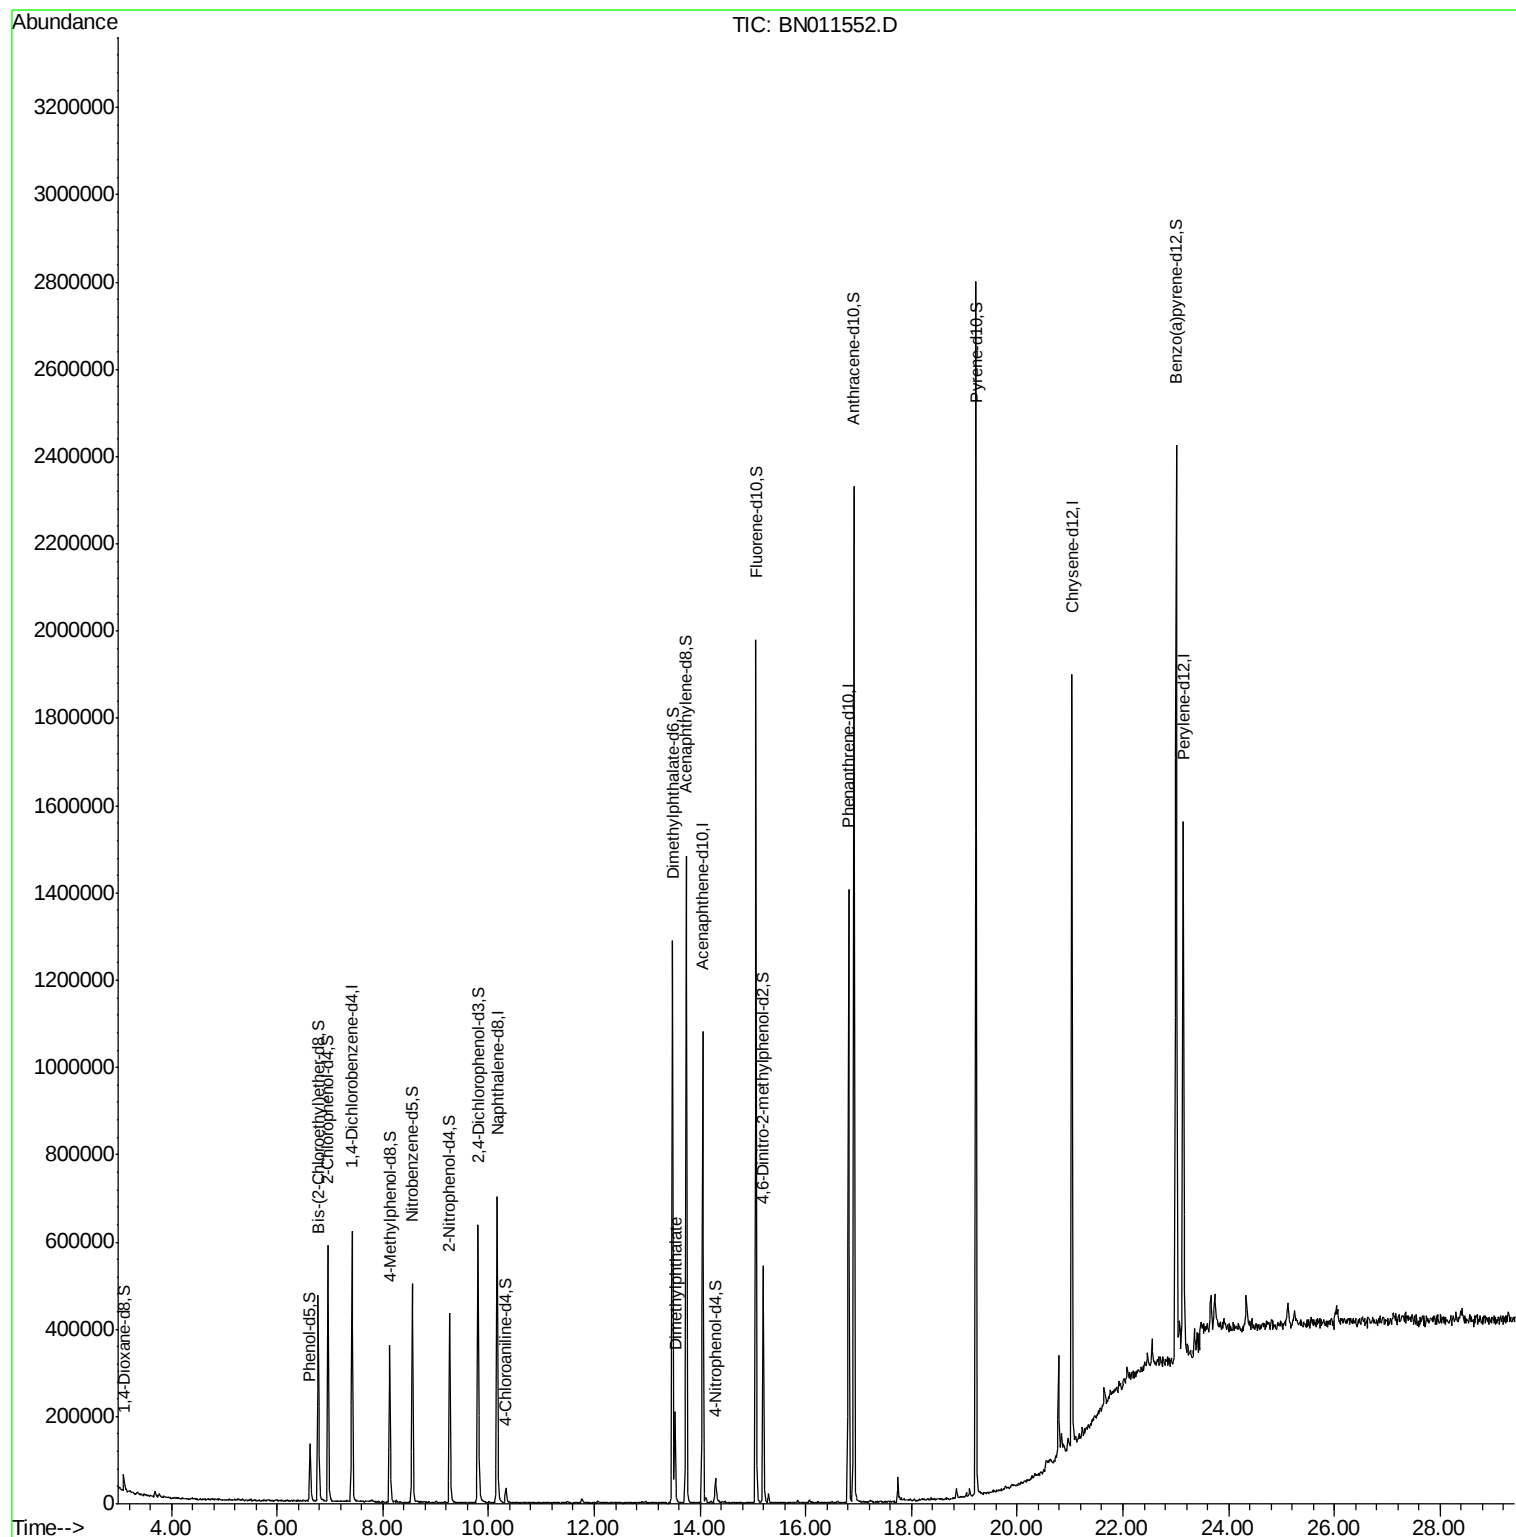

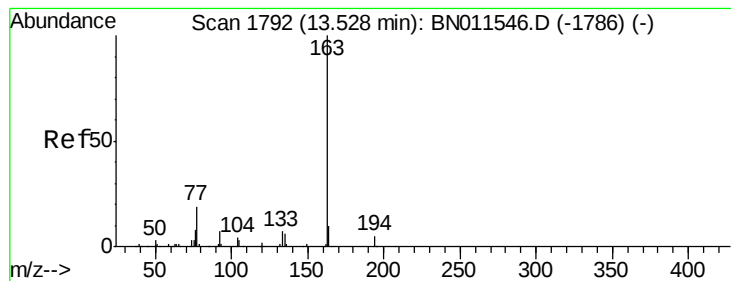

#45
 Dimethylphthalate
 Concen: 4.759 ng/ul
 RT: 13.53 min Scan# 1792
 Delta R.T. -0.01 min
 Lab File: BN011552.D
 Acq: 21 Aug 2020 08:52

Instrument :
 BNA_N
 ClientSampleId :
 DBFW1

Tot Ion	Ratio	Lower	Upper
163	100		
194	4.3	3.8	5.6
164	10.1	8.7	13.1

