

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN082020\
 Data File : BN011553.D
 Acq On : 21 Aug 2020 09:28
 Operator : CG/JU
 Sample : L3708-15
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBFW3

Quant Time: Aug 21 11:01:40 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081420MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Aug 21 04:54:28 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.42	152	173888	20.00	ng/ul	0.00
18) Naphthalene-d8	10.16	136	670534	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.05	164	425845	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.81	188	930579	20.00	ng/ul	0.00
78) Chrysene-d12	21.03	240	935851	20.00	ng/ul	0.00
86) Perylene-d12	23.14	264	936225	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.10	96	23401	6.46	ng/uL	0.00
5) Phenol-d5	6.62	99	79132	6.44	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.78	67	186386	29.74	ng/ul	0.00
9) 2-Chlorophenol-d4	6.96	132	254558	23.10	ng/ul	0.00
13) 4-Methylphenol-d8	8.13	113	155069	15.53	ng/ul	0.00
19) Nitrobenzene-d5	8.56	128	153135	29.47	ng/ul	0.00
22) 2-Nitrophenol-d4	9.27	143	171759	29.39	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.80	165	295153	26.73	ng/ul	0.00
29) 4-Chloroaniline-d4	10.33	131	26252	1.99	ng/ul	0.01
44) Dimethylphthalate-d6	13.48	166	1049906	31.66	ng/ul	0.00
47) Acenaphthylene-d8	13.74	160	1218359	30.53	ng/ul	0.00
52) 4-Nitrophenol-d4	14.29	143	27311	4.86	ng/ul	0.00
58) Fluorene-d10	15.06	176	933397	32.16	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.19	200	167161	27.09	ng/ul	0.00
71) Anthracene-d10	16.91	188	1584222	35.64	ng/ul	0.00
79) Pyrene-d10	19.22	212	1824145	37.94	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.01	264	1660331	31.93	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.53	163	146479	4.304	ng/ul#	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN082020\
Data File : BN011553.D
Acq On : 21 Aug 2020 09:28
Operator : CG/JU
Sample : L3708-15
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBFW3

Quant Time: Aug 21 11:01:40 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081420MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Aug 21 04:54:28 2020
Response via : Initial Calibration

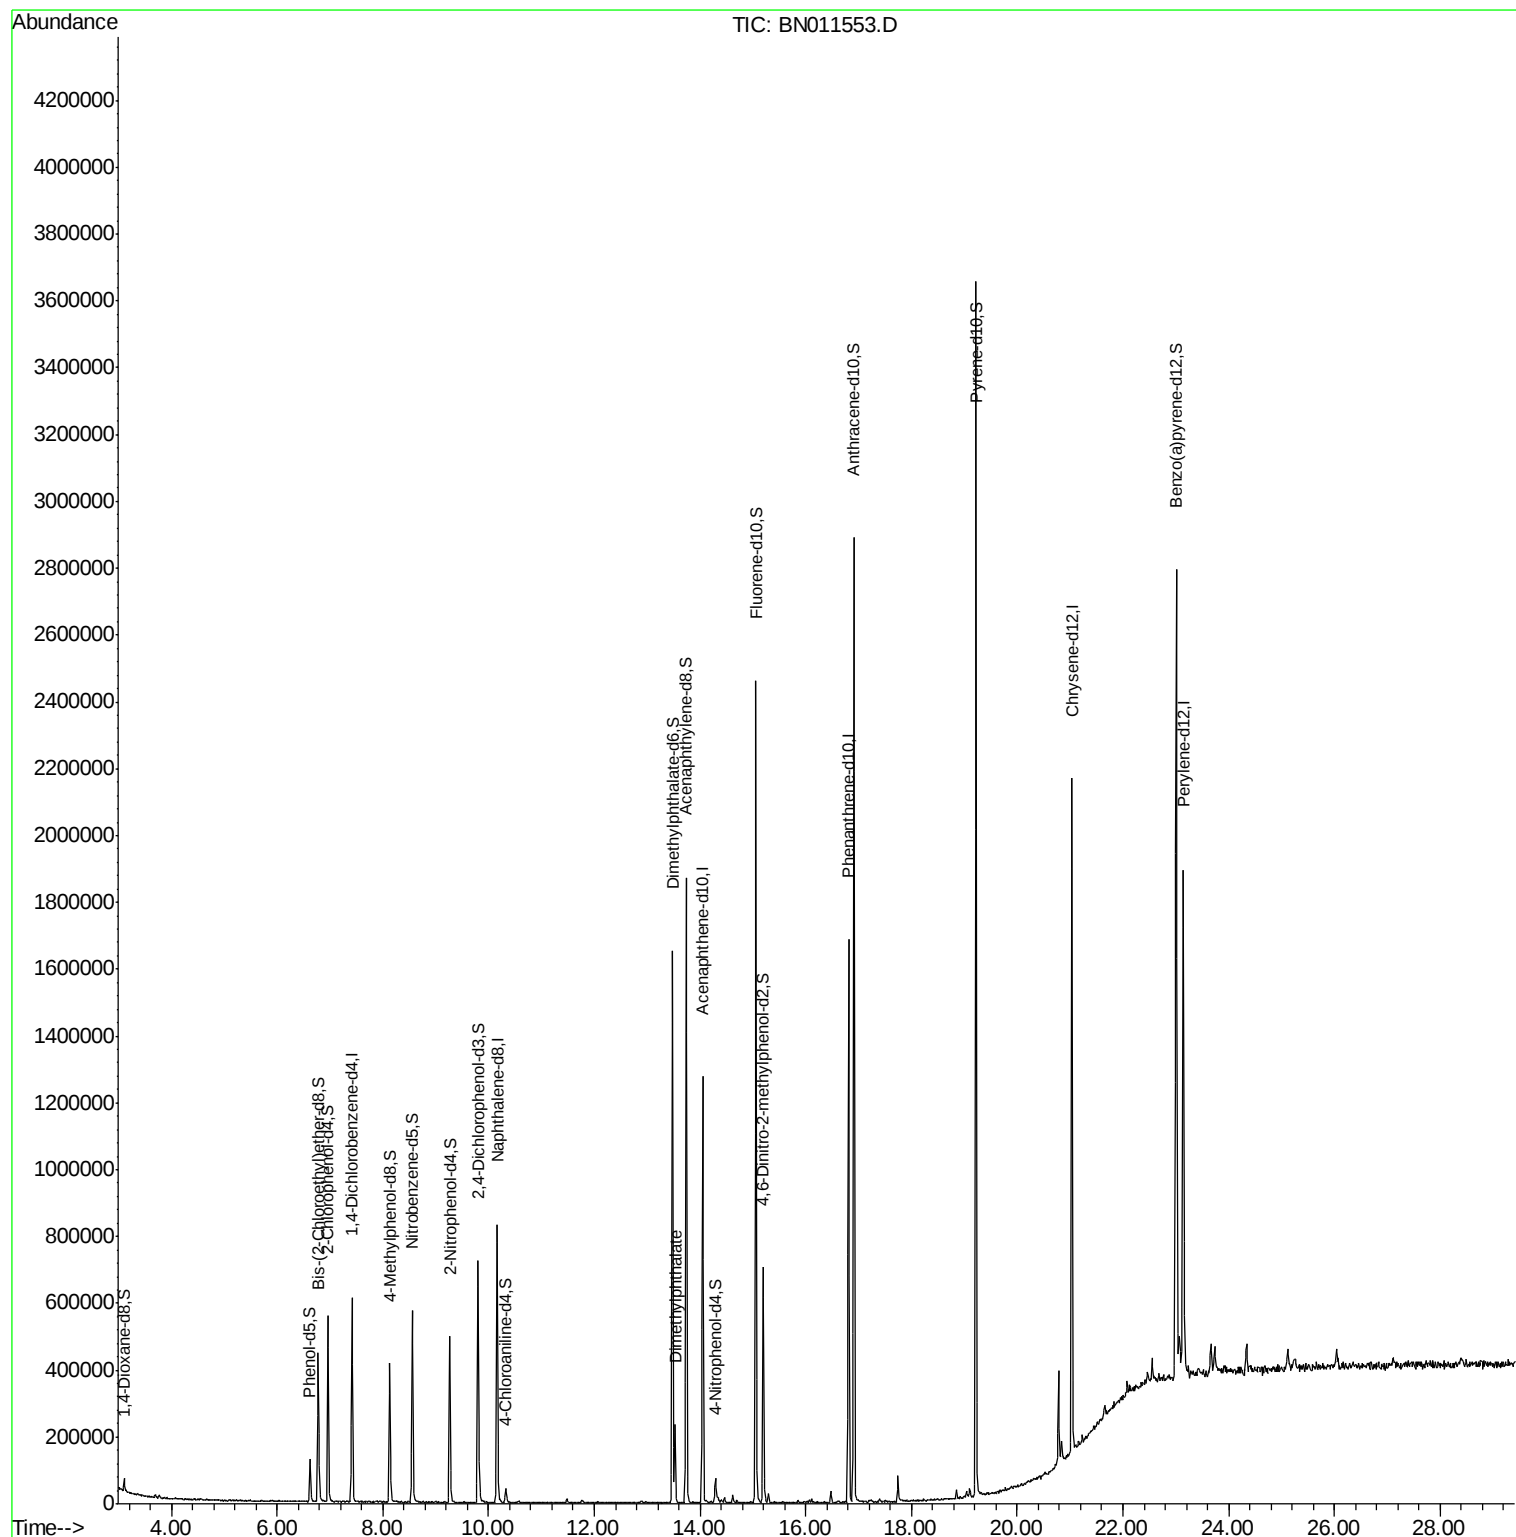

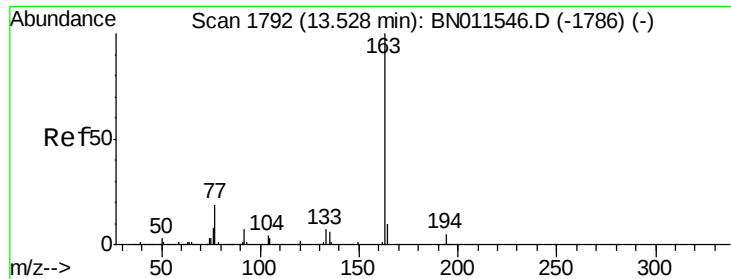

#45

Dimethylphthalate

Concen: 4.304 ng/ul

RT: 13.53 min Scan# 1792

Delta R.T. -0.01 min

Lab File: BN011553.D

Acq: 21 Aug 2020 09:28

Instrument :

BNA_N

ClientSampleId :

DBFW3


Tot Ion:163 Resp: 146479

Ion Ratio Lower Upper

163 100

194 4.1 3.8 5.6

164 7.8 8.7 13.1#

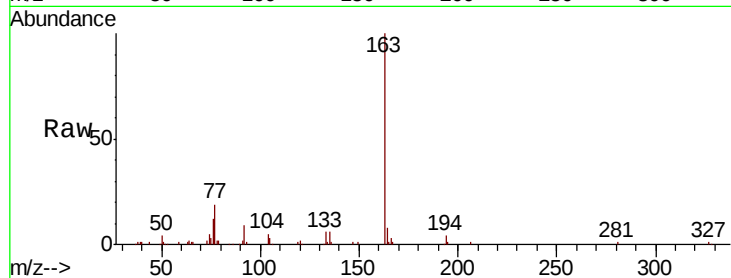

Abundance Ion 163.00 (162.70 to 163.70): E

150000 Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

