

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN082020\
 Data File : BN011523.D
 Acq On : 20 Aug 2020 13:42
 Operator : CG/JU
 Sample : PB131043BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK43

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081420MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.111	18	21	30	rVB	44628	67108	1.67%	0.174%
2	3.622	106	108	111	rBV4	4567	6724	0.17%	0.017%
3	3.787	131	136	138	rBV4	6072	8056	0.20%	0.021%
4	4.175	201	202	206	rVB3	5951	4476	0.11%	0.012%
5	4.222	208	210	213	rBV2	5804	4361	0.11%	0.011%
6	4.387	234	238	239	rBV3	4026	4649	0.12%	0.012%
7	4.628	278	279	284	rBV5	3567	4147	0.10%	0.011%
8	4.858	316	318	321	rVB3	3545	4396	0.11%	0.011%
9	6.628	613	619	628	rBV	681403	1049735	26.08%	2.725%
10	6.787	640	646	660	rVV	526969	838724	20.84%	2.178%
11	6.881	660	662	667	rVV4	3511	4339	0.11%	0.011%
12	6.969	670	677	686	rVV	794201	1218341	30.27%	3.163%
13	7.422	748	754	762	rBV	515583	801692	19.92%	2.081%
14	8.040	855	859	862	rBV5	2719	4263	0.11%	0.011%
15	8.134	869	875	888	rBV	880085	1366070	33.94%	3.547%
16	8.563	941	948	956	rBV	645867	1035358	25.72%	2.688%
17	8.816	989	991	996	rVB3	3013	4405	0.11%	0.011%
18	9.016	1022	1025	1028	rBV3	2779	4061	0.10%	0.011%
19	9.269	1062	1068	1076	rBV	553095	926907	23.03%	2.407%
20	9.805	1152	1159	1172	rBV	882925	1494167	37.12%	3.879%
21	10.169	1213	1221	1228	rBV	675523	1096977	27.25%	2.848%
22	10.316	1239	1246	1261	rBV	801779	1401885	34.83%	3.640%
23	10.822	1329	1332	1335	rBV4	2982	4350	0.11%	0.011%
24	11.769	1487	1493	1502	rBV6	11804	23363	0.58%	0.061%
25	13.487	1779	1785	1801	rVB	1574235	2208767	54.87%	5.735%
26	13.745	1822	1829	1838	rBV	1714331	2530589	62.86%	6.570%
27	13.922	1856	1859	1862	rBV5	4161	5273	0.13%	0.014%
28	14.057	1876	1882	1891	rBV2	1011054	1444107	35.87%	3.749%
29	14.287	1915	1921	1936	rVV	567036	909363	22.59%	2.361%
30	15.063	2046	2053	2061	rBV	2402239	3265558	81.12%	8.479%
31	15.198	2070	2076	2089	rBV	534973	752911	18.70%	1.955%
32	15.304	2089	2094	2100	rVB3	28178	37129	0.92%	0.096%
33	15.598	2142	2144	2149	rBV4	3882	7476	0.19%	0.019%
34	15.857	2184	2188	2190	rBV3	9274	11444	0.28%	0.030%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN082020\
 Data File : BN011523.D
 Acq On : 20 Aug 2020 13:42
 Operator : CG/JU
 Sample : PB131043BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK43

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081420MA.M
 Title : SVOA CALIBRATION

35	16.598	2312	2314	2318	rVB2	4253	5335	0.13%	0.014%
36	16.816	2345	2351	2361	rBV	1248104	1683378	41.82%	4.371%
37	16.916	2361	2368	2383	rVV2	2308393	3345555	83.11%	8.686%
38	17.592	2481	2483	2484	rBV	6895	4666	0.12%	0.012%
39	17.745	2502	2509	2515	rVV7	9163	18650	0.46%	0.048%
40	17.816	2517	2521	2524	rBV3	3225	5747	0.14%	0.015%
41	18.033	2555	2558	2559	rBV	4979	4343	0.11%	0.011%
42	18.116	2569	2572	2575	rBV4	4183	6211	0.15%	0.016%
43	18.504	2635	2638	2640	rBV3	2973	4154	0.10%	0.011%
44	18.616	2655	2657	2660	rVB4	5352	5187	0.13%	0.013%
45	18.651	2660	2663	2666	rBV5	7473	11007	0.27%	0.029%
46	18.857	2695	2698	2702	rBV3	28348	42666	1.06%	0.111%
47	19.051	2729	2731	2734	rVB3	8184	6545	0.16%	0.017%
48	19.110	2737	2741	2744	rBV2	22423	25652	0.64%	0.067%
49	19.228	2754	2761	2770	rBV	2865177	4025449	100.00%	10.451%
50	19.469	2800	2802	2803	rBV	7920	6704	0.17%	0.017%
51	19.575	2818	2820	2822	rBV3	6267	7242	0.18%	0.019%
52	19.622	2827	2828	2831	rBV3	11051	10626	0.26%	0.028%
53	19.710	2840	2843	2845	rBV3	11039	12594	0.31%	0.033%
54	20.839	3032	3035	3042	rBV3	44992	72893	1.81%	0.189%
55	21.039	3063	3069	3075	rBV	1359138	1785330	44.35%	4.635%
56	23.016	3398	3405	3413	rBV	1782127	3169201	78.73%	8.228%
57	23.145	3422	3427	3438	rVB	918494	1634519	40.60%	4.244%
58	27.474	4162	4163	4166	rBV2	65586	70692	1.76%	0.184%


Sum of corrected areas: 38515517

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN082020\
Data File : BN011523.D
Acq On : 20 Aug 2020 13:42
Operator : CG/JU
Sample : PB131043BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK43

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081420MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

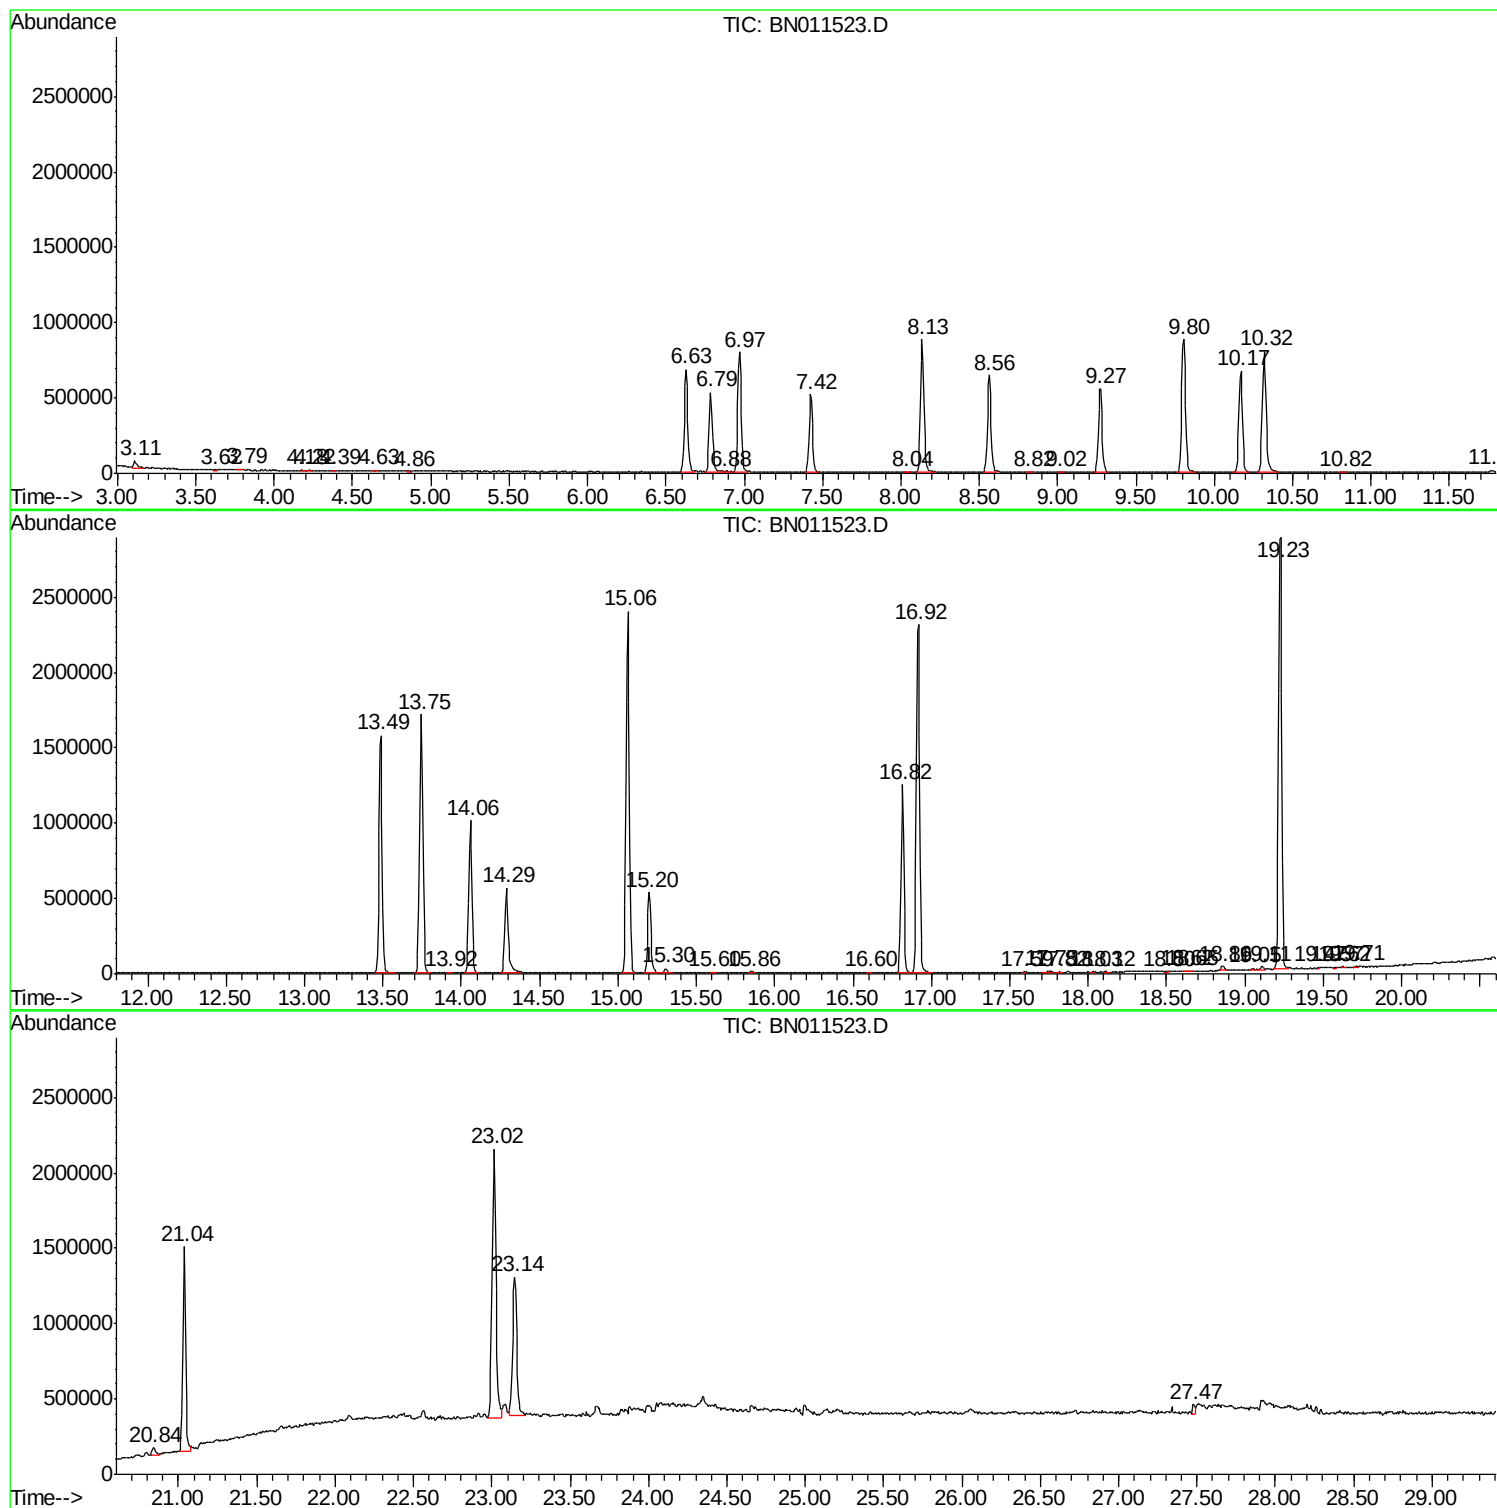

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN082020\
Data File : BN011523.D
Acq On : 20 Aug 2020 13:42
Operator : CG/JU
Sample : PB131043BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK43

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081420MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN082020\
Data File : BN011523.D
Acq On : 20 Aug 2020 13:42
Operator : CG/JU
Sample : PB131043BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK43

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081420MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc