

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN082020\
 Data File : BN011524.D
 Acq On : 20 Aug 2020 14:54
 Operator : CG/JU
 Sample : PB131045BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK45

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081420MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.052	9	11	13	rBV3	5627	4644	0.11%	0.011%
2	3.111	17	21	26	rVB	36665	55135	1.36%	0.136%
3	3.617	104	107	113	rVB3	19651	30895	0.76%	0.076%
4	3.781	131	135	139	rVV5	7543	10681	0.26%	0.026%
5	3.846	143	146	149	rVB3	4224	5749	0.14%	0.014%
6	6.105	526	530	532	rVB4	3858	4724	0.12%	0.012%
7	6.628	613	619	633	rVB	675934	1049362	25.82%	2.592%
8	6.787	639	646	659	rBV	498829	792520	19.50%	1.957%
9	6.969	670	677	689	rBV	801584	1223353	30.11%	3.022%
10	7.422	747	754	764	rBV	603412	925833	22.78%	2.287%
11	8.134	869	875	887	rBV	867579	1363048	33.54%	3.367%
12	8.563	940	948	959	rBV	590553	970630	23.89%	2.397%
13	8.752	977	980	986	rVB4	2912	4719	0.12%	0.012%
14	9.269	1061	1068	1082	rBV	526356	867368	21.35%	2.142%
15	9.805	1152	1159	1173	rBV	891584	1479401	36.41%	3.654%
16	10.169	1213	1221	1229	rBV	742698	1228431	30.23%	3.034%
17	10.316	1238	1246	1265	rBV	747388	1325457	32.62%	3.274%
18	11.769	1487	1493	1497	rBV5	9807	18091	0.45%	0.045%
19	13.487	1778	1785	1798	rBV	1441476	2056235	50.60%	5.079%
20	13.746	1822	1829	1841	rBV	1702150	2480499	61.04%	6.127%
21	13.922	1854	1859	1862	rBV4	3208	5280	0.13%	0.013%
22	14.057	1875	1882	1890	rBV	1211962	1732040	42.62%	4.278%
23	14.287	1915	1921	1936	rBV	540273	899371	22.13%	2.221%
24	15.063	2046	2053	2062	rBV	2223213	3138418	77.24%	7.752%
25	15.198	2070	2076	2089	rBV	516812	708453	17.43%	1.750%
26	15.298	2089	2093	2100	rVB2	22141	33269	0.82%	0.082%
27	15.851	2181	2187	2191	rBV5	7896	12509	0.31%	0.031%
28	16.492	2295	2296	2300	rBV3	4728	5649	0.14%	0.014%
29	16.604	2313	2315	2321	rVB2	5464	5982	0.15%	0.015%
30	16.816	2345	2351	2359	rBV	1500620	2091920	51.48%	5.167%
31	16.916	2359	2368	2376	rBV	2323773	3356398	82.60%	8.290%
32	17.751	2506	2510	2513	rBV4	7339	10494	0.26%	0.026%
33	18.145	2574	2577	2578	rVB2	4364	4069	0.10%	0.010%
34	18.175	2581	2582	2585	rBV2	4018	4837	0.12%	0.012%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN082020\
 Data File : BN011524.D
 Acq On : 20 Aug 2020 14:54
 Operator : CG/JU
 Sample : PB131045BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK45

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081420MA.M
 Title : SVOA CALIBRATION

35	18.557	2646	2647	2652	rBV4	2604	4203	0.10%	0.010%
36	18.857	2694	2698	2703	rBV2	23840	33618	0.83%	0.083%
37	18.957	2713	2715	2718	rBV3	4601	4074	0.10%	0.010%
38	19.022	2725	2726	2728	rBV2	4900	4182	0.10%	0.010%
39	19.110	2738	2741	2746	rVB	21580	24027	0.59%	0.059%
40	19.222	2753	2760	2773	rBV	3082539	4063453	100.00%	10.037%
41	19.428	2792	2795	2796	rBV3	6702	7852	0.19%	0.019%
42	19.480	2801	2804	2805	rBV3	8273	10002	0.25%	0.025%
43	19.810	2858	2860	2861	rVB2	12711	6314	0.16%	0.016%
44	19.822	2861	2862	2864	rBV2	7849	6864	0.17%	0.017%
45	20.263	2932	2937	2940	rBV7	18067	32308	0.80%	0.080%
46	20.786	3023	3026	3031	rBV2	58820	87196	2.15%	0.215%
47	20.839	3031	3035	3041	rBV	145920	205705	5.06%	0.508%
48	21.033	3063	3068	3081	rBV	1838824	2407193	59.24%	5.946%
49	23.010	3398	3404	3412	rBV	2000550	3311103	81.48%	8.178%
50	23.139	3421	3426	3440	rVB2	1180101	2167613	53.34%	5.354%
51	23.669	3513	3516	3522	rVB3	139065	205471	5.06%	0.508%


Sum of corrected areas: 40486642

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN082020\
Data File : BN011524.D
Acq On : 20 Aug 2020 14:54
Operator : CG/JU
Sample : PB131045BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK45

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081420MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

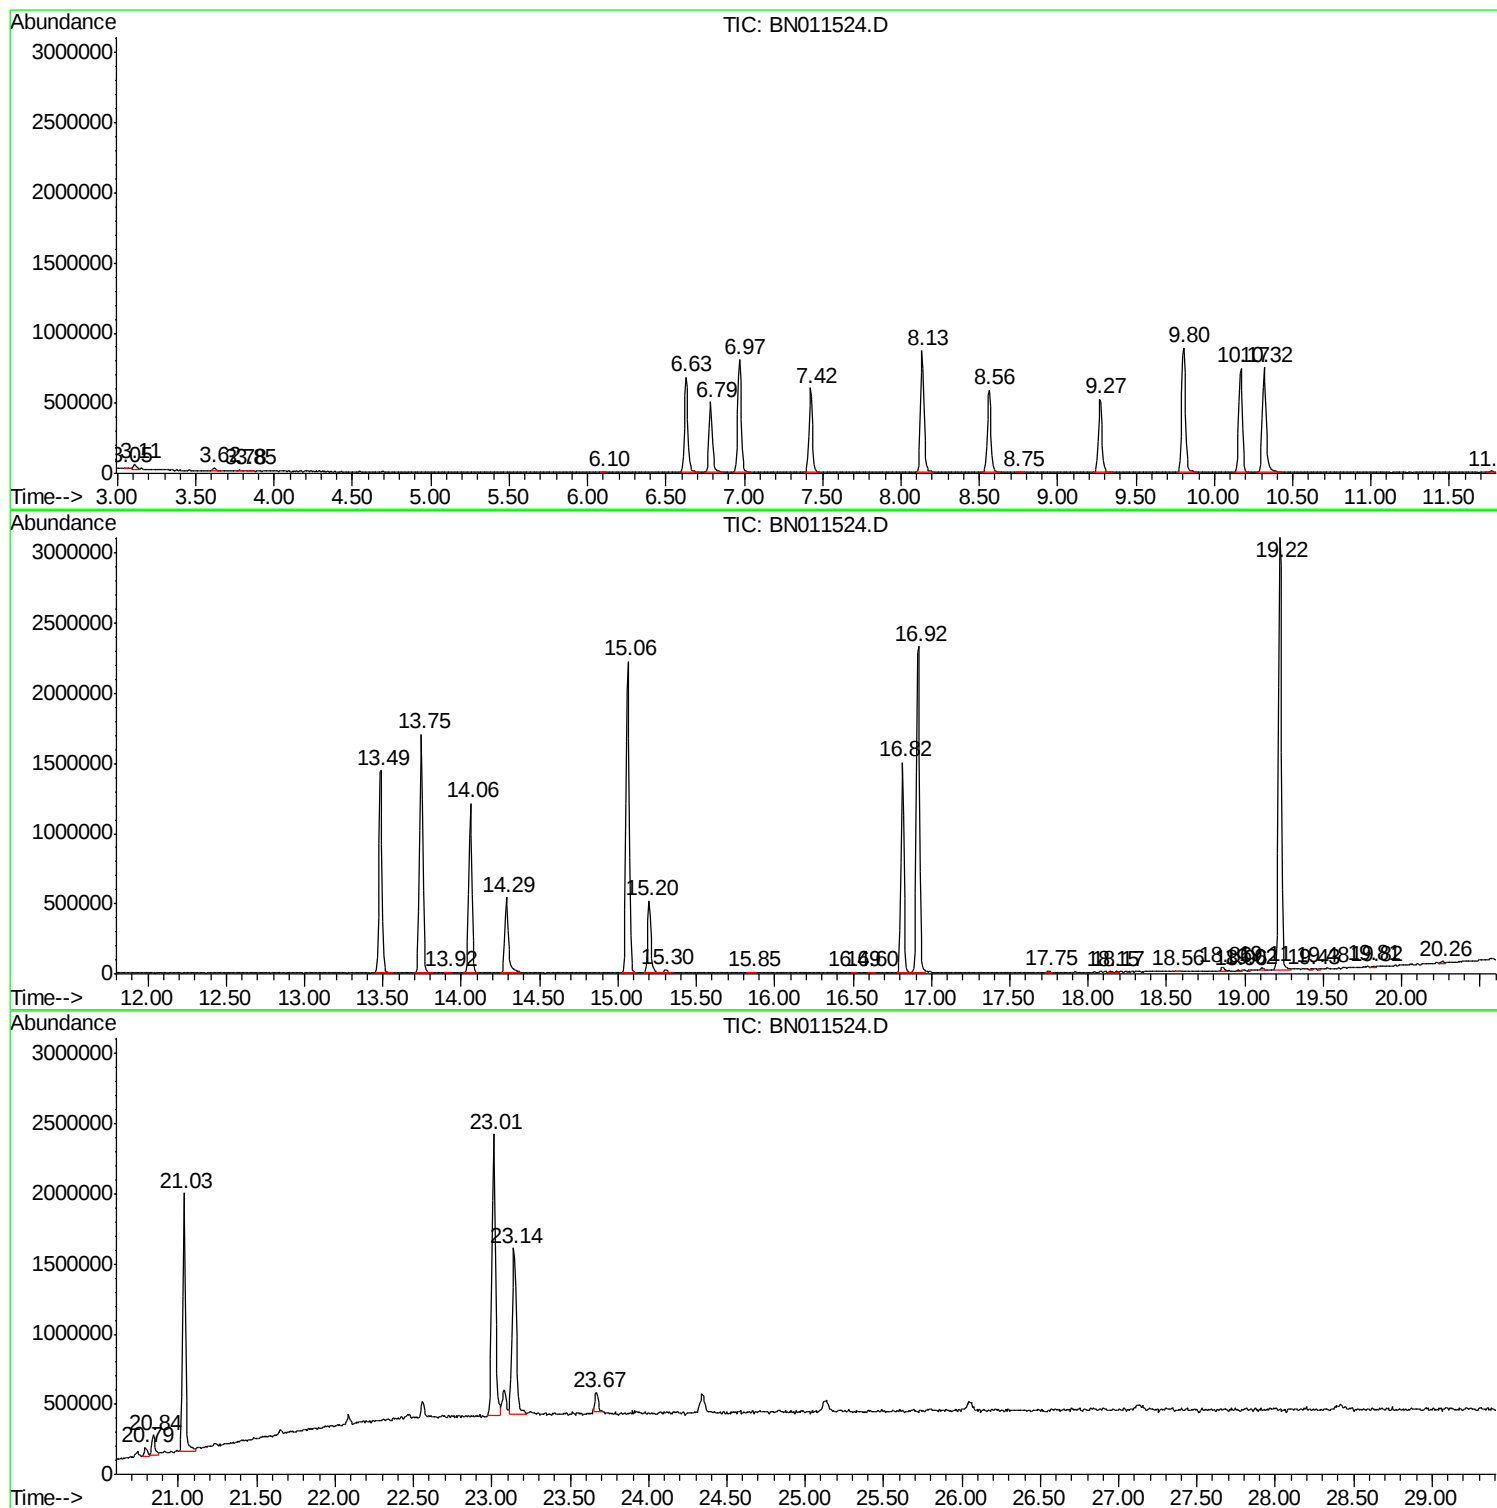

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN082020\
Data File : BN011524.D
Acq On : 20 Aug 2020 14:54
Operator : CG/JU
Sample : PB131045BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK45

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081420MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN082020\
Data File : BN011524.D
Acq On : 20 Aug 2020 14:54
Operator : CG/JU
Sample : PB131045BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK45

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081420MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc