

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN082020\
 Data File : BN011526.D
 Acq On : 20 Aug 2020 16:06
 Operator : CG/JU
 Sample : L3668-02DL2 50X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBFS4DL2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081420MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.358	62	63	66	rVB3	4271	3144	0.16%	0.026%
2	3.764	131	132	134	rBV2	5443	5151	0.26%	0.042%
3	3.958	163	165	168	rBV3	2214	2877	0.15%	0.024%
4	4.822	310	312	315	rBV2	2637	3121	0.16%	0.026%
5	4.869	318	320	323	rBV3	3258	3179	0.16%	0.026%
6	4.987	338	340	343	rVB3	4034	4164	0.21%	0.034%
7	5.052	348	351	355	rBV4	1976	2988	0.15%	0.025%
8	5.152	364	368	369	rBV4	3299	4135	0.21%	0.034%
9	5.493	423	426	427	rBV2	3121	2895	0.15%	0.024%
10	5.746	466	469	471	rBV4	3817	4330	0.22%	0.036%
11	6.287	559	561	563	rBV3	2868	3033	0.16%	0.025%
12	6.346	567	571	572	rVB3	2086	2495	0.13%	0.020%
13	6.369	572	575	577	rBV3	2372	2748	0.14%	0.023%
14	6.458	588	590	595	rVB5	2676	3595	0.18%	0.030%
15	6.793	640	647	650	rBV3	5030	9174	0.47%	0.075%
16	6.975	673	678	682	rBV5	6050	9612	0.49%	0.079%
17	7.046	687	690	693	rBV2	1702	2855	0.15%	0.023%
18	7.081	693	696	700	rVV3	5637	8140	0.42%	0.067%
19	7.152	704	708	714	rVB2	9686	14766	0.76%	0.121%
20	7.422	748	754	767	rVB	498979	792231	40.69%	6.504%
21	7.505	767	768	771	rBV3	2758	2928	0.15%	0.024%
22	7.528	771	772	777	rVB5	2452	2933	0.15%	0.024%
23	7.663	792	795	797	rBV3	1960	2730	0.14%	0.022%
24	7.775	813	814	821	rVB5	4437	7085	0.36%	0.058%
25	7.946	839	843	848	rBV	28415	41923	2.15%	0.344%
26	8.152	875	878	883	rBV4	4048	6342	0.33%	0.052%
27	8.263	894	897	904	rVB5	5355	9673	0.50%	0.079%
28	8.575	943	950	956	rVB6	6552	16382	0.84%	0.134%
29	8.757	977	981	984	rVV5	2783	4548	0.23%	0.037%
30	8.881	996	1002	1009	rVV7	6474	15996	0.82%	0.131%
31	8.946	1009	1013	1016	rVB3	3714	4883	0.25%	0.040%
32	9.193	1051	1055	1057	rVB3	3729	5072	0.26%	0.042%
33	9.281	1067	1070	1074	rBV4	5199	5854	0.30%	0.048%
34	9.434	1093	1096	1099	rVB2	2014	2768	0.14%	0.023%

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN082020\
 Data File : BN011526.D
 Acq On : 20 Aug 2020 16:06
 Operator : CG/JU
 Sample : L3668-02DL2 50X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBFS4DL2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081420MA.M
 Title : SVOA CALIBRATION

35	9.816	1158	1161	1162	rBV2	2878	3579	0.18%	0.029%
36	10.169	1214	1221	1225	rVV	655773	1103270	56.66%	9.057%
37	10.216	1225	1229	1239	rVV	1056953	1694180	87.01%	13.908%
38	10.334	1243	1249	1256	rVB	63065	110072	5.65%	0.904%
39	10.446	1266	1268	1270	rBV2	2922	2756	0.14%	0.023%
40	10.504	1275	1278	1282	rVB3	1718	3153	0.16%	0.026%
41	10.957	1352	1355	1359	rBV3	2100	3105	0.16%	0.025%
42	11.728	1483	1486	1490	rVB4	3345	4916	0.25%	0.040%
43	11.840	1499	1505	1515	rBV	101570	162941	8.37%	1.338%
44	11.951	1522	1524	1527	rBV3	4200	4988	0.26%	0.041%
45	12.063	1537	1543	1551	rVB	56205	96051	4.93%	0.789%
46	12.275	1578	1579	1583	rBV2	1964	2579	0.13%	0.021%
47	12.887	1677	1683	1688	rVV2	23889	33653	1.73%	0.276%
48	13.228	1736	1741	1747	rVB6	4757	9665	0.50%	0.079%
49	13.375	1763	1766	1772	rVB3	5300	8296	0.43%	0.068%
50	13.487	1780	1785	1790	rVV	19506	27593	1.42%	0.227%
51	13.534	1790	1793	1797	rVB3	1744	2722	0.14%	0.022%
52	13.616	1804	1807	1810	rBV2	2345	2882	0.15%	0.024%
53	13.745	1824	1829	1832	rBV	20677	28663	1.47%	0.235%
54	13.775	1832	1834	1837	rVB2	5231	6430	0.33%	0.053%
55	13.934	1858	1861	1862	rBV2	3357	2973	0.15%	0.024%
56	14.057	1876	1882	1888	rBV	1028924	1451281	74.53%	11.914%
57	14.122	1888	1893	1901	rVB	102302	147135	7.56%	1.208%
58	14.198	1901	1906	1911	rBV	21600	34168	1.75%	0.280%
59	14.463	1946	1951	1958	rBV	58453	86476	4.44%	0.710%
60	14.622	1974	1978	1983	rVB6	5119	7452	0.38%	0.061%
61	14.834	2011	2014	2018	rBV3	1495	2618	0.13%	0.021%
62	14.963	2033	2036	2041	rBV3	1571	2555	0.13%	0.021%
63	15.063	2048	2053	2057	rBV	30211	44075	2.26%	0.362%
64	15.122	2058	2063	2068	rVB	48952	66049	3.39%	0.542%
65	15.239	2076	2083	2087	rVB3	3493	6521	0.33%	0.054%
66	15.798	2175	2178	2179	rBV2	3459	3044	0.16%	0.025%
67	15.939	2198	2202	2205	rVB3	2683	4210	0.22%	0.035%
68	16.104	2226	2230	2235	rBV2	6666	11471	0.59%	0.094%
69	16.192	2242	2245	2249	rVB3	2028	2807	0.14%	0.023%
70	16.481	2286	2294	2298	rBV5	5410	10369	0.53%	0.085%
71	16.551	2301	2306	2307	rVB4	2023	3182	0.16%	0.026%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN082020\
 Data File : BN011526.D
 Acq On : 20 Aug 2020 16:06
 Operator : CG/JU
 Sample : L3668-02DL2 50X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBFS4DL2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081420MA.M
 Title : SVOA CALIBRATION

72	16.598	2312	2314	2317	rBV2	3070	3103	0.16%	0.025%
73	16.634	2317	2320	2324	rVB2	3217	3536	0.18%	0.029%
74	16.816	2343	2351	2356	rVV	1281336	1730807	88.89%	14.209%
75	16.851	2356	2357	2362	rVV2	43567	49910	2.56%	0.410%
76	16.916	2364	2368	2379	rVV2	36370	61938	3.18%	0.508%
77	17.069	2391	2394	2397	rVB2	1655	2529	0.13%	0.021%
78	17.228	2416	2421	2427	rBV	86650	119576	6.14%	0.982%
79	17.398	2446	2450	2455	rBV4	7128	12758	0.66%	0.105%
80	17.639	2489	2491	2494	rVV3	2603	2776	0.14%	0.023%
81	17.751	2506	2510	2514	rVB4	5669	8193	0.42%	0.067%
82	18.039	2556	2559	2561	rBV3	3590	3689	0.19%	0.030%
83	18.110	2568	2571	2574	rBV4	3255	3794	0.19%	0.031%
84	18.139	2574	2576	2580	rVB4	4744	4543	0.23%	0.037%
85	18.180	2580	2583	2585	rBV3	3180	3285	0.17%	0.027%
86	18.457	2627	2630	2631	rBV3	3617	3856	0.20%	0.032%
87	18.645	2660	2662	2665	rBV4	3824	4527	0.23%	0.037%
88	18.716	2673	2674	2677	rBV3	2782	2852	0.15%	0.023%
89	18.939	2711	2712	2715	rBV3	4787	3984	0.20%	0.033%
90	19.080	2733	2736	2737	rBV3	4013	4572	0.23%	0.038%
91	19.110	2739	2741	2743	rBV3	3634	3765	0.19%	0.031%
92	19.169	2749	2751	2753	rBV3	3721	3686	0.19%	0.030%
93	19.222	2757	2760	2766	rVB2	39719	59569	3.06%	0.489%
94	19.351	2780	2782	2784	rBV3	4061	3993	0.21%	0.033%
95	19.422	2792	2794	2797	rBV3	5643	7170	0.37%	0.059%
96	20.786	3023	3026	3030	rBV2	58876	74852	3.84%	0.614%
97	20.839	3031	3035	3041	rVV	152355	203699	10.46%	1.672%
98	21.033	3063	3068	3079	rBV	1549453	1947146	100.00%	15.985%
99	23.139	3421	3426	3436	rVB2	864816	1591502	81.74%	13.065%
100	25.515	3829	3830	3832	rBV	60736	44058	2.26%	0.362%


Sum of corrected areas: 12181298

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN082020\
Data File : BN011526.D
Acq On : 20 Aug 2020 16:06
Operator : CG/JU
Sample : L3668-02DL2 50X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBFS4DL2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081420MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

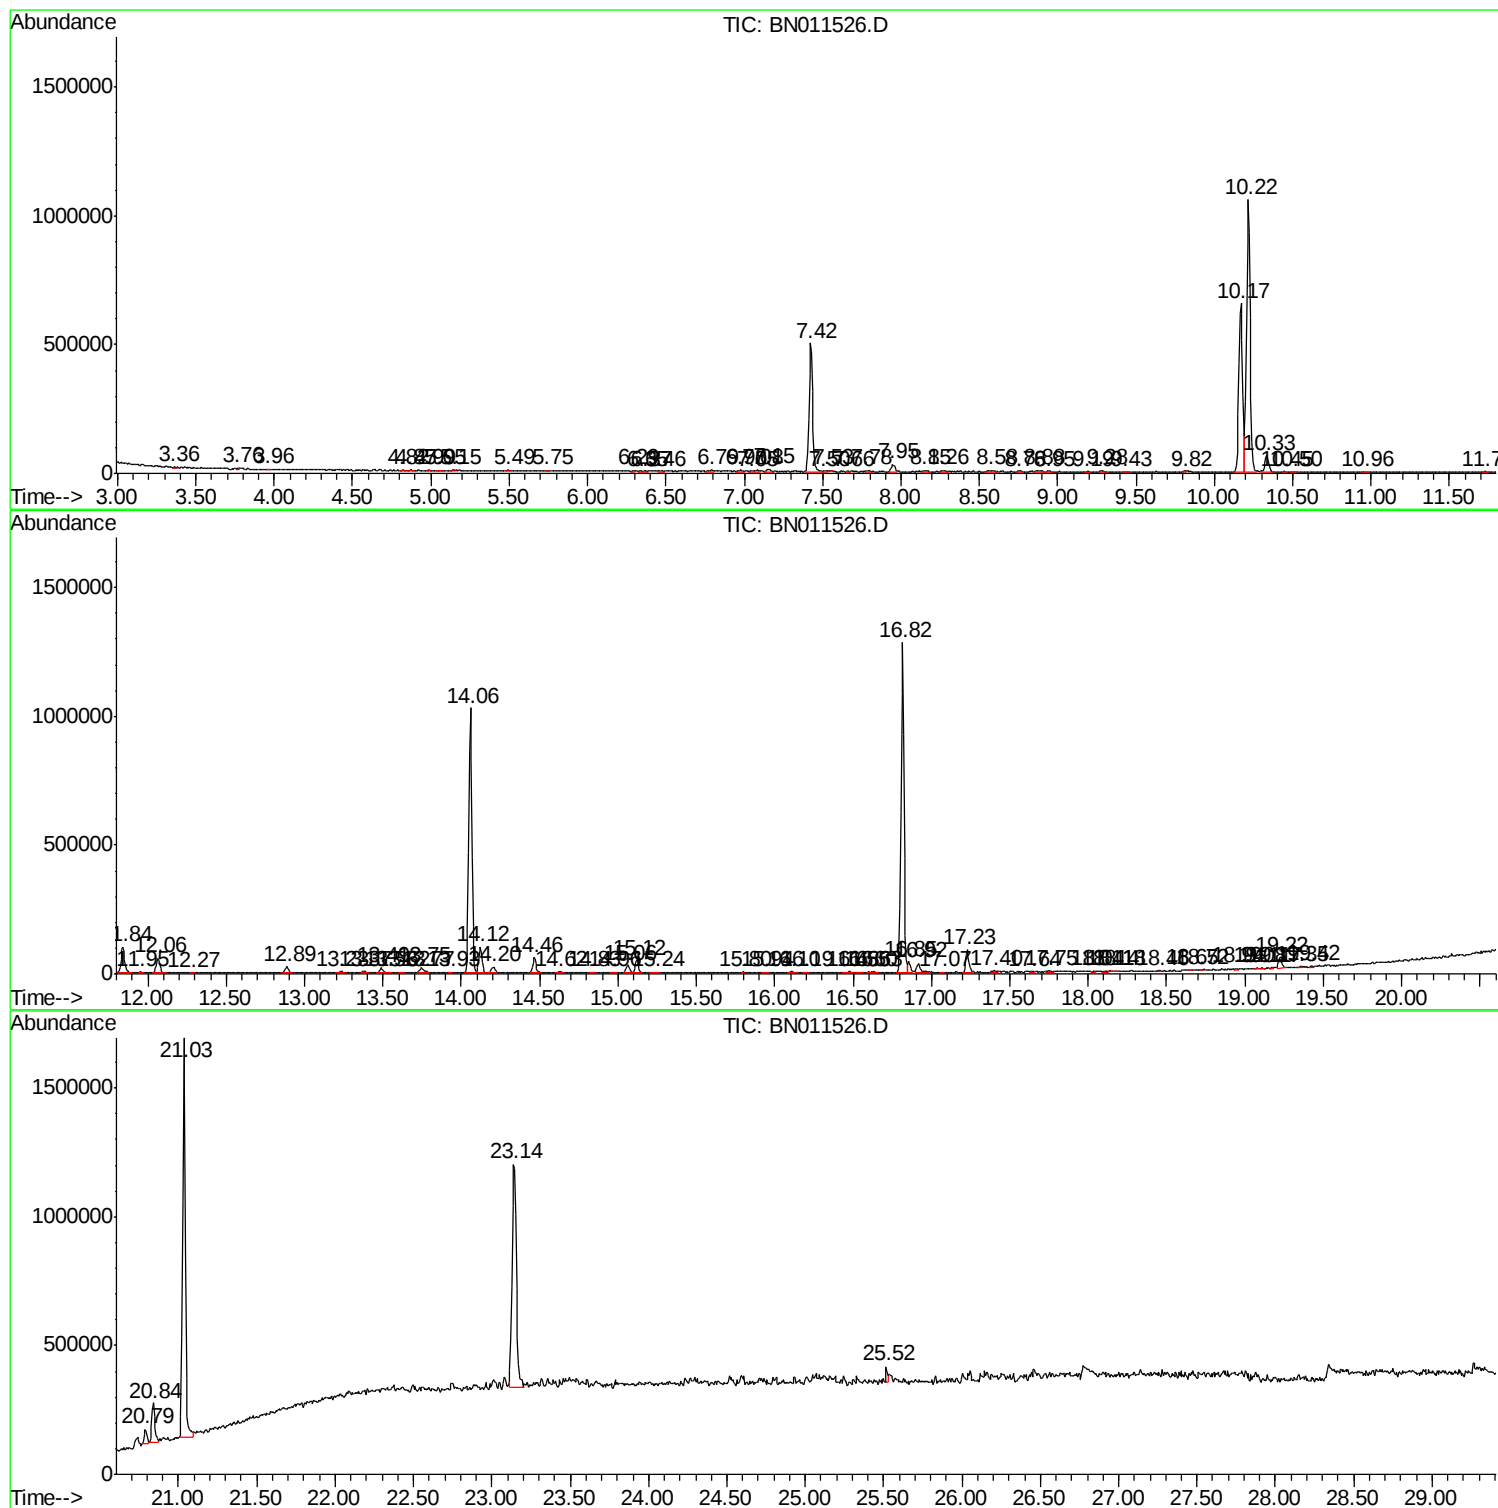

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN082020\
Data File : BN011526.D
Acq On : 20 Aug 2020 16:06
Operator : CG/JU
Sample : L3668-02DL2 50X
Misc :
ALS Vial : 6 Sample Multiplier: 1










Instrument :
BNA_N
ClientSampleId :
DBFS4DL2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081420MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2,2'-(Ethane-1,2-diylbis(ox... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.		
20.84	2.09 ng/ul	203699	Chrysene-d12	21.03		
Hit# of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2,2'-(Ethane-1,2-diylbis(oxv))bi...	358	C20H22O6	1000366-99-4	78	
2	3-Benzoylamino-2-benzyl-butvric ...	311	C19H21NO3	1000193-12-7	78	
3	Benzoic acid, 2-(3-nitrophenyl)e...	271	C15H13NO4	1000368-22-4	72	
4	Diethylene glycol dibenzoate	314	C18H18O5	000120-55-8	64	
5	Benzoic acid, 2-(2-chlorophenoxy...	276	C15H13ClO3	1000368-25-9	64	

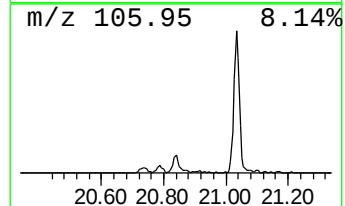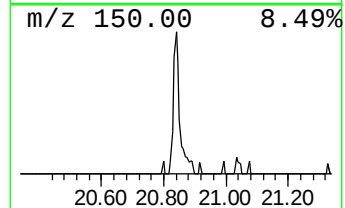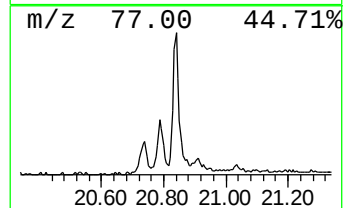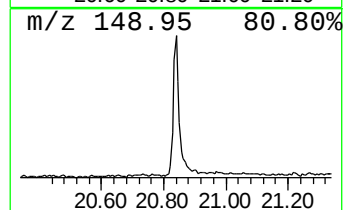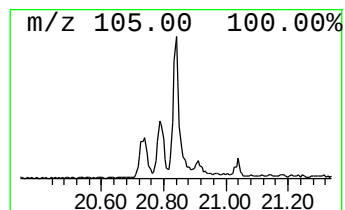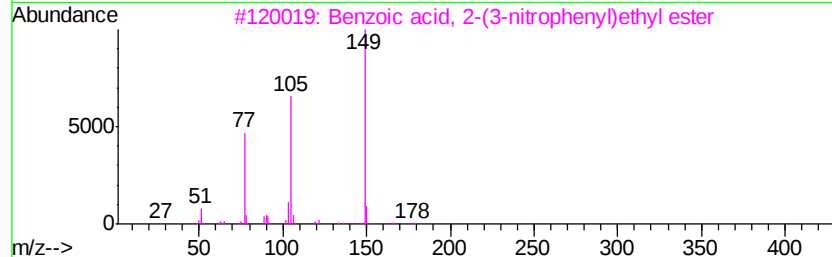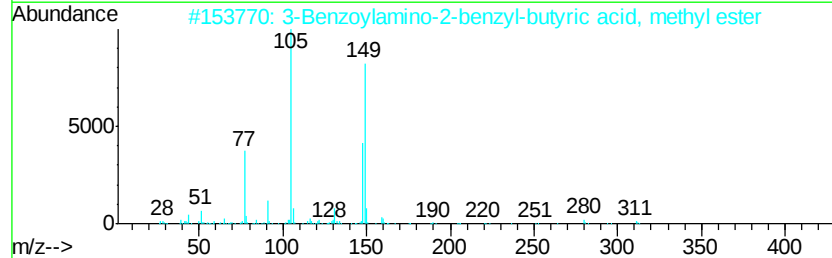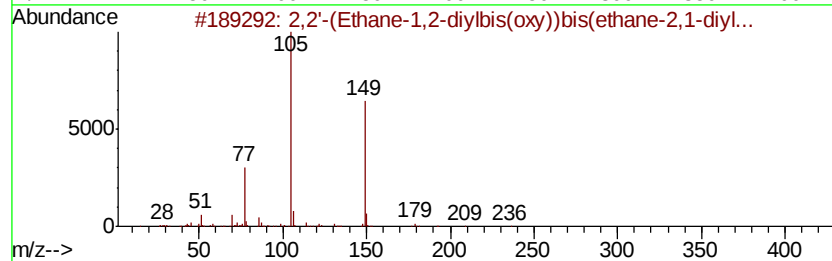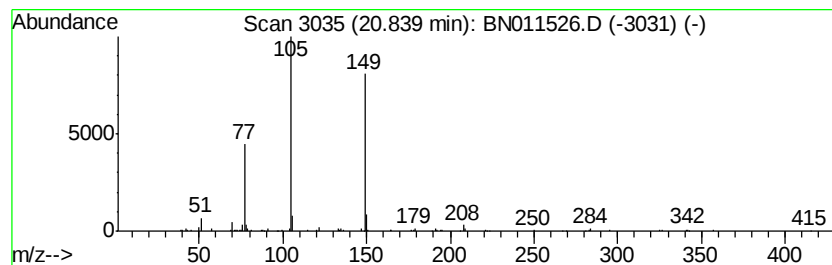

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN082020\
Data File : BN011526.D
Acq On : 20 Aug 2020 16:06
Operator : CG/JU
Sample : L3668-02DL2 50X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBFS4DL2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081420MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2,2'-(Ethane-1,2-...	20.84	2.1	ng/ul	203699	5	21.03	1947150	20.0