

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082021\
 Data File : BN015998.D
 Acq On : 20 Aug 2021 22:40
 Operator : CG/JU
 Sample : M3448-12
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBKF1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN015998.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.740	109	111	116	rBV2	107540	156143	2.35%	0.264%
2	7.034	666	671	680	rVB	203190	348988	5.25%	0.590%
3	7.205	694	700	711	rVB	749822	1266325	19.06%	2.139%
4	7.405	727	734	745	rVB	793283	1331014	20.03%	2.249%
5	7.875	807	814	823	rBV	815859	1343235	20.22%	2.269%
6	8.440	908	910	913	rBV3	5705	7613	0.11%	0.013%
7	8.581	927	934	941	rVB	581632	971197	14.62%	1.641%
8	9.034	1003	1011	1018	rBV	1011394	1753131	26.39%	2.962%
9	9.463	1081	1084	1087	rBV4	7863	9396	0.14%	0.016%
10	9.758	1127	1134	1143	rVB	754117	1297680	19.53%	2.192%
11	10.293	1218	1225	1233	rBV	1041997	1810596	27.25%	3.059%
12	10.463	1250	1254	1257	rBV3	10953	14024	0.21%	0.024%
13	10.675	1282	1290	1298	rBV	1105795	1898336	28.57%	3.207%
14	10.810	1305	1313	1323	rBV	984724	1713448	25.79%	2.895%
15	11.458	1420	1423	1427	rBV5	4172	6905	0.10%	0.012%
16	11.881	1492	1495	1498	rBV4	6681	8595	0.13%	0.015%
17	11.963	1505	1509	1512	rVB5	6673	8204	0.12%	0.014%
18	12.263	1555	1560	1567	rVB4	17224	32976	0.50%	0.056%
19	12.757	1639	1644	1645	rBV4	6920	9491	0.14%	0.016%
20	12.881	1658	1665	1670	rBV6	9047	20968	0.32%	0.035%
21	13.128	1700	1707	1708	rBV6	6620	9510	0.14%	0.016%
22	13.346	1739	1744	1748	rVB5	4247	8783	0.13%	0.015%
23	13.481	1761	1767	1769	rBV6	5618	8793	0.13%	0.015%
24	13.804	1816	1822	1823	rBV4	6420	7545	0.11%	0.013%
25	13.922	1834	1842	1854	rBV	2112751	3102988	46.70%	5.242%
26	14.204	1883	1890	1899	rVB	2371674	3562310	53.62%	6.018%
27	14.410	1921	1925	1929	rBV7	6098	9914	0.15%	0.017%
28	14.510	1932	1942	1950	rVV	1603701	2457735	36.99%	4.152%
29	14.569	1950	1952	1957	rVB6	5534	6908	0.10%	0.012%
30	14.704	1969	1975	1984	rBV2	170821	270878	4.08%	0.458%
31	15.328	2073	2081	2085	rBV6	11253	25762	0.39%	0.044%
32	15.363	2085	2087	2095	rVB5	4584	8810	0.13%	0.015%
33	15.504	2104	2111	2118	rBV	3099309	4538811	68.31%	7.668%
34	15.616	2124	2130	2142	rBV	920057	1302863	19.61%	2.201%
35	15.740	2148	2151	2156	rVB2	34955	49978	0.75%	0.084%
36	15.922	2180	2182	2190	rBV6	6848	11116	0.17%	0.019%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082021\
 Data File : BN015998.D
 Acq On : 20 Aug 2021 22:40
 Operator : CG/JU
 Sample : M3448-12
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBKF1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
 Title : SVOA CALIBRATION

37	16.293	2241	2245	2249	rBV6	10190	16595	0.25%	0.028%
38	16.393	2259	2262	2270	rVB7	10390	16266	0.24%	0.027%
39	16.557	2286	2290	2294	rBV5	5705	10236	0.15%	0.017%
40	16.663	2305	2308	2313	rBV6	3927	7161	0.11%	0.012%
41	16.751	2316	2323	2326	rBV5	4820	10139	0.15%	0.017%
42	17.175	2394	2395	2401	rVB5	6983	9228	0.14%	0.016%
43	17.257	2401	2409	2416	rBV	1983037	2898503	43.62%	4.897%
44	17.357	2419	2426	2438	rVV	3724163	5401679	81.30%	9.125%
45	17.640	2469	2474	2479	rBV8	6931	13295	0.20%	0.022%
46	17.781	2493	2498	2499	rBV4	4635	7381	0.11%	0.012%
47	17.934	2520	2524	2532	rVB10	10271	15585	0.23%	0.026%
48	18.228	2573	2574	2578	rVB4	9374	10107	0.15%	0.017%
49	18.345	2591	2594	2595	rBV3	6370	6877	0.10%	0.012%
50	18.969	2695	2700	2701	rBV5	6198	9013	0.14%	0.015%
51	19.216	2738	2742	2749	rVB7	23900	32377	0.49%	0.055%
52	19.287	2749	2754	2758	rBV2	45503	65853	0.99%	0.111%
53	19.534	2794	2796	2801	rBV3	19469	27900	0.42%	0.047%
54	19.651	2809	2816	2823	rBV	4615172	6332055	95.30%	10.697%
55	19.881	2851	2855	2860	rBV	202160	261146	3.93%	0.441%
56	19.992	2870	2874	2877	rBV6	15838	19114	0.29%	0.032%
57	20.651	2981	2986	2993	rBV	572715	745267	11.22%	1.259%
58	21.157	3068	3072	3078	rBV6	62691	106668	1.61%	0.180%
59	21.439	3115	3120	3132	rVB	2404749	3253601	48.97%	5.496%
60	23.116	3401	3405	3412	rVB6	96978	146895	2.21%	0.248%
61	23.686	3494	3502	3509	rBV2	3256089	6644173	100.00%	11.224%
62	23.839	3521	3528	3537	rVB2	1607567	3435039	51.70%	5.803%
63	24.463	3630	3634	3643	rVB3	150747	301339	4.54%	0.509%




Sum of corrected areas: 59194461

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082021\
Data File : BN015998.D
Acq On : 20 Aug 2021 22:40
Operator : CG/JU
Sample : M3448-12
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBKF1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

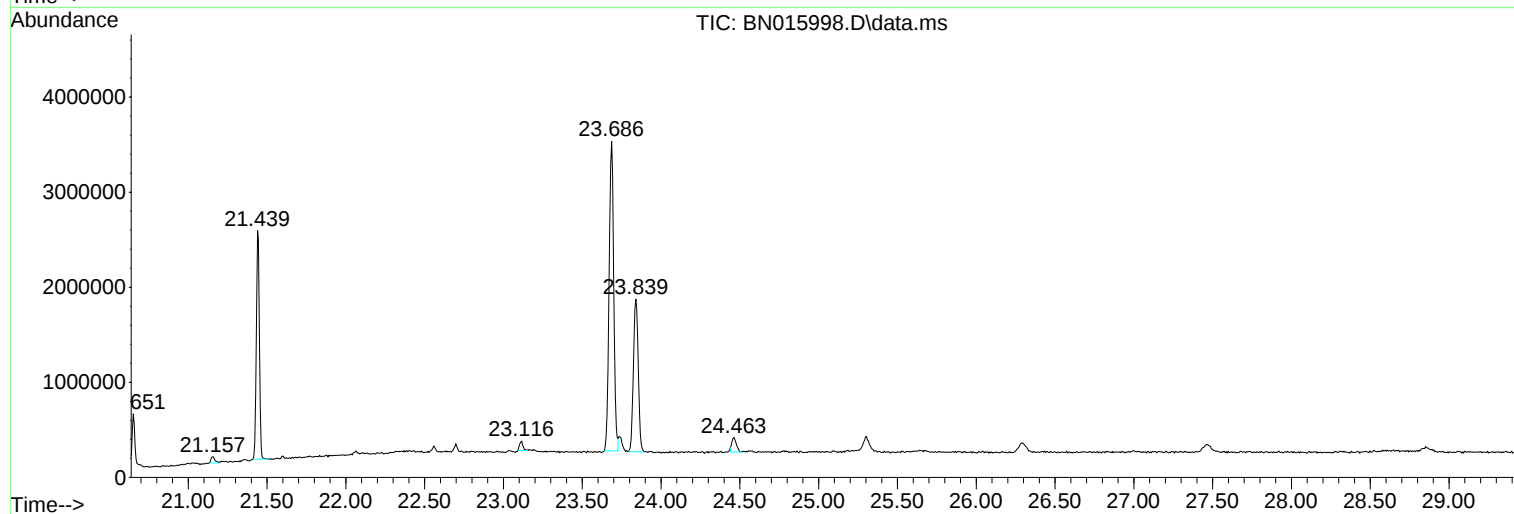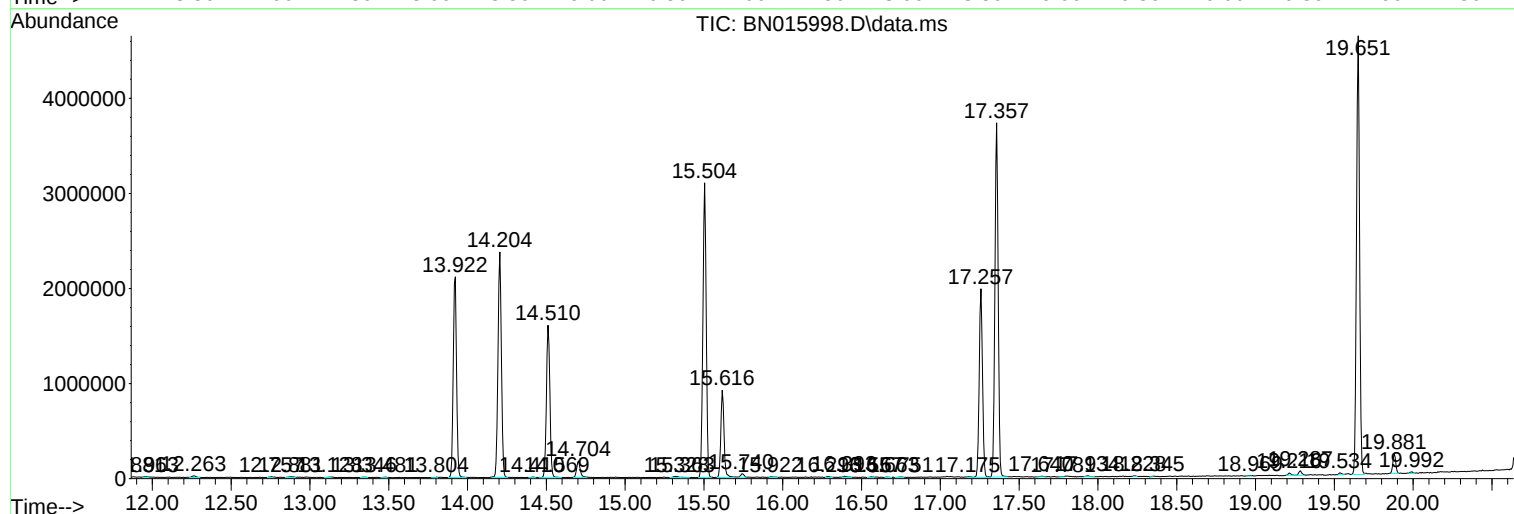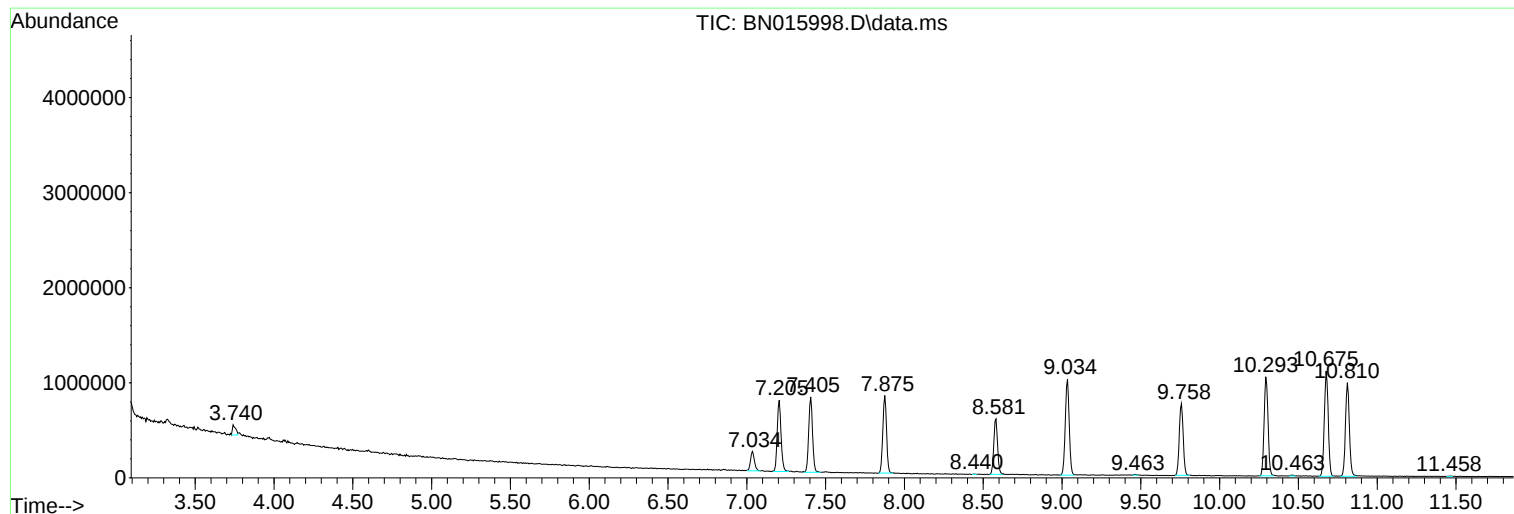

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082021\
Data File : BN015998.D
Acq On : 20 Aug 2021 22:40
Operator : CG/JU
Sample : M3448-12
Misc :
ALS Vial : 12 Sample Multiplier: 1










Instrument :
BNA_N
ClientSampleId :
DBKF1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Hexanedioic acid, bis(2-eth... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.	
20.651	4.58 ng/ul	745267	Chrysene-d12	21.439	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	Hexanedioic acid, bis(2-ethylhex...	370	C22H42O4	000103-23-1	91
2	Hexanedioic acid, dioctyl ester	370	C22H42O4	000123-79-5	90
3	Hexanedioic acid, bis(2-ethylhex...	370	C22H42O4	000103-23-1	90
4	Adipic acid, 2-ethylhexyl octyl ...	370	C22H42O4	1000324-48-6	90
5	Hexanedioic acid, bis(2-ethylhex...	370	C22H42O4	000103-23-1	87

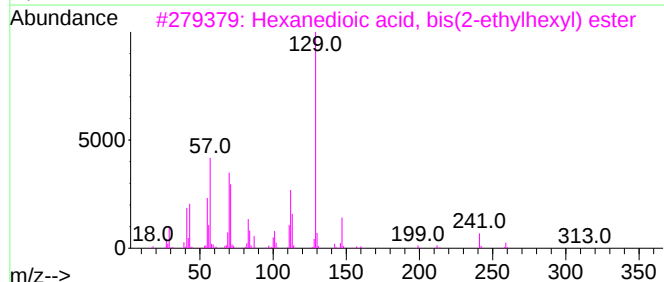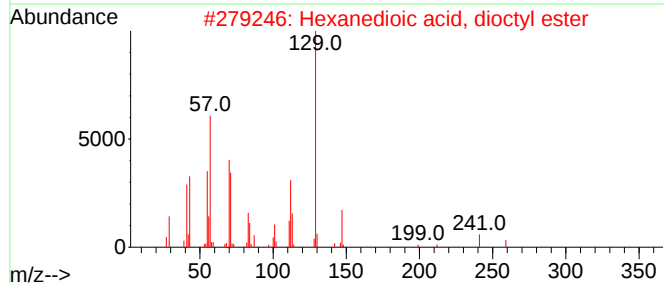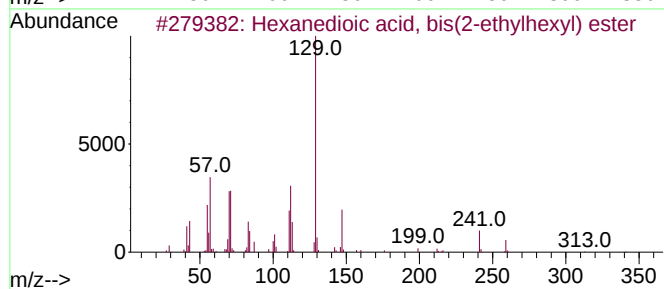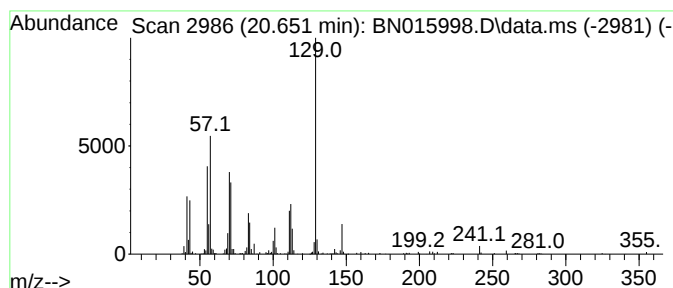

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082021\
Data File : BN015998.D
Acq On : 20 Aug 2021 22:40
Operator : CG/JU
Sample : M3448-12
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBKF1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Hexanedioic aci...	20.651	4.6	ng/u1	745267	5	21.439	3253600	20.0