

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082021\
 Data File : BN016001.D
 Acq On : 21 Aug 2021 00:30
 Operator : CG/JU
 Sample : M3448-16
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBKG1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN016001.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.740	108	111	121	rVB2	144200	282804	4.30%	0.455%
2	7.034	666	671	680	rVB	401622	665720	10.12%	1.071%
3	7.205	694	700	708	rBV	729506	1247508	18.97%	2.008%
4	7.405	727	734	744	rVB	915470	1536806	23.36%	2.473%
5	7.875	807	814	821	rBV	887721	1450468	22.05%	2.334%
6	8.575	926	933	942	rBV	929025	1567288	23.83%	2.522%
7	9.034	1001	1011	1020	rBV	1007676	1746052	26.55%	2.810%
8	9.140	1028	1029	1035	rVB5	4934	6831	0.10%	0.011%
9	9.346	1063	1064	1070	rBV6	5987	10661	0.16%	0.017%
10	9.758	1127	1134	1146	rVB	751968	1325412	20.15%	2.133%
11	10.293	1217	1225	1234	rBV	1181951	2043816	31.07%	3.289%
12	10.452	1247	1252	1258	rBV2	63174	108508	1.65%	0.175%
13	10.675	1283	1290	1298	rVB	1191647	2059248	31.31%	3.314%
14	10.810	1304	1313	1322	rBV	970966	1701802	25.87%	2.739%
15	11.499	1419	1430	1434	rBV8	16519	36036	0.55%	0.058%
16	11.963	1502	1509	1512	rBV8	6032	10732	0.16%	0.017%
17	12.263	1554	1560	1566	rVB3	19937	31087	0.47%	0.050%
18	12.757	1639	1644	1649	rVB6	8039	16755	0.25%	0.027%
19	12.875	1659	1664	1672	rVB8	7940	15724	0.24%	0.025%
20	13.134	1704	1708	1711	rVB4	6626	9489	0.14%	0.015%
21	13.922	1835	1842	1853	rBV	2201002	3354926	51.01%	5.399%
22	14.204	1883	1890	1900	rVB	2477091	3717204	56.51%	5.982%
23	14.510	1934	1942	1950	rBV	1744638	2657538	40.40%	4.277%
24	14.704	1967	1975	1981	rVV	238317	389341	5.92%	0.627%
25	14.746	1981	1982	1986	rVV4	12486	14445	0.22%	0.023%
26	14.798	1989	1991	1996	rVV7	4791	7273	0.11%	0.012%
27	14.857	1998	2001	2007	rVB5	6358	12774	0.19%	0.021%
28	15.251	2063	2068	2072	rBV6	8531	15570	0.24%	0.025%
29	15.322	2074	2080	2085	rBV8	10924	20740	0.32%	0.033%
30	15.504	2104	2111	2122	rBV	3186874	4688142	71.28%	7.545%
31	15.616	2124	2130	2145	rBV	946076	1338008	20.34%	2.153%
32	15.745	2148	2152	2156	rVB5	22033	31841	0.48%	0.051%
33	15.945	2184	2186	2191	rVB5	7069	8354	0.13%	0.013%
34	16.293	2240	2245	2246	rBV4	5107	7558	0.11%	0.012%
35	16.393	2257	2262	2266	rBV5	8530	18620	0.28%	0.030%
36	16.857	2336	2341	2346	rVB6	11925	20010	0.30%	0.032%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082021\
 Data File : BN016001.D
 Acq On : 21 Aug 2021 00:30
 Operator : CG/JU
 Sample : M3448-16
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBKG1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
 Title : SVOA CALIBRATION

37	16.940	2351	2355	2358	rBV6	4819	7174	0.11%	0.012%
38	17.045	2369	2373	2378	rVB5	8836	17169	0.26%	0.028%
39	17.257	2402	2409	2416	rBV	2205161	3121356	47.46%	5.023%
40	17.357	2419	2426	2435	rBV	3785812	5576106	84.78%	8.974%
41	17.540	2454	2457	2460	rVB5	8343	6970	0.11%	0.011%
42	17.634	2466	2473	2474	rBV5	8676	9735	0.15%	0.016%
43	17.792	2497	2500	2503	rBV5	6734	8330	0.13%	0.013%
44	17.934	2519	2524	2530	rVB8	11672	22491	0.34%	0.036%
45	18.051	2541	2544	2548	rVB4	7776	13099	0.20%	0.021%
46	18.157	2558	2562	2568	rVV7	5963	14183	0.22%	0.023%
47	18.228	2571	2574	2578	rVB2	15810	20590	0.31%	0.033%
48	18.645	2642	2645	2649	rBV5	6642	8349	0.13%	0.013%
49	18.775	2662	2667	2671	rVB8	7455	11852	0.18%	0.019%
50	19.063	2715	2716	2719	rBV3	6687	6965	0.11%	0.011%
51	19.216	2737	2742	2746	rBV2	43831	62036	0.94%	0.100%
52	19.286	2749	2754	2761	rVB	42379	71690	1.09%	0.115%
53	19.422	2775	2777	2780	rBV4	7584	8155	0.12%	0.013%
54	19.651	2809	2816	2823	rBV	4752602	6492748	98.71%	10.449%
55	19.733	2827	2830	2832	rVB4	10571	12739	0.19%	0.021%
56	20.651	2982	2986	2991	rBV	541835	653217	9.93%	1.051%
57	21.157	3068	3072	3077	rBV5	77413	130711	1.99%	0.210%
58	21.439	3115	3120	3130	rBV	2692500	3523003	53.56%	5.670%
59	23.686	3494	3502	3509	rBV	3301961	6577472	100.00%	10.585%
60	23.839	3521	3528	3537	rVB	1765396	3587699	54.55%	5.774%




Sum of corrected areas: 62138930

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082021\
Data File : BN016001.D
Acq On : 21 Aug 2021 00:30
Operator : CG/JU
Sample : M3448-16
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBKG1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

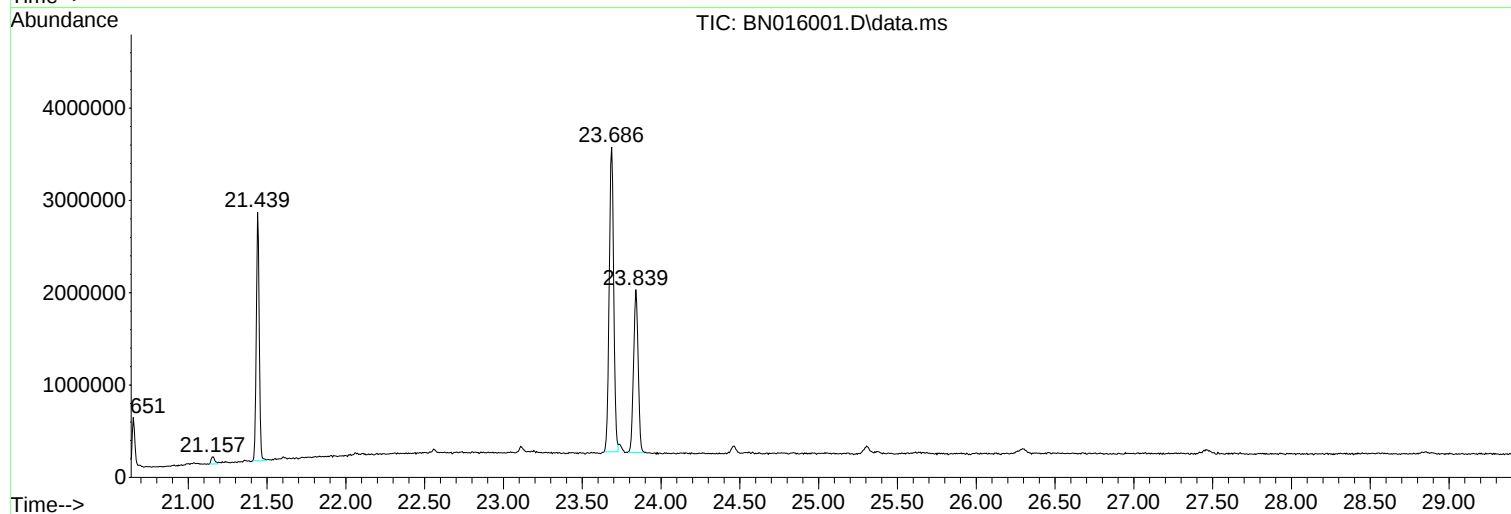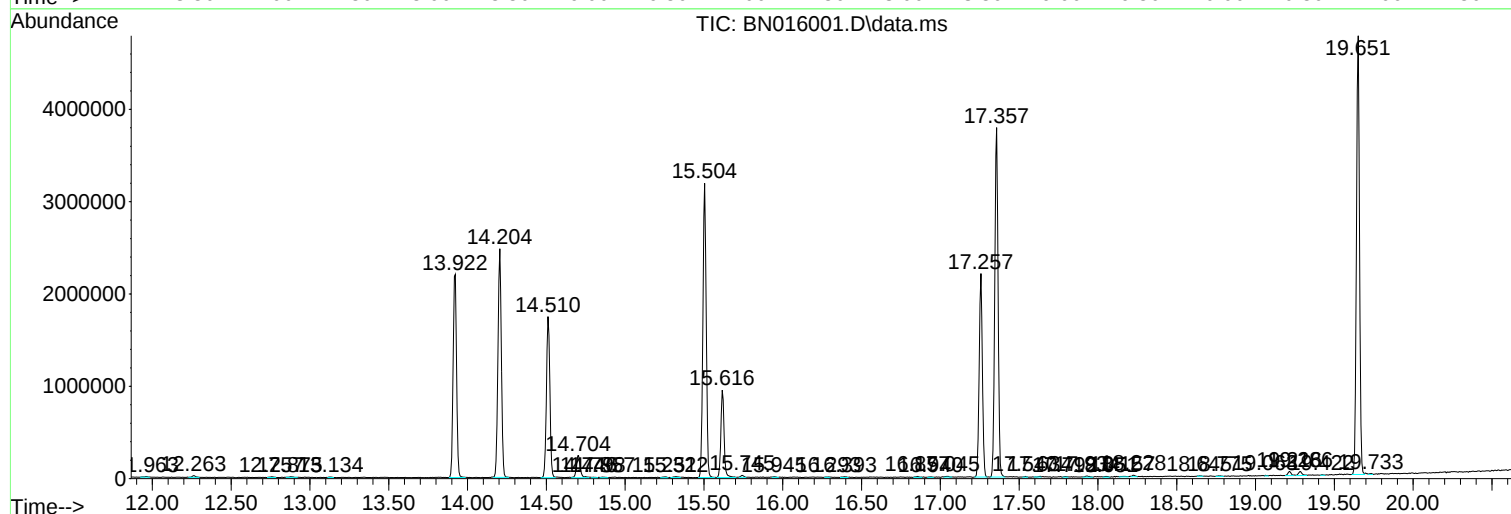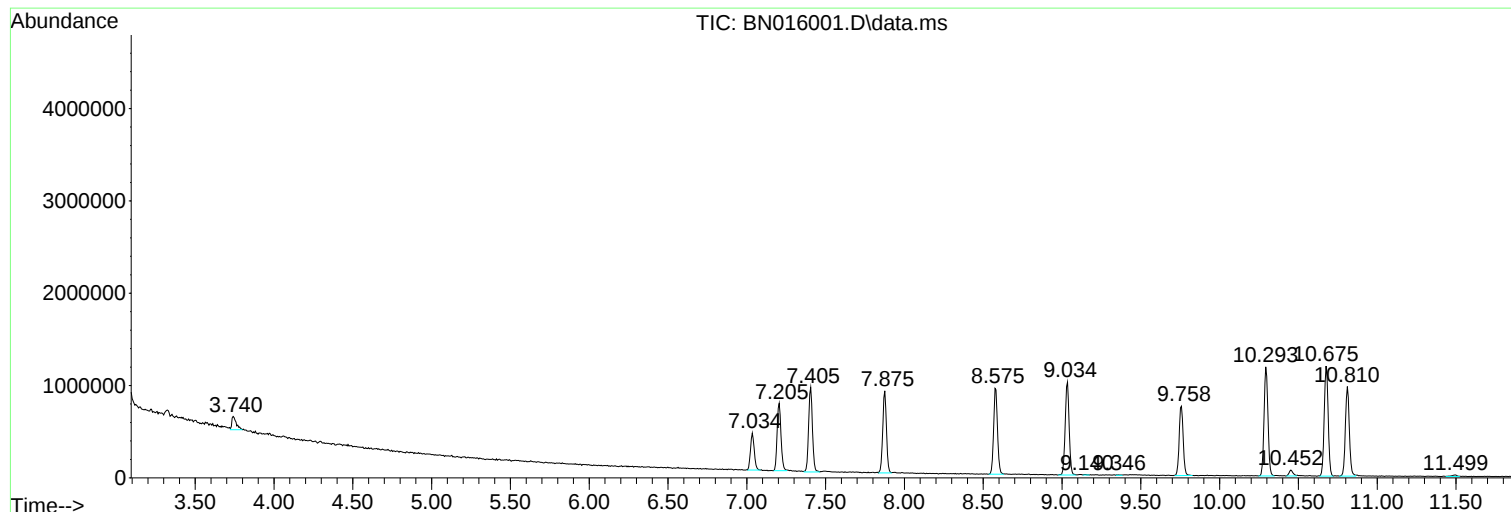

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082021\
Data File : BN016001.D
Acq On : 21 Aug 2021 00:30
Operator : CG/JU
Sample : M3448-16
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBKG1










Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Hexanedioic acid, dioctyl e... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
20.651	3.71 ng/ul	653217	Chrysene-d12	21.439

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Hexanedioic acid, dioctyl ester	370	C22H42O4	000123-79-5	90
2			Diisooctyl adipate	370	C22H42O4	001330-86-5	90
3			Hexanedioic acid, dioctyl ester	370	C22H42O4	000123-79-5	87
4			Hexanedioic acid, bis(2-ethylhex...	370	C22H42O4	000103-23-1	83
5			Hexanedioic acid, bis(2-ethylhex...	370	C22H42O4	000103-23-1	83

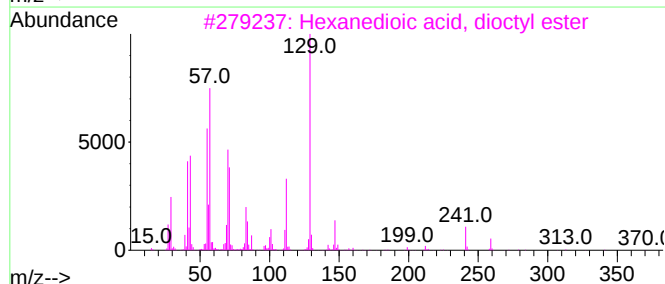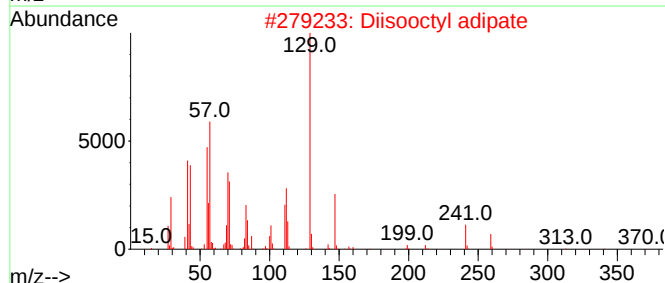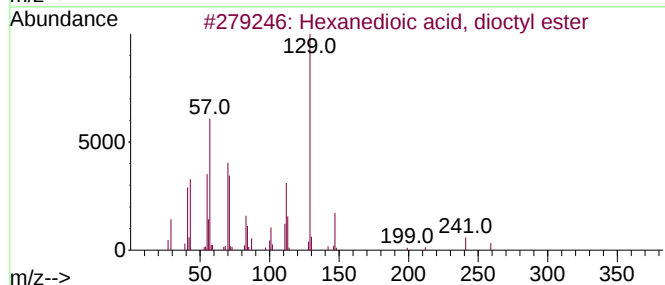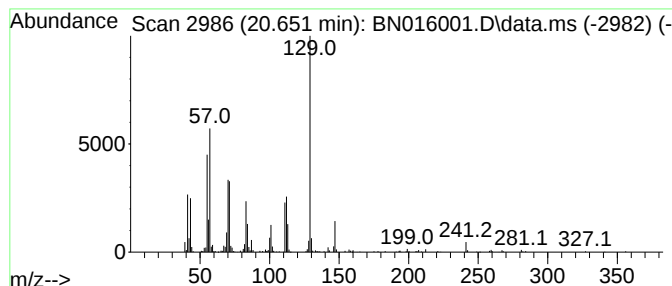

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082021\
Data File : BN016001.D
Acq On : 21 Aug 2021 00:30
Operator : CG/JU
Sample : M3448-16
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBKG1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Hexanedioic aci...	20.651	3.7	ng/ul	653217	5	21.439	3523000	20.0