

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082021\
 Data File : BN016004.D
 Acq On : 21 Aug 2021 02:20
 Operator : CG/JU
 Sample : M3448-07
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBKE6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN016004.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	7.034	666	671	679	rVB	254330	438878	6.35%	0.708%
2	7.205	694	700	712	rVB	810508	1361462	19.69%	2.196%
3	7.405	727	734	742	rVB	850379	1426895	20.64%	2.301%
4	7.875	807	814	822	rVB	815044	1401715	20.28%	2.261%
5	8.575	927	933	944	rBV	674371	1129172	16.33%	1.821%
6	9.034	1004	1011	1020	rVB	1109560	1906332	27.58%	3.075%
7	9.757	1126	1134	1145	rBV	781054	1383081	20.01%	2.231%
8	9.899	1155	1158	1162	rBV5	6890	9752	0.14%	0.016%
9	10.293	1218	1225	1235	rBV	1163512	1996448	28.88%	3.220%
10	10.675	1283	1290	1297	rVB	1162835	1993053	28.83%	3.215%
11	10.810	1304	1313	1325	rBV	1057900	1837451	26.58%	2.964%
12	11.322	1398	1400	1403	rBV3	5281	7146	0.10%	0.012%
13	11.951	1505	1507	1514	rVB7	5379	8771	0.13%	0.014%
14	12.263	1555	1560	1566	rVB4	21469	35865	0.52%	0.058%
15	12.751	1640	1643	1649	rBV4	6362	12095	0.17%	0.020%
16	12.887	1663	1666	1671	rVB6	4618	7634	0.11%	0.012%
17	13.304	1733	1737	1741	rVB4	4099	7516	0.11%	0.012%
18	13.916	1834	1841	1851	rBV	2183467	3271758	47.33%	5.277%
19	14.204	1880	1890	1903	rVB	2545584	3889900	56.27%	6.274%
20	14.510	1935	1942	1953	rBV	1697552	2587057	37.42%	4.173%
21	14.698	1969	1974	1983	rBV	178865	287927	4.16%	0.464%
22	15.310	2075	2078	2079	rBV3	8229	7851	0.11%	0.013%
23	15.334	2079	2082	2085	rVB5	8806	10221	0.15%	0.016%
24	15.504	2104	2111	2118	rBV	3284440	4764416	68.92%	7.685%
25	15.616	2123	2130	2140	rBV	934428	1309098	18.94%	2.111%
26	15.739	2147	2151	2156	rVB3	37658	53288	0.77%	0.086%
27	16.292	2239	2245	2247	rBV4	6137	8894	0.13%	0.014%
28	16.386	2258	2261	2263	rBV4	6306	7747	0.11%	0.012%
29	17.039	2366	2372	2377	rBV4	8836	16742	0.24%	0.027%
30	17.122	2382	2386	2388	rBV4	5695	7139	0.10%	0.012%
31	17.175	2392	2395	2400	rVB6	5412	7153	0.10%	0.012%
32	17.257	2402	2409	2418	rVB	2147318	3018710	43.67%	4.869%
33	17.357	2418	2426	2437	rBV	4017007	5860906	84.78%	9.453%
34	17.628	2470	2472	2476	rBV4	6663	7761	0.11%	0.013%
35	17.922	2521	2522	2527	rVB3	6823	8146	0.12%	0.013%
36	18.051	2541	2544	2548	rVB5	6435	8018	0.12%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082021\
 Data File : BN016004.D
 Acq On : 21 Aug 2021 02:20
 Operator : CG/JU
 Sample : M3448-07
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBKE6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
 Title : SVOA CALIBRATION

37	18.222	2572	2573	2580	rVB5	6909	8366	0.12%	0.013%
38	19.063	2712	2716	2719	rVB5	5595	7754	0.11%	0.013%
39	19.210	2738	2741	2748	rVV6	25873	41839	0.61%	0.067%
40	19.286	2748	2754	2760	rVV	40881	68723	0.99%	0.111%
41	19.533	2793	2796	2801	rBV2	16603	22818	0.33%	0.037%
42	19.586	2801	2805	2807	rBV4	6990	9305	0.13%	0.015%
43	19.651	2809	2816	2825	rBV	5100423	6854134	99.15%	11.055%
44	20.198	2906	2909	2910	rBV3	8872	10249	0.15%	0.017%
45	20.469	2953	2955	2957	rBV3	9476	9198	0.13%	0.015%
46	20.651	2981	2986	2996	rVV	435046	600857	8.69%	0.969%
47	21.439	3114	3120	3130	rBV	2653404	3472376	50.23%	5.601%
48	23.110	3402	3404	3416	rVB9	86930	125682	1.82%	0.203%
49	23.686	3494	3502	3509	rBV2	3296529	6913090	100.00%	11.150%
50	23.839	3520	3528	3539	rVB2	1671328	3482205	50.37%	5.616%
51	24.462	3629	3634	3641	rVB4	135250	277278	4.01%	0.447%




Sum of corrected areas: 61999872

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082021\
Data File : BN016004.D
Acq On : 21 Aug 2021 02:20
Operator : CG/JU
Sample : M3448-07
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBKE6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

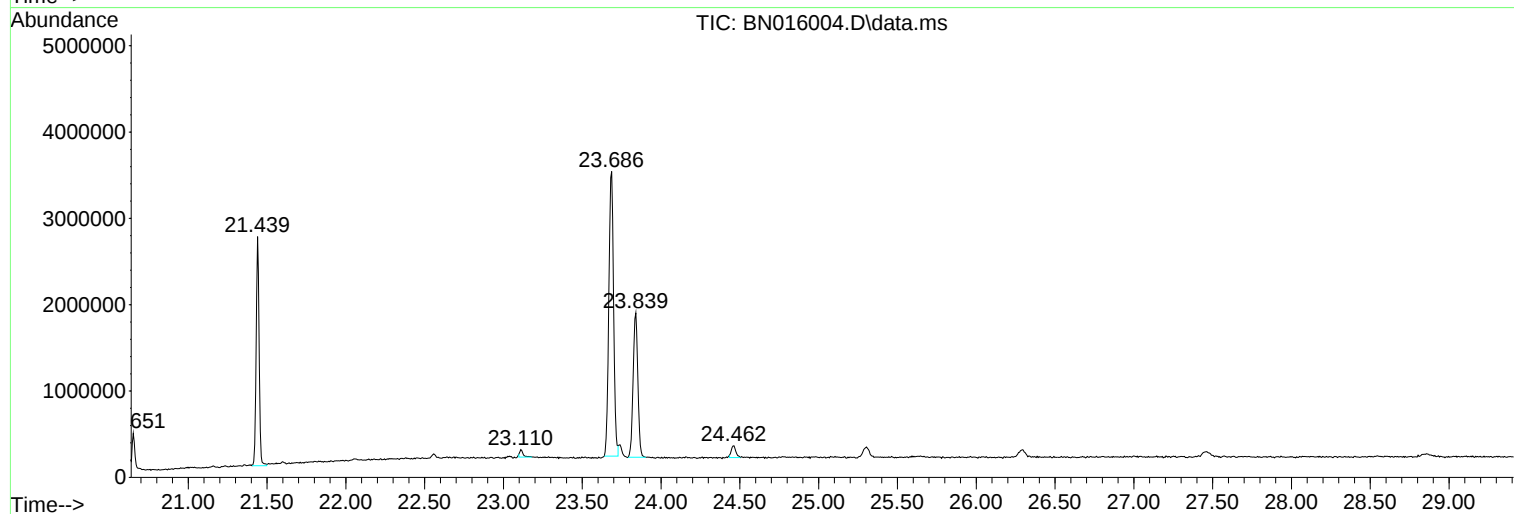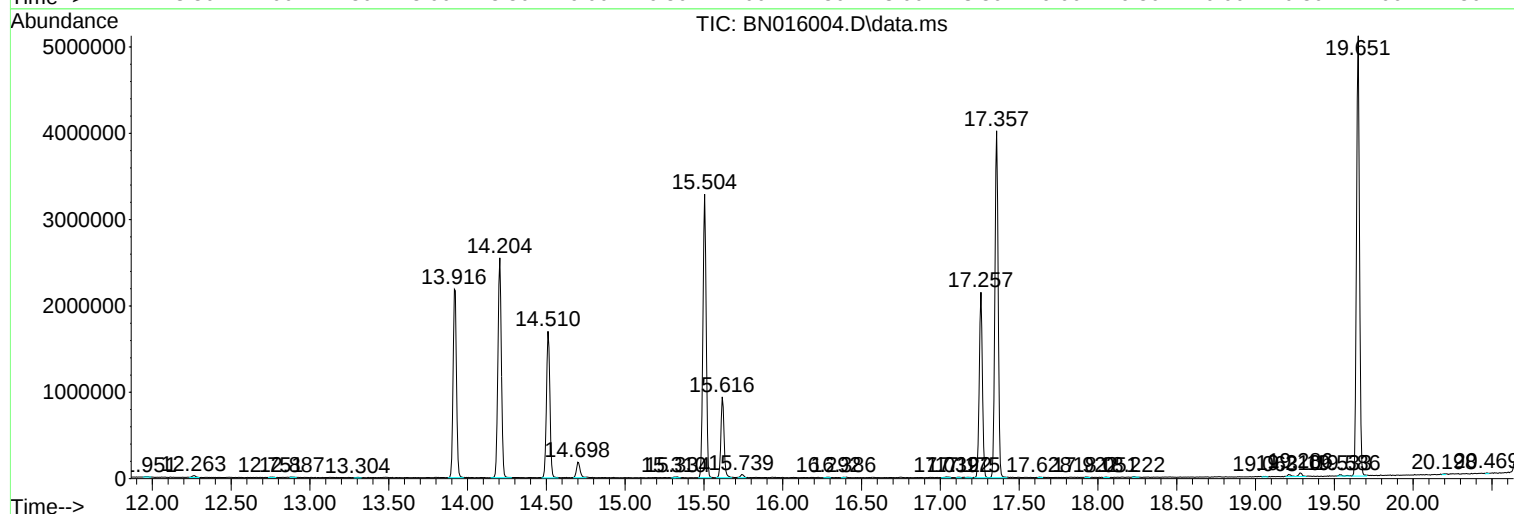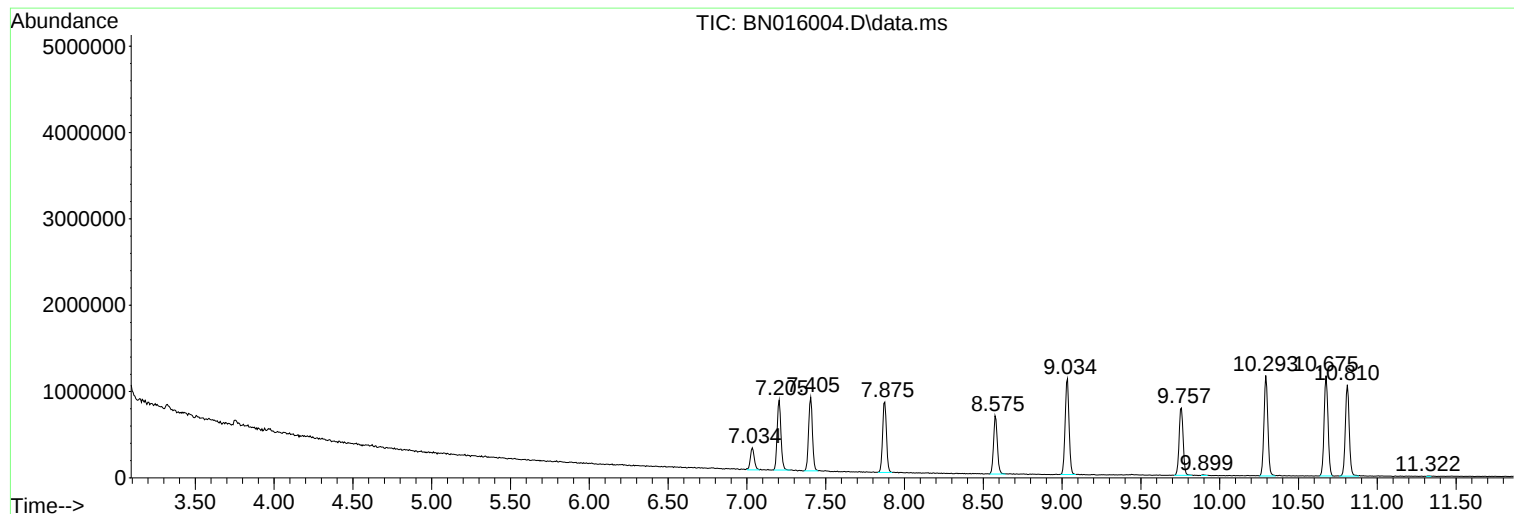

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082021\
Data File : BN016004.D
Acq On : 21 Aug 2021 02:20
Operator : CG/JU
Sample : M3448-07
Misc :
ALS Vial : 18 Sample Multiplier: 1










Instrument :
BNA_N
ClientSampleId :
DBKE6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Hexanedioic acid, bis(2-eth... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.	
20.651	3.46 ng/ul	600857	Chrysene-d12	21.439	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	Hexanedioic acid, bis(2-ethylhex...	370	C22H42O4	000103-23-1	91
2	Adipic acid, 2-ethylhexyl octyl ...	370	C22H42O4	1000324-48-6	91
3	Diisooctyl adipate	370	C22H42O4	001330-86-5	90
4	Hexanedioic acid, dioctyl ester	370	C22H42O4	000123-79-5	87
5	Hexanedioic acid, bis(2-ethylhex...	370	C22H42O4	000103-23-1	80

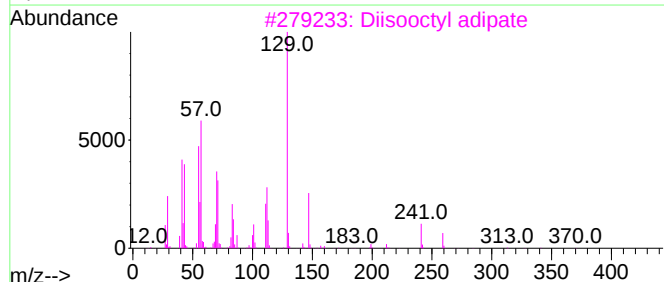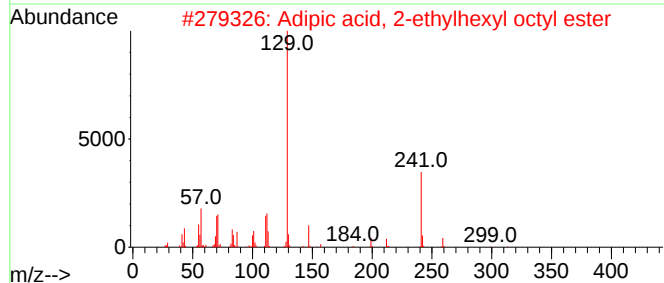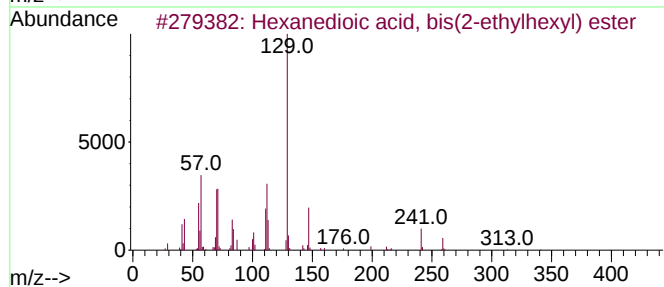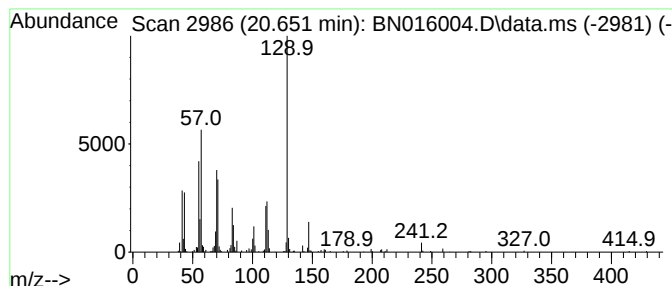

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082021\
Data File : BN016004.D
Acq On : 21 Aug 2021 02:20
Operator : CG/JU
Sample : M3448-07
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBKE6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Hexanedioic aci...	20.651	3.5	ng/u1	600857	5	21.439	3472380	20.0