

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082024\
 Data File : BN033519.D
 Acq On : 20 Aug 2024 23:06
 Operator : MA/JU
 Sample : P3666-02
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SP-201-20240816

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/21/2024
 Supervised By :mohammad ahmed 08/22/2024

Quant Time: Aug 20 23:33:24 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN081924.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 19 23:32:18 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.552	152	6956	0.400	ng	0.00
7) Naphthalene-d8	10.314	136	17989	0.400	ng	# 0.00
13) Acenaphthene-d10	14.189	164	8326	0.400	ng	0.00
19) Phenanthrene-d10	16.929	188	15938	0.400	ng	#-0.01
29) Chrysene-d12	21.139	240	10259	0.400	ng	# 0.00
35) Perylene-d12	23.312	264	10334	0.400	ng	# 0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.183	112	2300	0.104	ng	0.00
5) Phenol-d6	6.736	99	1625	0.062	ng	0.00
8) Nitrobenzene-d5	8.681	82	4846	0.325	ng	-0.01
11) 2-Methylnaphthalene-d10	11.907	152	7657	0.298	ng	0.00
14) 2,4,6-Tribromophenol	15.688	330	978	0.219	ng	0.00
15) 2-Fluorobiphenyl	12.809	172	11526	0.339	ng	0.00
27) Fluoranthene-d10	18.975	212	13818	0.361	ng	0.00
31) Terphenyl-d14	19.593	244	10940	0.469	ng	0.00
Target Compounds						Qvalue
34) Bis(2-ethylhexyl)phtha...	21.086	149	1269m	0.054	ng	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082024\
Data File : BN033519.D
Acq On : 20 Aug 2024 23:06
Operator : MA/JU
Sample : P3666-02
Misc :
ALS Vial : 14 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
SP-201-20240816

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/21/2024
Supervised By :mohammad ahmed 08/22/2024

Quant Time: Aug 20 23:33:24 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN081924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 19 23:32:18 2024
Response via : Initial Calibration

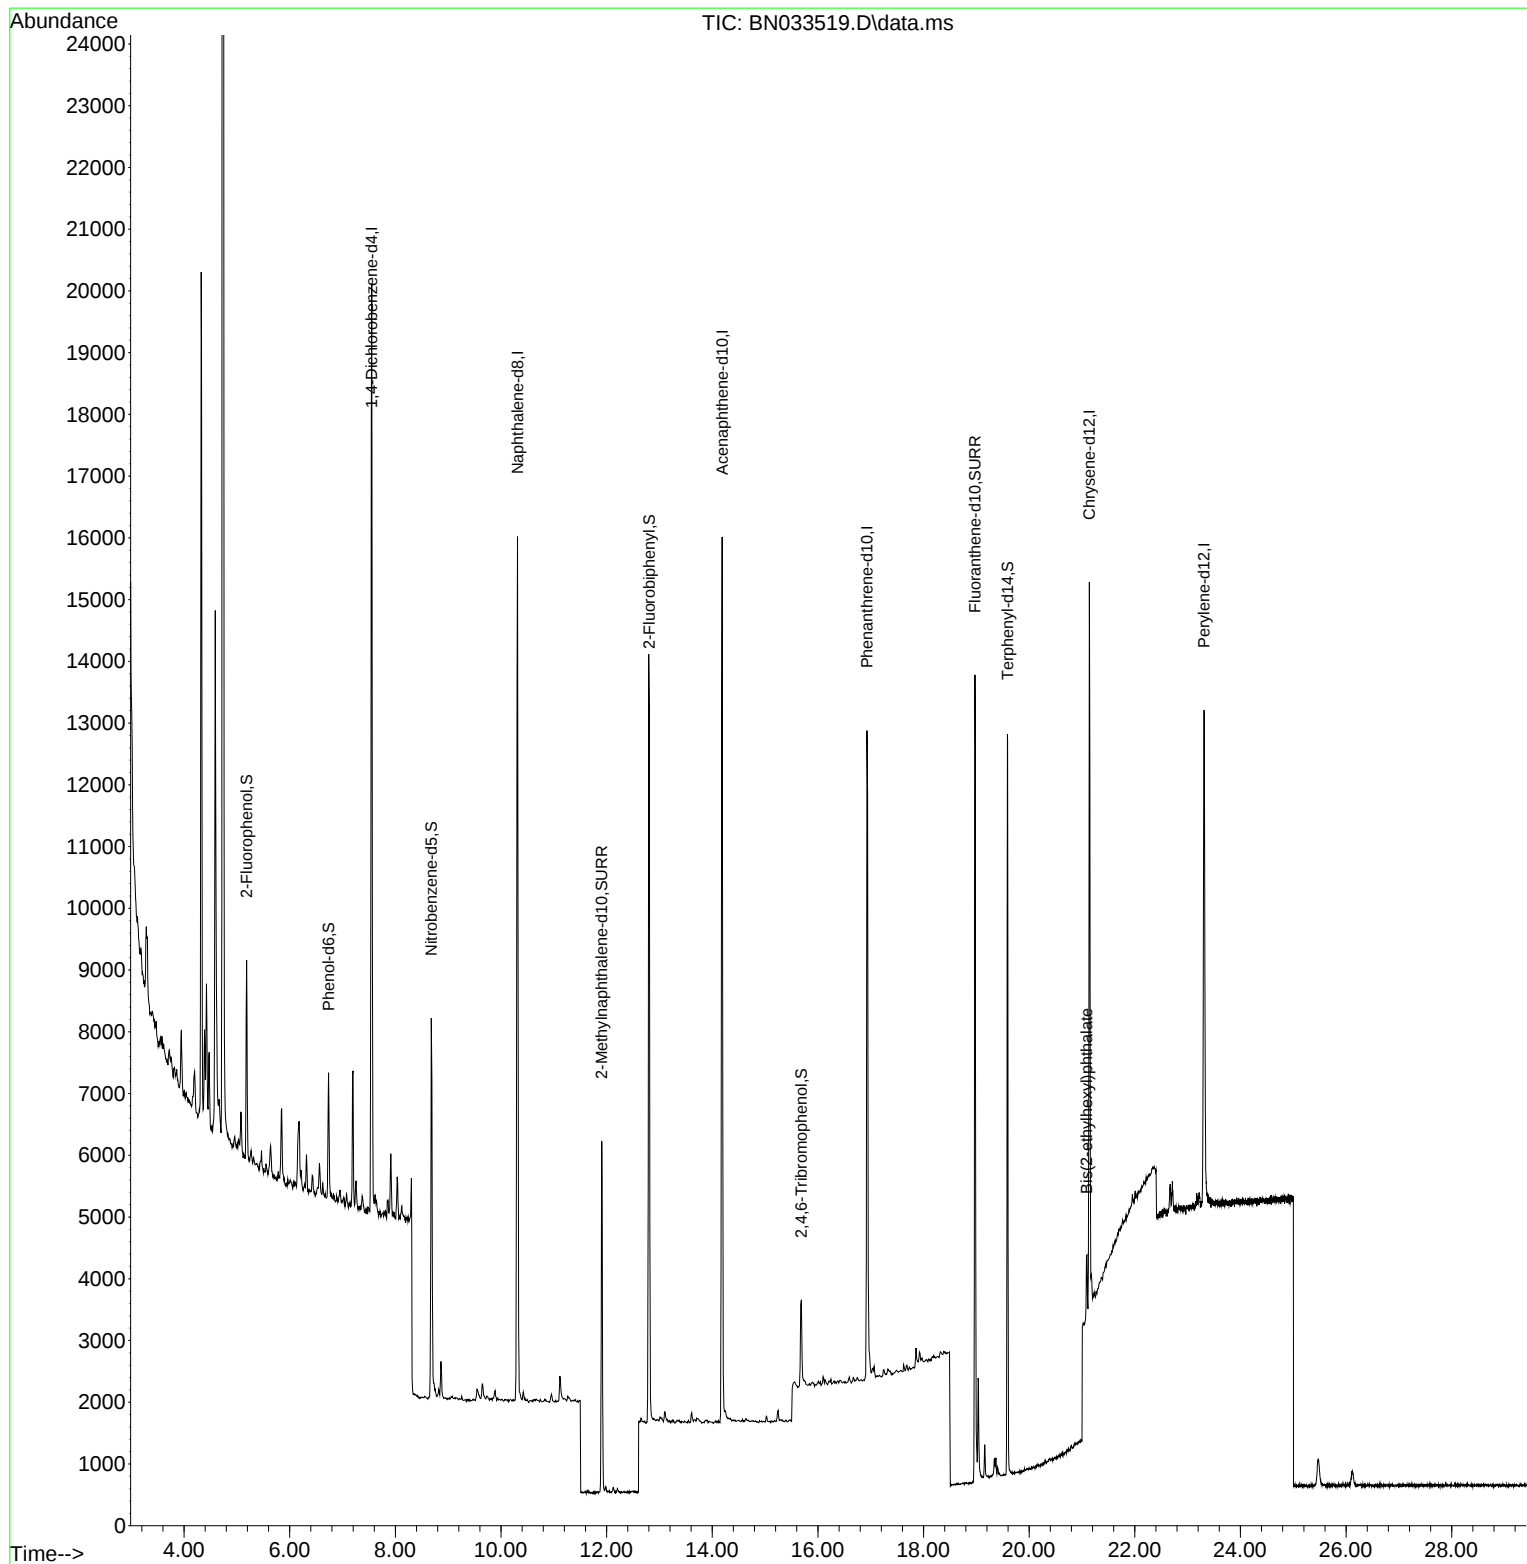




#1
1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.552 min Scan# 61
Delta R.T. -0.007 min
Lab File: BN033519.D
Acq: 20 Aug 2024 23:06

Instrument :

BNA_N

ClientSampleId :

SP-201-20240816






Tgt Ion:152 Resp: 6950
Ion Ratio Lower Upper
152 100
150 152.5 122.2 183.2
115 60.8 47.2 70.8

Manual Integrations

APPROVED




Reviewed By :Yogesh Patel 08/21/2024


Supervised By :mohammad ahmed 08/22/2024

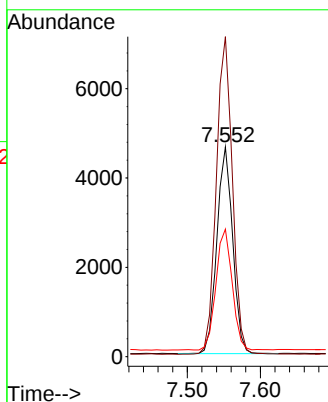

#4
2-Fluorophenol
Concen: 0.104 ng
RT: 5.183 min Scan# 305
Delta R.T. -0.007 min
Lab File: BN033519.D
Acq: 20 Aug 2024 23:06


Tgt Ion:112 Resp: 2300
Ion Ratio Lower Upper
112 100
64 59.0 47.1 70.7
63 32.7 24.9 37.3

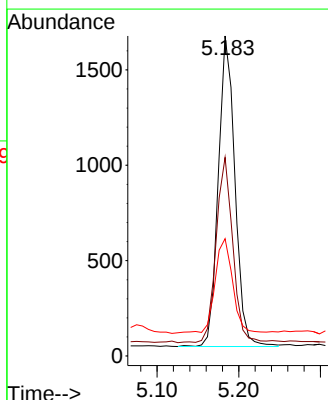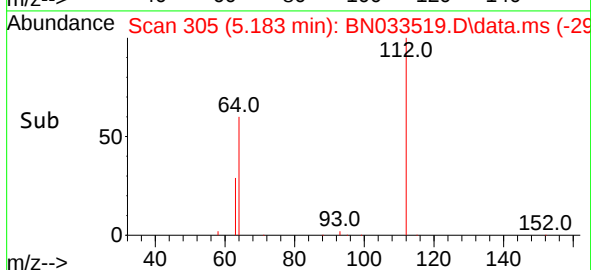



#5
Phenol-d6
Concen: 0.062 ng
RT: 6.736 min Scan# 51
Delta R.T. -0.007 min
Lab File: BN033519.D
Acq: 20 Aug 2024 23:06




Instrument :
BNA_N
ClientSampleId :
SP-201-20240816



Tgt Ion: 99 Resp: 162
Ion Ratio Lower Upper
99 100
42 23.0 16.6 24.8
71 39.2 26.2 39.4




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 08/21/2024
Supervised By :mohammad ahmed 08/22/2024

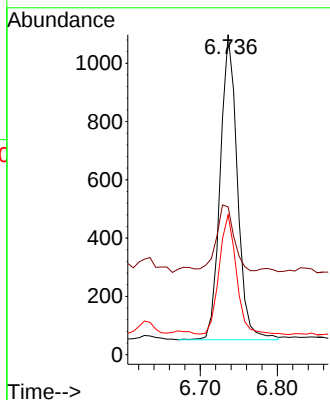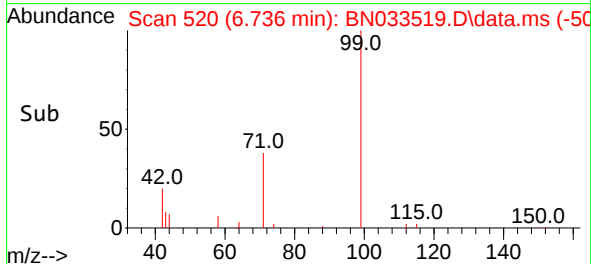

#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.314 min Scan# 926
Delta R.T. -0.000 min
Lab File: BN033519.D
Acq: 20 Aug 2024 23:06


Tgt Ion:136 Resp: 17989
Ion Ratio Lower Upper
136 100
137 11.2 9.0 13.6
54 7.3 8.3 12.5#
68 5.4 5.9 8.9#

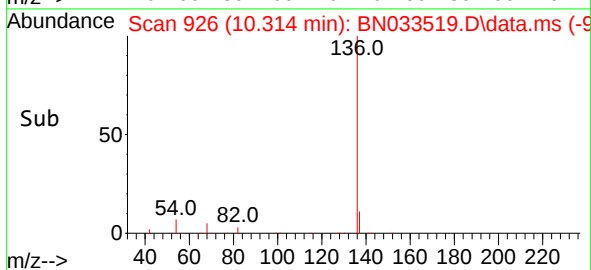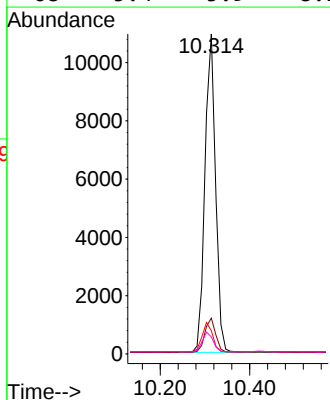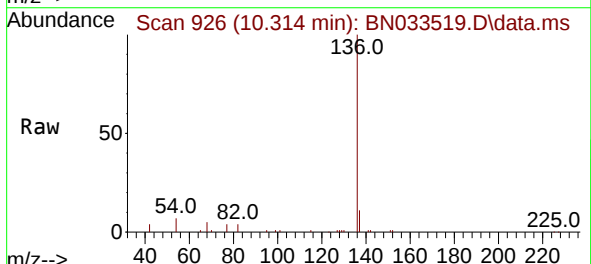



#8
Nitrobenzene-d5
Concen: 0.325 ng
RT: 8.681 min Scan# 71
Delta R.T. -0.011 min
Lab File: BN033519.D
Acq: 20 Aug 2024 23:06




Instrument :
BNA_N
ClientSampleId :
SP-201-20240816



Tgt Ion: 82 Resp: 4840
Ion Ratio Lower Upper
82 100
128 37.5 36.0 54.0
54 58.5 42.0 63.0




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 08/21/2024
Supervised By :mohammad ahmed 08/22/2024

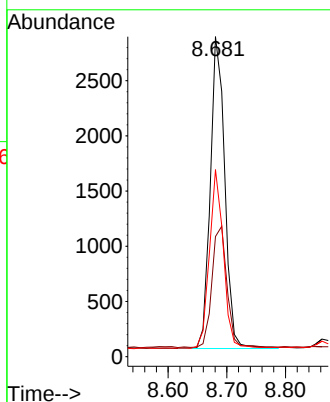

#11
2-Methylnaphthalene-d10
Concen: 0.298 ng
RT: 11.907 min Scan# 1143
Delta R.T. -0.008 min
Lab File: BN033519.D
Acq: 20 Aug 2024 23:06


Tgt Ion:152 Resp: 7657
Ion Ratio Lower Upper
152 100
151 21.1 16.6 25.0

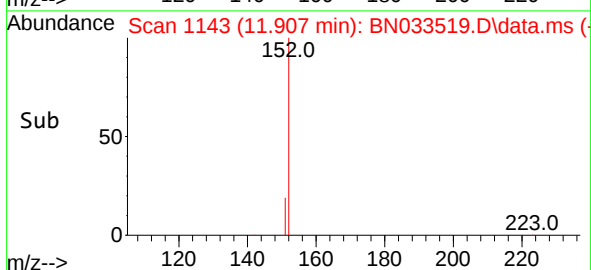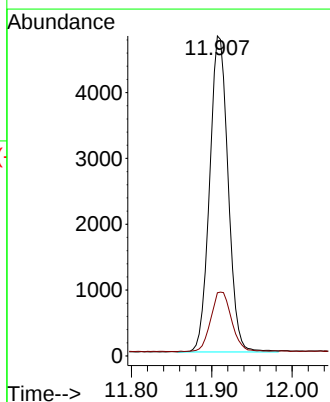



#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.189 min Scan# 1476
Delta R.T. -0.000 min
Lab File: BN033519.D
Acq: 20 Aug 2024 23:06




Instrument :
BNA_N
ClientSampleId :
SP-201-20240816




Tgt Ion:164 Resp: 8320
Ion Ratio Lower Upper
164 100
162 104.1 83.5 125.3
160 50.2 40.2 60.4

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 08/21/2024
Supervised By :mohammad ahmed 08/22/2024

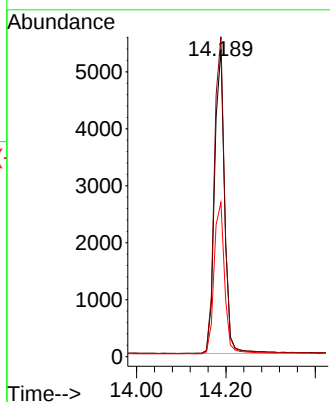


#14
2,4,6-Tribromophenol
Concen: 0.219 ng
RT: 15.688 min Scan# 1614
Delta R.T. -0.000 min
Lab File: BN033519.D
Acq: 20 Aug 2024 23:06




Tgt Ion:330 Resp: 978
Ion Ratio Lower Upper
330 100
332 96.1 77.5 116.3
141 41.1 33.9 50.9

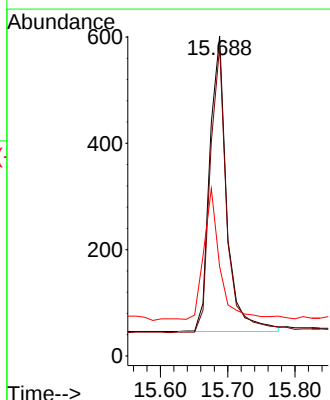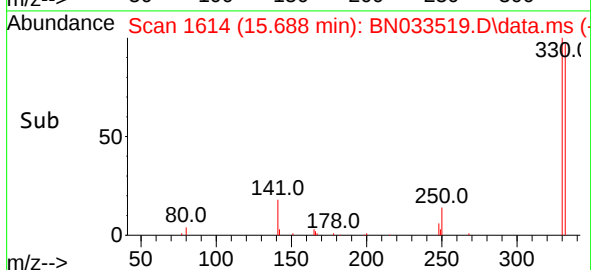

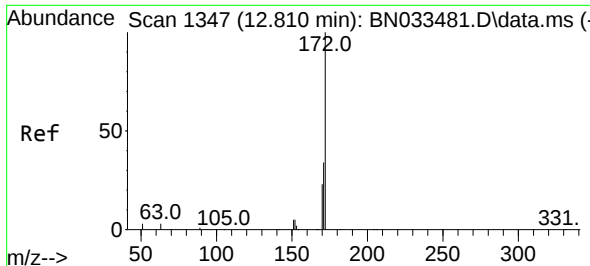

#15
2-Fluorobiphenyl
Concen: 0.339 ng
RT: 12.809 min Scan# 11520
Delta R.T. -0.000 min
Lab File: BN033519.D
Acq: 20 Aug 2024 23:06




Instrument :
BNA_N
ClientSampleId :
SP-201-20240816

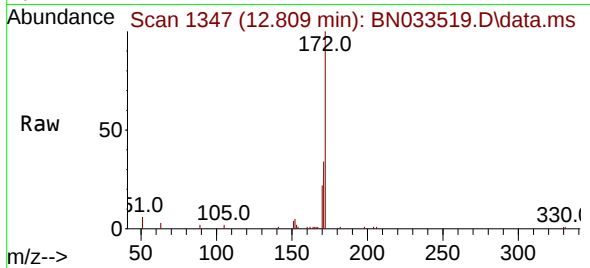

Tgt Ion:172 Resp: 11520
Ion Ratio Lower Upper
172 100
171 34.2 27.7 41.5
170 22.5 18.3 27.5




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 08/21/2024
Supervised By :mohammad ahmed 08/22/2024

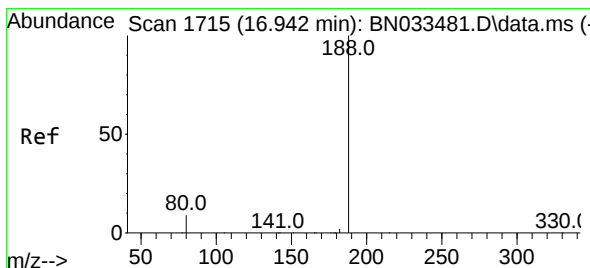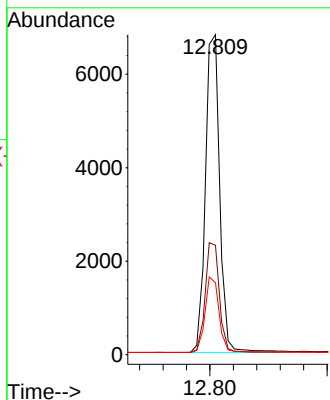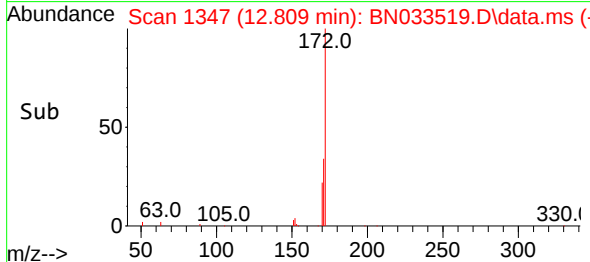

#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 16.929 min Scan# 1714
Delta R.T. -0.012 min
Lab File: BN033519.D
Acq: 20 Aug 2024 23:06

Tgt Ion:188 Resp: 15938
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 15.7 7.8 11.8

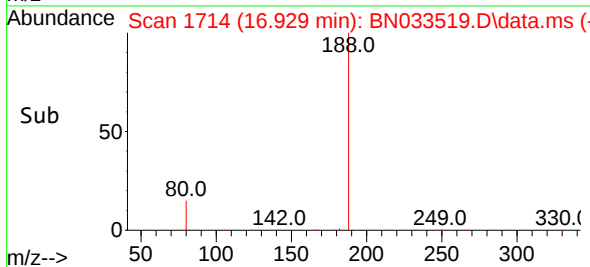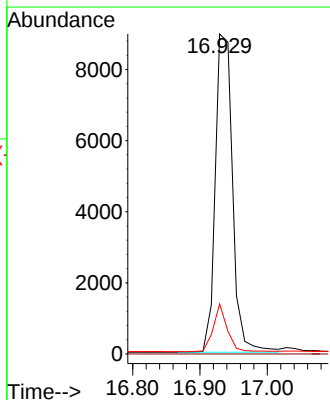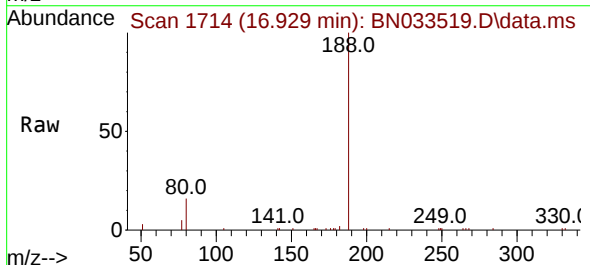

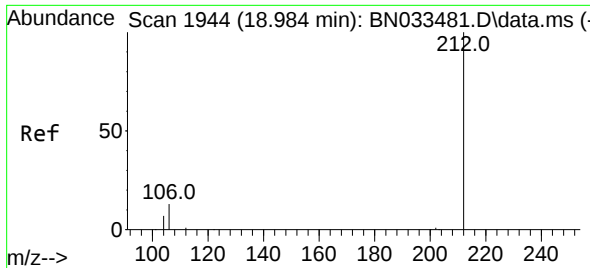


#27
Fluoranthene-d10
Concen: 0.361 ng
RT: 18.975 min Scan# 1942
Delta R.T. -0.009 min
Lab File: BN033519.D
Acq: 20 Aug 2024 23:06

Instrument :

BNA_N

ClientSampleId :




SP-201-20240816

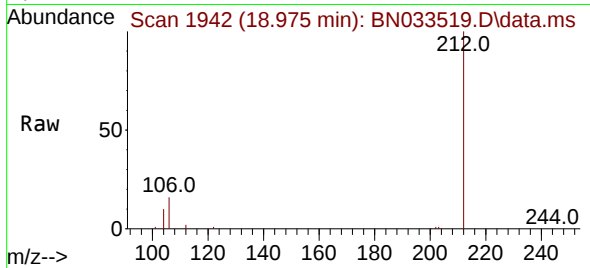

Tgt Ion:212 Resp: 13818
Ion Ratio Lower Upper
212 100
106 15.3 12.3 18.5
104 8.8 7.0 10.4




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 08/21/2024
Supervised By :mohammad ahmed 08/22/2024

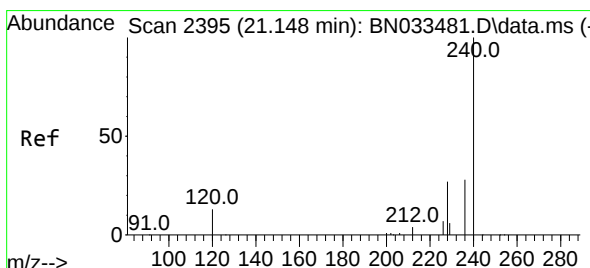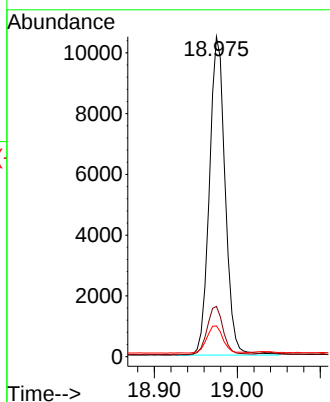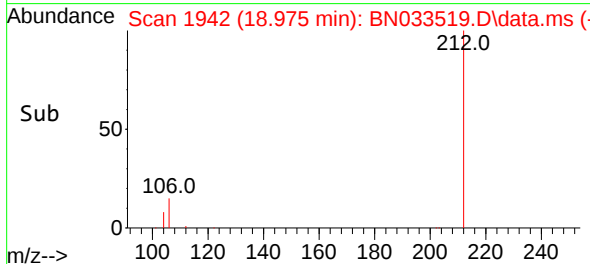

#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.139 min Scan# 2394
Delta R.T. -0.009 min
Lab File: BN033519.D
Acq: 20 Aug 2024 23:06

Tgt Ion:240 Resp: 10259
Ion Ratio Lower Upper
240 100
120 19.9 12.4 18.6#
236 30.0 23.0 34.6

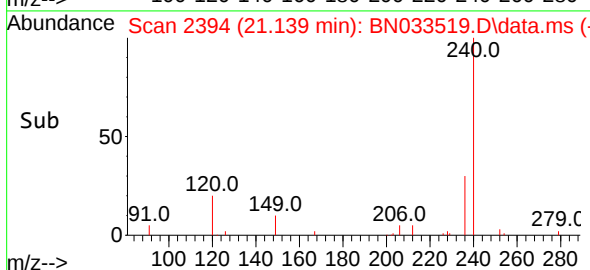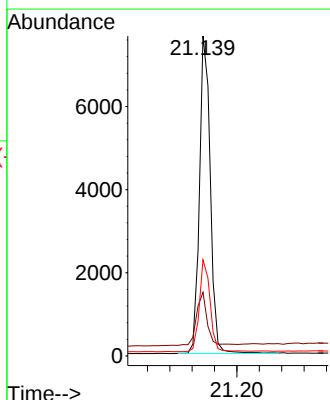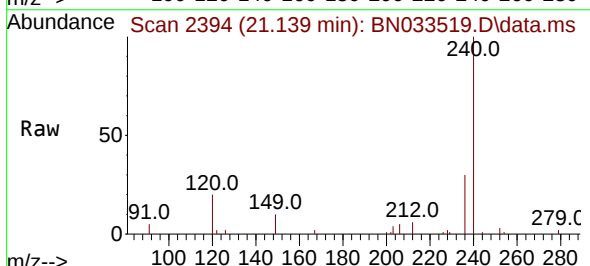




#31
 Terphenyl-d14
 Concen: 0.469 ng
 RT: 19.593 min Scan# 2075
 Delta R.T. -0.005 min
 Lab File: BN033519.D
 Acq: 20 Aug 2024 23:06

Instrument :

BNA_N

ClientSampleId :

SP-201-20240816






Tgt Ion:244 Resp: 10940
 Ion Ratio Lower Upper
 244 100
 212 9.8 7.8 11.6
 122 16.3 13.3 19.9

Manual Integrations

APPROVED




Reviewed By :Yogesh Patel 08/21/2024


Supervised By :mohammad ahmed 08/22/2024

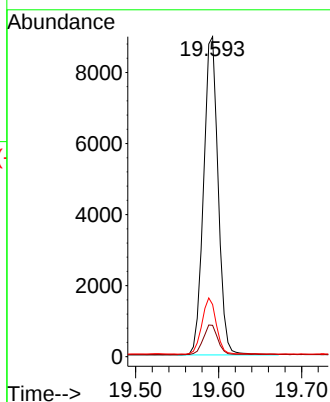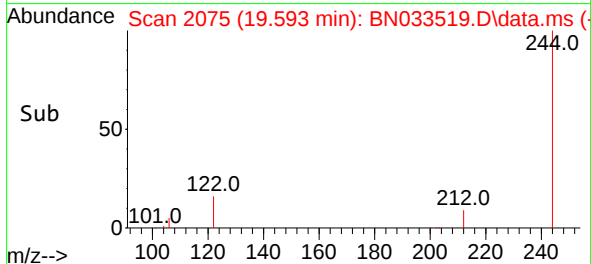

#34
 Bis(2-ethylhexyl)phthalate
 Concen: 0.054 ng m
 RT: 21.086 min Scan# 2388
 Delta R.T. -0.009 min
 Lab File: BN033519.D
 Acq: 20 Aug 2024 23:06


Tgt Ion:149 Resp: 1269
 Ion Ratio Lower Upper
 149 100
 167 31.8 21.5 32.3
 279 0.0 2.2 3.2#

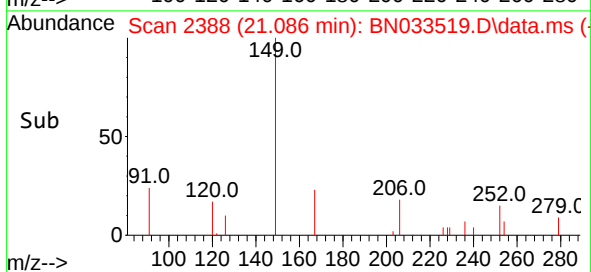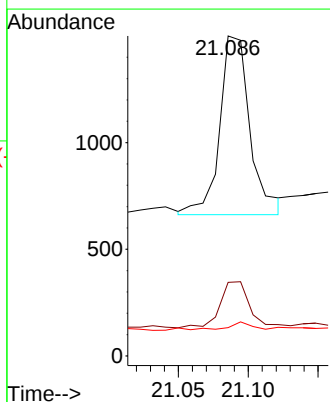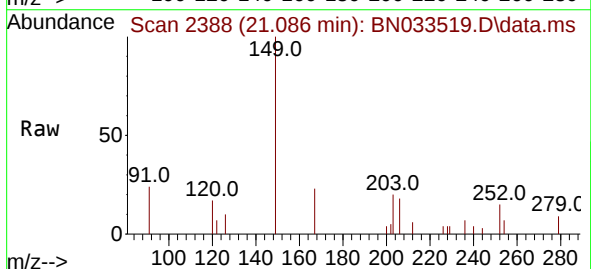

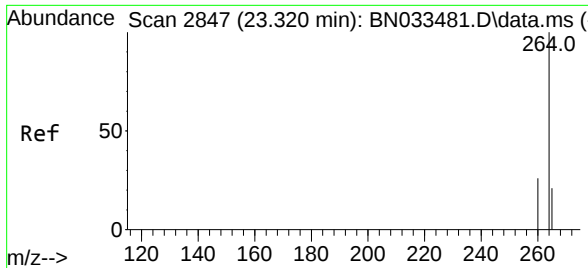

#35
 Perylene-d12
 Concen: 0.400 ng
 RT: 23.312 min Scan# 21
 Delta R.T. -0.009 min
 Lab File: BN033519.D
 Acq: 20 Aug 2024 23:06

Instrument :
 BNA_N
 ClientSampleId :
 SP-201-20240816

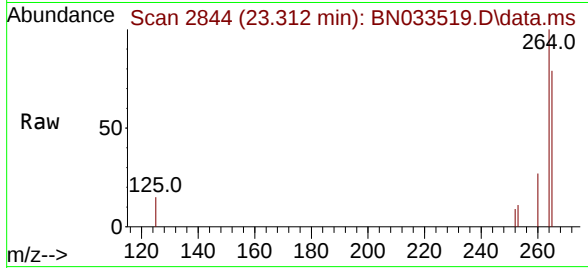

Tgt Ion:264 Resp: 10334
 Ion Ratio Lower Upper
 264 100
 260 27.0 20.8 31.2
 265 79.1 52.2 78.2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/21/2024
 Supervised By :mohammad ahmed 08/22/2024

