

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082024\
 Data File : BN033520.D
 Acq On : 20 Aug 2024 23:42
 Operator : MA/JU
 Sample : P3666-03
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SP-303-20240816

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 08/21/2024
 Supervised By :mohammad ahmed 08/22/2024

Quant Time: Aug 21 00:11:47 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN081924.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 19 23:32:18 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.552	152	7349	0.400	ng	0.00
7) Naphthalene-d8	10.314	136	18908	0.400	ng	# 0.00
13) Acenaphthene-d10	14.189	164	8775	0.400	ng	0.00
19) Phenanthrene-d10	16.929	188	16959	0.400	ng	#-0.01
29) Chrysene-d12	21.139	240	11478	0.400	ng	0.00
35) Perylene-d12	23.311	264	11439	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.183	112	2245	0.096	ng	0.00
5) Phenol-d6	6.736	99	1614	0.058	ng	0.00
8) Nitrobenzene-d5	8.681	82	4491	0.286	ng	-0.01
11) 2-Methylnaphthalene-d10	11.911	152	7257	0.268	ng	0.00
14) 2,4,6-Tribromophenol	15.688	330	985	0.209	ng	0.00
15) 2-Fluorobiphenyl	12.799	172	10843	0.303	ng	-0.01
27) Fluoranthene-d10	18.975	212	14174	0.348	ng	0.00
31) Terphenyl-d14	19.588	244	12292	0.471	ng	0.00
Target Compounds						Qvalue
34) Bis(2-ethylhexyl)phtha...	21.085	149	1217m	0.046	ng	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082024\
Data File : BN033520.D
Acq On : 20 Aug 2024 23:42
Operator : MA/JU
Sample : P3666-03
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SP-303-20240816

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 08/21/2024
Supervised By :mohammad ahmed 08/22/2024


Quant Time: Aug 21 00:11:47 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN081924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 19 23:32:18 2024
Response via : Initial Calibration

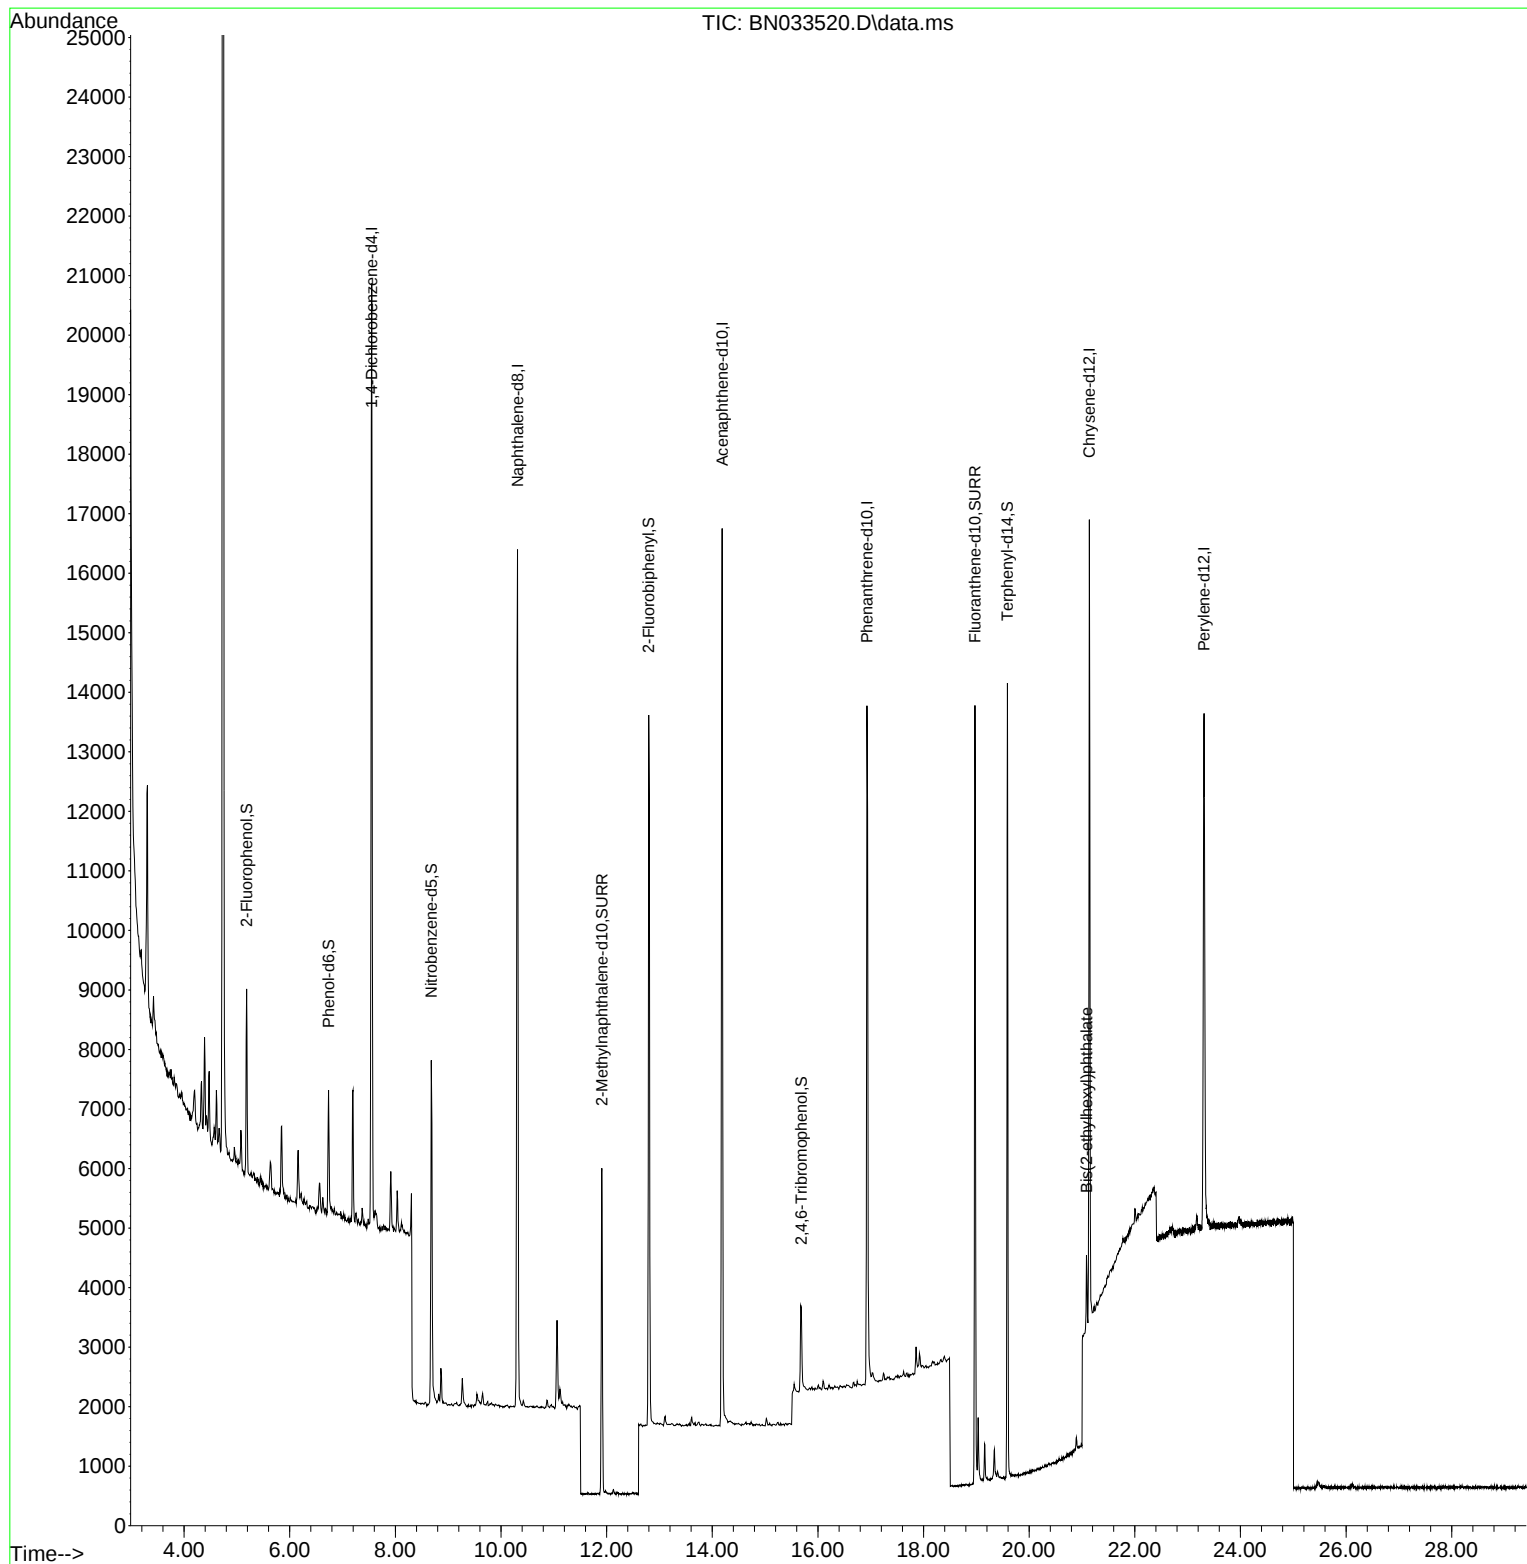



#1
1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.552 min Scan# 61
Delta R.T. -0.007 min
Lab File: BN033520.D
Acq: 20 Aug 2024 23:42




Instrument :
BNA_N
ClientSampleId :
SP-303-20240816

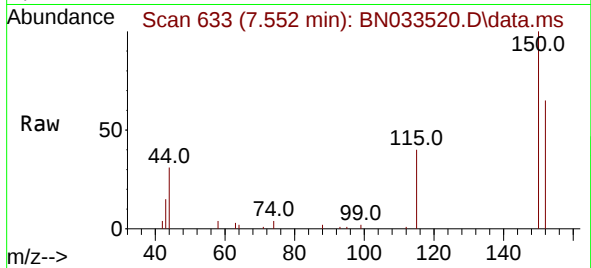

Tgt Ion:152 Resp: 7349
Ion Ratio Lower Upper
152 100
150 154.2 122.2 183.2
115 61.5 47.2 70.8




Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 08/21/2024
Supervised By :mohammad ahmed 08/22/2024

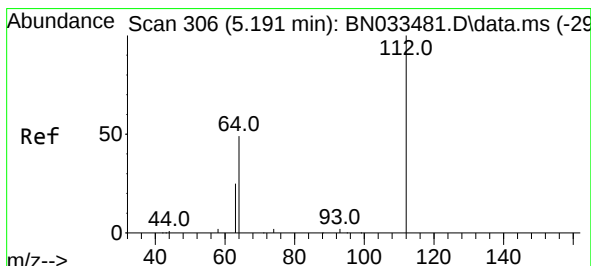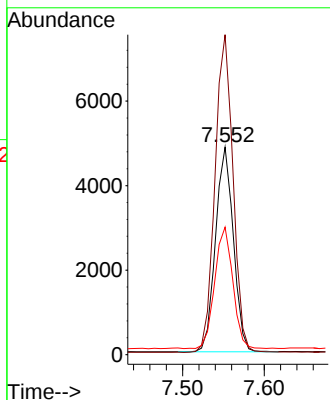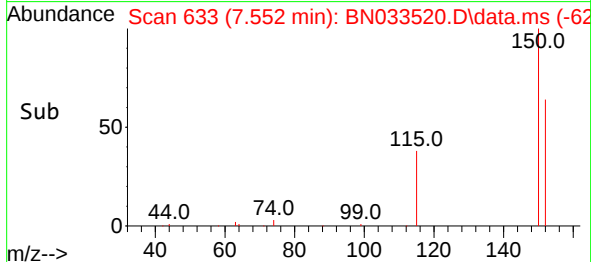

#4
2-Fluorophenol
Concen: 0.096 ng
RT: 5.183 min Scan# 305
Delta R.T. -0.007 min
Lab File: BN033520.D
Acq: 20 Aug 2024 23:42


Tgt Ion:112 Resp: 2245
Ion Ratio Lower Upper
112 100
64 60.4 47.1 70.7
63 33.2 24.9 37.3

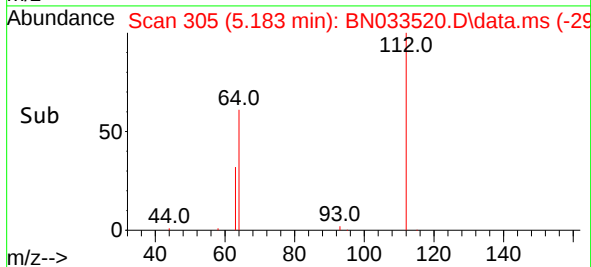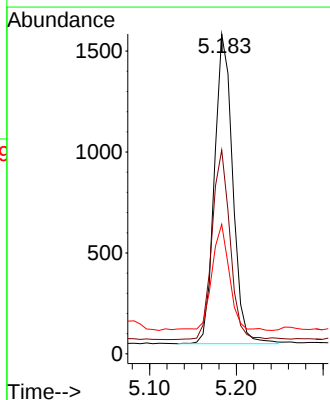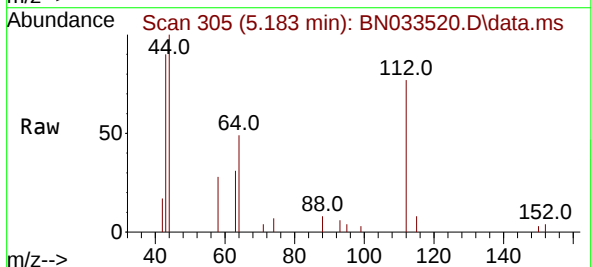



#5
Phenol-d6
Concen: 0.058 ng
RT: 6.736 min Scan# 51
Delta R.T. -0.007 min
Lab File: BN033520.D
Acq: 20 Aug 2024 23:42




Instrument :
BNA_N
ClientSampleId :
SP-303-20240816

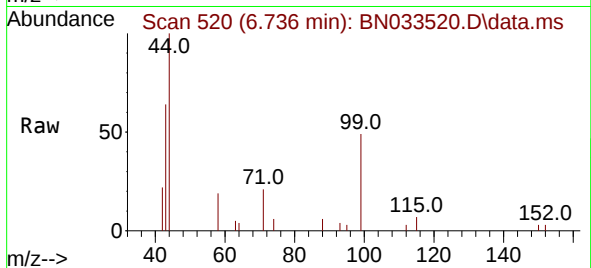

Tgt Ion: 99 Resp: 1614
Ion Ratio Lower Upper
99 100
42 23.6 16.6 24.8
71 39.8 26.2 39.4




Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 08/21/2024
Supervised By :mohammad ahmed 08/22/2024

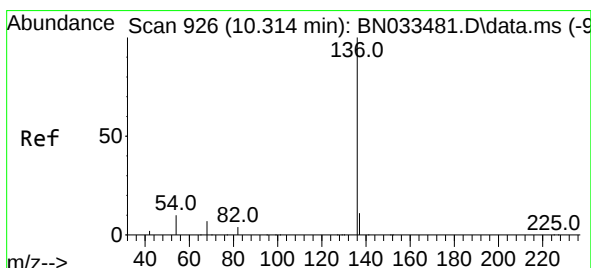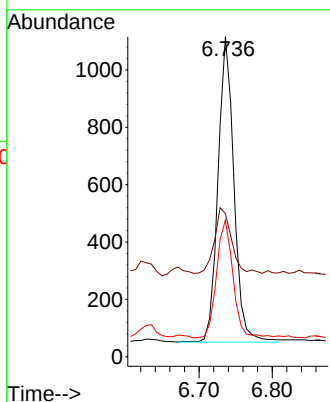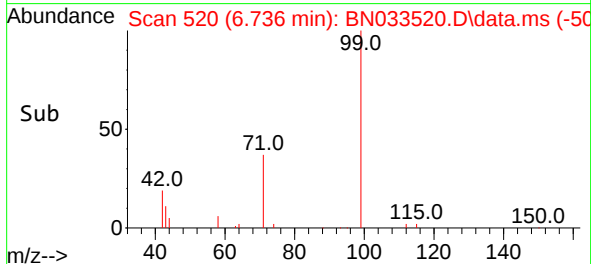

#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.314 min Scan# 926
Delta R.T. -0.000 min
Lab File: BN033520.D
Acq: 20 Aug 2024 23:42


Tgt Ion:136 Resp: 18908
Ion Ratio Lower Upper
136 100
137 11.4 9.0 13.6
54 7.7 8.3 12.5#
68 5.4 5.9 8.9#

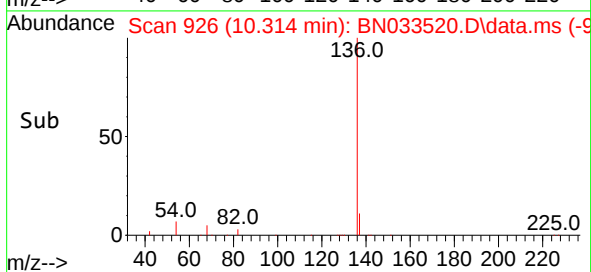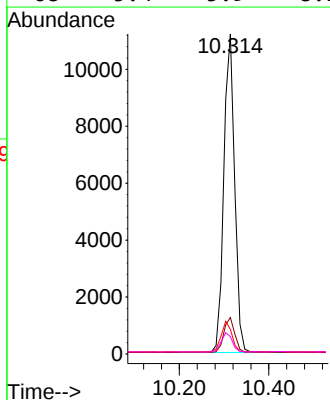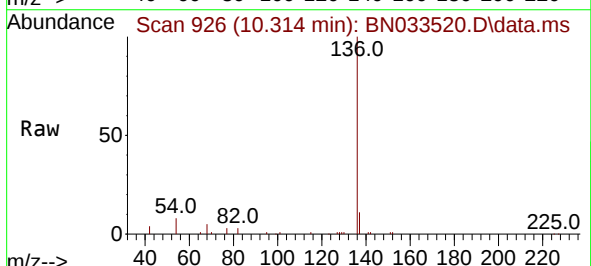



#8
Nitrobenzene-d5
Concen: 0.286 ng
RT: 8.681 min Scan# 71
Delta R.T. -0.011 min
Lab File: BN033520.D
Acq: 20 Aug 2024 23:42




Instrument :
BNA_N
ClientSampleId :
SP-303-20240816

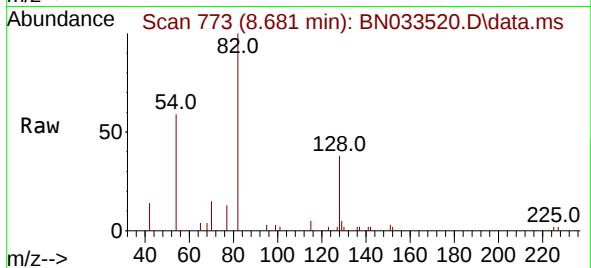

Tgt Ion: 82 Resp: 449
Ion Ratio Lower Upper
82 100
128 38.1 36.0 54.0
54 59.4 42.0 63.0




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 08/21/2024
Supervised By :mohammad ahmed 08/22/2024

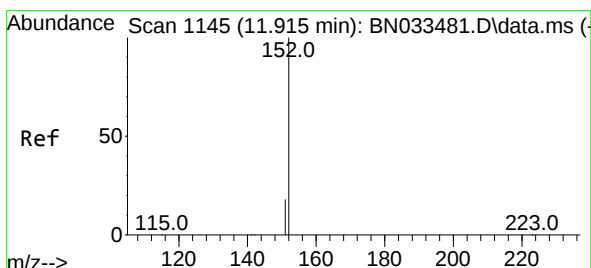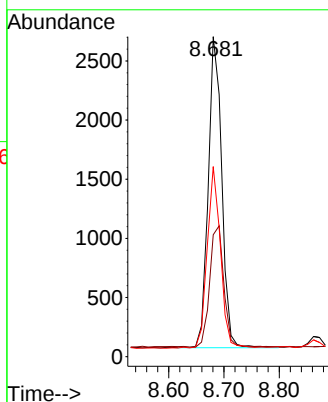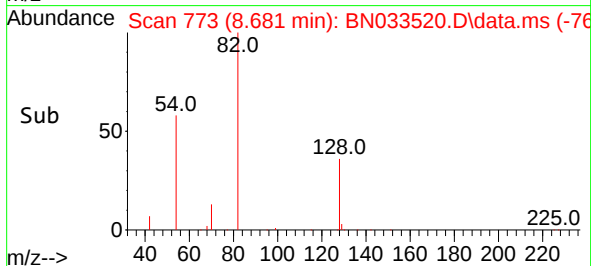

#11
2-Methylnaphthalene-d10
Concen: 0.268 ng
RT: 11.911 min Scan# 1144
Delta R.T. -0.004 min
Lab File: BN033520.D
Acq: 20 Aug 2024 23:42


Tgt Ion:152 Resp: 7257
Ion Ratio Lower Upper
152 100
151 20.8 16.6 25.0

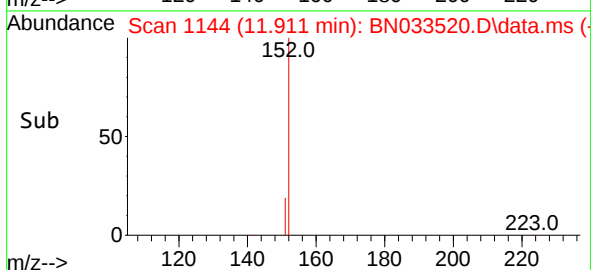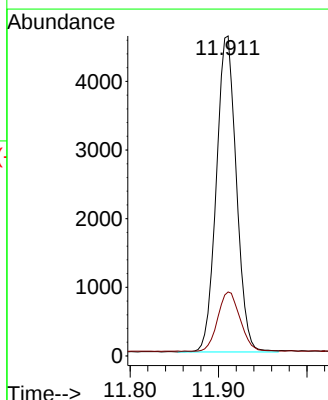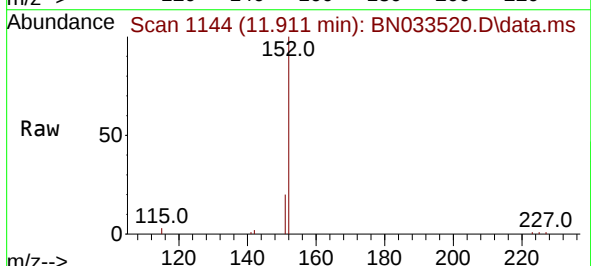

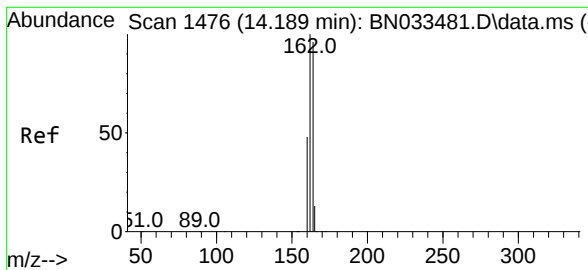

#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.189 min Scan# 1476
Delta R.T. -0.000 min
Lab File: BN033520.D
Acq: 20 Aug 2024 23:42




Instrument :
BNA_N
ClientSampleId :
SP-303-20240816

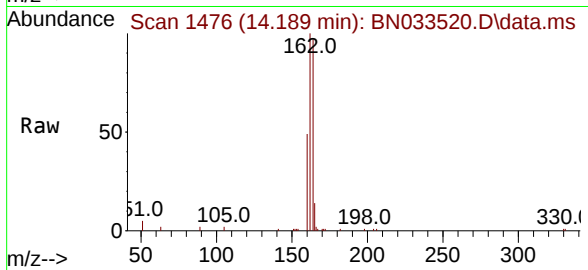


Tgt Ion:164 Resp: 8775
Ion Ratio Lower Upper
164 100
162 102.7 83.5 125.3
160 50.1 40.2 60.4

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 08/21/2024
Supervised By :mohammad ahmed 08/22/2024

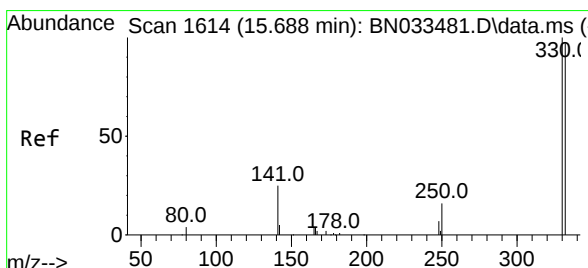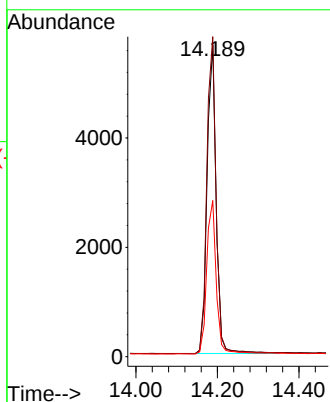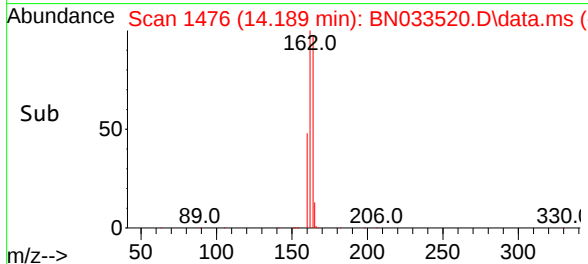


#14
2,4,6-Tribromophenol
Concen: 0.209 ng
RT: 15.688 min Scan# 1614
Delta R.T. -0.000 min
Lab File: BN033520.D
Acq: 20 Aug 2024 23:42

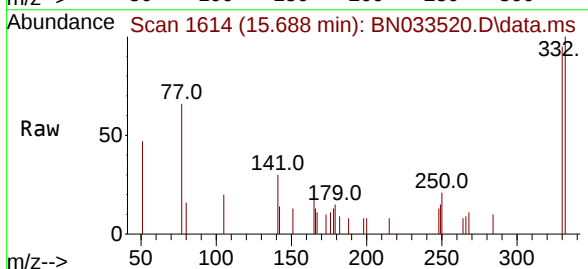

Tgt Ion:330 Resp: 985
Ion Ratio Lower Upper
330 100
332 100.6 77.5 116.3
141 41.6 33.9 50.9

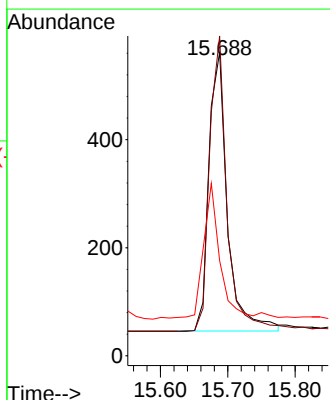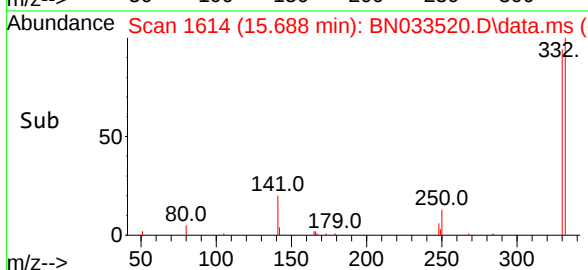

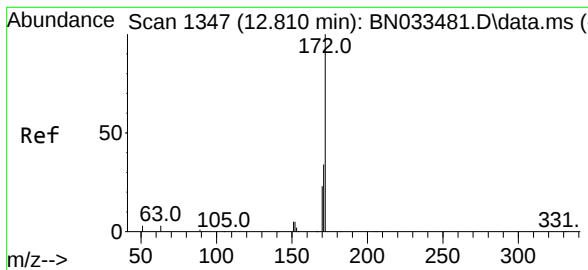


#15
2-Fluorobiphenyl
Concen: 0.303 ng
RT: 12.799 min Scan# 11
Delta R.T. -0.011 min
Lab File: BN033520.D
Acq: 20 Aug 2024 23:42

Instrument :

BNA_N

ClientSampleId :

SP-303-20240816



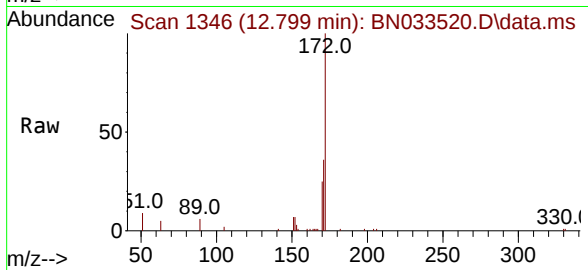


Tgt Ion:172 Resp: 1084
Ion Ratio Lower Upper
172 100
171 35.7 27.7 41.5
170 24.6 18.3 27.5

Manual Integrations




APPROVED


Reviewed By :Jagrut Upadhyay 08/21/2024
Supervised By :mohammad ahmed 08/22/2024

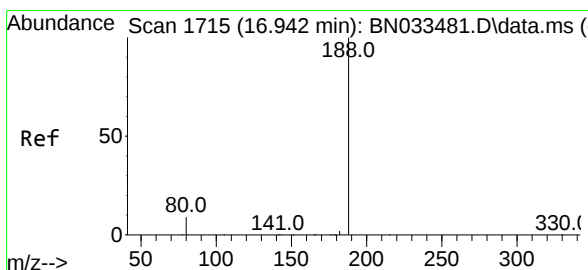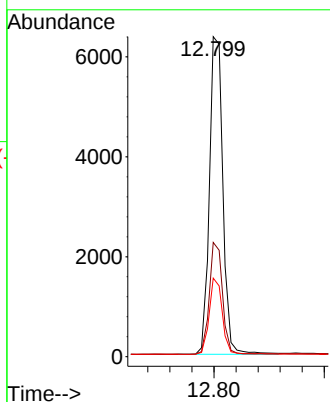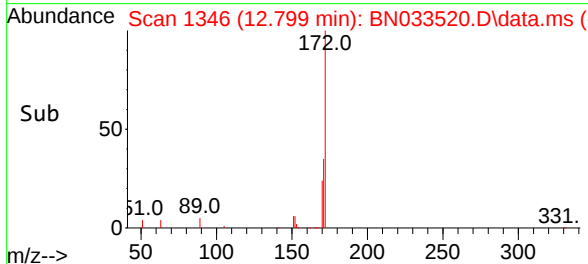

#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 16.929 min Scan# 1714
Delta R.T. -0.013 min
Lab File: BN033520.D
Acq: 20 Aug 2024 23:42

Tgt Ion:188 Resp: 16959
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 15.1 7.8 11.8

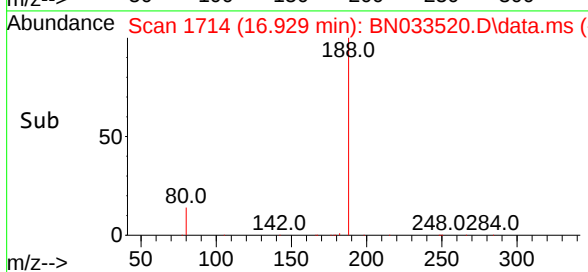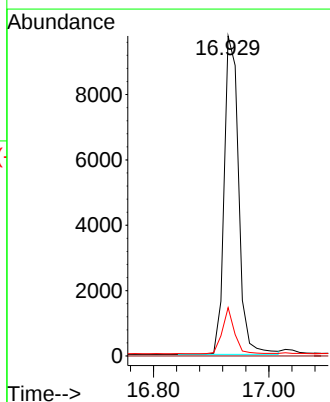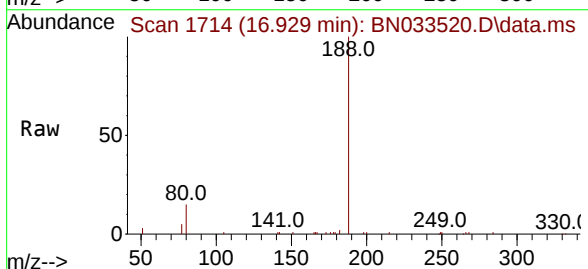

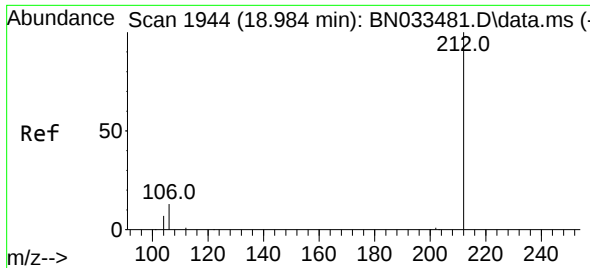


#27
Fluoranthene-d10
Concen: 0.348 ng
RT: 18.975 min Scan# 1942
Delta R.T. -0.009 min
Lab File: BN033520.D
Acq: 20 Aug 2024 23:42

Instrument :

BNA_N

ClientSampleId :

SP-303-20240816



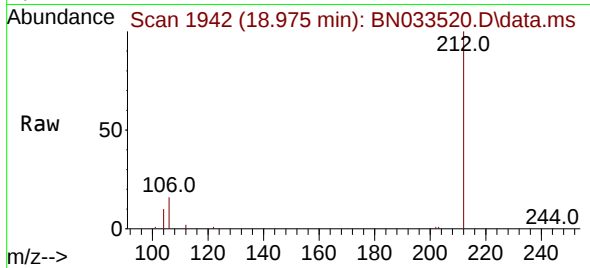


Tgt Ion:212 Resp: 14174
Ion Ratio Lower Upper
212 100
106 15.5 12.3 18.5
104 8.8 7.0 10.4

Manual Integrations




APPROVED


Reviewed By :Jagrut Upadhyay 08/21/2024
Supervised By :mohammad ahmed 08/22/2024

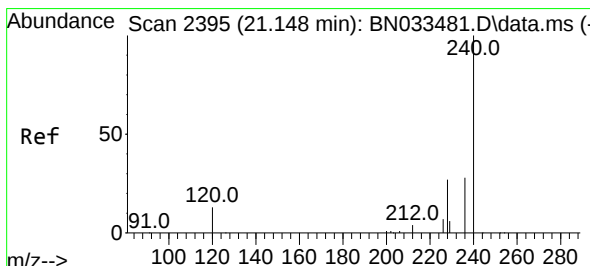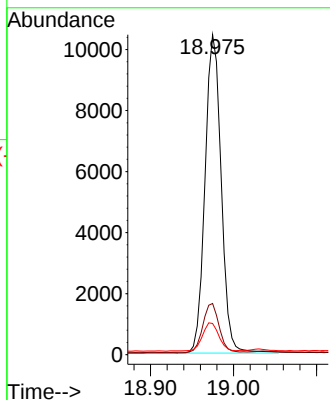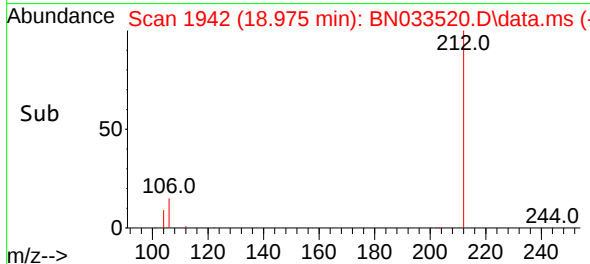

#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.139 min Scan# 2394
Delta R.T. -0.009 min
Lab File: BN033520.D
Acq: 20 Aug 2024 23:42

Tgt Ion:240 Resp: 11478
Ion Ratio Lower Upper
240 100
120 17.2 12.4 18.6
236 29.2 23.0 34.6

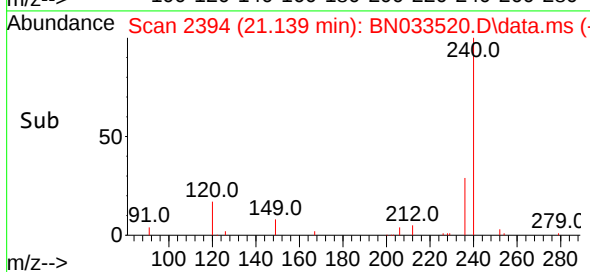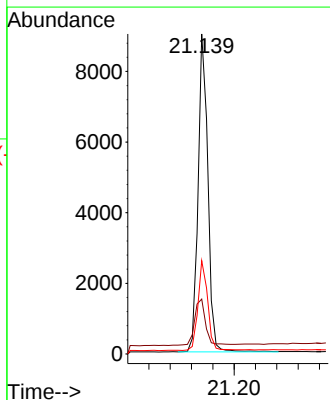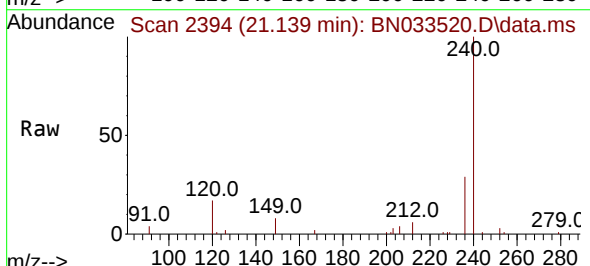

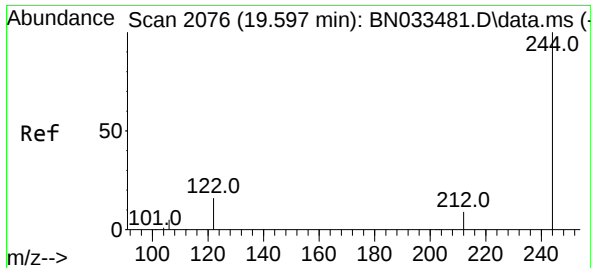

#31
 Terphenyl-d14
 Concen: 0.471 ng
 RT: 19.588 min Scan# 2074
 Delta R.T. -0.009 min
 Lab File: BN033520.D
 Acq: 20 Aug 2024 23:42

Instrument :

BNA_N

ClientSampleId :





SP-303-20240816

Tgt Ion:244 Resp: 12292
 Ion Ratio Lower Upper
 244 100
 212 9.9 7.8 11.6
 122 18.0 13.3 19.9

Manual Integrations




APPROVED


Reviewed By :Jagrut Upadhyay 08/21/2024
 Supervised By :mohammad ahmed 08/22/2024

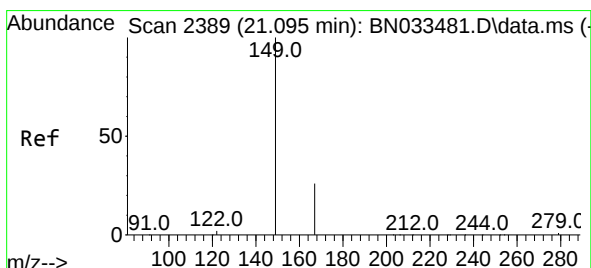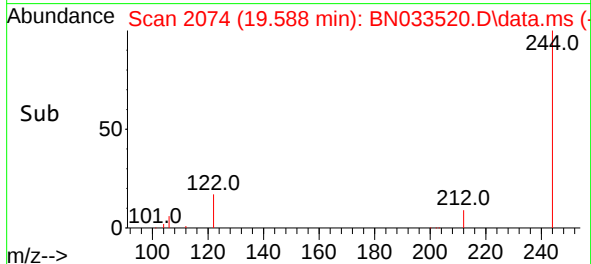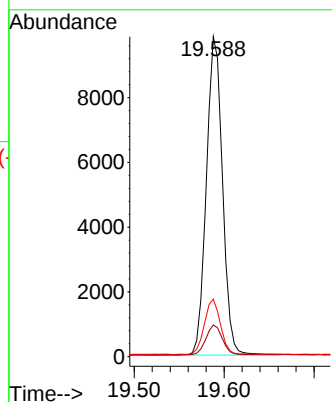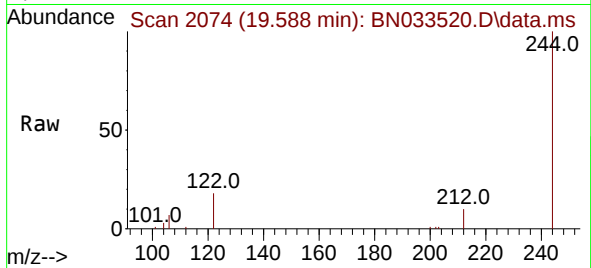

#34
 Bis(2-ethylhexyl)phthalate
 Concen: 0.046 ng m
 RT: 21.085 min Scan# 2388
 Delta R.T. -0.009 min
 Lab File: BN033520.D
 Acq: 20 Aug 2024 23:42


Tgt Ion:149 Resp: 1217
 Ion Ratio Lower Upper
 149 100
 167 36.9 21.5 32.3#
 279 0.0 2.2 3.2#

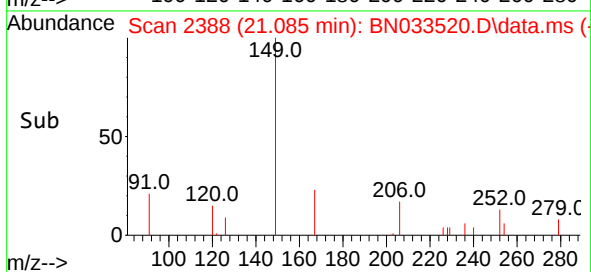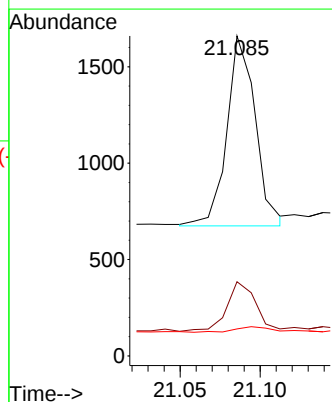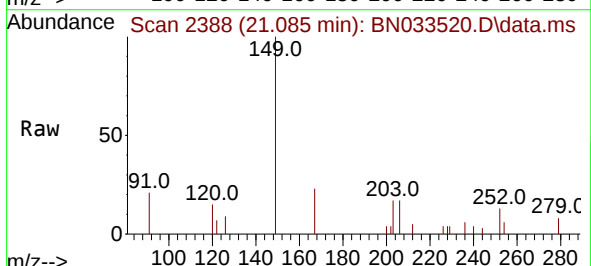

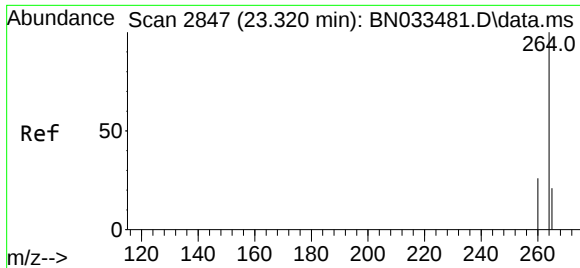

#35
 Perylene-d12
 Concen: 0.400 ng
 RT: 23.311 min Scan# 21
 Delta R.T. -0.009 min
 Lab File: BN033520.D
 Acq: 20 Aug 2024 23:42

Instrument :
 BNA_N
 ClientSampleId :
 SP-303-20240816

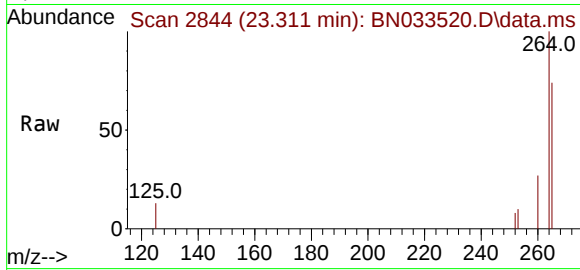

Tgt Ion:264 Resp: 11439

Ion	Ratio	Lower	Upper
264	100		
260	26.6	20.8	31.2
265	73.9	52.2	78.2

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 08/21/2024
 Supervised By :mohammad ahmed 08/22/2024

