


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082024\
Data File : BN033525.D
Acq On : 21 Aug 2024 03:22
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN081924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Aug 19 23:32:18 2024

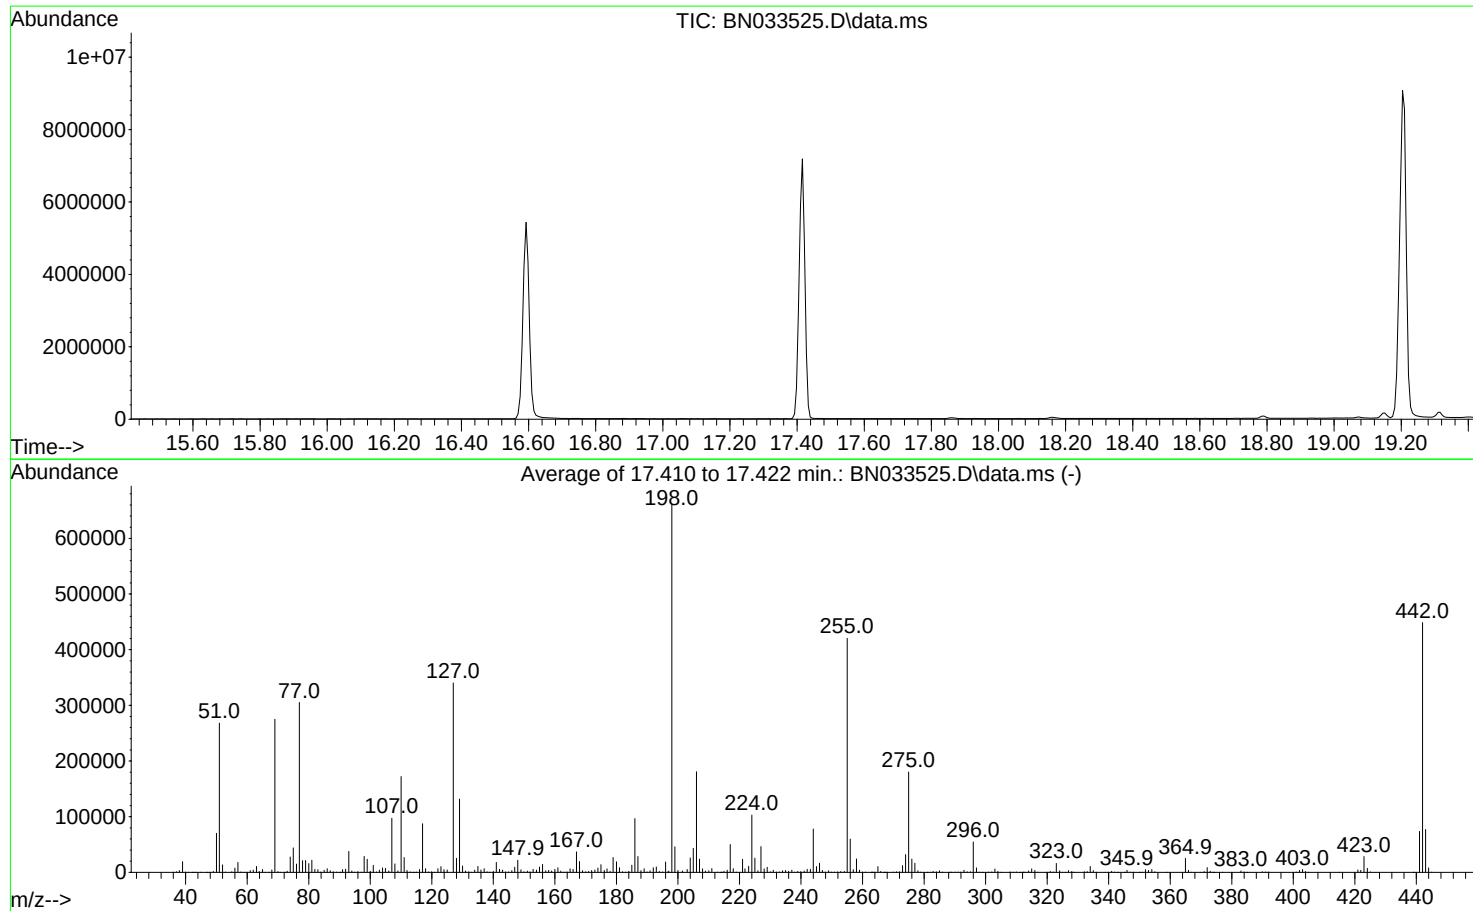




AutoFind: Scans 2452, 2453, 2454; Background Corrected with Scan 2445

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.6	268086	PASS
68	69	0.00	2	1.6	4473	PASS
69	198	0.00	100	41.6	275136	PASS
70	69	0.00	2	0.5	1354	PASS
127	198	10	80	51.5	340352	PASS
197	198	0.00	2	0.4	2392	PASS
198	198	100	100	100.0	660843	PASS
199	198	5	9	7.0	46093	PASS
275	198	10	60	27.3	180224	PASS
365	198	1	100	3.8	24901	PASS
441	198	0.01	100	11.1	73576	PASS
442	442	50	100	100.0	448619	PASS
443	442	15	24	17.2	76992	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082024\
Data File : BN033525.D
Acq On : 21 Aug 2024 03:22
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 21 05:33:24 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 21 05:32:13 2024
Response via : Initial Calibration

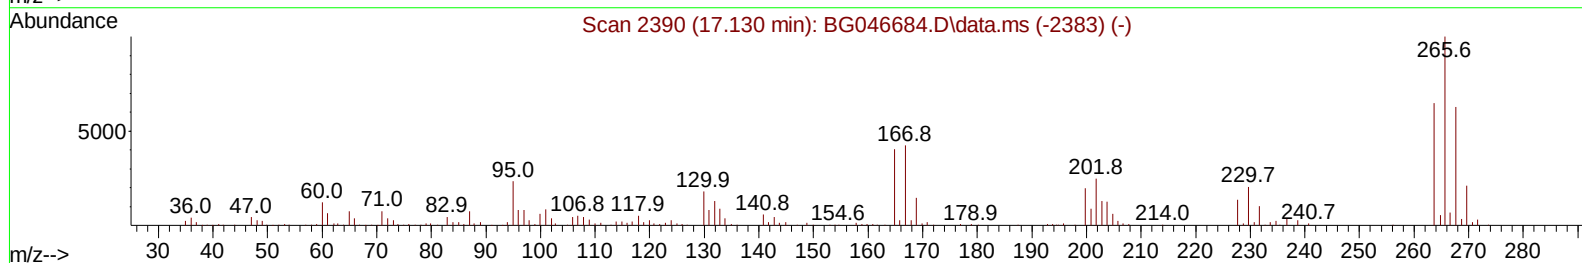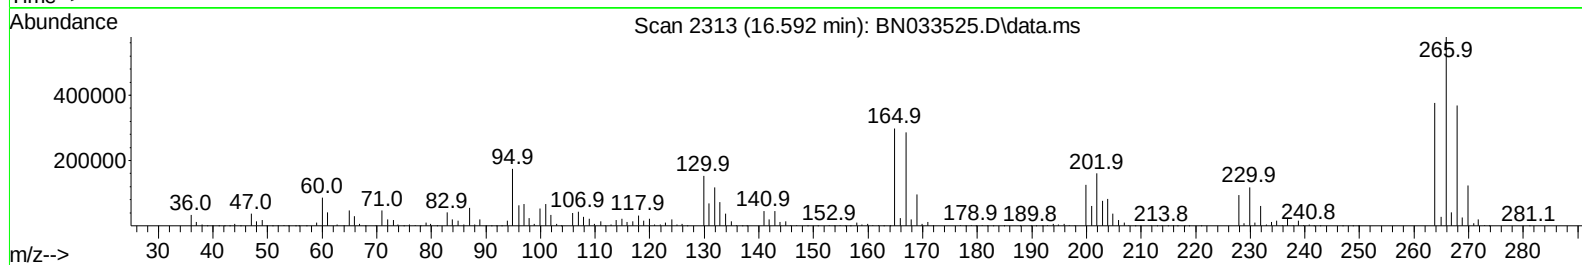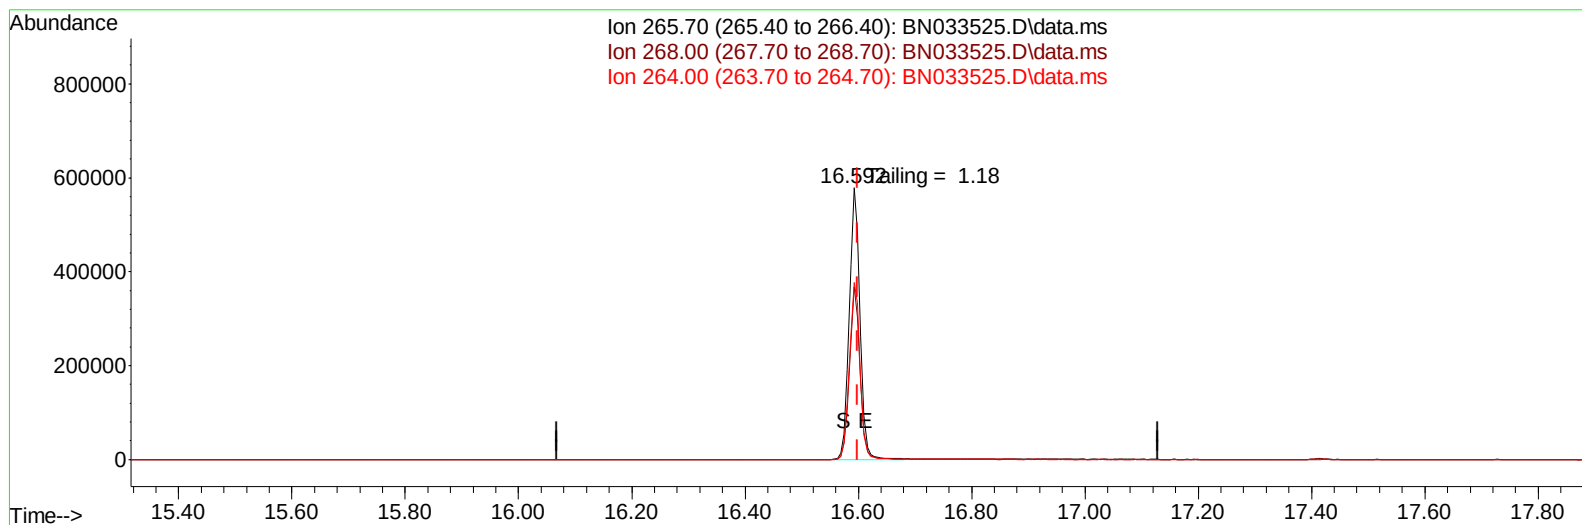

TIC: BN033525.D\data.ms

(70) Pentachlorophenol (C)

16.592min (-0.006) 21261.92 ng




response 767214

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.62
264.00	61.60	65.22
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082024\
Data File : BN033525.D
Acq On : 21 Aug 2024 03:22
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 21 05:33:24 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 21 05:32:13 2024
Response via : Initial Calibration

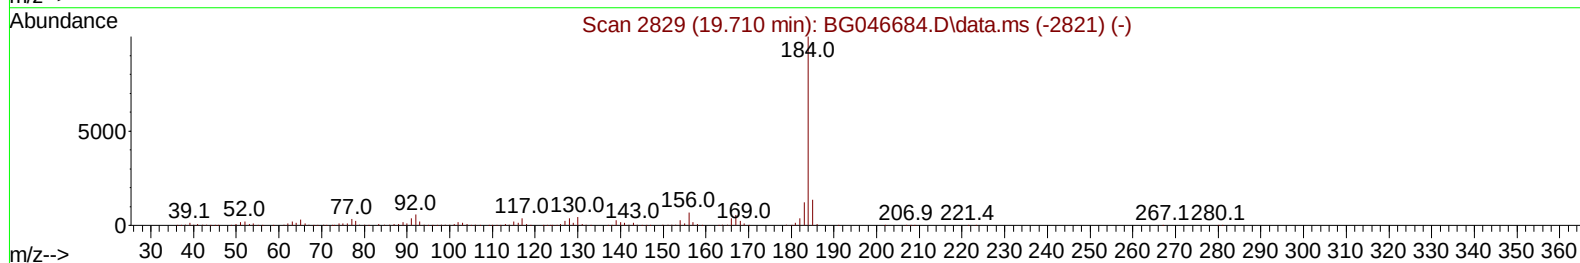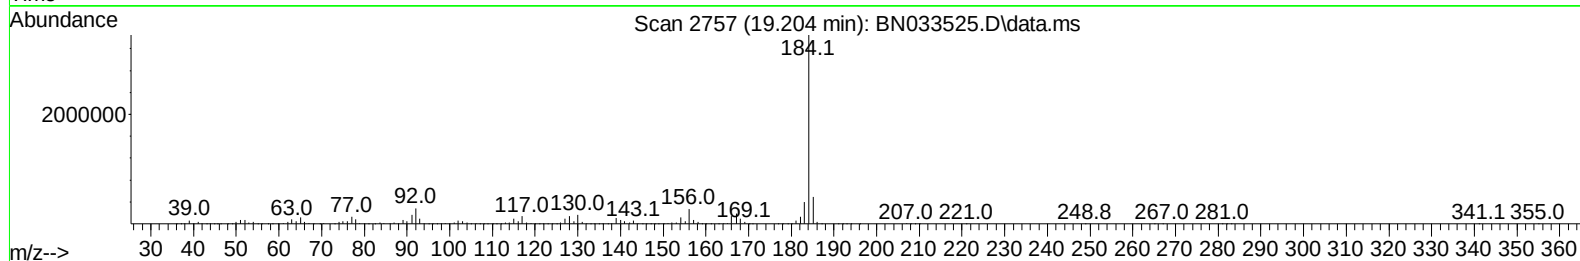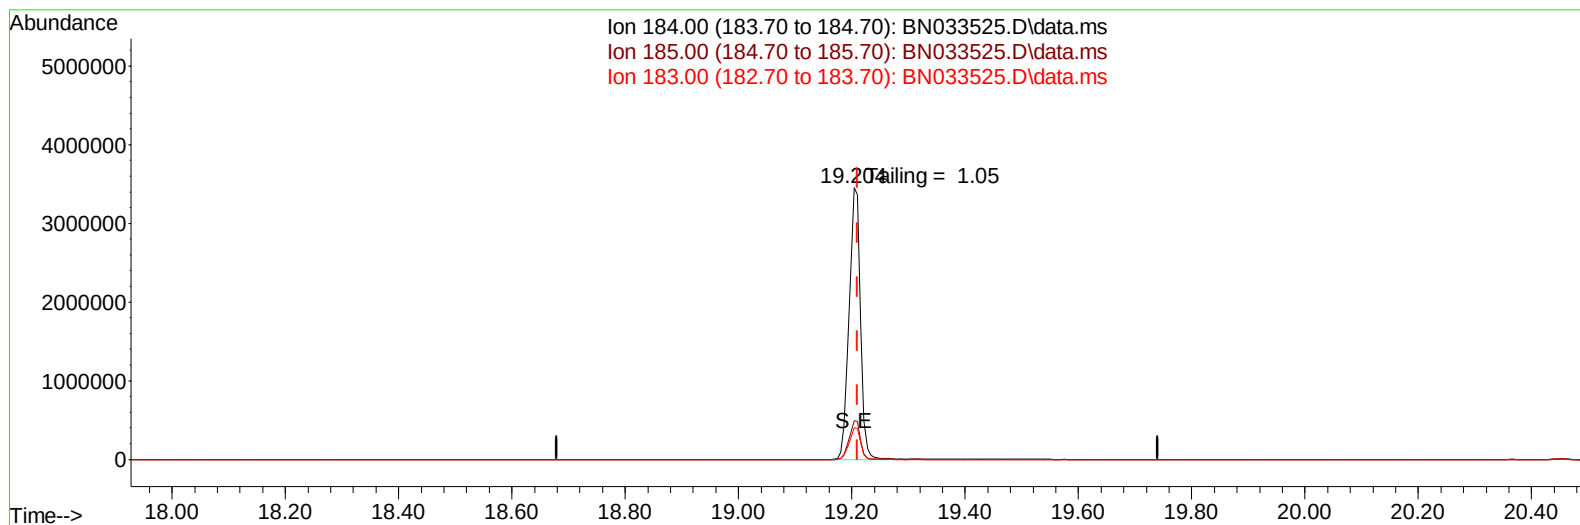

TIC: BN033525.D\data.ms

(77) Benzidine

19.204min (-0.006) 0.00 ng

response 4854251

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.28
183.00	13.20	11.64
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/20/2024	BNA_N	<u>BN033525.D</u>
Compound Name	Response	Retention Time
DDT	2231070	20.451
DDD	67613	20.004
DDE	1201	19.498
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
68814	2299884	2.99

Instrument :
BNA_N
ClientSampleId :
DFTPP