

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082222\
 Data File : BN021307.D
 Acq On : 22 Aug 2022 19:25
 Operator : CG/JU
 Sample : PB147154BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK154

Quant Time: Aug 23 04:03:20 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN082222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 22 18:06:52 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.097	152	2638	0.400	ng/ul	0.00
4) Naphthalene-d8	10.933	136	8734	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.754	164	4778	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.502	188	9622	0.400	ng/ul	0.00
17) Chrysene-d12	21.691	240	7062	0.400	ng/ul	# 0.00
23) Perylene-d12	24.225	264	8200	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.384	96	18865	5.544	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.517	152	4163	0.315	ng/ul	0.00
18) Fluoranthene-d10	19.525	212	8072	0.371	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.892	202	1287	0.038	ng/ul#	1
26) Benzo(a)pyrene	24.062	252	2785	0.084	ng/ul#	69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082222\
Data File : BN021307.D
Acq On : 22 Aug 2022 19:25
Operator : CG/JU
Sample : PB147154BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK154

Quant Time: Aug 23 04:03:20 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN082222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 22 18:06:52 2022
Response via : Initial Calibration




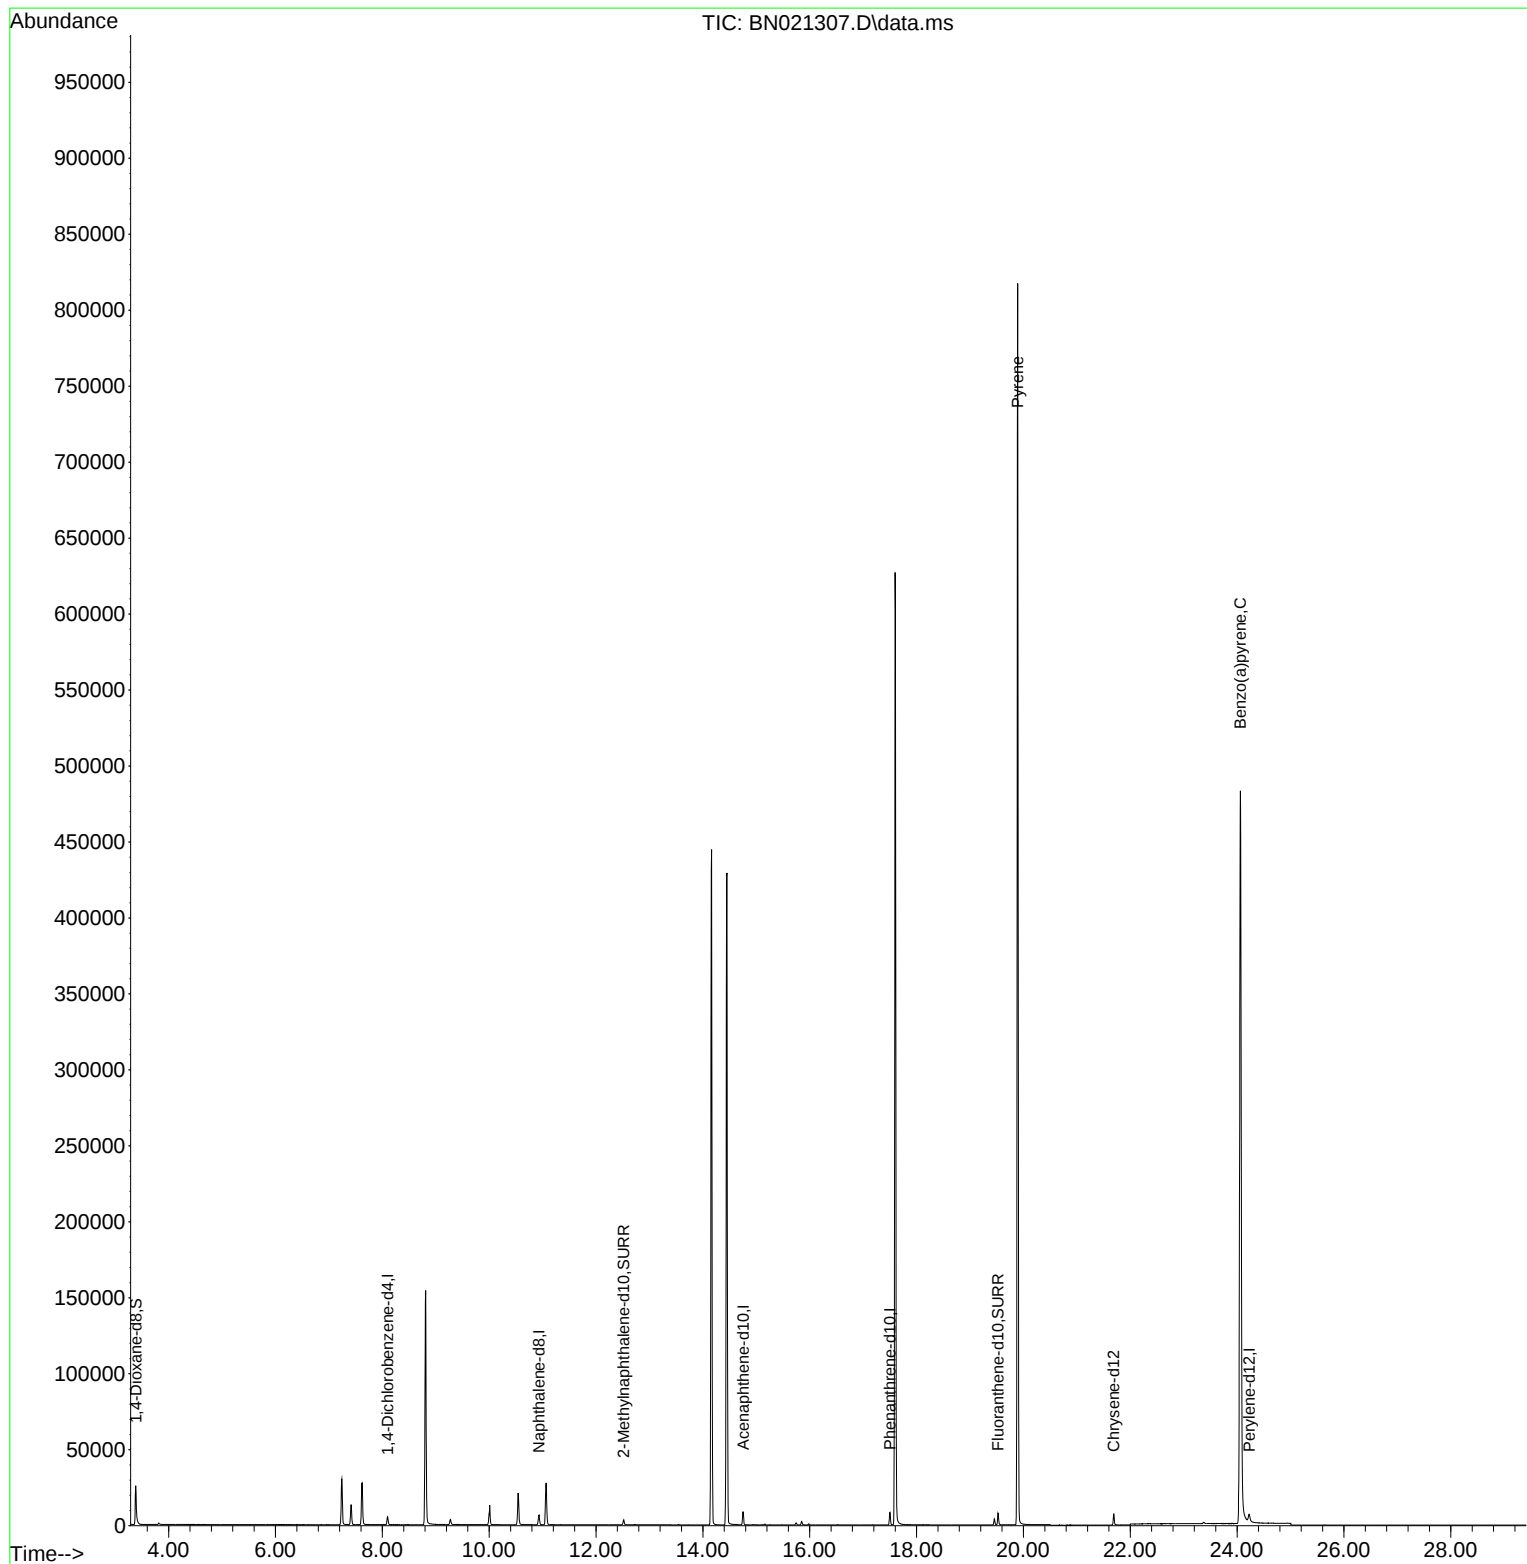


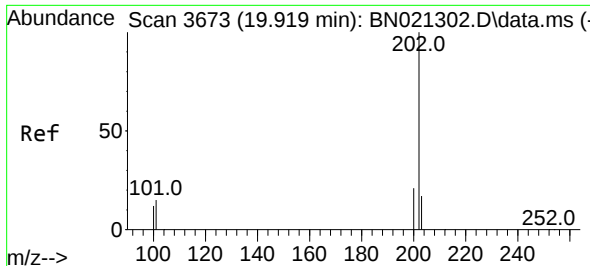

#20
Pyrene
Concen: 0.038 ng/ul
RT: 19.892 min Scan# 3667
Delta R.T. -0.028 min
Lab File: BN021307.D
Acq: 22 Aug 2022 19:25

Instrument :
BNA_N
ClientSampleId :
SBLK154

Tgt Ion:202 Resp: 1287
Ion Ratio Lower Upper
202 100
101 159.2 11.3 16.9#
100 1131.6 9.0 13.4#

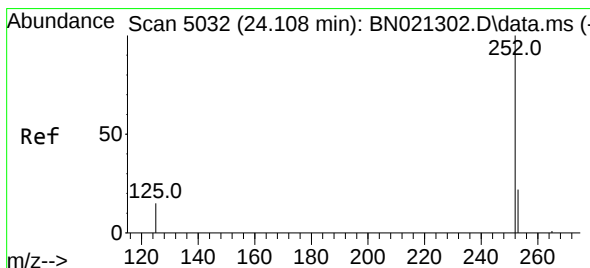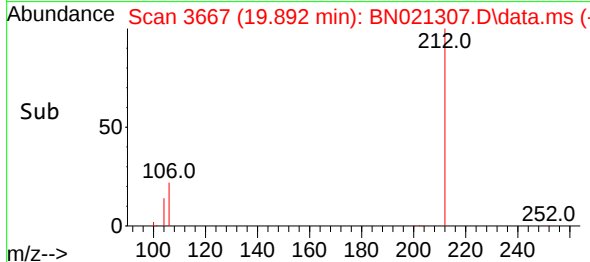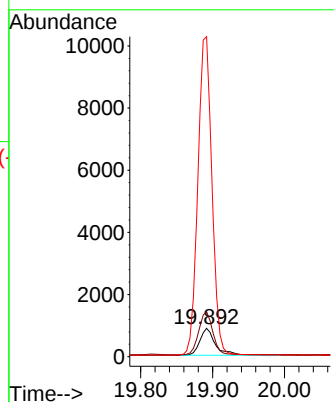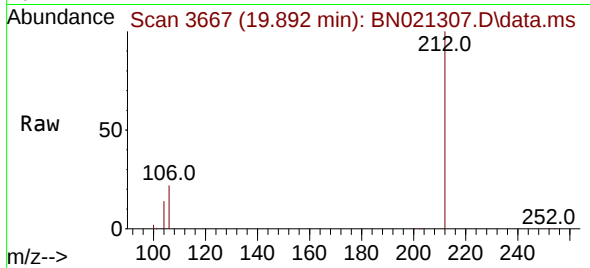

#26
Benzo(a)pyrene
Concen: 0.084 ng/ul
RT: 24.062 min Scan# 5016
Delta R.T. -0.047 min
Lab File: BN021307.D
Acq: 22 Aug 2022 19:25

Tgt Ion:252 Resp: 2785
Ion Ratio Lower Upper
252 100
253 39.7 22.1 33.1#
125 37.8 14.7 22.1#

