

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082222\
 Data File : BN021314.D
 Acq On : 23 Aug 2022 00:24
 Operator : CG/JU
 Sample : PB147177BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK177

Quant Time: Aug 23 04:05:03 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN082222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 22 18:06:52 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.097	152	2815	0.400	ng/ul	0.00
4) Naphthalene-d8	10.927	136	9511	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.749	164	5299	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.498	188	11037	0.400	ng/ul	0.00
17) Chrysene-d12	21.685	240	8148	0.400	ng/ul	# 0.00
23) Perylene-d12	24.219	264	9094	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.384	96	22539	6.207	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.516	152	5197	0.361	ng/ul	0.00
18) Fluoranthene-d10	19.524	212	10457	0.416	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.744	166	1593	0.068	ng/ul#	14
20) Pyrene	19.892	202	1536	0.040	ng/ul#	1
26) Benzo(a)pyrene	24.056	252	3430	0.093	ng/ul#	75


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082222\
Data File : BN021314.D
Acq On : 23 Aug 2022 00:24
Operator : CG/JU
Sample : PB147177BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK177

Quant Time: Aug 23 04:05:03 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN082222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 22 18:06:52 2022
Response via : Initial Calibration




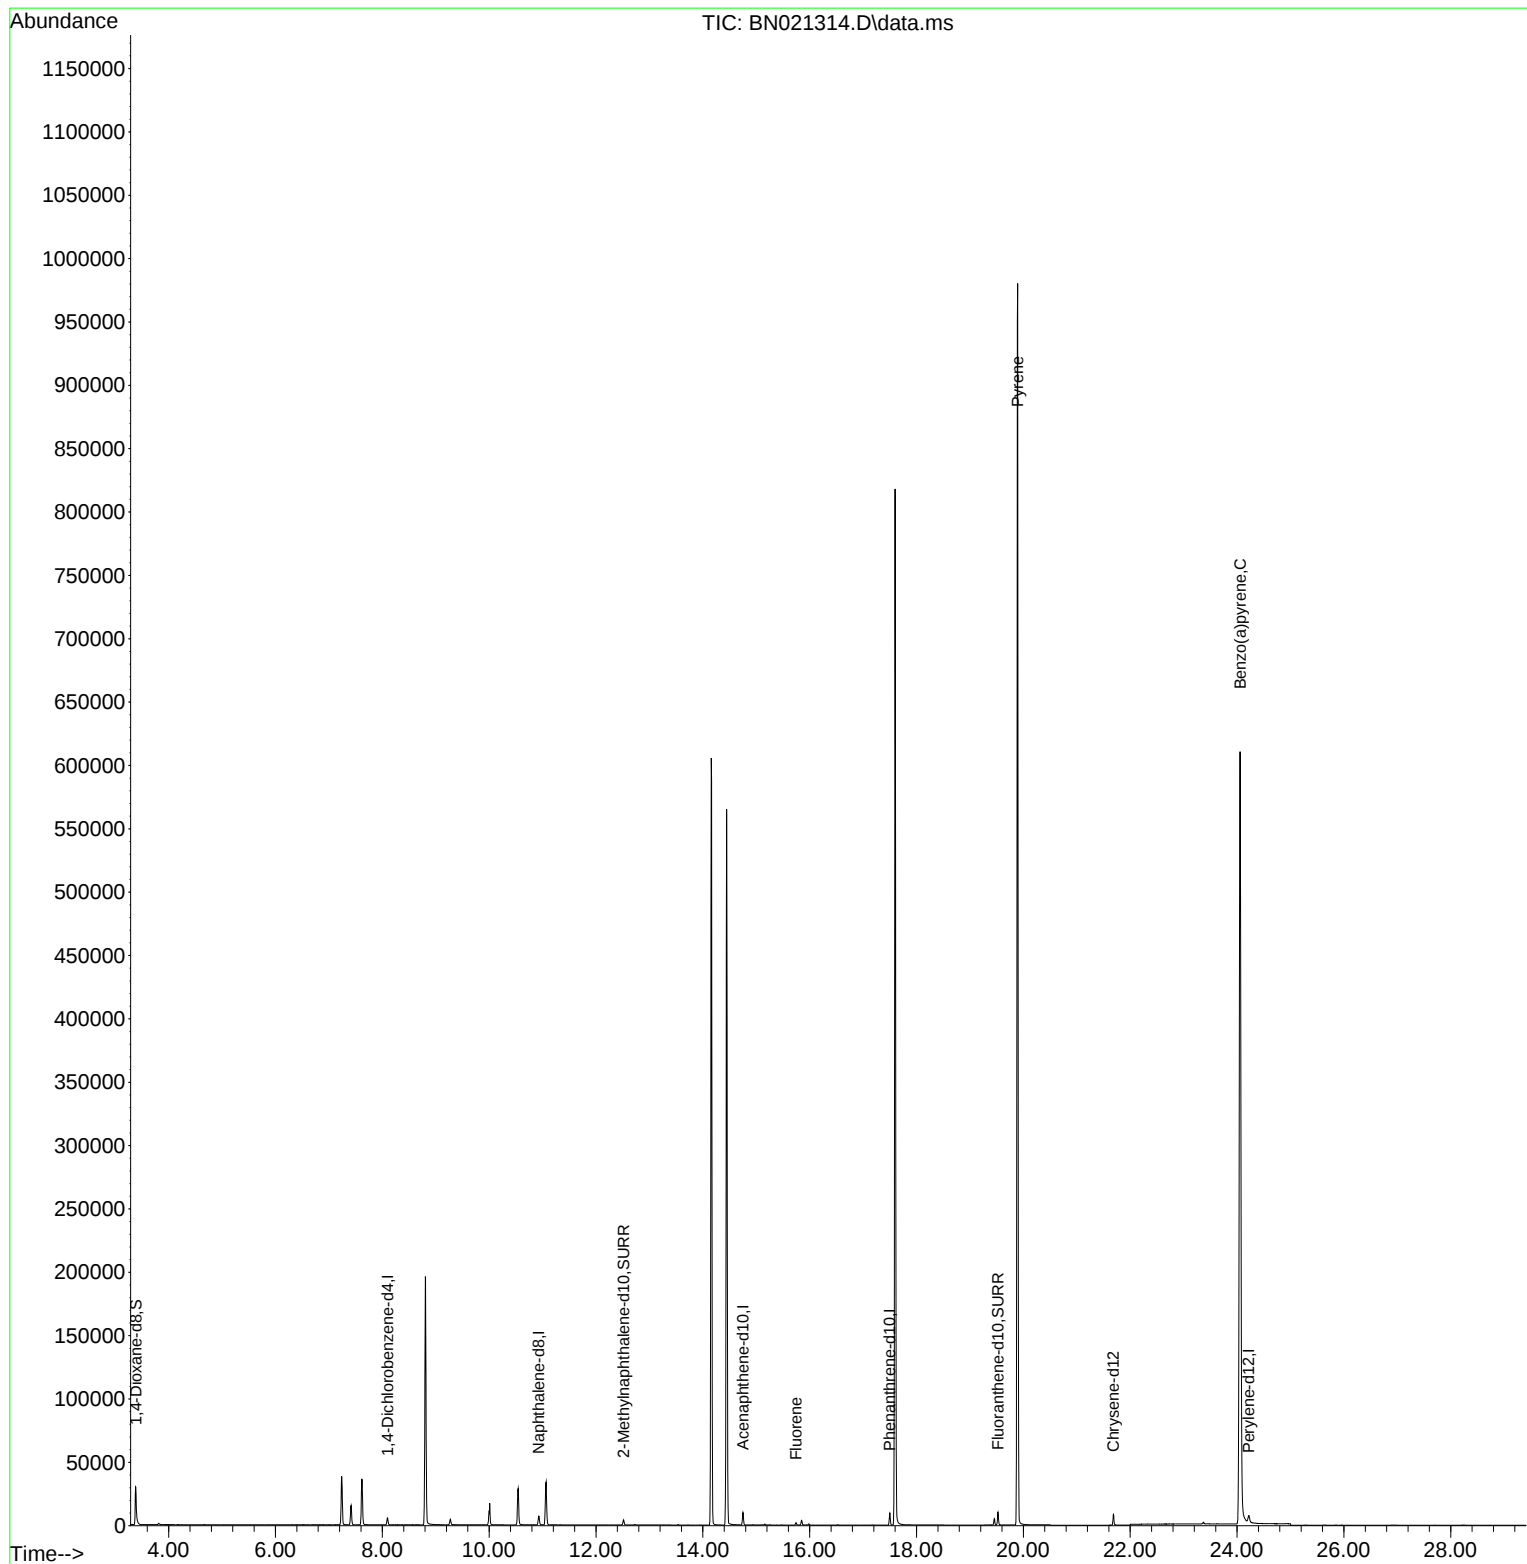


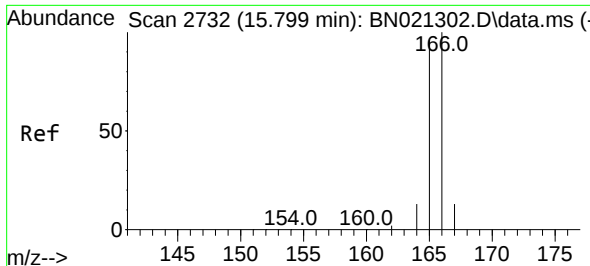

#12
Fluorene
Concen: 0.068 ng/ul
RT: 15.744 min Scan# 21
Delta R.T. -0.055 min
Lab File: BN021314.D
Acq: 23 Aug 2022 00:24




Instrument :
BNA_N
ClientSampleId :
SBLK177


Tgt Ion:166 Resp: 1593
Ion Ratio Lower Upper
166 100
165 8.2 78.6 117.8#
167 35.7 11.8 17.6#

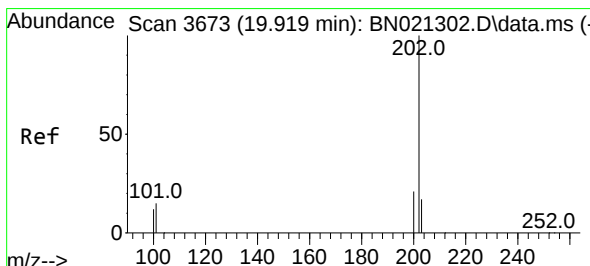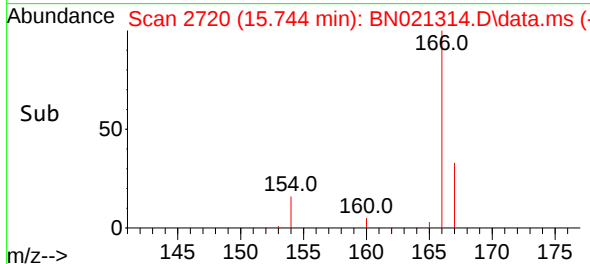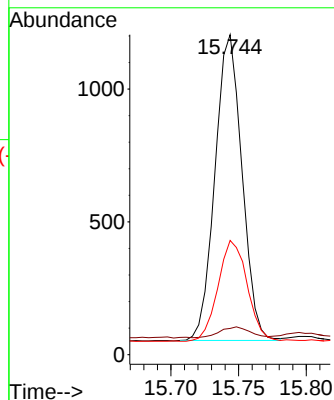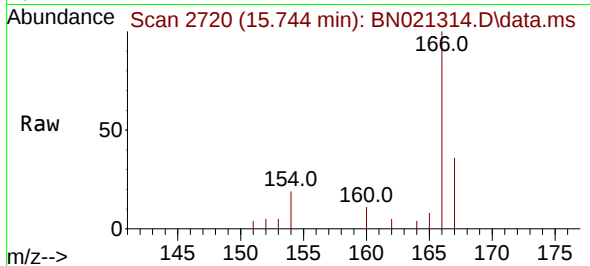

#20
Pyrene
Concen: 0.040 ng/ul
RT: 19.892 min Scan# 3667
Delta R.T. -0.028 min
Lab File: BN021314.D
Acq: 23 Aug 2022 00:24

Tgt Ion:202 Resp: 1536
Ion Ratio Lower Upper
202 100
101 155.4 11.3 16.9#
100 1090.1 9.0 13.4#

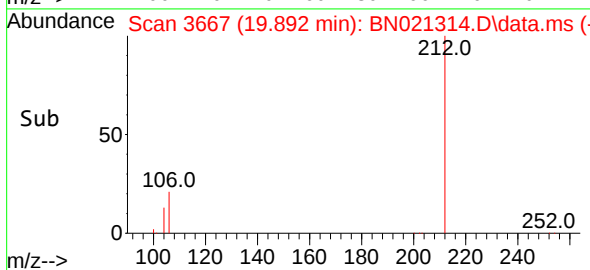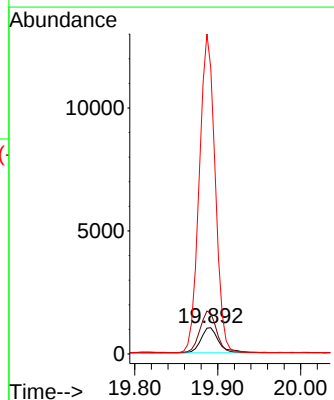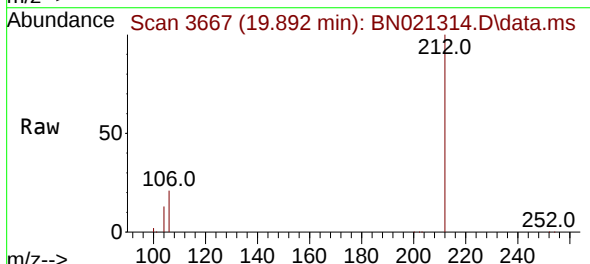

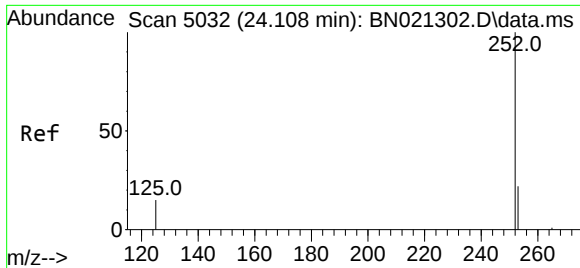

#26

Benzo(a)pyrene

Concen: 0.093 ng/ul

RT: 24.056 min Scan# 50

Delta R.T. -0.053 min

Lab File: BN021314.D


Acq: 23 Aug 2022 00:24

Instrument :

BNA_N

ClientSampleId :

SBLK177

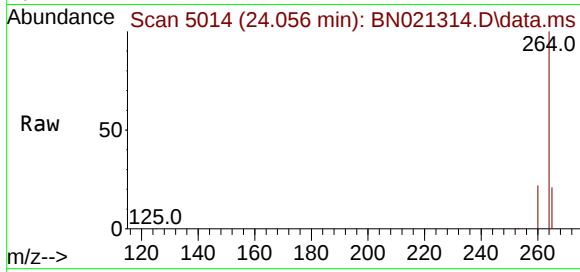

Tgt Ion:252 Resp: 3430

Ion Ratio Lower Upper

252 100

253 36.9 22.1 33.1#

125 34.4 14.7 22.1#

