

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082222\
 Data File : BN021309.D
 Acq On : 22 Aug 2022 20:40
 Operator : CG/JU
 Sample : N4251-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BGN66

Quant Time: Aug 23 04:03:52 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN082222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 22 18:06:52 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.097	152	2509	0.400	ng/ul	0.00
4) Naphthalene-d8	10.927	136	8494	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.749	164	4662	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.502	188	9753	0.400	ng/ul	0.00
17) Chrysene-d12	21.688	240	7779	0.400	ng/ul	# 0.00
23) Perylene-d12	24.217	264	9096	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.385	96	15623	4.827	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.517	152	4381	0.341	ng/ul	0.00
18) Fluoranthene-d10	19.525	212	11095	0.463	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.422	88	218	0.064	ng/ul#	62


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082222\
Data File : BN021309.D
Acq On : 22 Aug 2022 20:40
Operator : CG/JU
Sample : N4251-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGN66


Quant Time: Aug 23 04:03:52 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN082222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 22 18:06:52 2022
Response via : Initial Calibration

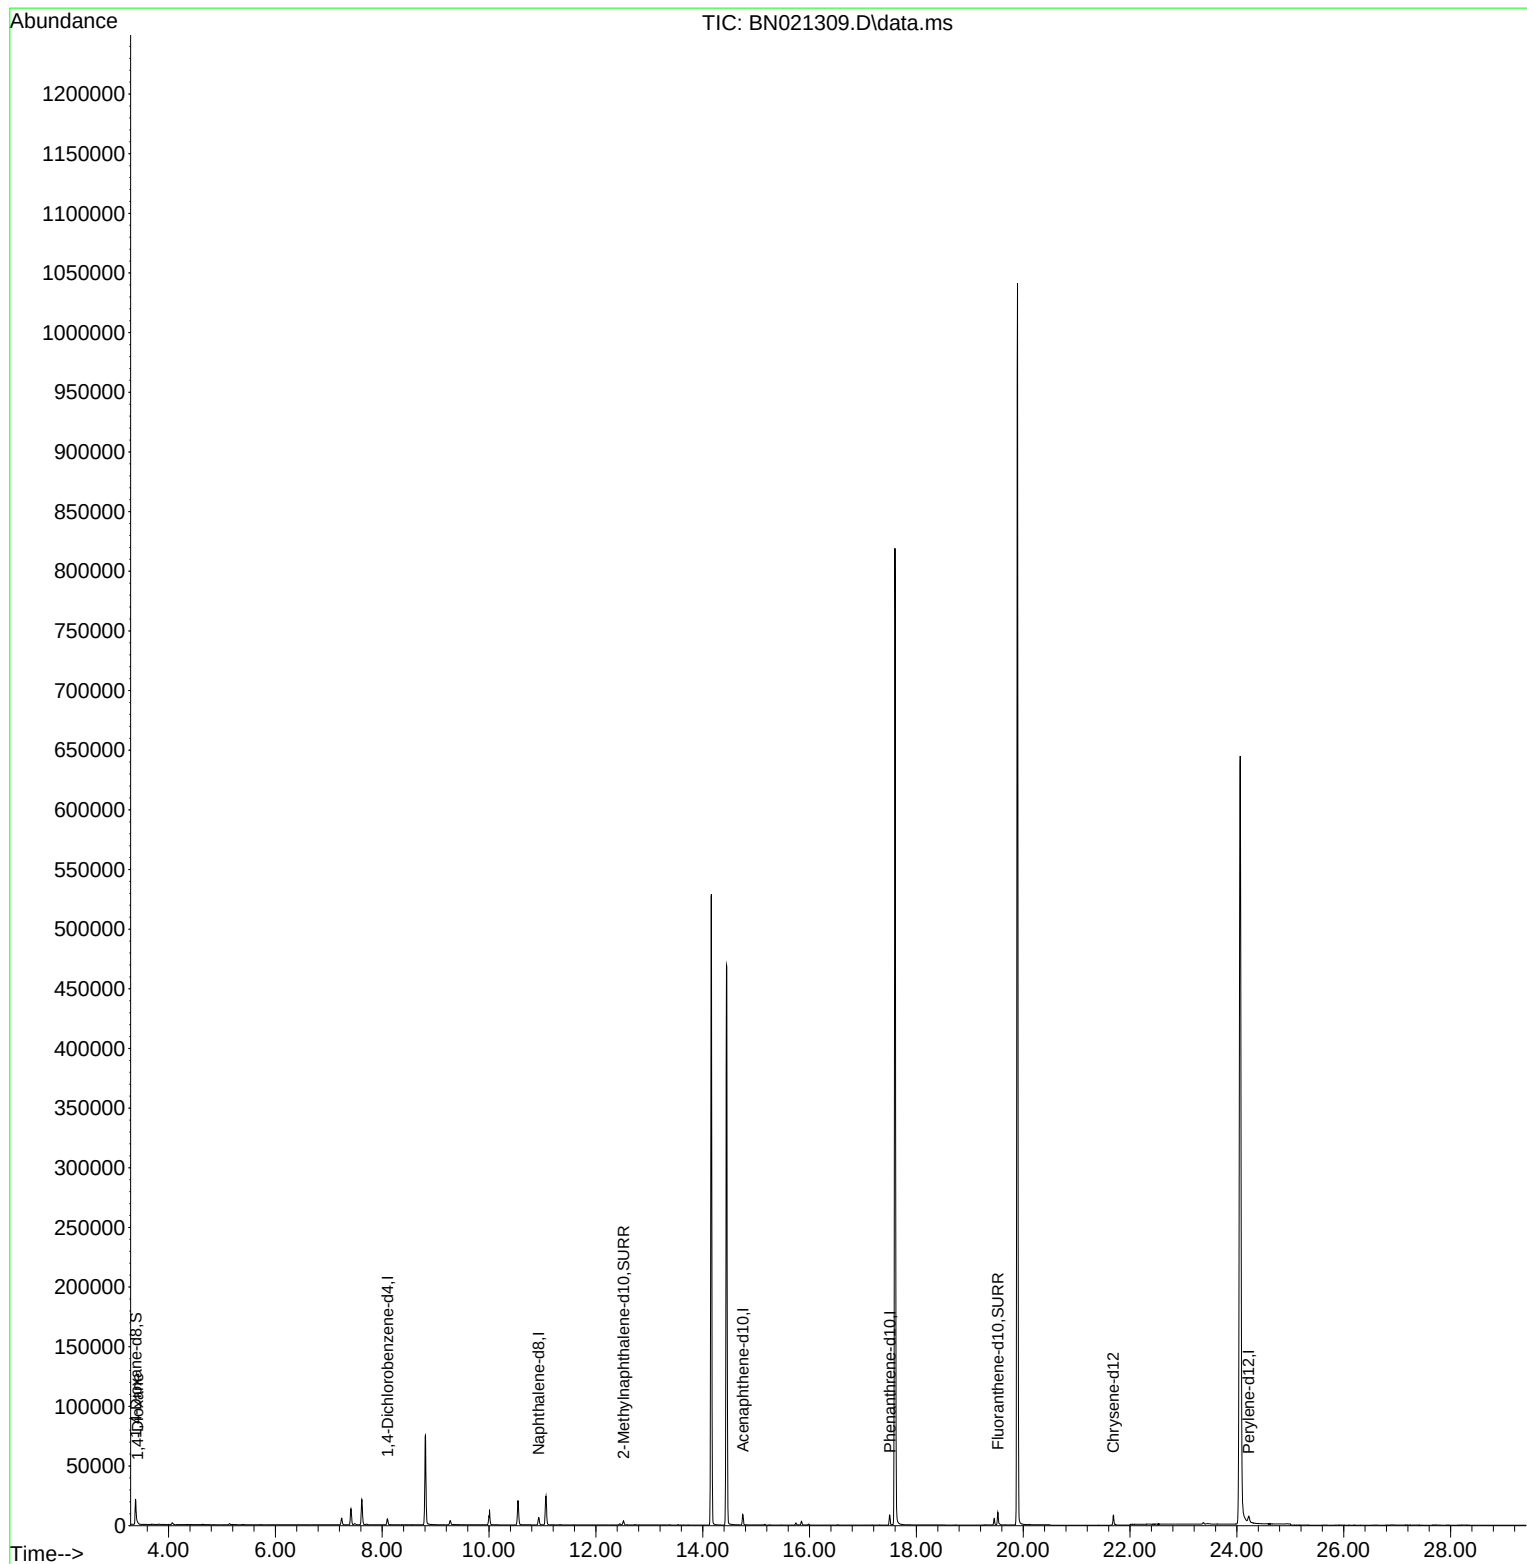

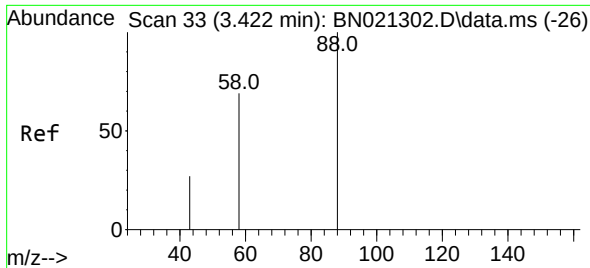

#2
 1,4-Dioxane
 Concen: 0.064 ng/ul
 RT: 3.422 min Scan# 33
 Delta R.T. 0.000 min
 Lab File: BN021309.D
 Acq: 22 Aug 2022 20:40

Instrument :
 BNA_N
 ClientSampleId :
 BGN66

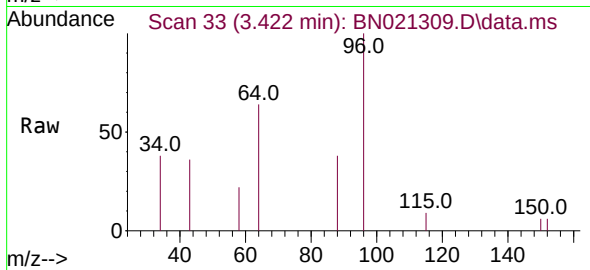

Tgt Ion:	88	Resp:	218
Ion	Ratio	Lower	Upper
88	100		
43	95.3	31.4	47.0#
58	58.7	49.0	73.6

