

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082222\
 Data File : BN021310.D
 Acq On : 22 Aug 2022 21:17
 Operator : CG/JU
 Sample : N4251-02
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BGN86

Quant Time: Aug 23 04:04:04 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN082222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 22 18:06:52 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.097	152	2355	0.400	ng/ul	0.00
4) Naphthalene-d8	10.933	136	7989	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.749	164	4540	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.502	188	9739	0.400	ng/ul	0.00
17) Chrysene-d12	21.688	240	7920	0.400	ng/ul	# 0.00
23) Perylene-d12	24.219	264	8941	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.385	96	14637	4.818	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.517	152	4397	0.364	ng/ul	0.00
18) Fluoranthene-d10	19.524	212	10585	0.434	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.422	88	1812	0.569	ng/ul#	75


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082222\
Data File : BN021310.D
Acq On : 22 Aug 2022 21:17
Operator : CG/JU
Sample : N4251-02
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGN86

Quant Time: Aug 23 04:04:04 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN082222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 22 18:06:52 2022
Response via : Initial Calibration

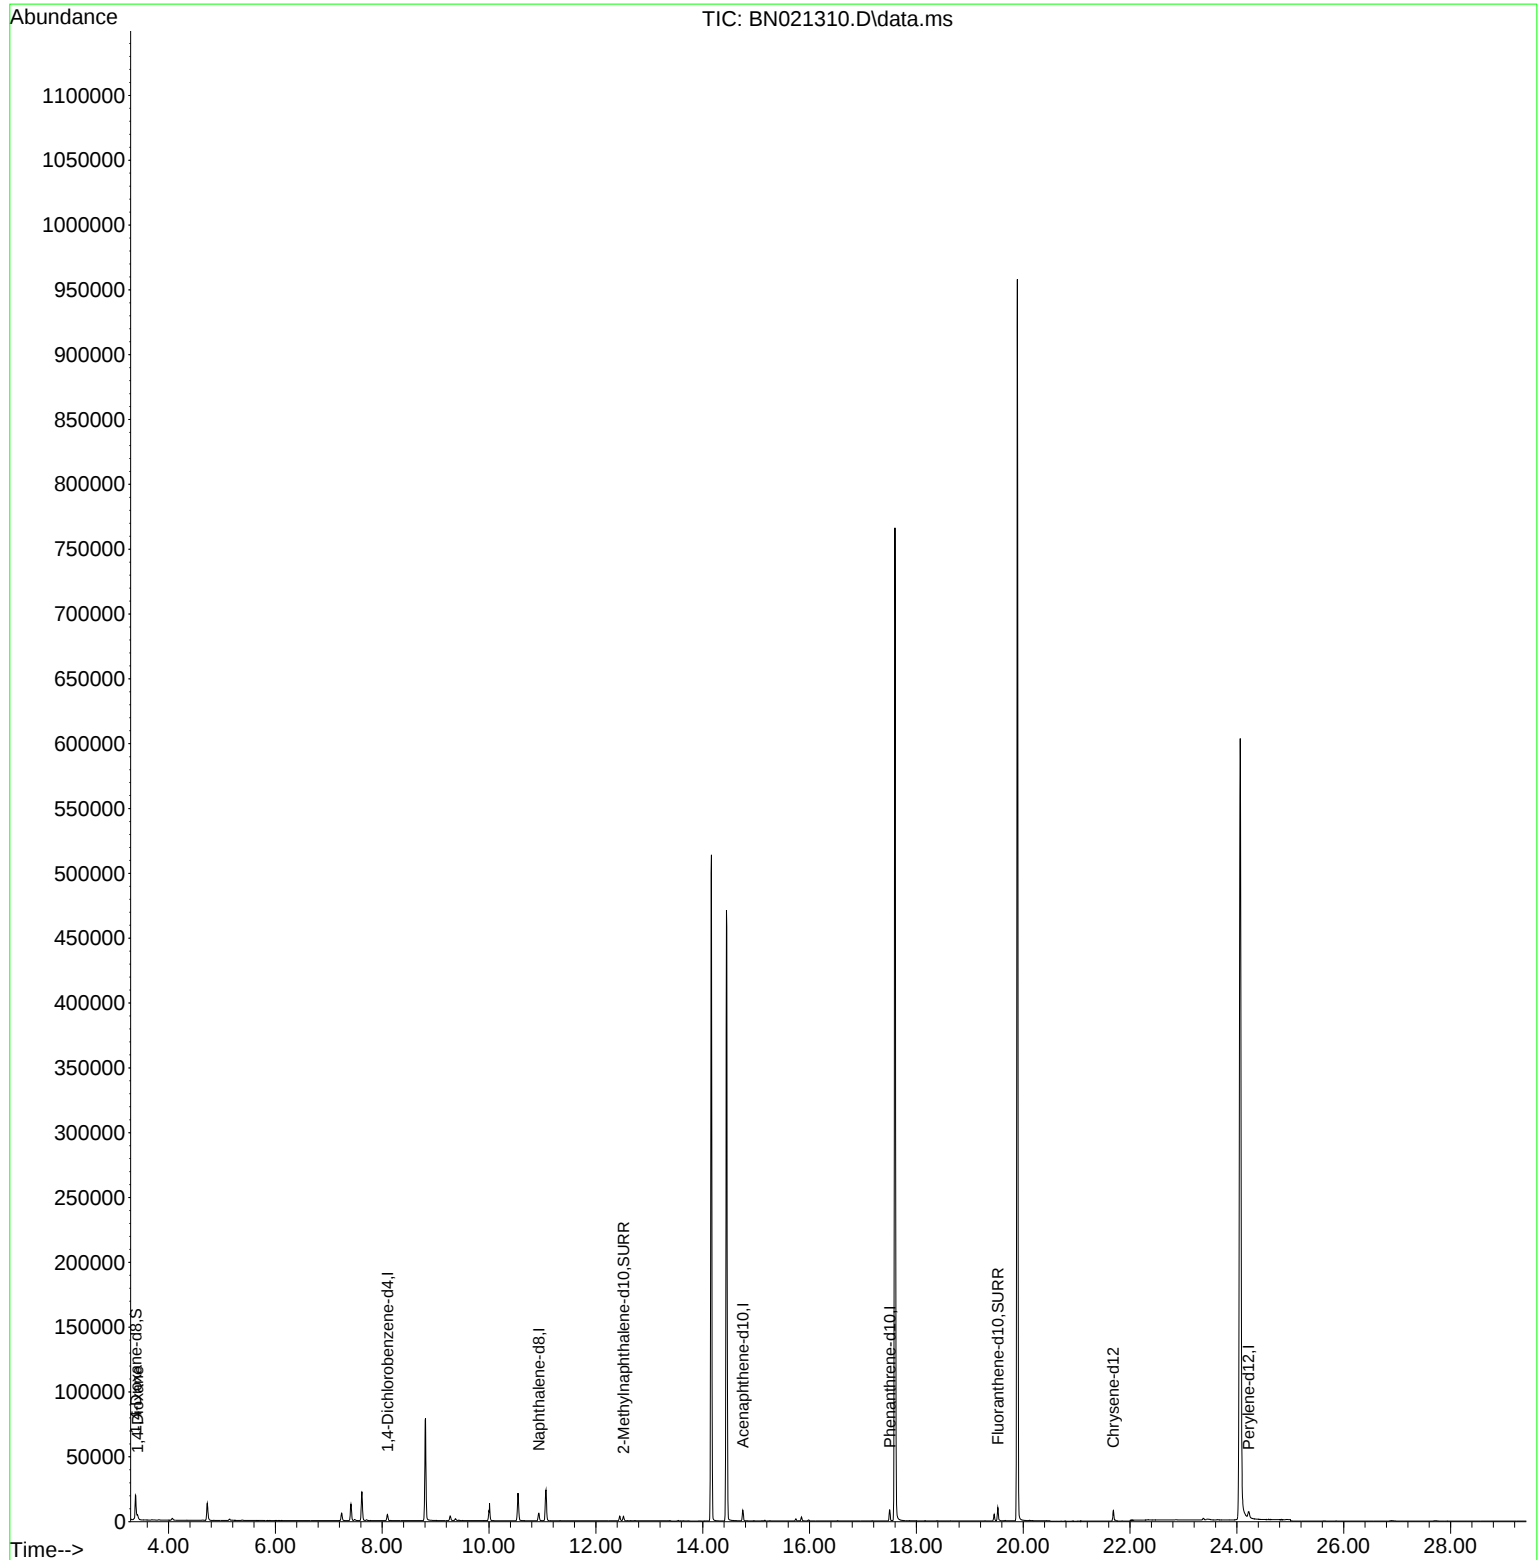

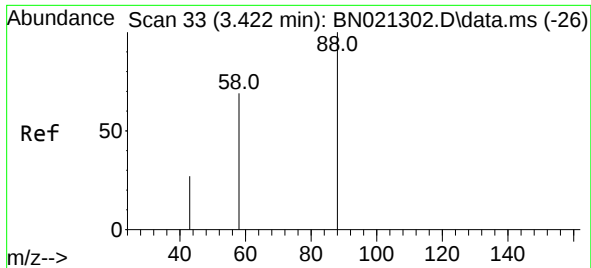

#2
 1,4-Dioxane
 Concen: 0.569 ng/ul
 RT: 3.422 min Scan# 33
 Delta R.T. 0.000 min
 Lab File: BN021310.D
 Acq: 22 Aug 2022 21:17

Instrument :
 BNA_N
 ClientSampleId :
 BGN86

Tgt Ion: 88 Resp: 1812
 Ion Ratio Lower Upper
 88 100
 43 62.6 31.4 47.0#
 58 74.1 49.0 73.6#

