

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082222\
 Data File : BN021316.D
 Acq On : 23 Aug 2022 01:38
 Operator : CG/JU
 Sample : N4251-05
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BGN60

Quant Time: Aug 23 04:05:33 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN082222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 22 18:06:52 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.097	152	2800	0.400	ng/ul	0.00
4) Naphthalene-d8	10.927	136	9587	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.749	164	5404	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.498	188	11462	0.400	ng/ul	0.00
17) Chrysene-d12	21.688	240	8885	0.400	ng/ul	0.00
23) Perylene-d12	24.220	264	10146	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.385	96	15097	4.180	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.517	152	4847	0.334	ng/ul	0.00
18) Fluoranthene-d10	19.525	212	11780	0.430	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.422	88	14652	3.872	ng/ul#	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082222\
Data File : BN021316.D
Acq On : 23 Aug 2022 01:38
Operator : CG/JU
Sample : N4251-05
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGN60


Quant Time: Aug 23 04:05:33 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN082222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 22 18:06:52 2022
Response via : Initial Calibration

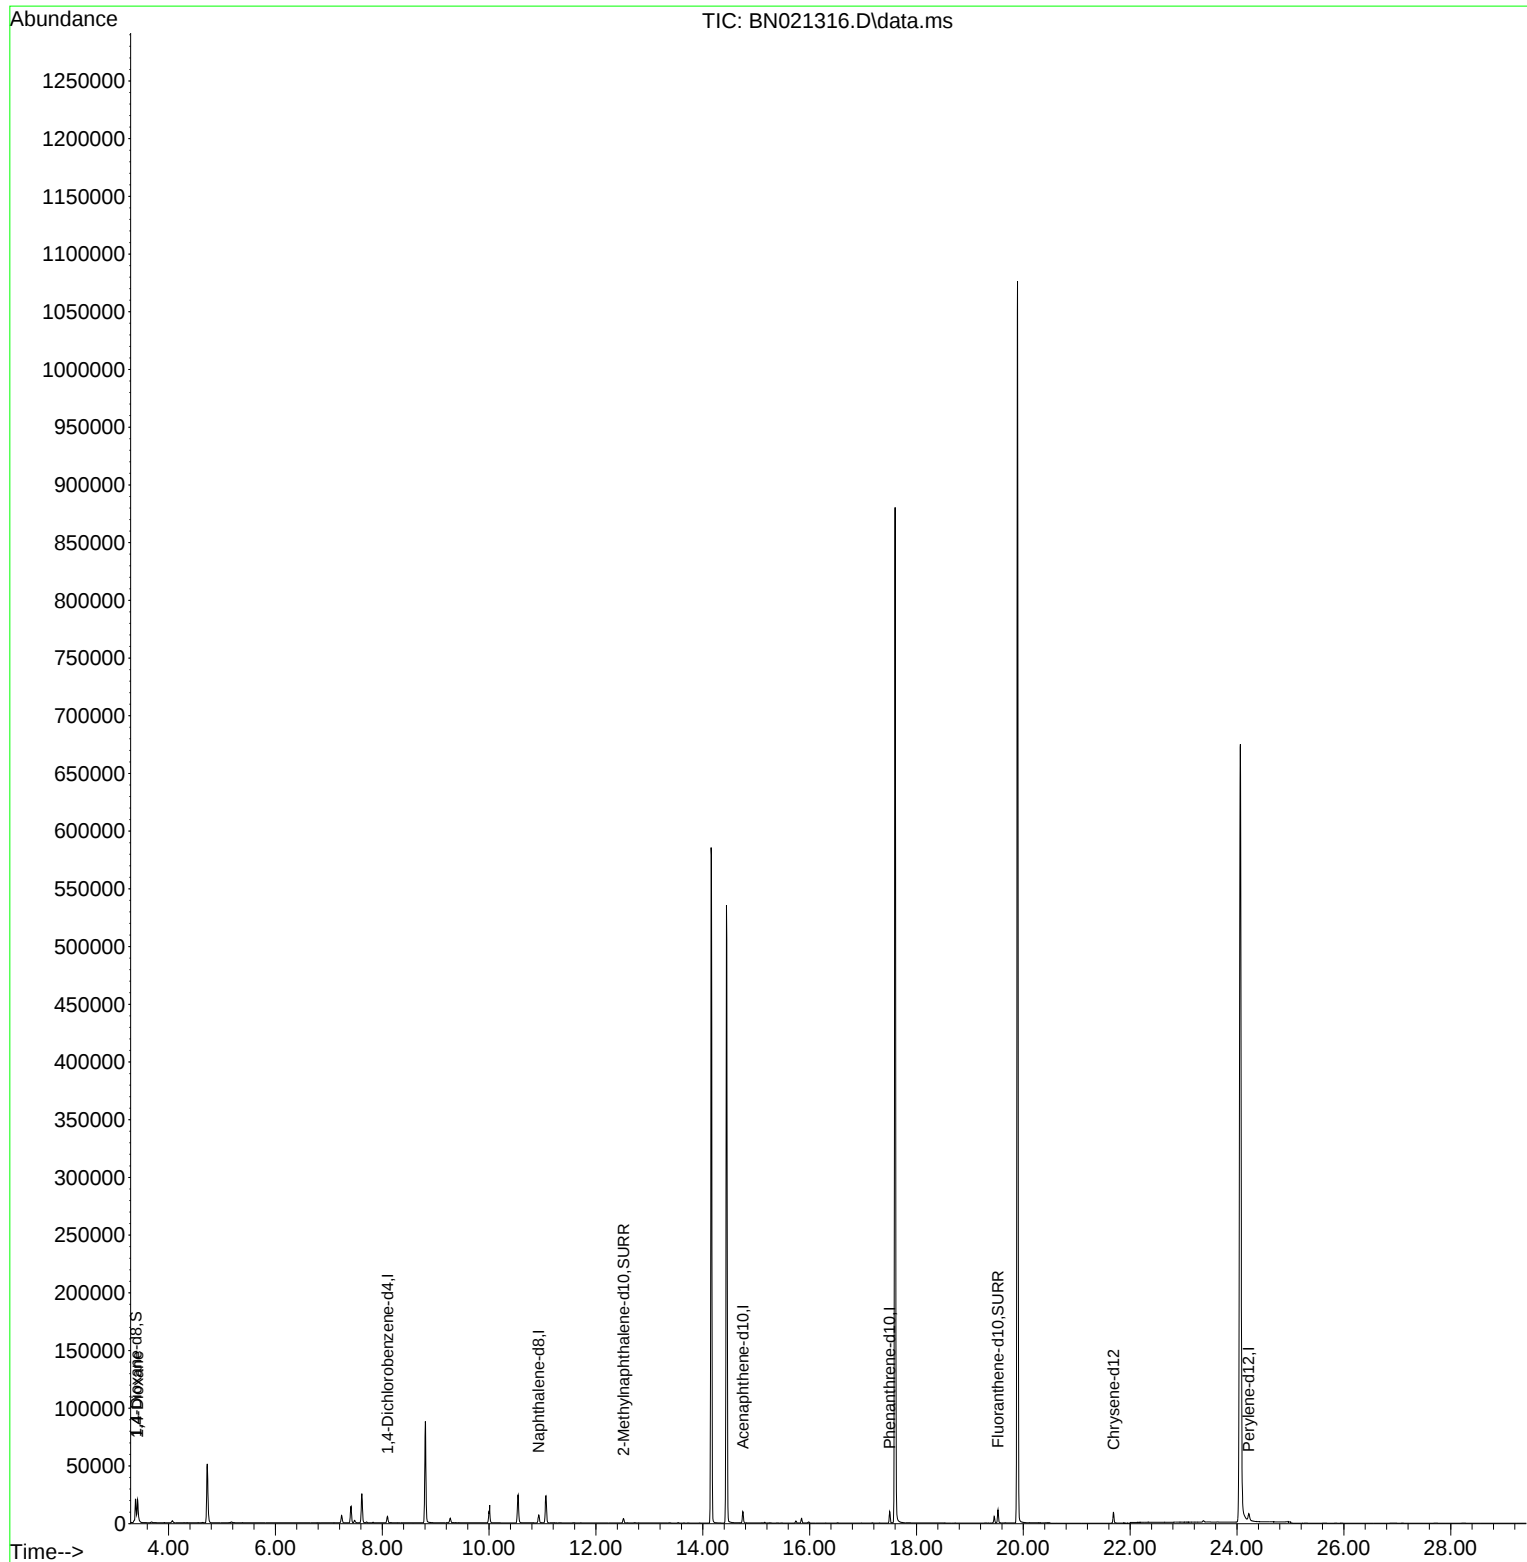

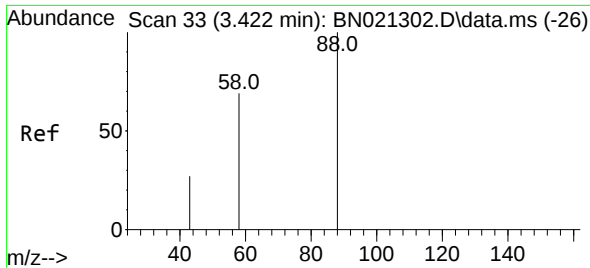

#2
 1,4-Dioxane
 Concen: 3.872 ng/ul
 RT: 3.422 min Scan# 33
 Delta R.T. 0.000 min
 Lab File: BN021316.D
 Acq: 23 Aug 2022 01:38

Instrument :
 BNA_N
 ClientSampleId :
 BGN60

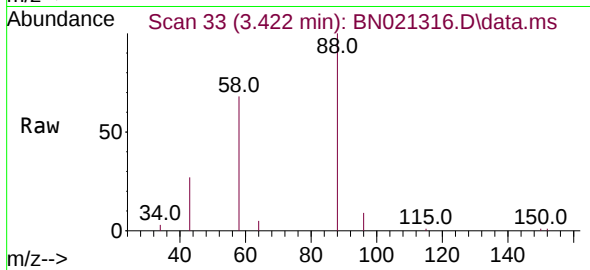

Tgt Ion: 88 Resp: 14652
 Ion Ratio Lower Upper
 88 100
 43 26.6 31.4 47.0#
 58 67.7 49.0 73.6

