
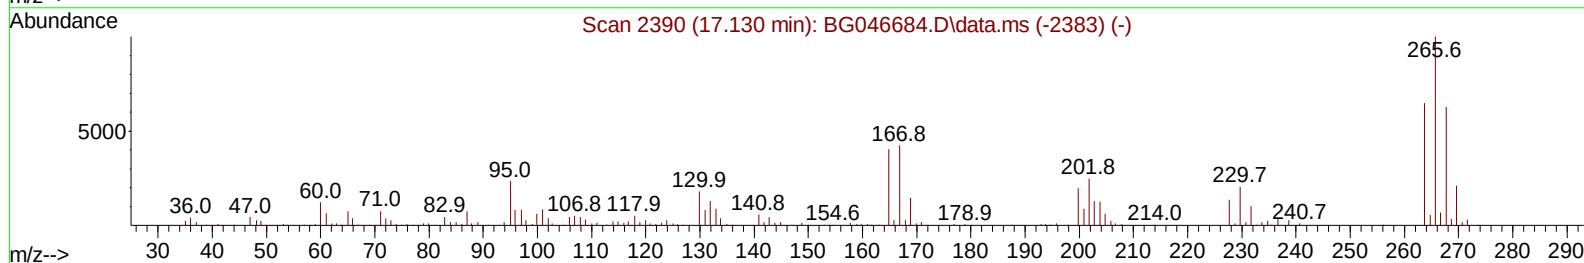
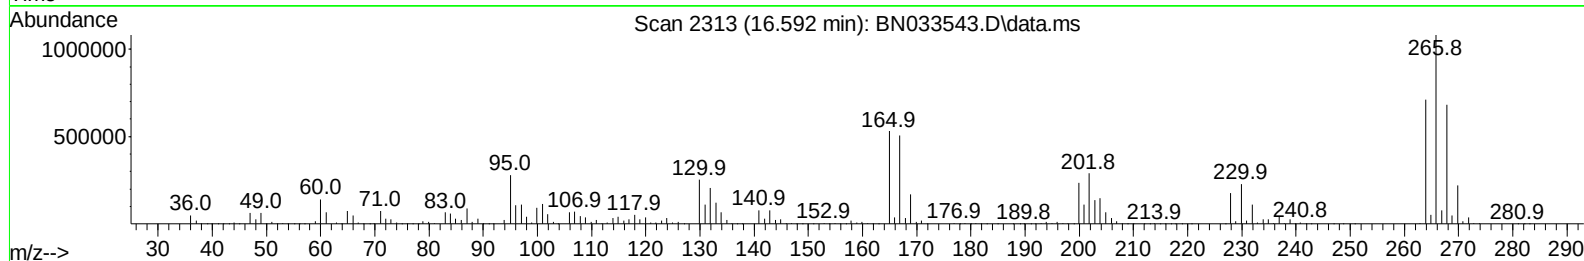


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082224\
Data File : BN033543.D
Acq On : 22 Aug 2024 09:12
Operator : MA/JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 23 07:43:02 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 23 07:42:58 2024
Response via : Initial Calibration

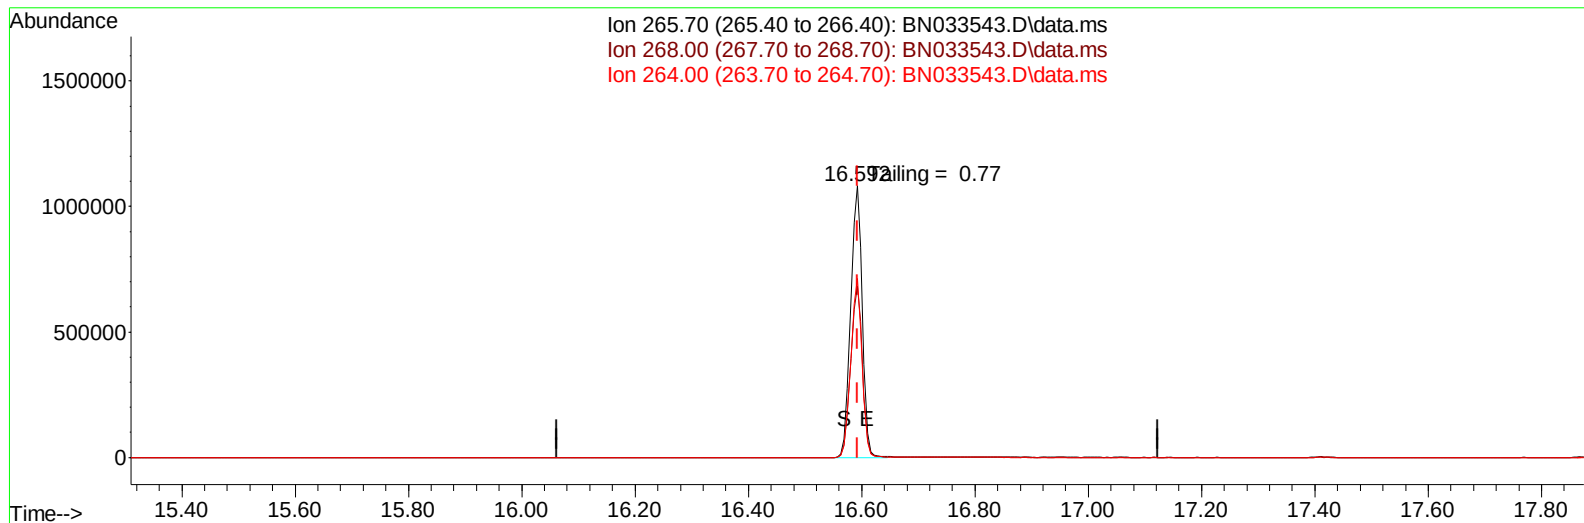

TIC: BN033543.D\data.ms

(70) Pentachlorophenol (C)




16.592min (0.000) 240843.19 ng

response 1551753

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.04
264.00	61.60	65.84
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082224\
Data File : BN033543.D
Acq On : 22 Aug 2024 09:12
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 23 07:43:02 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 23 07:42:58 2024
Response via : Initial Calibration

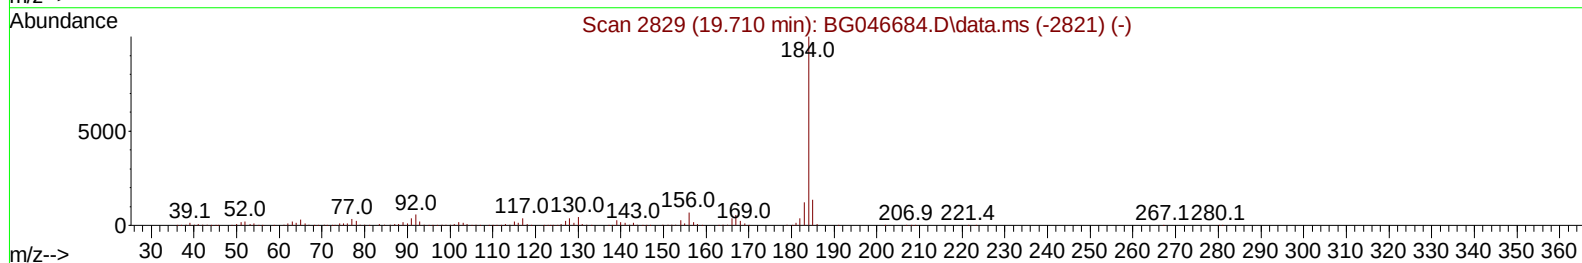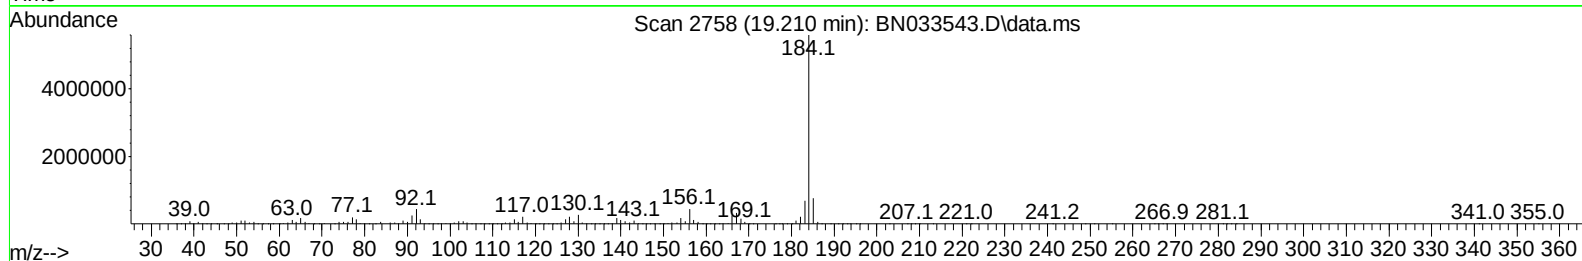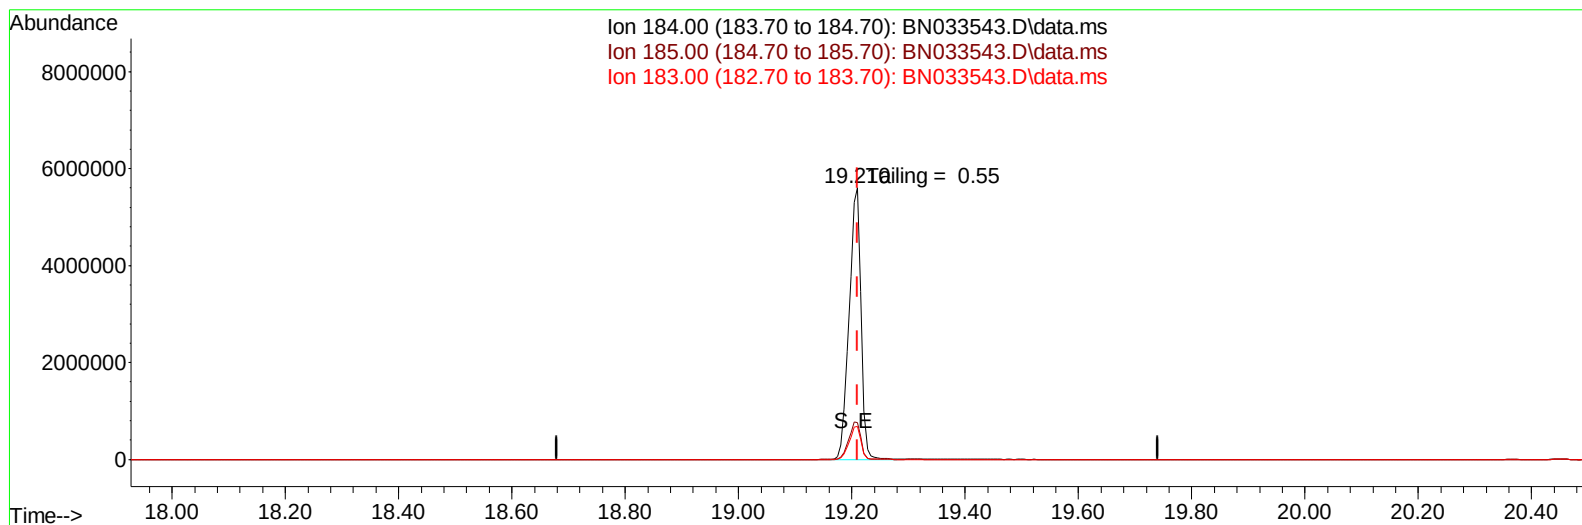

TIC: BN033543.D\data.ms

(77) Benzidine**19.210min (0.000) 4565.62 ng****response 8235503**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.70
183.00	13.20	12.11
0.00	0.00	0.00