
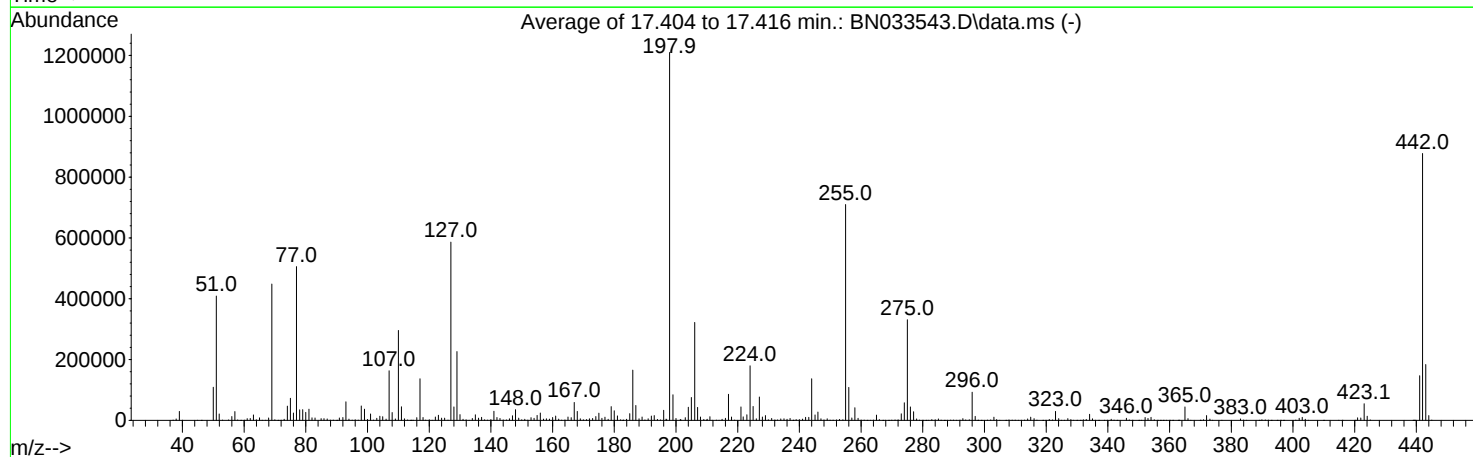


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082224\
Data File : BN033543.D
Acq On : 22 Aug 2024 09:12
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN081924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Aug 23 00:22:18 2024

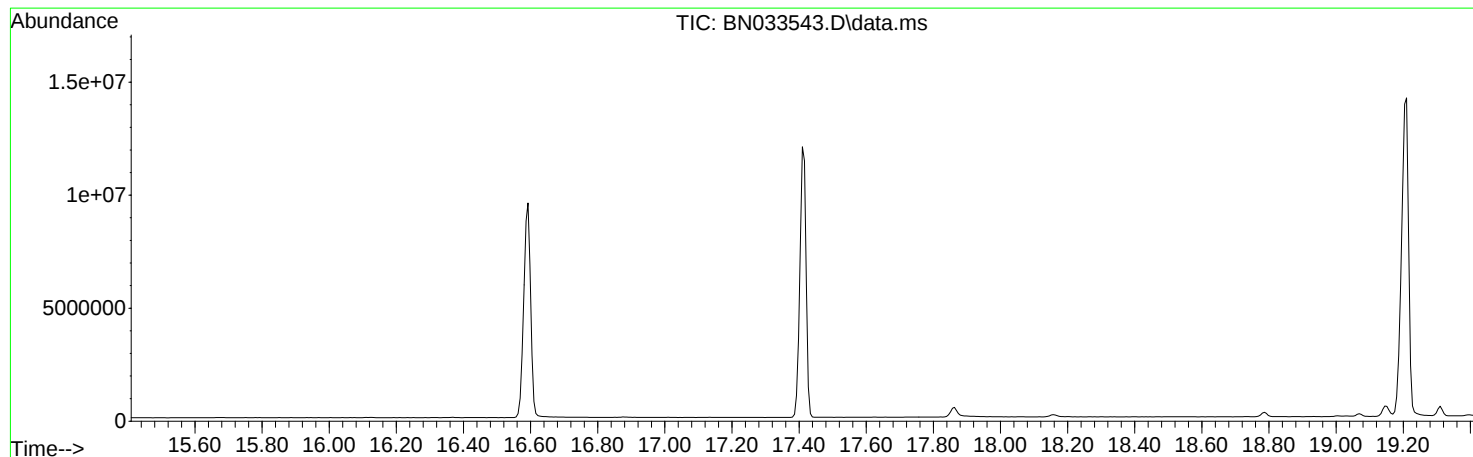




AutoFind: Scans 2451, 2452, 2453; Background Corrected with Scan 2444

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.8	408937	PASS
68	69	0.00	2	1.7	7689	PASS
69	198	0.00	100	37.0	448106	PASS
70	69	0.00	2	0.4	2010	PASS
127	198	10	80	48.5	586368	PASS
197	198	0.00	2	0.3	4108	PASS
198	198	100	100	100.0	1209749	PASS
199	198	5	9	7.0	84115	PASS
275	198	10	60	27.3	330795	PASS
365	198	1	100	3.7	44160	PASS
441	198	0.01	100	12.1	146845	PASS
442	442	50	100	100.0	877653	PASS
443	442	15	24	20.9	183427	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082224\
Data File : BN033543.D
Acq On : 22 Aug 2024 09:12
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 23 07:43:02 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 23 07:42:58 2024
Response via : Initial Calibration

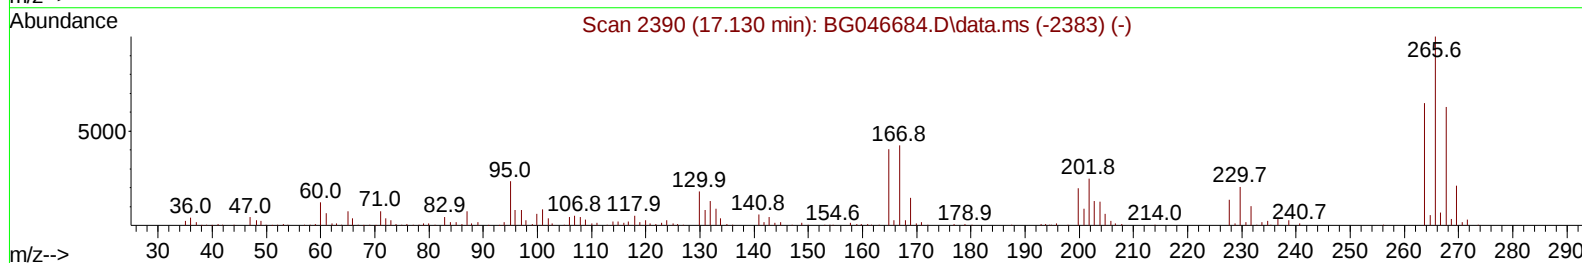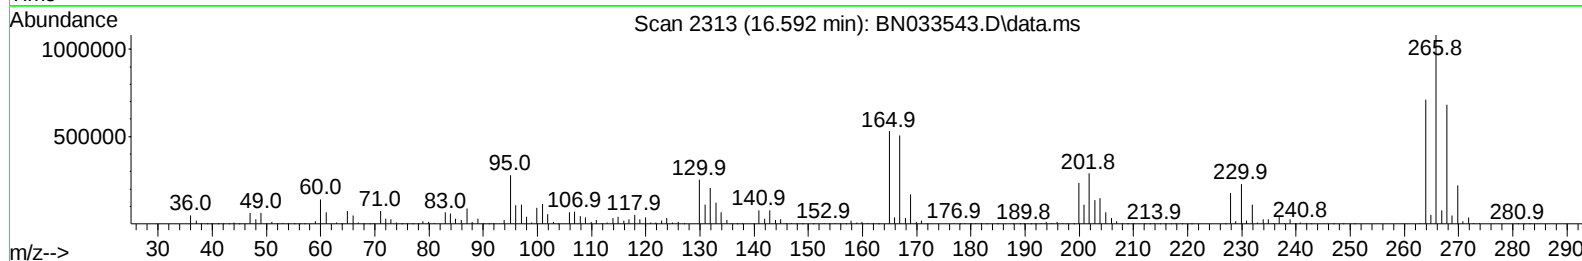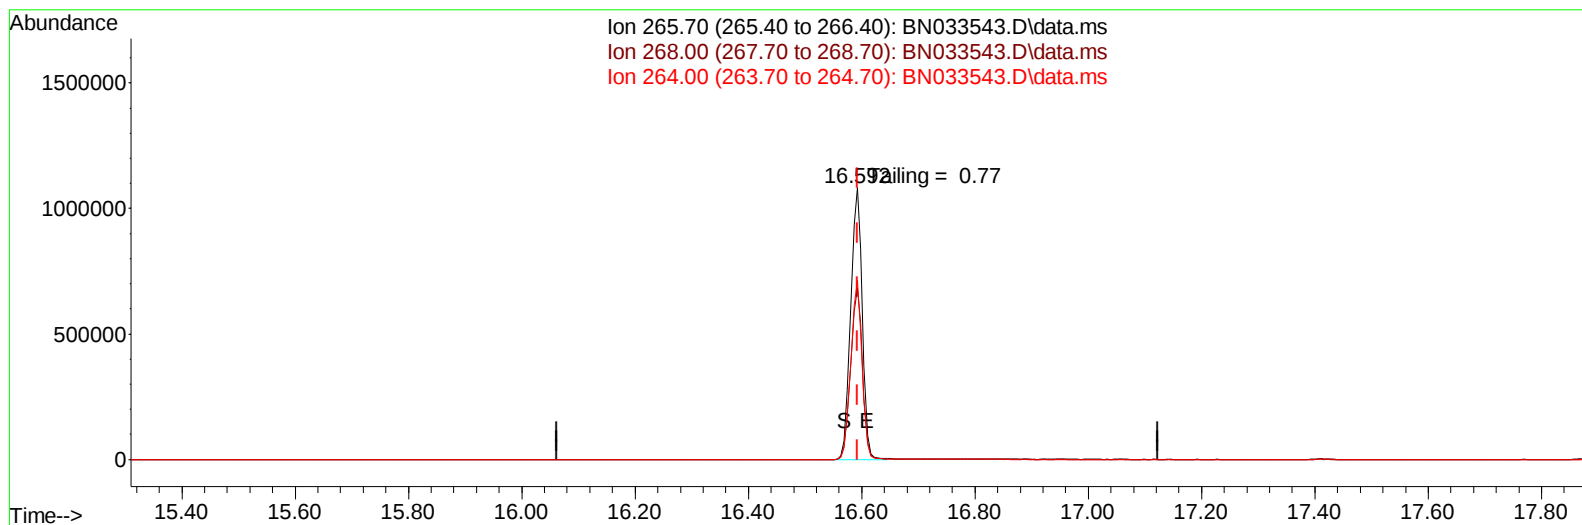

TIC: BN033543.D\data.ms

(70) Pentachlorophenol (C)

16.592min (0.000) 240843.19 ng




response 1551753

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.04
264.00	61.60	65.84
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082224\
Data File : BN033543.D
Acq On : 22 Aug 2024 09:12
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 23 07:43:02 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 23 07:42:58 2024
Response via : Initial Calibration

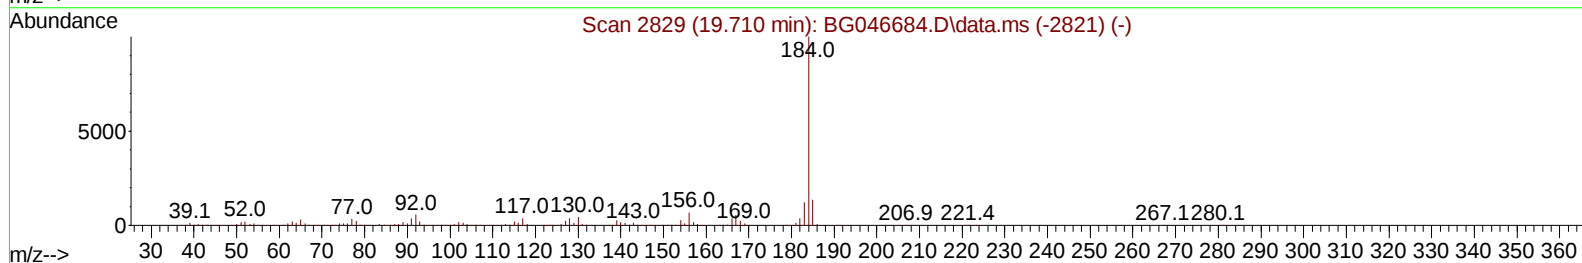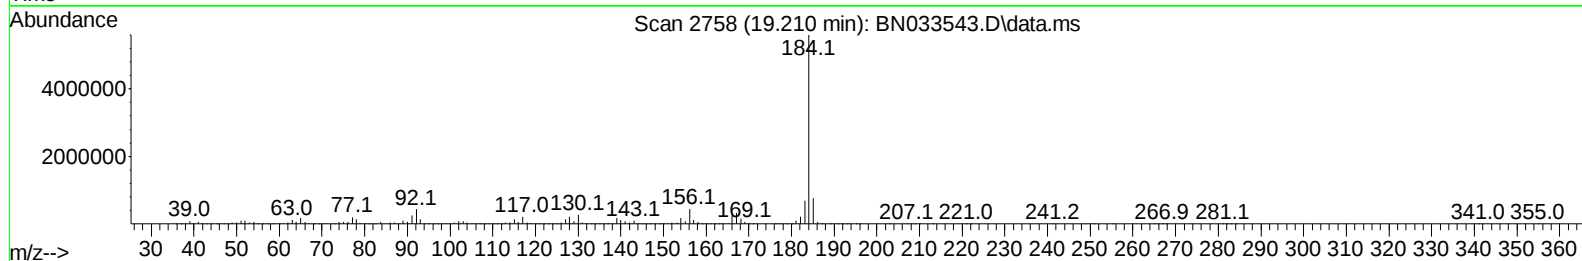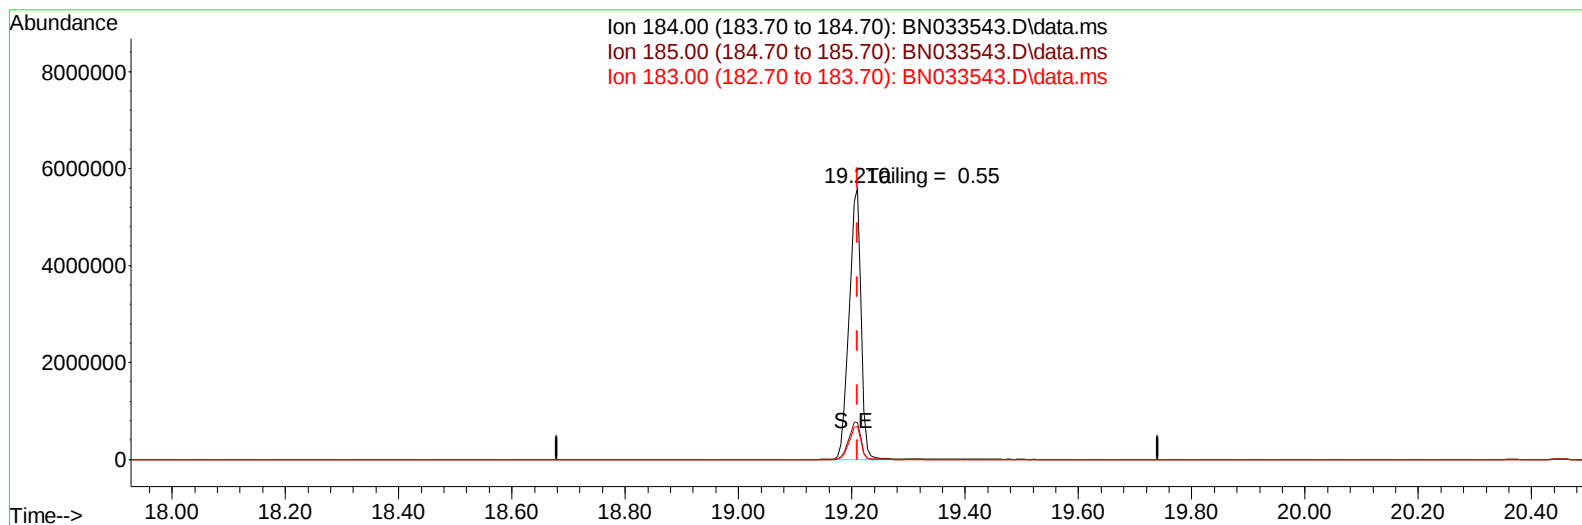

TIC: BN033543.D\data.ms

(77) Benzidine

19.210min (0.000) 4565.62 ng

response 8235503

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.70
183.00	13.20	12.11
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/22/2024	BNA_N	<u>BN033543.D</u>
Compound Name	Response	Retention Time
DDT	4014888	20.451
DDD	72062	20.057
DDE	1341	19.492
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
73403	4088291	1.80

Instrument :
BNA_N
ClientSampleId :
DFTPP