


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082324\
Data File : BN033598.D
Acq On : 23 Aug 2024 20:51
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN081924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Aug 23 00:22:18 2024

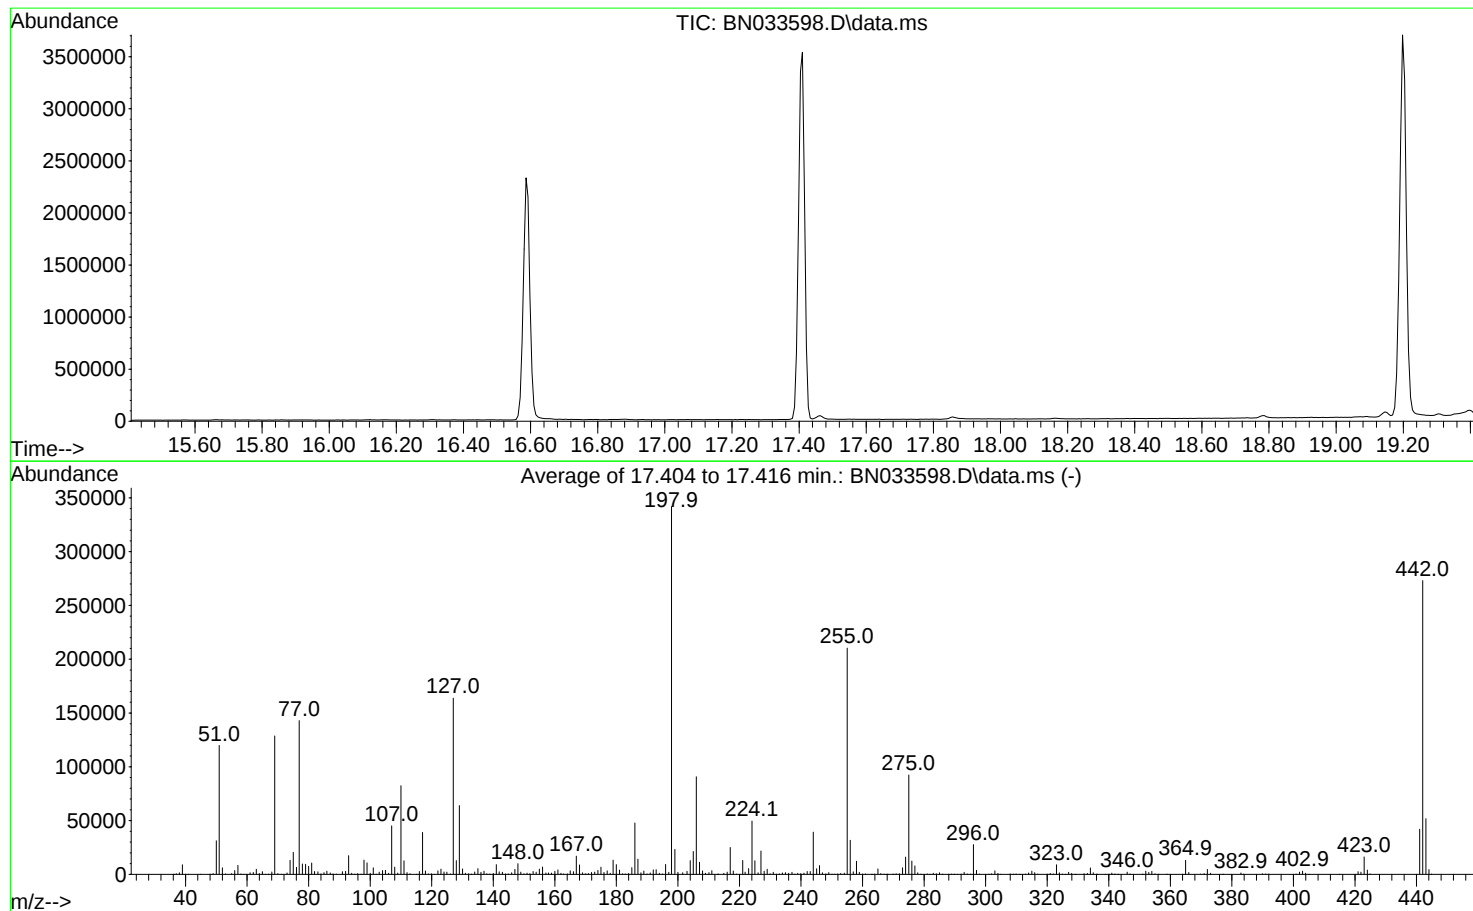

AutoFind: Scans 2451, 2452, 2453; Background Corrected with Scan 2444

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.1	119878	PASS
68	69	0.00	2	1.7	2196	PASS
69	198	0.00	100	37.6	128634	PASS
70	69	0.00	2	0.6	771	PASS
127	198	10	80	47.9	163808	PASS
197	198	0.00	2	0.6	1988	PASS
198	198	100	100	100.0	341952	PASS
199	198	5	9	6.8	23268	PASS
275	198	10	60	27.0	92328	PASS
365	198	1	100	3.8	13090	PASS
441	198	0.01	100	12.3	41963	PASS
442	442	50	100	100.0	273045	PASS
443	442	15	24	18.9	51704	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/23/2024	BNA_N	<u>BN033598.D</u>
Compound Name	Response	Retention Time
DDT	316046	20.445
DDD	482833	20.004
DDE	703	19.492
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
483536	799582	60.47

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082324\
Data File : BN033598.D
Acq On : 23 Aug 2024 20:51
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 24 06:45:58 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Aug 24 06:44:36 2024
Response via : Initial Calibration

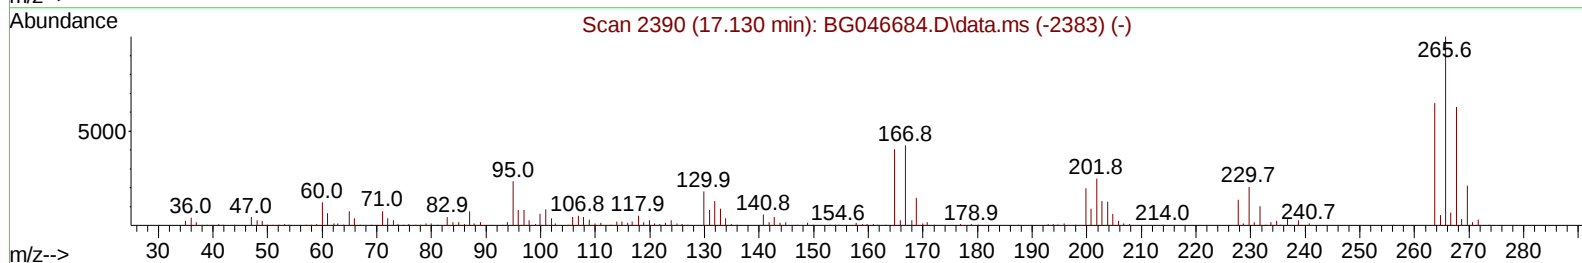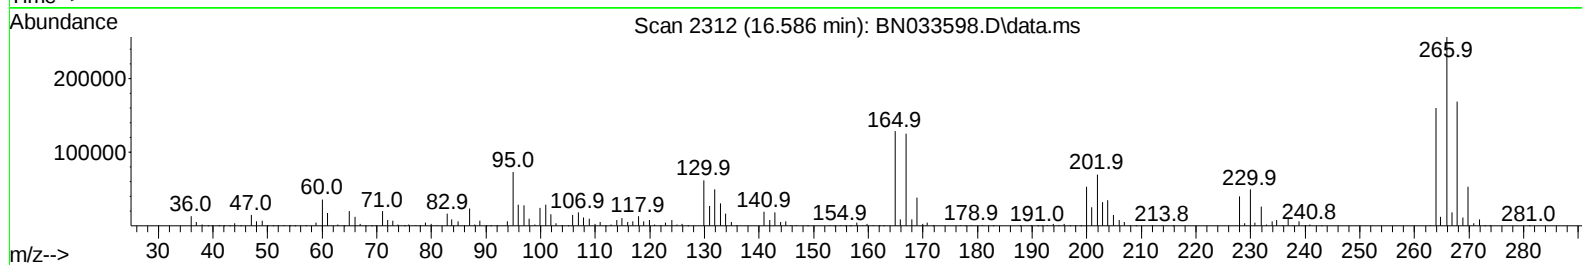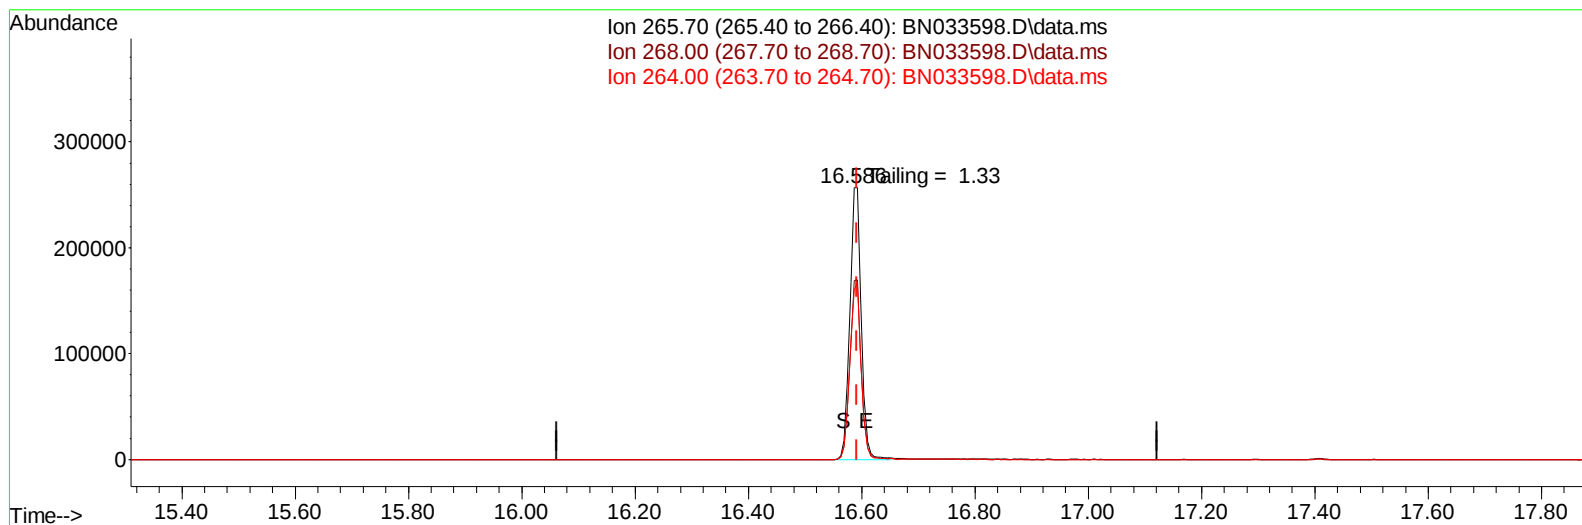

TIC: BN033598.D\data.ms

(70) Pentachlorophenol (C)

16.586min (-0.006) 229085.58 ng




response 361359

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.92
264.00	61.60	62.48
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082324\
Data File : BN033598.D
Acq On : 23 Aug 2024 20:51
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 24 06:45:58 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Aug 24 06:44:36 2024
Response via : Initial Calibration

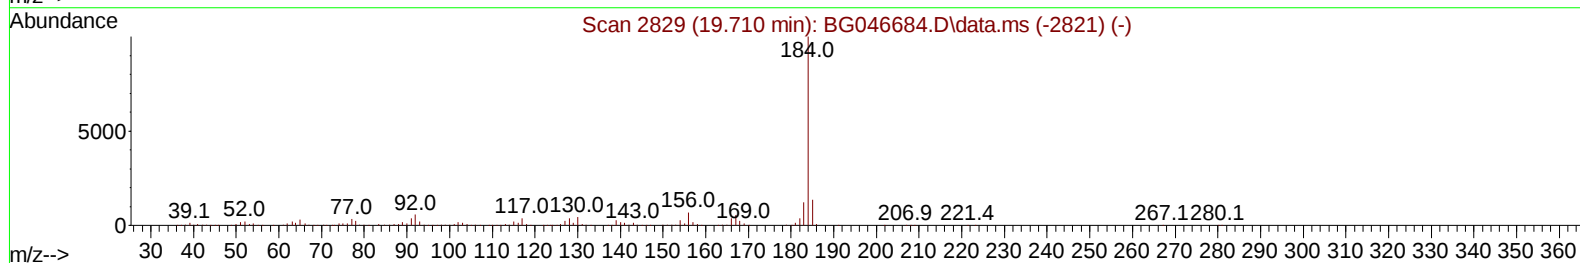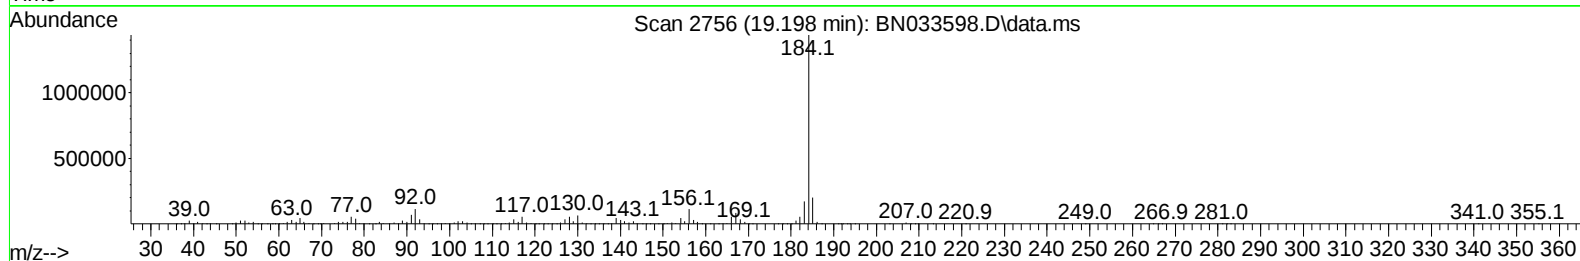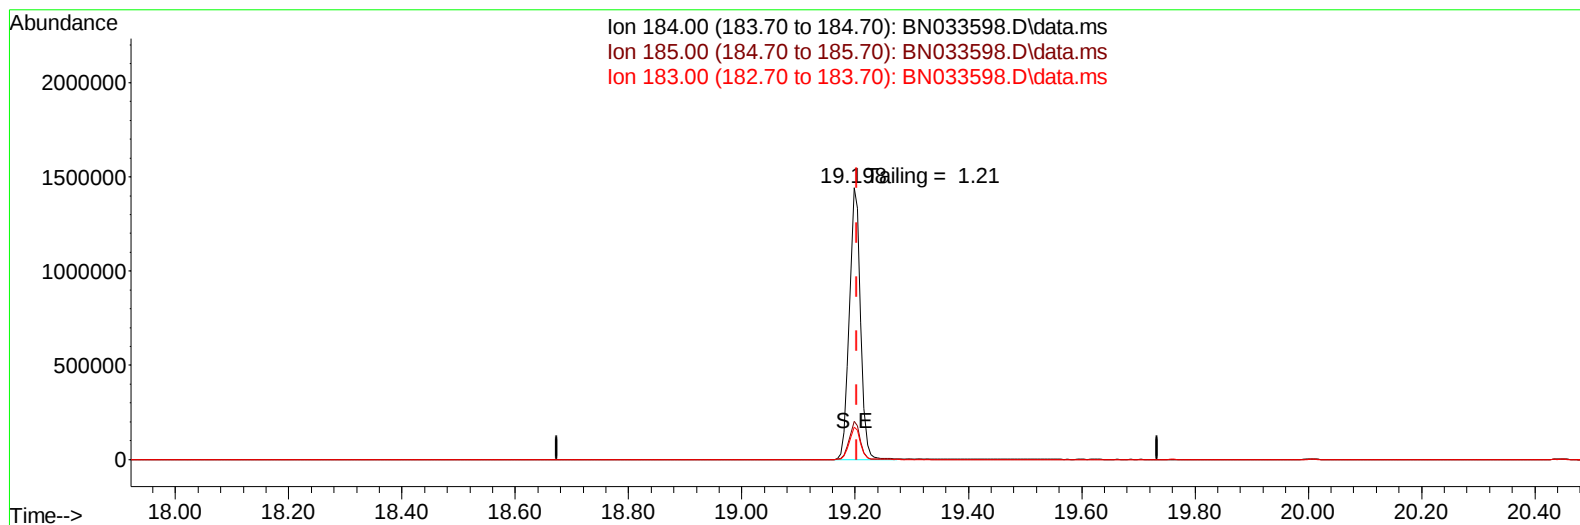

TIC: BN033598.D\data.ms

(77) Benzidine

19.198min (-0.006) 14681.39 ng

response 1986736

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.97
183.00	13.20	11.90
0.00	0.00	0.00