

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082422\
 Data File : BN021368.D
 Acq On : 25 Aug 2022 12:14
 Operator : CG/JU
 Sample : N4245-16
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 RE126D3-20220817

Quant Time: Aug 25 16:23:32 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN082422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 25 06:55:06 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.083	152	3139	0.400	ng	0.00
7) Naphthalene-d8	10.920	136	9574	0.400	ng	0.00
13) Acenaphthene-d10	14.739	164	5176	0.400	ng	0.00
19) Phenanthrene-d10	17.490	188	10834	0.400	ng	0.00
29) Chrysene-d12	21.682	240	8589	0.400	ng	0.00
35) Perylene-d12	24.206	264	6913	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.606	112	599	0.071	ng	0.00
5) Phenol-d6	7.231	99	411	0.039	ng	0.00
8) Nitrobenzene-d5	9.254	82	1719	0.237	ng	0.00
11) 2-Methylnaphthalene-d10	12.501	152	4431	0.274	ng	0.00
14) 2,4,6-Tribromophenol	16.229	330	490	0.207	ng	0.00
15) 2-Fluorobiphenyl	13.371	172	8596	0.371	ng	0.00
27) Fluoranthene-d10	19.514	212	9624	0.297	ng	0.00
31) Terphenyl-d14	20.106	244	7294	0.402	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.411	88	550	0.126	ng	Qvalue # 88
20) 4,6-Dinitro-2-methylph...	15.573	198	3	0.211	ng	94
34) Bis(2-ethylhexyl)phtha...	21.575	149	1020	0.065	ng	# 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082422\
Data File : BN021368.D
Acq On : 25 Aug 2022 12:14
Operator : CG/JU
Sample : N4245-16
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
RE126D3-20220817


Quant Time: Aug 25 16:23:32 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN082422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 25 06:55:06 2022
Response via : Initial Calibration

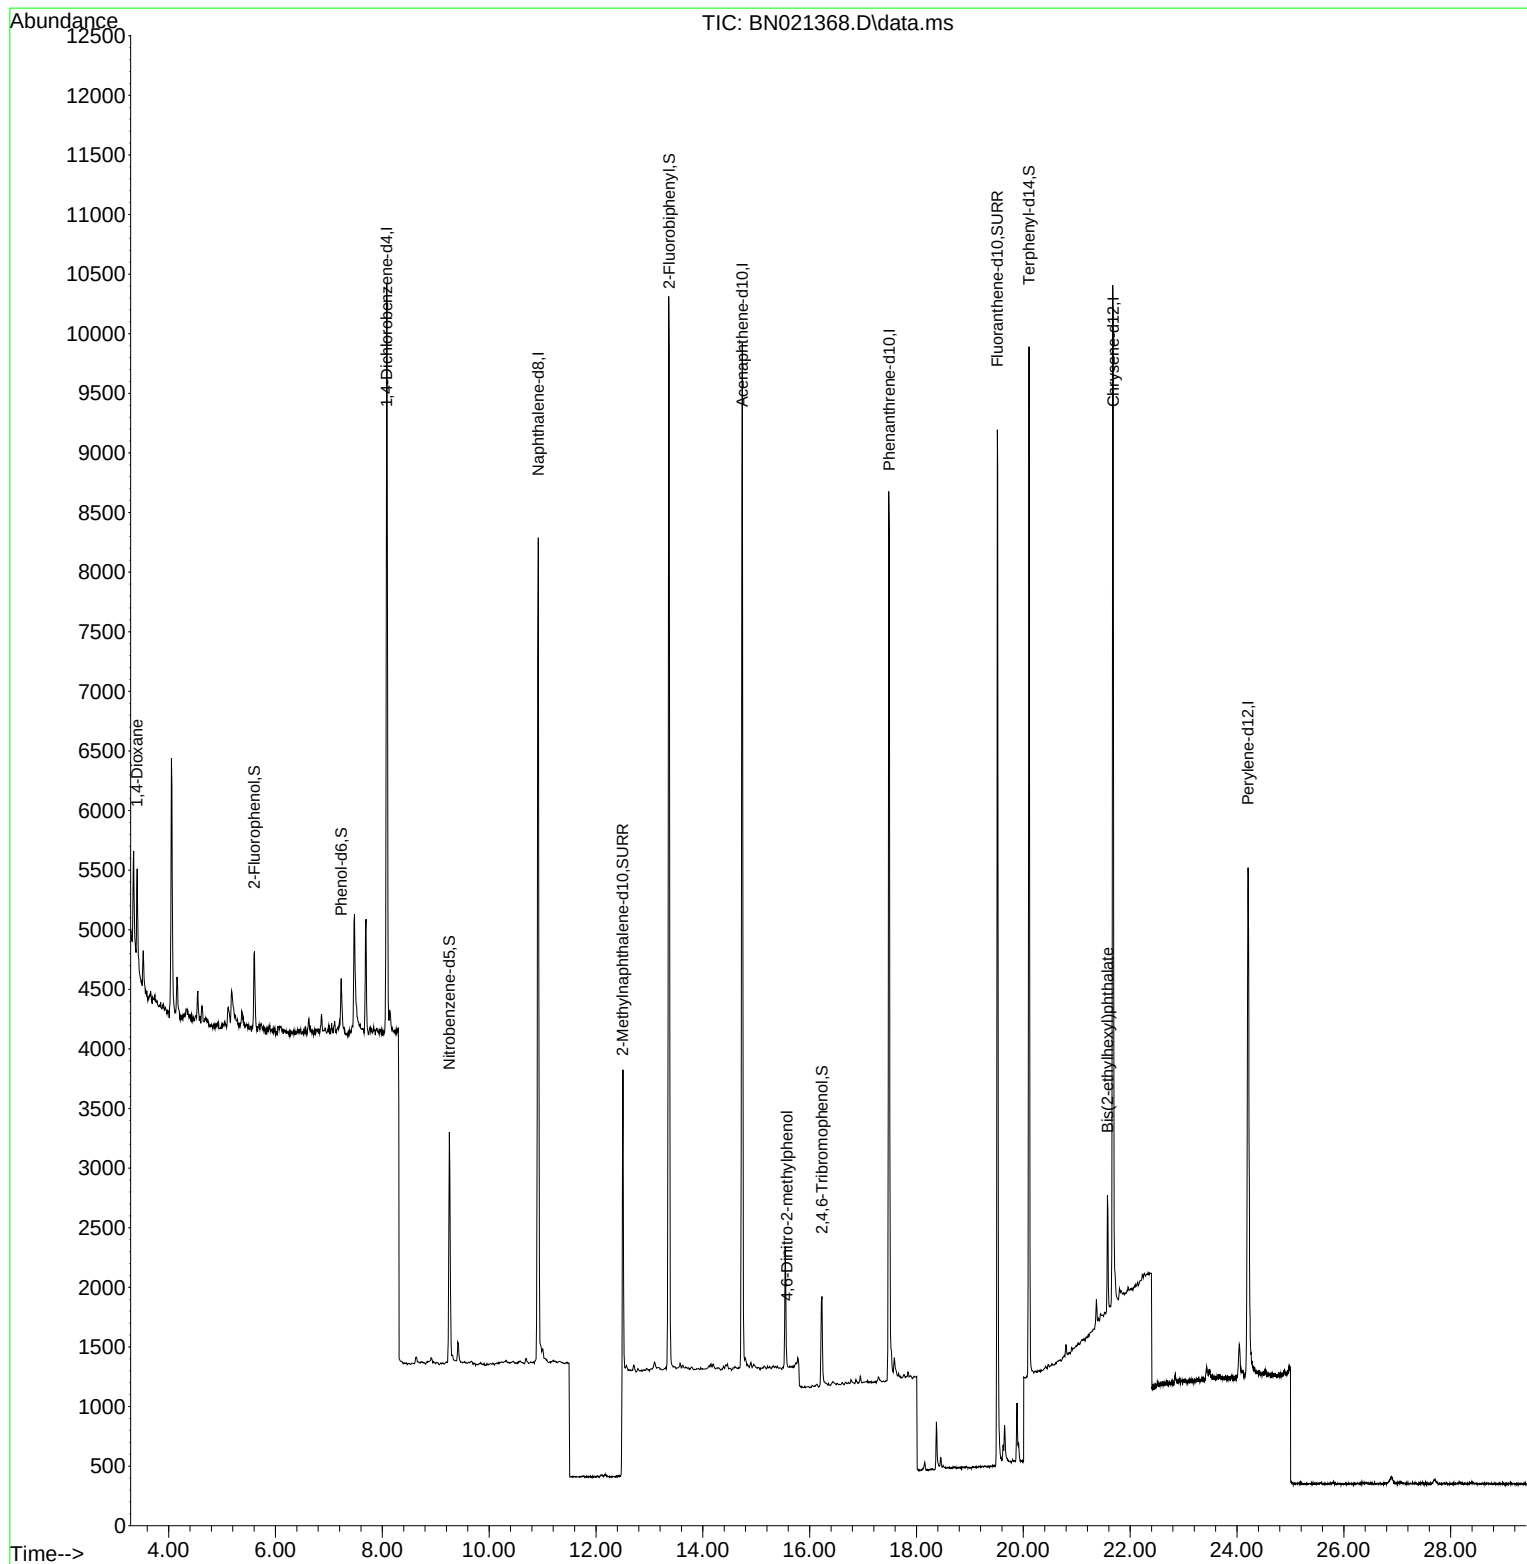



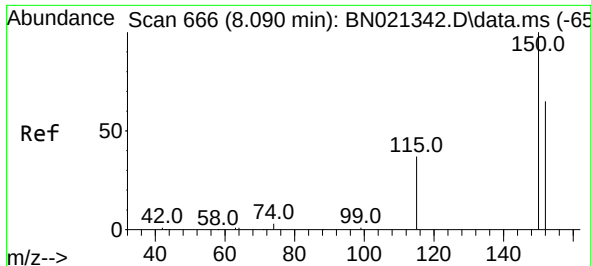


#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 8.083 min Scan# 6
 Delta R.T. -0.007 min
 Lab File: BN021368.D
 Acq: 25 Aug 2022 12:14

Instrument :
 BNA_N
 ClientSampleId :
 RE126D3-20220817



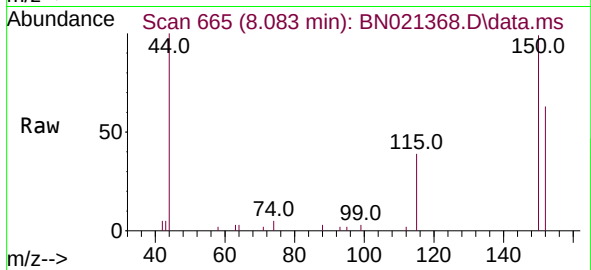



Tgt Ion:152 Resp: 3139
 Ion Ratio Lower Upper
 152 100
 150 156.0 121.4 182.0
 115 60.8 48.6 72.8

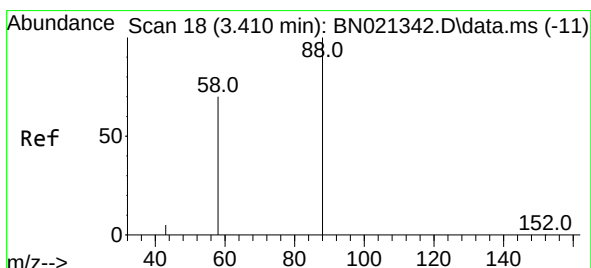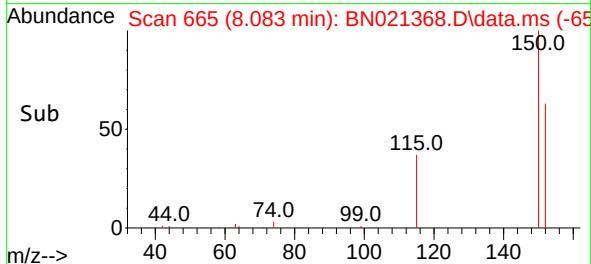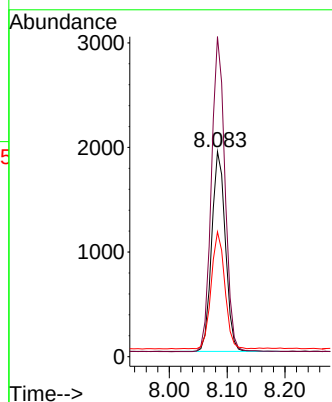

#2
 1,4-Dioxane
 Concen: 0.126 ng
 RT: 3.411 min Scan# 18
 Delta R.T. 0.000 min
 Lab File: BN021368.D
 Acq: 25 Aug 2022 12:14

Tgt Ion: 88 Resp: 550
 Ion Ratio Lower Upper
 88 100
 43 28.9 35.8 53.8#
 58 74.5 57.1 85.7

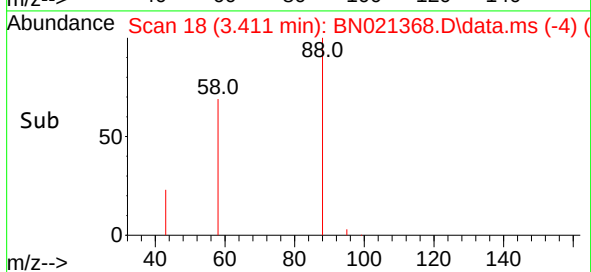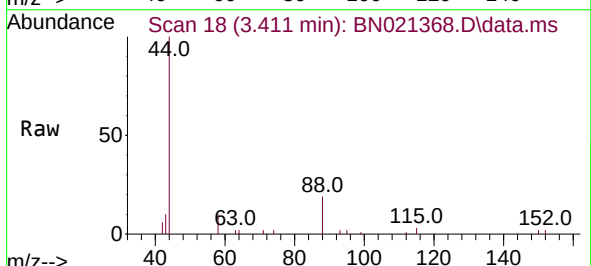

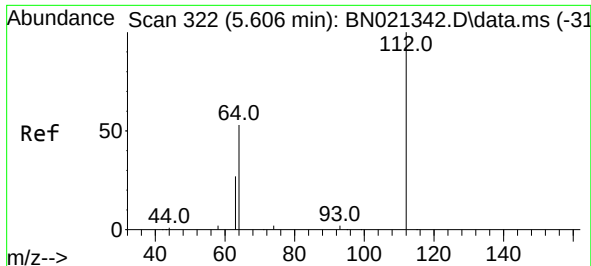

#4

2-Fluorophenol

Concen: 0.071 ng

RT: 5.606 min Scan# 31

Delta R.T. 0.000 min

Lab File: BN021368.D


Acq: 25 Aug 2022 12:14

Instrument :




BNA_N

ClientSampleId :

RE126D3-20220817

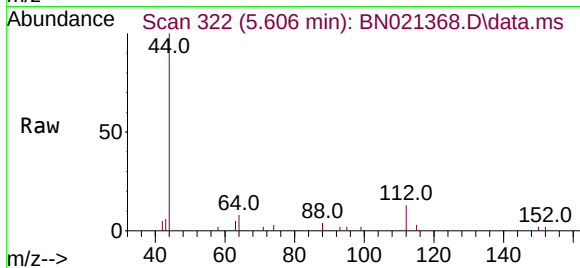

Tgt Ion:	112	Resp:	599
Ion	Ratio	Lower	Upper
112	100		
64	55.3	43.5	65.3
63	28.4	22.6	34.0

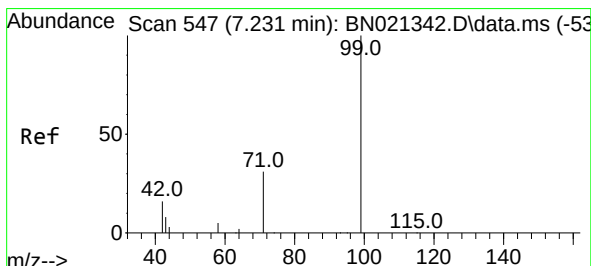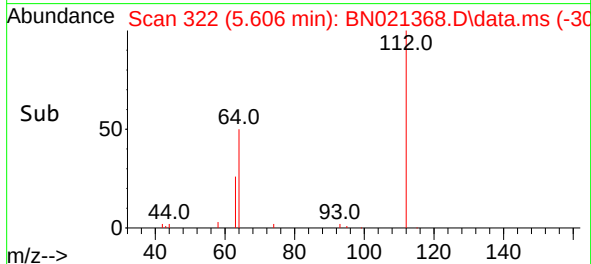

#5

Phenol-d6

Concen: 0.039 ng




RT: 7.231 min Scan# 547


Delta R.T. 0.000 min

Lab File: BN021368.D

Acq: 25 Aug 2022 12:14

Tgt Ion:	99	Resp:	411
Ion	Ratio	Lower	Upper
99	100		
42	23.6	15.5	23.3#
71	46.0	24.2	36.2#


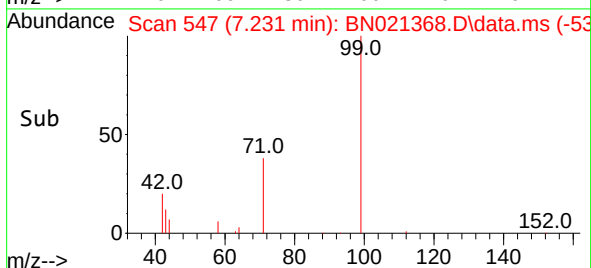
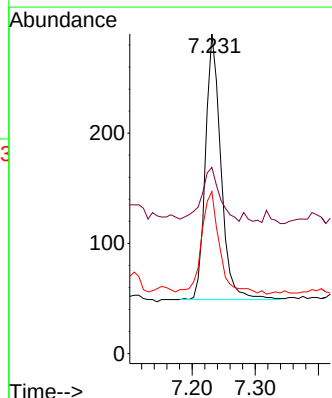
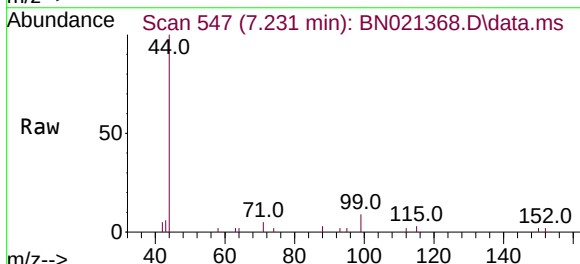


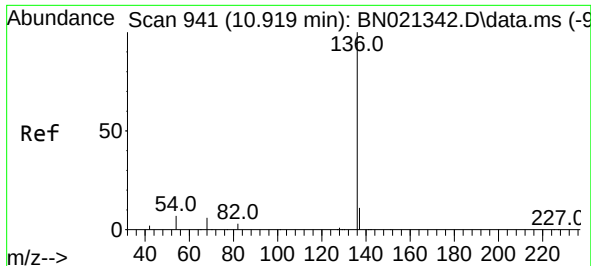

#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.920 min Scan# 941
Delta R.T. 0.000 min
Lab File: BN021368.D
Acq: 25 Aug 2022 12:14




Instrument :
BNA_N
ClientSampleId :
RE126D3-20220817


Tgt Ion:	136	Resp:	9574
Ion	Ratio	Lower	Upper
136	100		
137	11.7	9.3	13.9
54	7.1	6.9	10.3
68	6.2	6.1	9.1

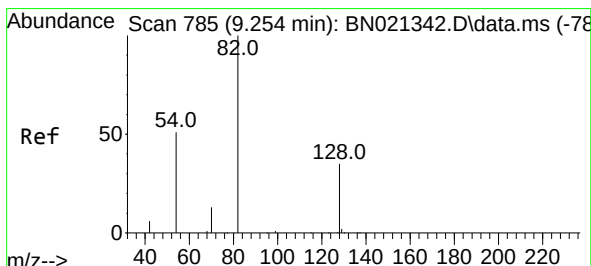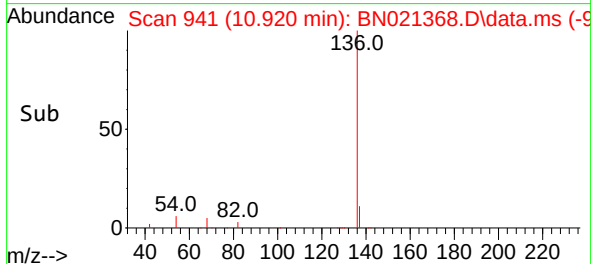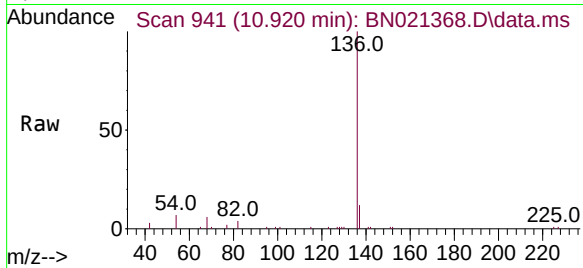

#8
Nitrobenzene-d5
Concen: 0.237 ng
RT: 9.254 min Scan# 785
Delta R.T. 0.000 min
Lab File: BN021368.D
Acq: 25 Aug 2022 12:14

Tgt Ion:	82	Resp:	1719
Ion	Ratio	Lower	Upper
82	100		
128	41.5	30.9	46.3
54	52.3	42.7	64.1


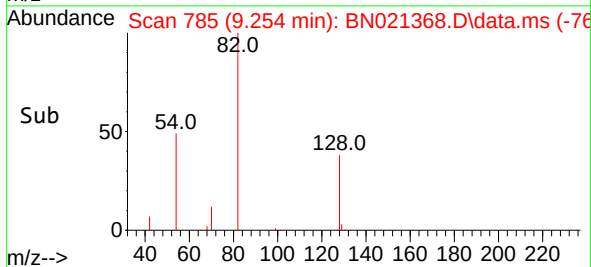

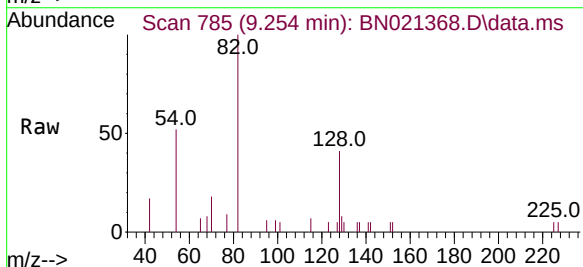


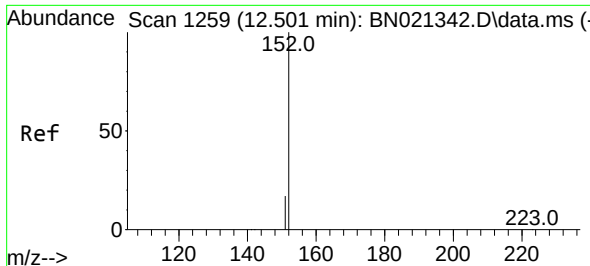

#11
2-Methylnaphthalene-d10
Concen: 0.274 ng
RT: 12.501 min Scan# 1259
Delta R.T. 0.000 min
Lab File: BN021368.D
Acq: 25 Aug 2022 12:14




Instrument :
BNA_N
ClientSampleId :
RE126D3-20220817


Tgt Ion:152 Resp: 4431
Ion Ratio Lower Upper
152 100
151 20.6 14.5 21.7

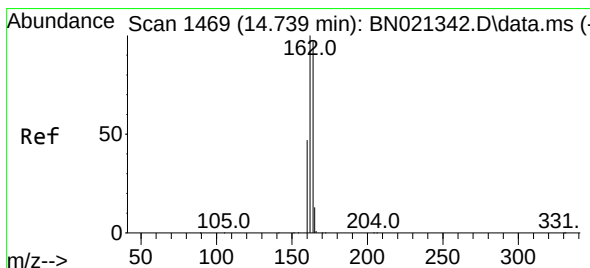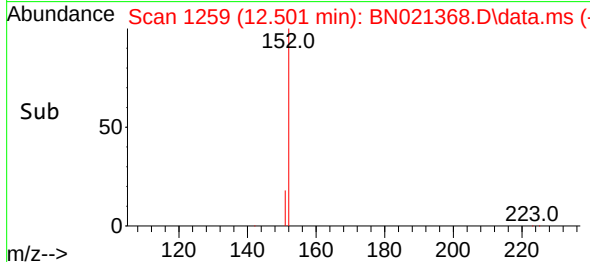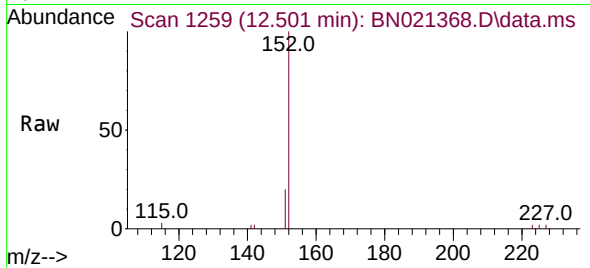

#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.739 min Scan# 1469
Delta R.T. 0.000 min
Lab File: BN021368.D
Acq: 25 Aug 2022 12:14

Tgt Ion:164 Resp: 5176
Ion Ratio Lower Upper
164 100
162 101.3 82.2 123.4
160 49.0 39.5 59.3


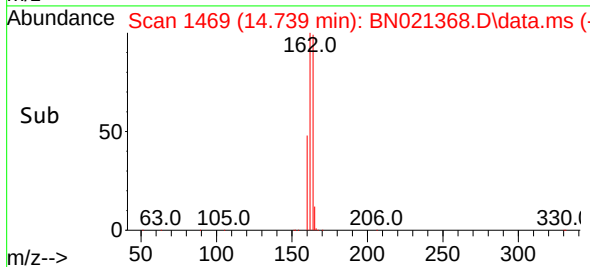

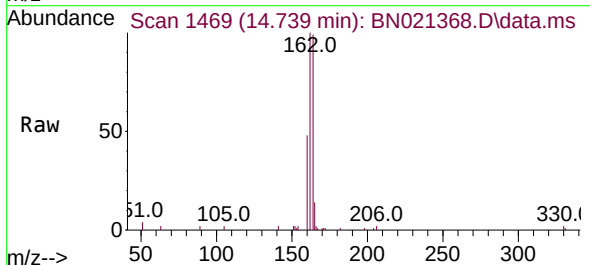


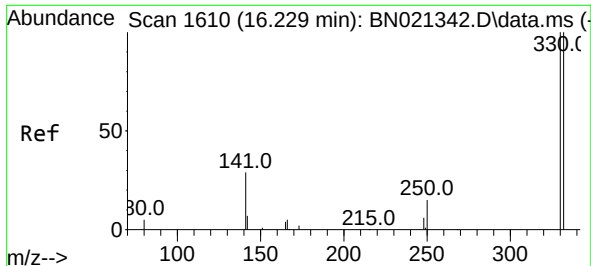

#14
 2,4,6-Tribromophenol
 Concen: 0.207 ng
 RT: 16.229 min Scan# 1610
 Delta R.T. 0.000 min
 Lab File: BN021368.D
 Acq: 25 Aug 2022 12:14




Instrument :
 BNA_N
 ClientSampleId :
 RE126D3-20220817


Tgt Ion:330 Resp: 490
 Ion Ratio Lower Upper
 330 100
 332 98.4 79.3 118.9
 141 47.8 37.1 55.7

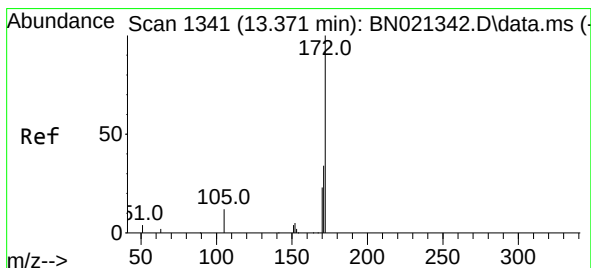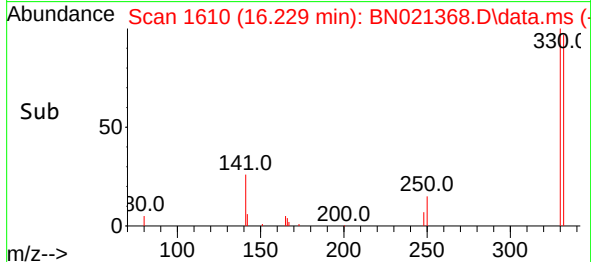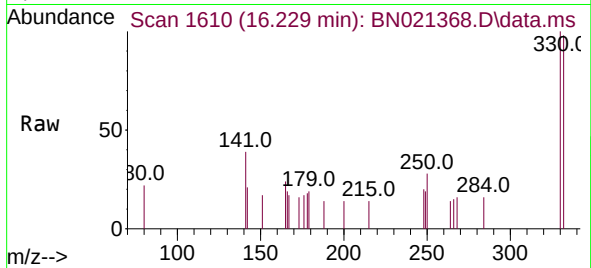

#15
 2-Fluorobiphenyl
 Concen: 0.371 ng
 RT: 13.371 min Scan# 1341
 Delta R.T. 0.000 min
 Lab File: BN021368.D
 Acq: 25 Aug 2022 12:14

Tgt Ion:172 Resp: 8596
 Ion Ratio Lower Upper
 172 100
 171 34.0 27.8 41.6
 170 23.0 18.6 28.0


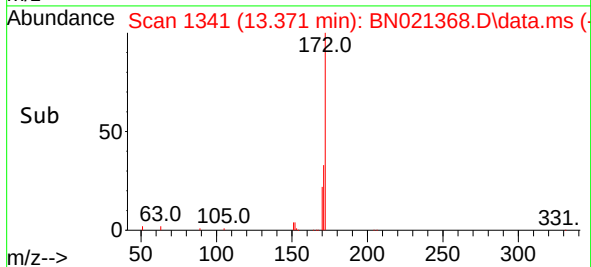

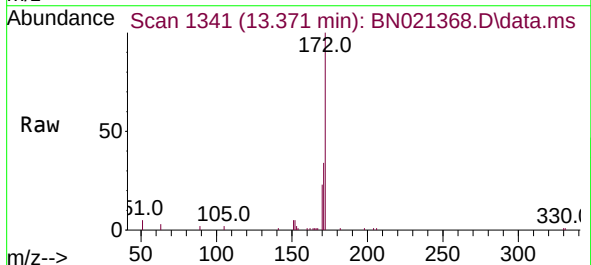


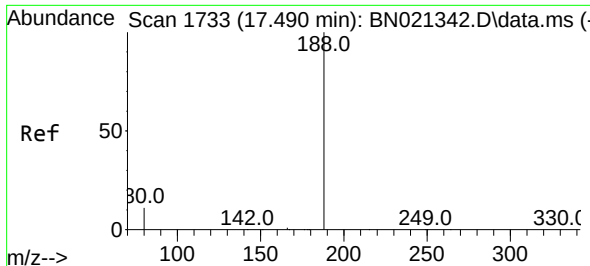

#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.490 min Scan# 11
Delta R.T. 0.000 min
Lab File: BN021368.D
Acq: 25 Aug 2022 12:14




Instrument :
BNA_N
ClientSampleId :
RE126D3-20220817


Tgt Ion:188 Resp: 10834
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 9.7 9.5 14.3

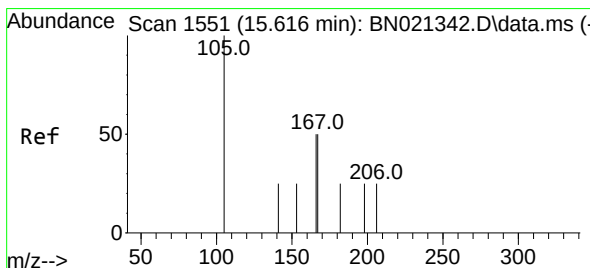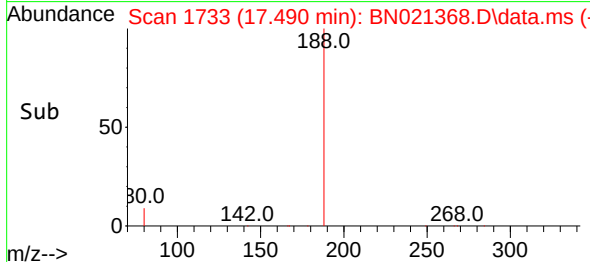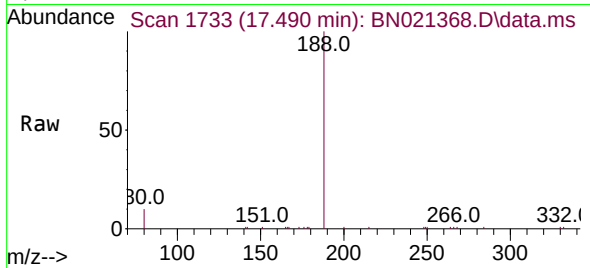

#20
4,6-Dinitro-2-methylphenol
Concen: 0.211 ng
RT: 15.573 min Scan# 1547
Delta R.T. -0.043 min
Lab File: BN021368.D
Acq: 25 Aug 2022 12:14

Tgt Ion:198 Resp: 3
Ion Ratio Lower Upper
198 100
182 102.2 86.6 130.0
77 0.0 0.0 0.0


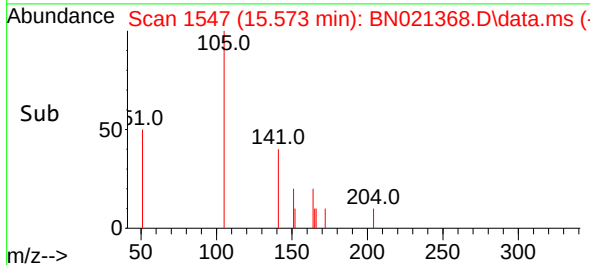

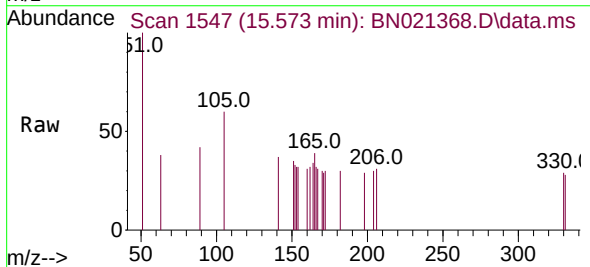


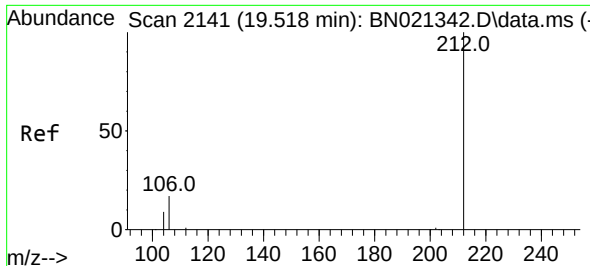

#27
Fluoranthene-d10
Concen: 0.297 ng
RT: 19.514 min Scan# 2141
Delta R.T. -0.004 min
Lab File: BN021368.D
Acq: 25 Aug 2022 12:14




Instrument :
BNA_N
ClientSampleId :
RE126D3-20220817


Tgt Ion:212 Resp: 9624
Ion Ratio Lower Upper
212 100
106 17.9 14.2 21.2
104 10.2 7.8 11.6

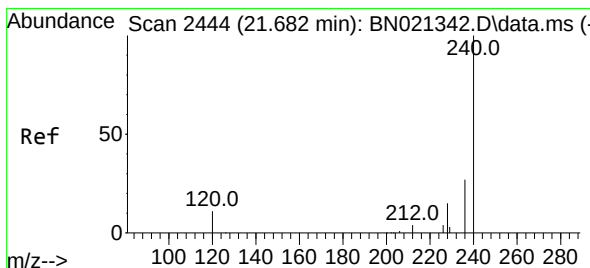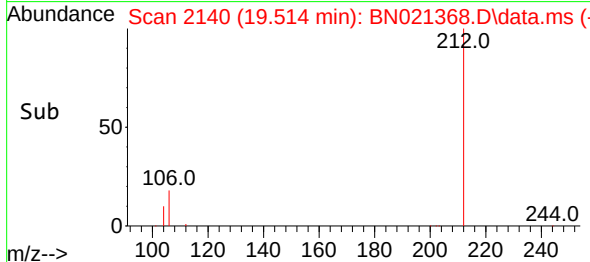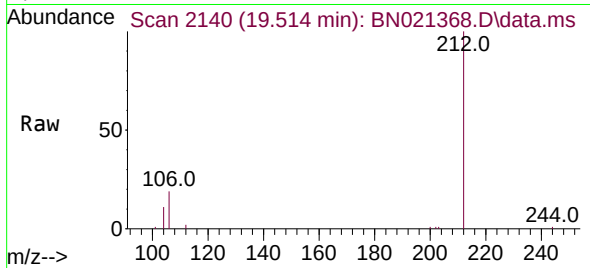

#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.682 min Scan# 2444
Delta R.T. 0.000 min
Lab File: BN021368.D
Acq: 25 Aug 2022 12:14

Tgt Ion:240 Resp: 8589
Ion Ratio Lower Upper
240 100
120 13.0 10.2 15.4
236 28.3 22.1 33.1

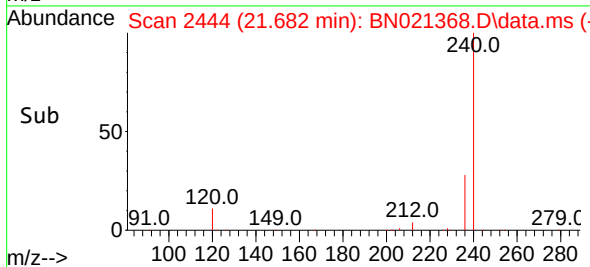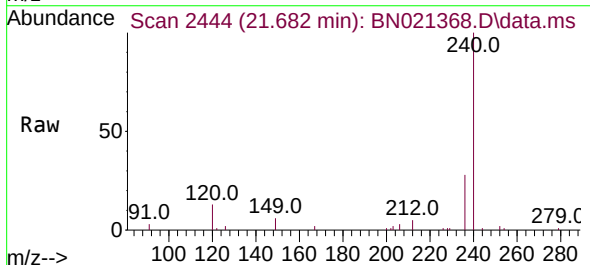

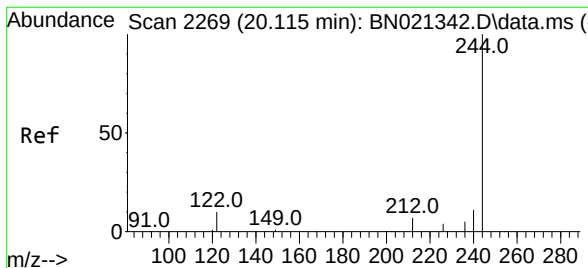

#31

Terphenyl-d14

Concen: 0.402 ng

RT: 20.106 min Scan# 21

Delta R.T. -0.009 min

Lab File: BN021368.D

Acq: 25 Aug 2022 12:14

Instrument :

BNA_N

ClientSampleId :

RE126D3-20220817





Tgt Ion:244 Resp: 7294

Ion Ratio Lower Upper

244 100

212 9.7 6.5 9.7

122 17.7 9.1 13.7#

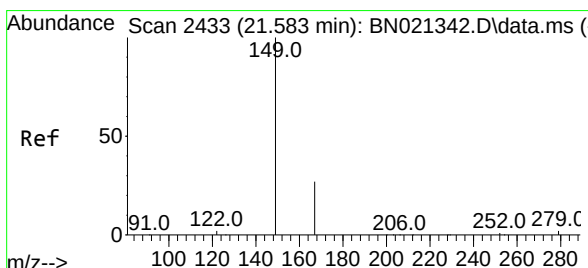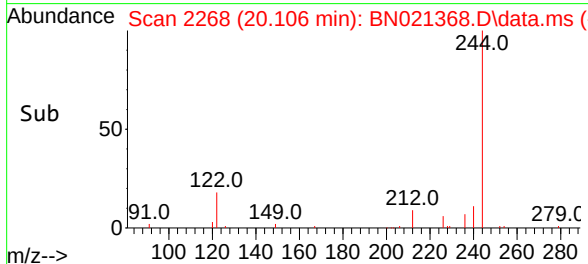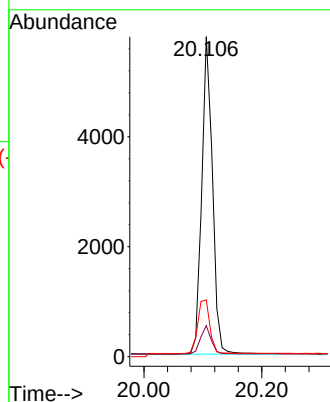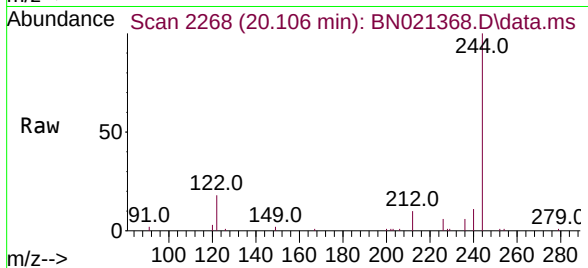

#34

Bis(2-ethylhexyl)phthalate

Concen: 0.065 ng

RT: 21.575 min Scan# 2432

Delta R.T. -0.009 min

Lab File: BN021368.D

Acq: 25 Aug 2022 12:14




Tgt Ion:149 Resp: 1020


Ion Ratio Lower Upper

149 100

167 26.6 21.4 32.0


279 4.6 2.2 3.2#

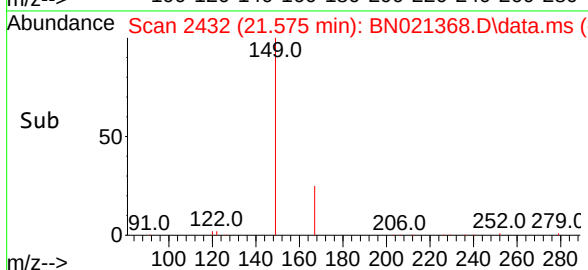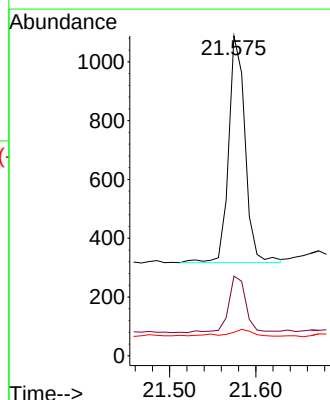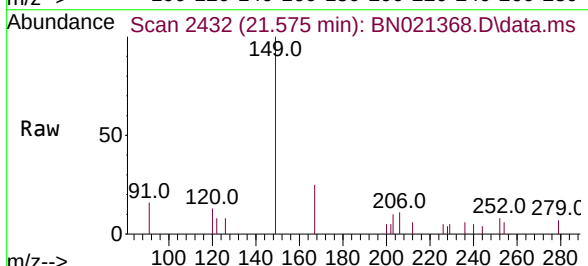

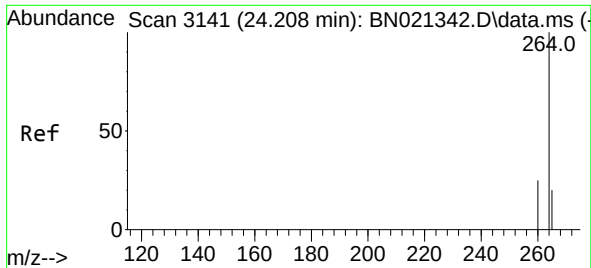

#35
 Perylene-d12
 Concen: 0.400 ng
 RT: 24.206 min Scan# 31
 Delta R.T. -0.003 min
 Lab File: BN021368.D
 Acq: 25 Aug 2022 12:14

Instrument :
 BNA_N
 ClientSampleId :
 RE126D3-20220817

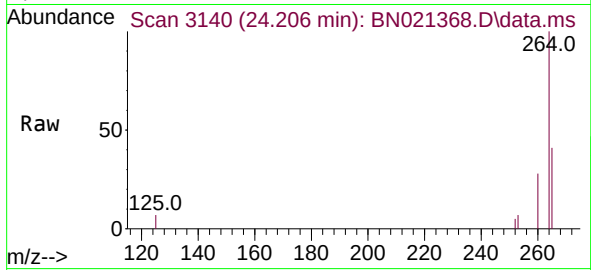

Tgt Ion:264 Resp: 6913

Ion	Ratio	Lower	Upper
264	100		
260	27.7	21.0	31.6
265	41.3	32.2	48.2

