
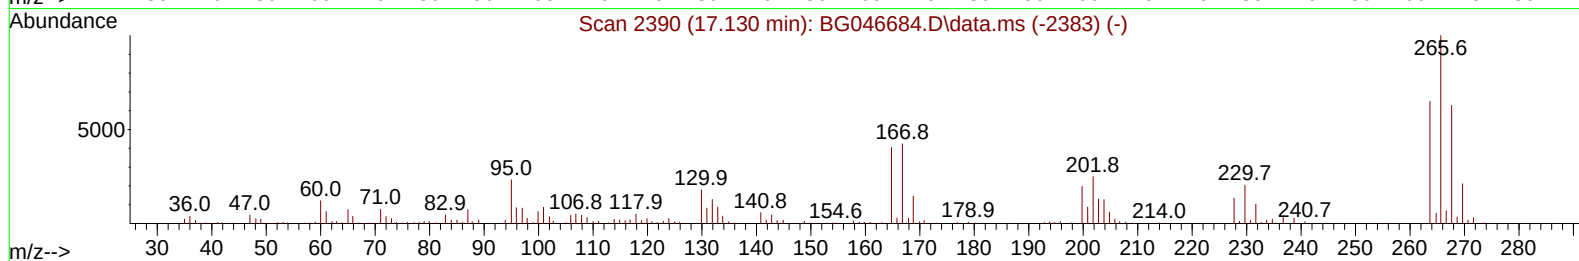
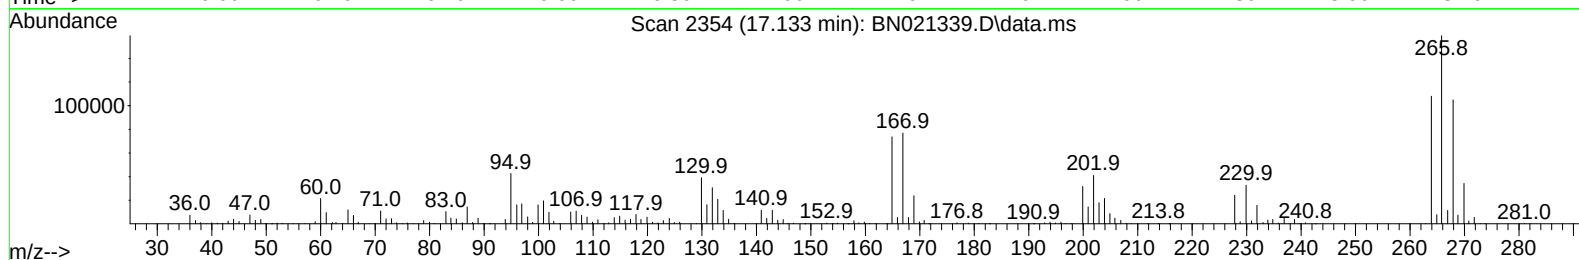


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082422\
Data File : BN021339.D
Acq On : 24 Aug 2022 15:55
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 25 08:22:01 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 25 08:21:54 2022
Response via : Initial Calibration

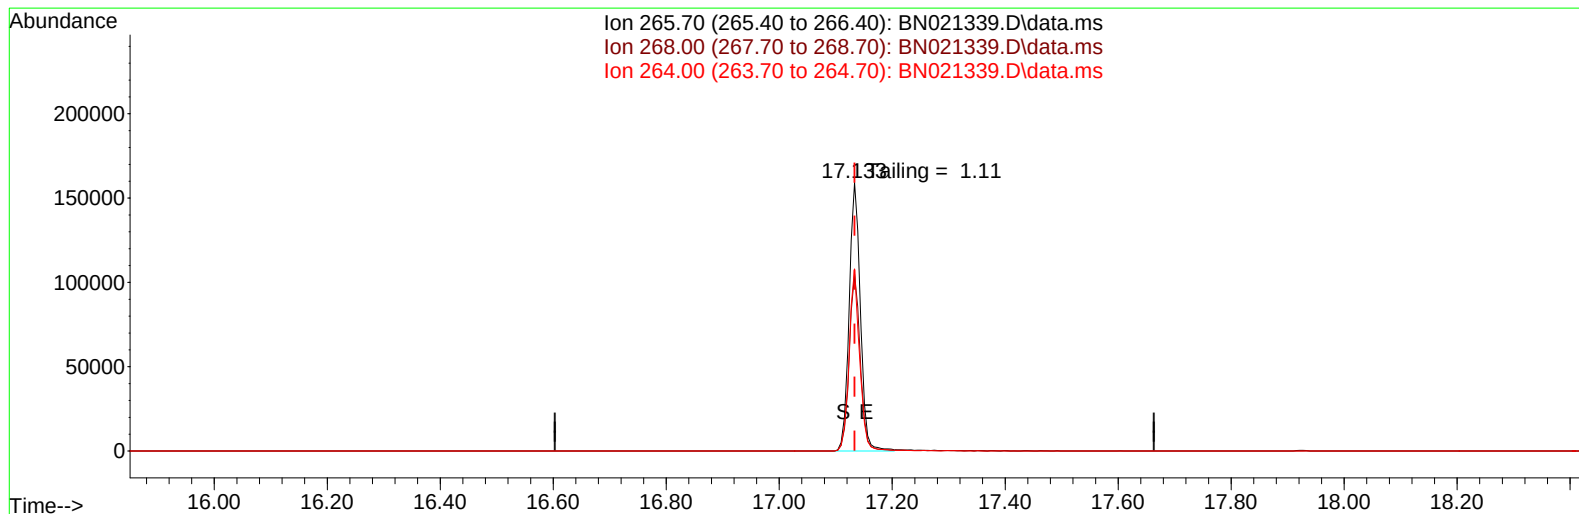

TIC: BN021339.D\data.ms

(70) Pentachlorophenol (C)




17.133min (0.000) 454958.94 ng

response 221365

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.93
264.00	61.60	67.85
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082422\
Data File : BN021339.D
Acq On : 24 Aug 2022 15:55
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 25 08:22:01 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 25 08:21:54 2022
Response via : Initial Calibration

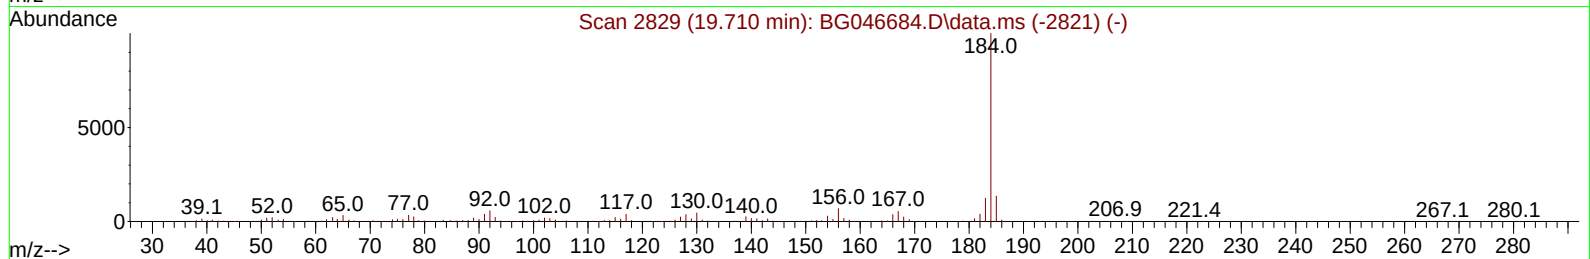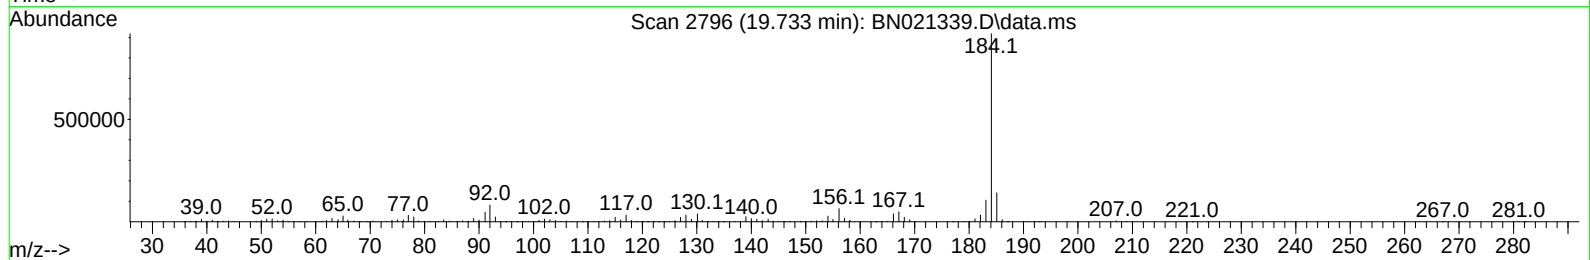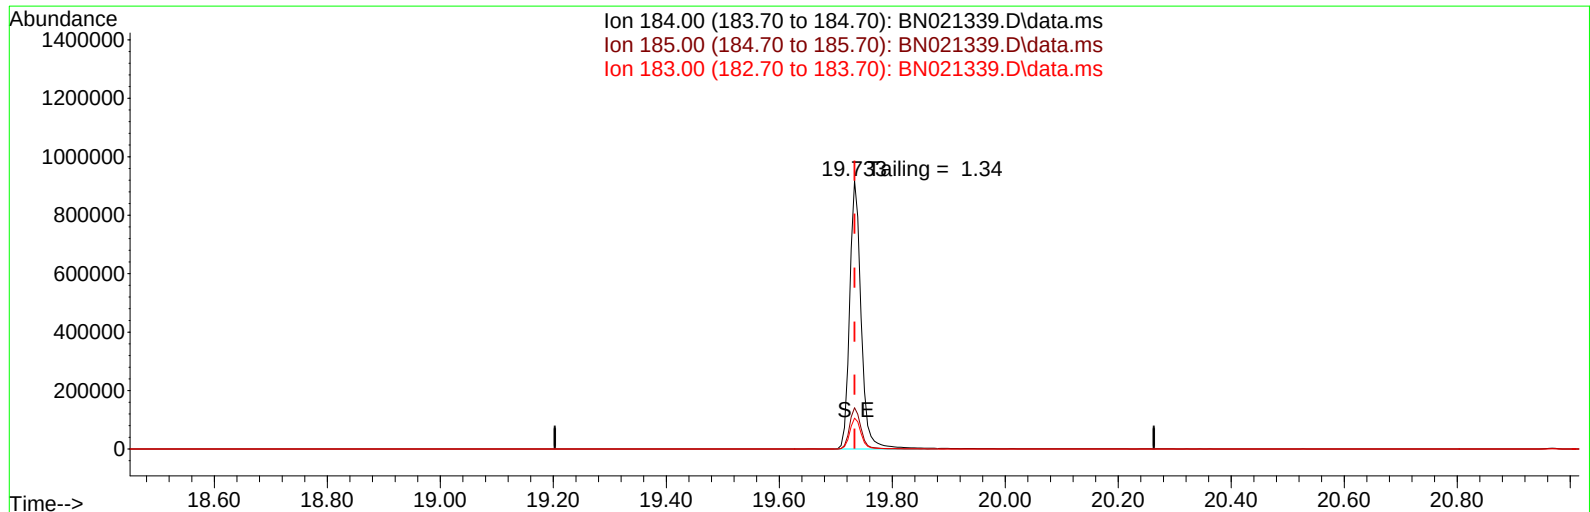

TIC: BN021339.D\data.ms

(77) Benzidine**19.733min (0.000) 52670.18 ng****response 1303733**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	15.42
183.00	13.20	11.53
0.00	0.00	0.00