
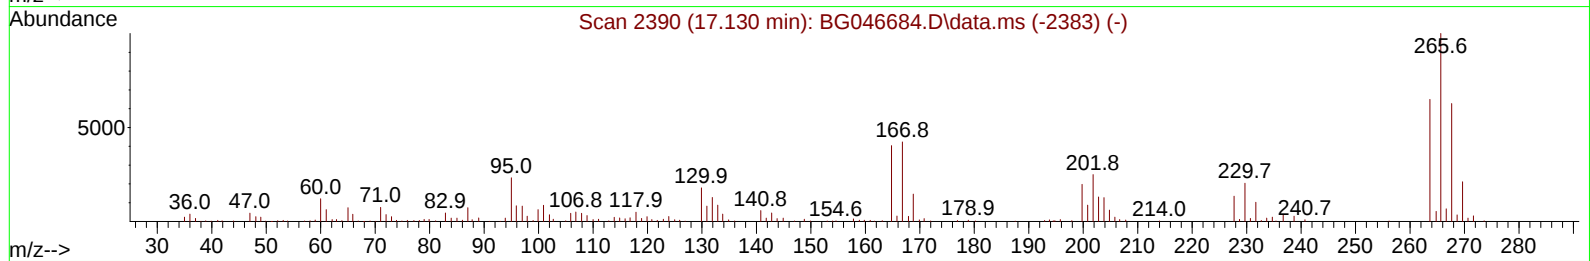
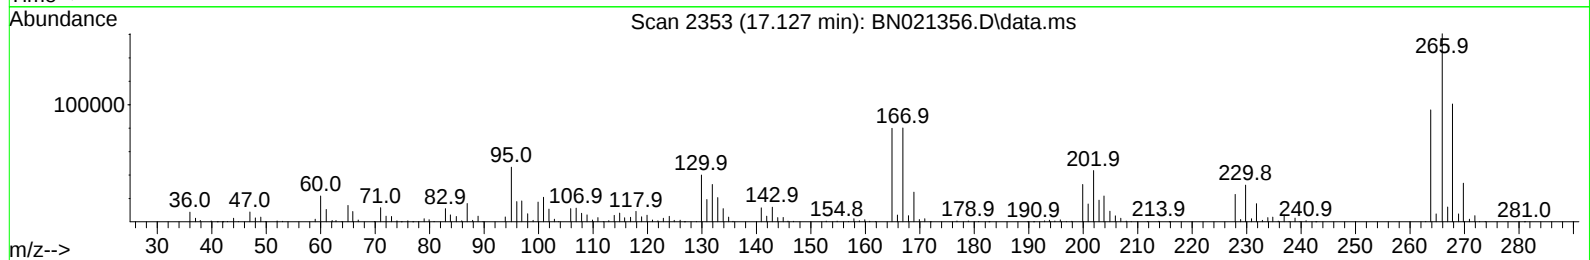


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082422\
Data File : BN021356.D
Acq On : 25 Aug 2022 04:41
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 25 08:23:30 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 25 08:21:54 2022
Response via : Initial Calibration

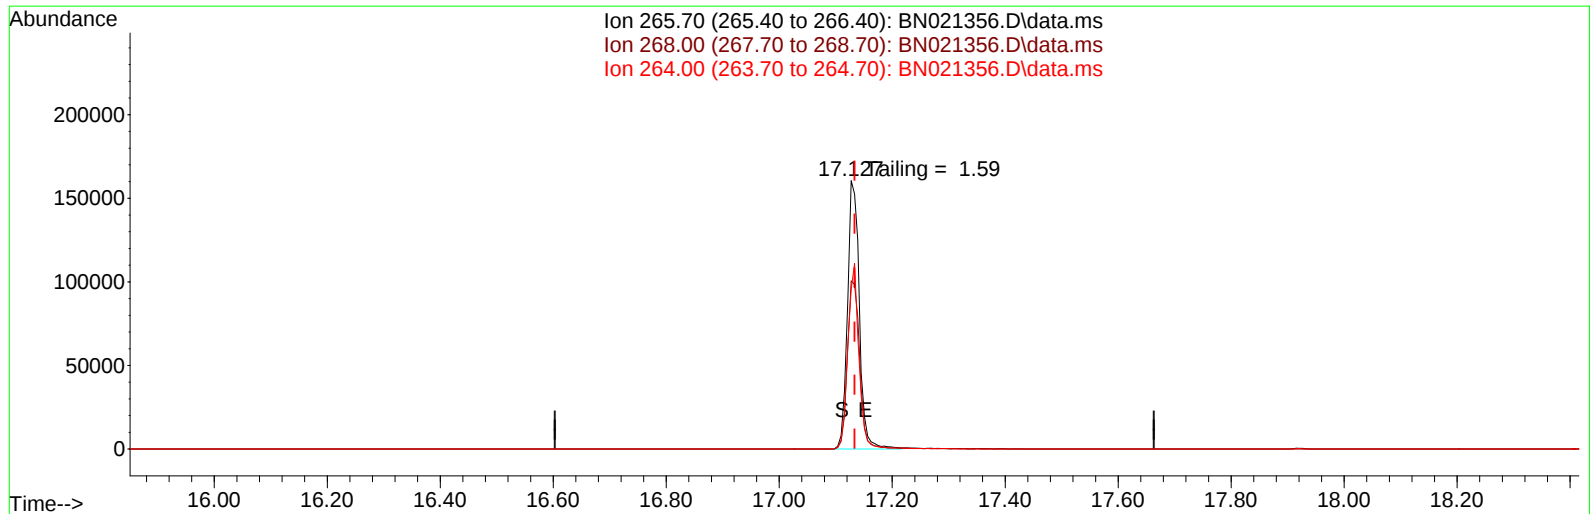

TIC: BN021356.D\data.ms

(70) Pentachlorophenol (C)




17.127min (-0.006) 20721.33 ng

response 235305

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.67
264.00	61.60	59.50
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082422\
Data File : BN021356.D
Acq On : 25 Aug 2022 04:41
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 25 08:23:30 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 25 08:21:54 2022
Response via : Initial Calibration

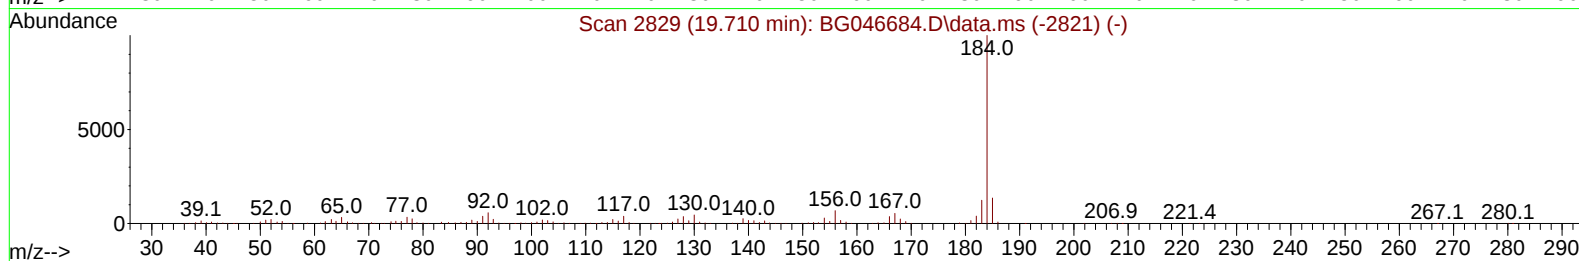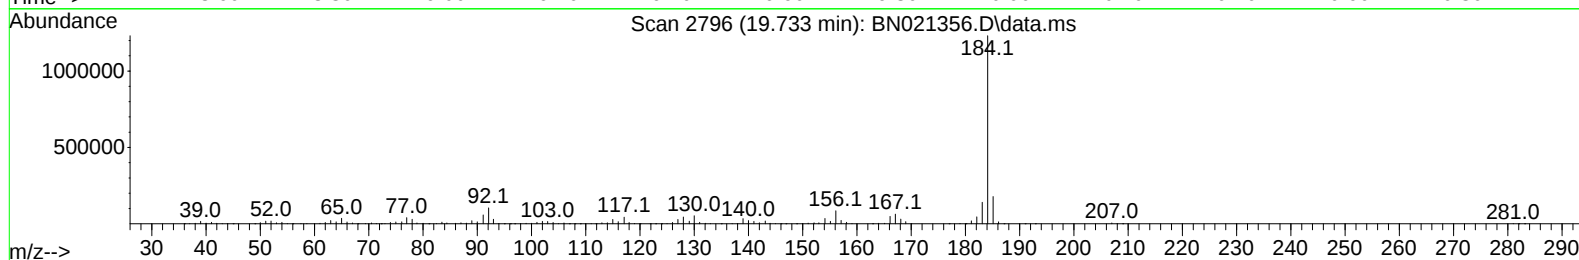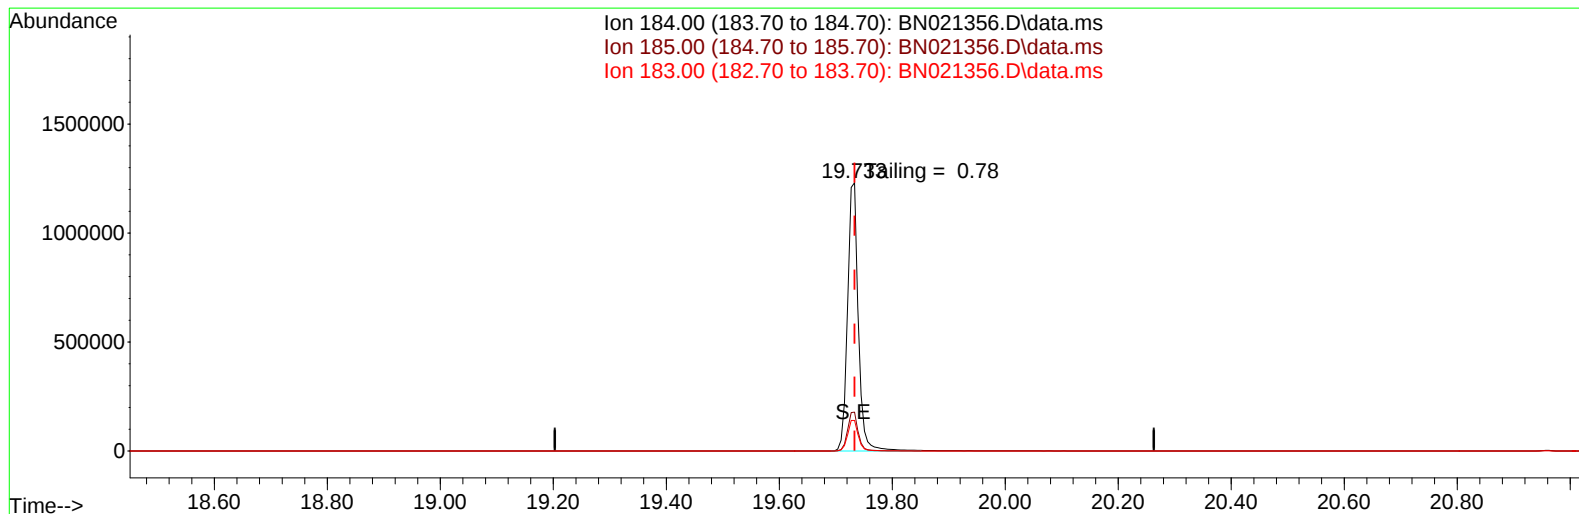

TIC: BN021356.D\data.ms

(77) Benzidine**19.733min (-0.000) 165579.00 ng****response 1633291**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.51
183.00	13.20	11.41
0.00	0.00	0.00