
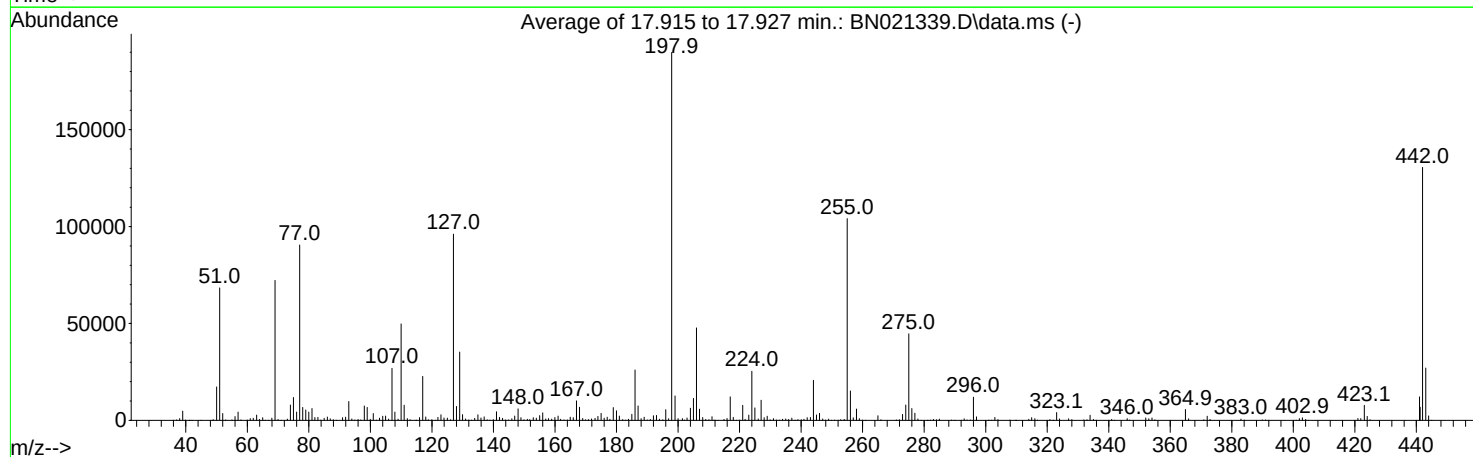


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082422\
 Data File : BN021339.D
 Acq On : 24 Aug 2022 15:55
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN082422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Aug 26 23:37:03 2022

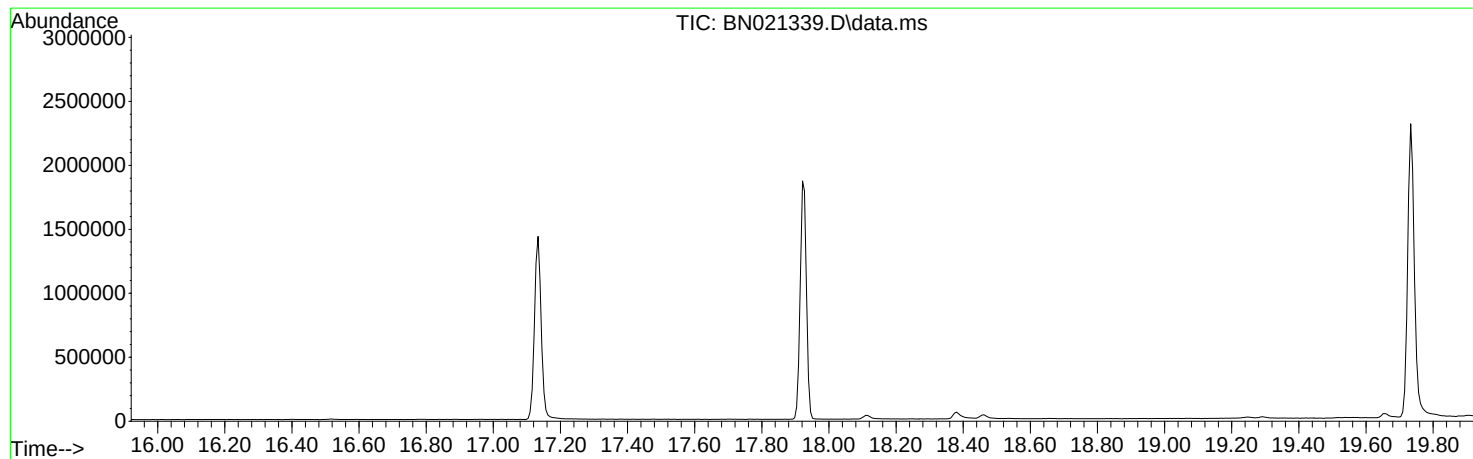

AutoFind: Scans 2487, 2488, 2489; Background Corrected with Scan 2481

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.0	68376	PASS
68	69	0.00	2	1.6	1154	PASS
69	198	0.00	100	38.1	72221	PASS
70	69	0.00	2	0.7	479	PASS
127	198	10	80	50.6	96072	PASS
197	198	0.00	2	0.4	824	PASS
198	198	100	100	100.0	189803	PASS
199	198	5	9	6.6	12620	PASS
275	198	10	60	23.5	44659	PASS
365	198	1	100	3.0	5614	PASS
441	198	0.01	100	6.4	12123	PASS
442	442	50	100	100.0	130499	PASS
443	442	15	24	20.7	26986	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/24/2022	BNA_N	<u>BN021339.D</u>
Compound Name	Response	Retention Time
DDT	594167	20.968
DDD	10870	20.527
DDE	136	20.015
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11006	605173	1.82

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082422\
 Data File : BN021339.D
 Acq On : 24 Aug 2022 15:55
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Aug 25 08:22:01 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 25 08:21:54 2022
 Response via : Initial Calibration

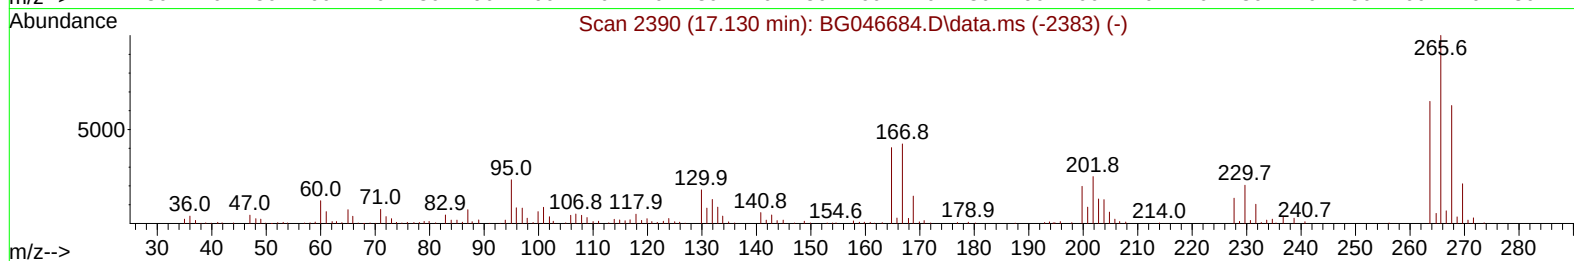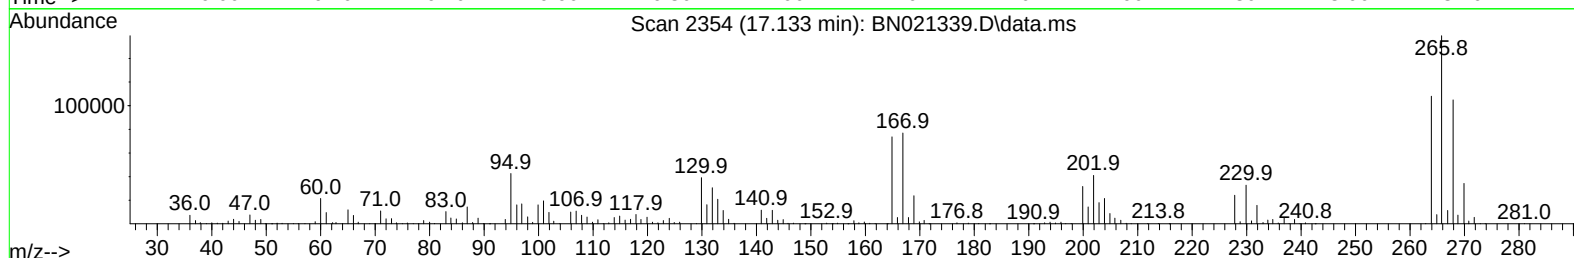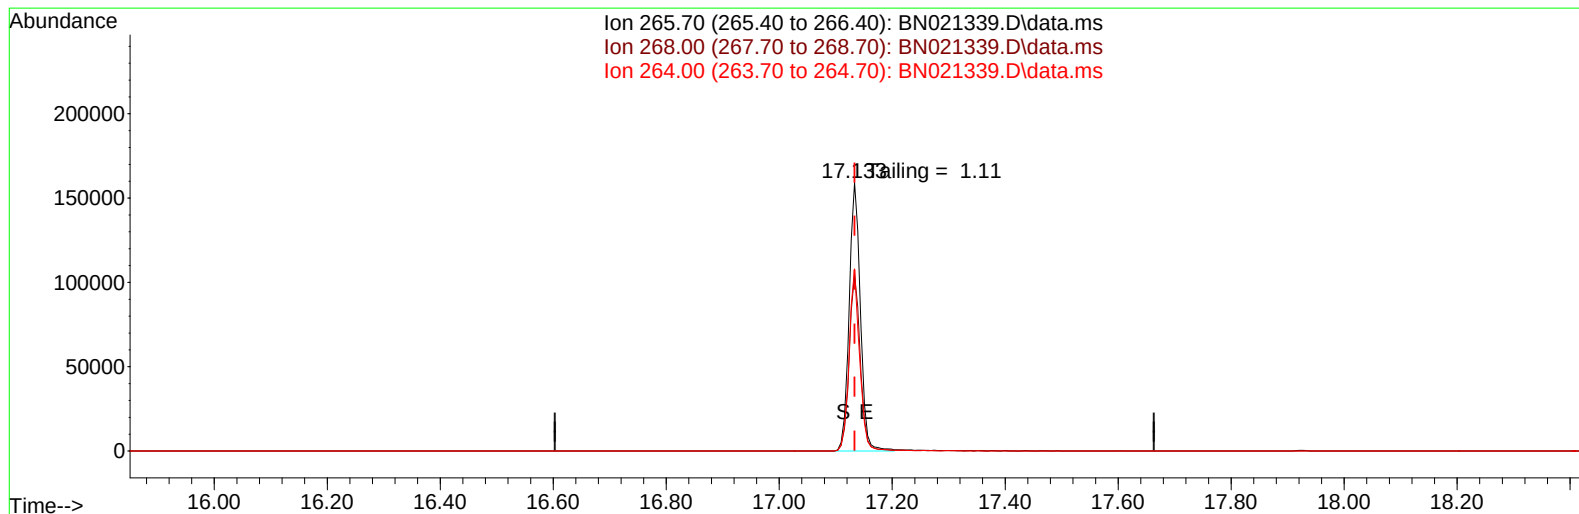

TIC: BN021339.D\data.ms

(70) Pentachlorophenol (C)

17.133min (0.000) 454958.94 ng




response 221365

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.93
264.00	61.60	67.85
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082422\
Data File : BN021339.D
Acq On : 24 Aug 2022 15:55
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 25 08:22:01 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 25 08:21:54 2022
Response via : Initial Calibration

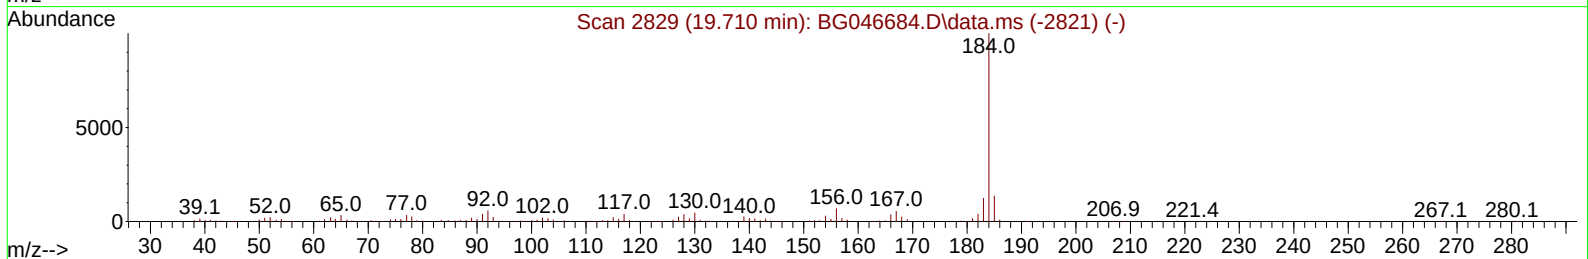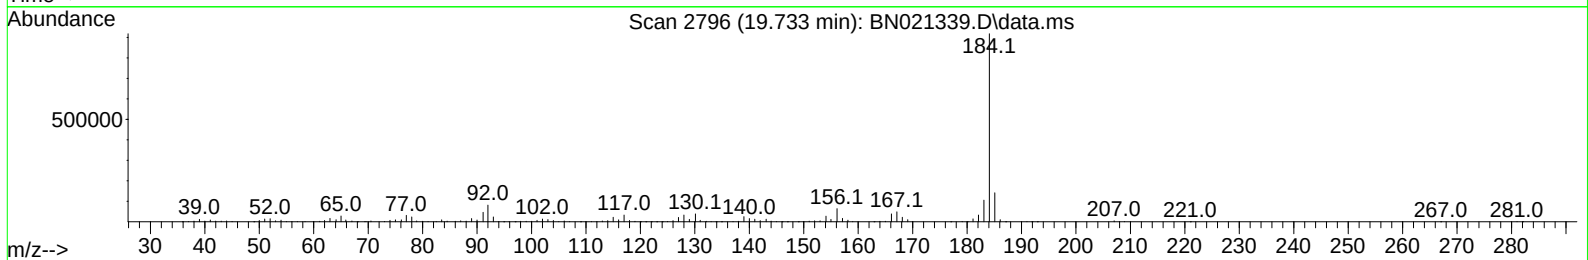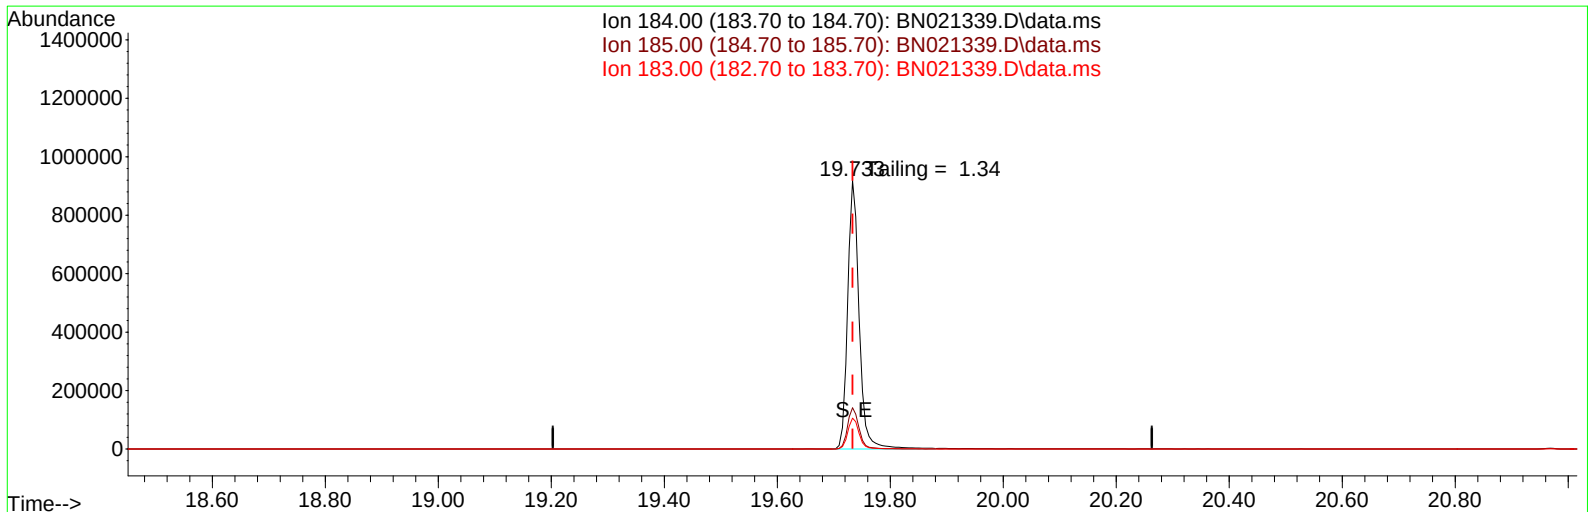

TIC: BN021339.D\data.ms

(77) Benzidine

19.733min (0.000) 52670.18 ng

response 1303733

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	15.42
183.00	13.20	11.53
0.00	0.00	0.00