
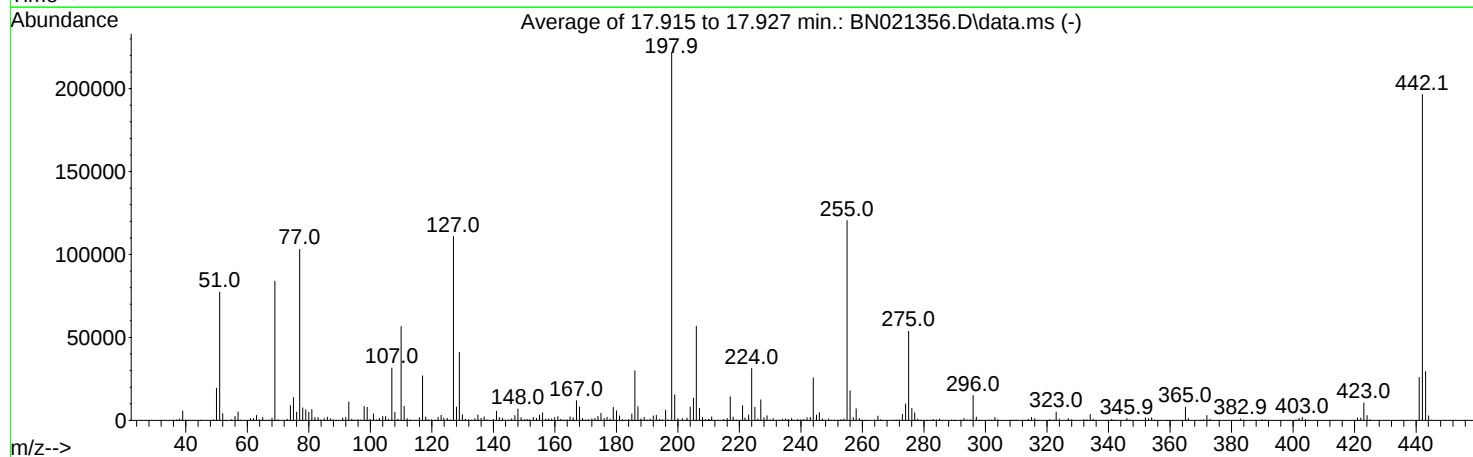


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082422\
 Data File : BN021356.D
 Acq On : 25 Aug 2022 04:41
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN082422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Aug 26 23:37:03 2022

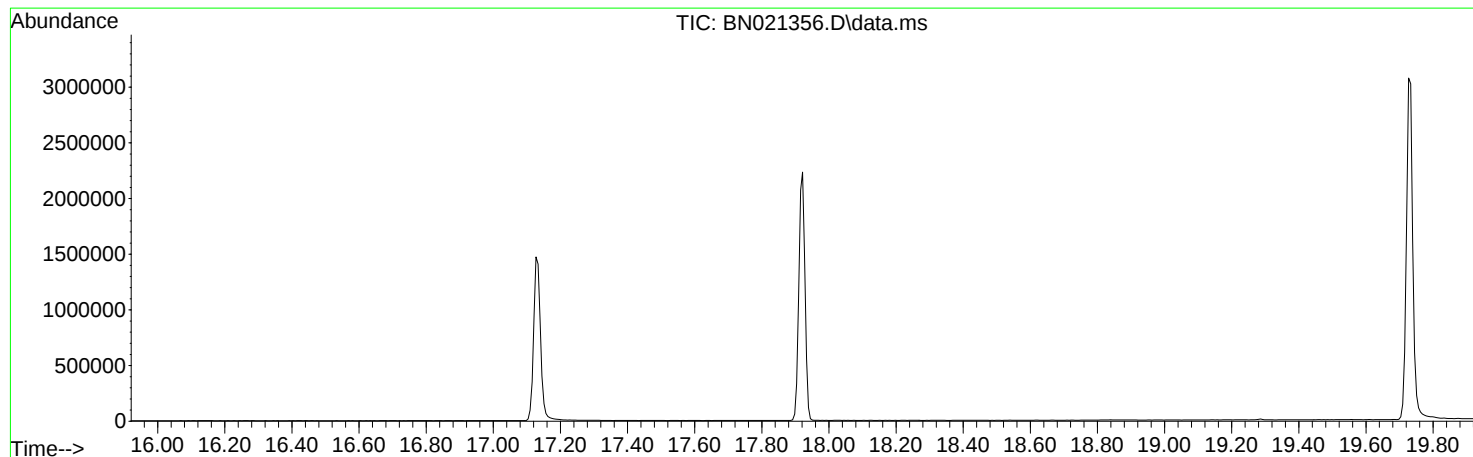

AutoFind: Scans 2487, 2488, 2489; Background Corrected with Scan 2480

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.9	77411	PASS
68	69	0.00	2	1.6	1353	PASS
69	198	0.00	100	37.8	83925	PASS
70	69	0.00	2	0.5	418	PASS
127	198	10	80	50.0	110917	PASS
197	198	0.00	2	0.1	283	PASS
198	198	100	100	100.0	221781	PASS
199	198	5	9	7.0	15467	PASS
275	198	10	60	24.2	53661	PASS
365	198	1	100	3.6	7885	PASS
441	198	0.01	100	11.7	25896	PASS
442	442	50	100	100.0	196395	PASS
443	442	15	24	15.0	29469	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/24/2022	BNA_N	<u>BN021356.D</u>
Compound Name	Response	Retention Time
DDT	700120	20.956
DDD	9371	20.521
DDE	305	20.009
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9676	709796	1.36

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082422\
Data File : BN021356.D
Acq On : 25 Aug 2022 04:41
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 25 08:23:30 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 25 08:21:54 2022
Response via : Initial Calibration

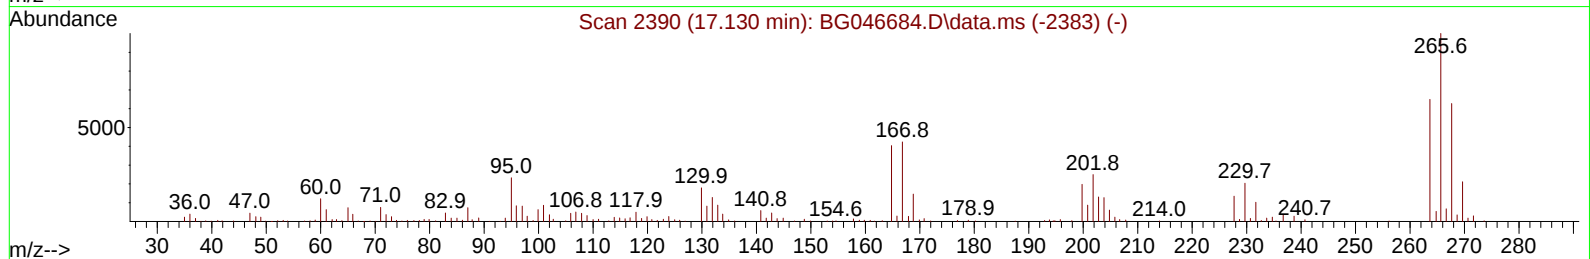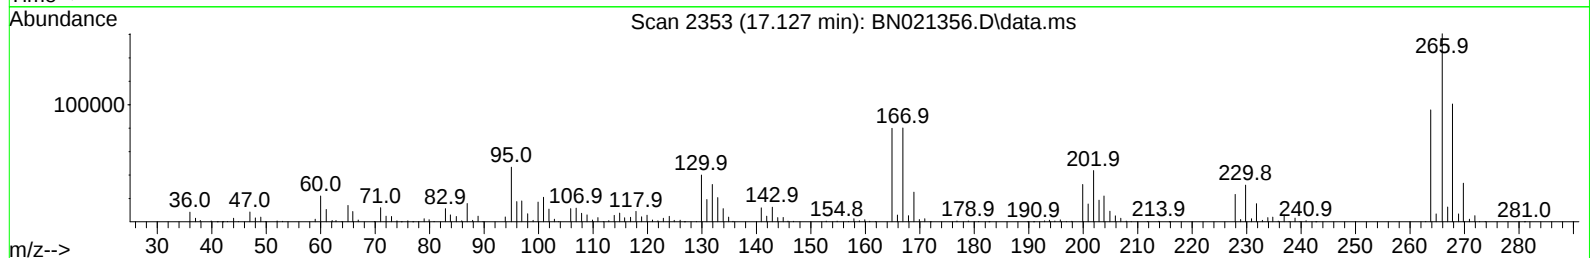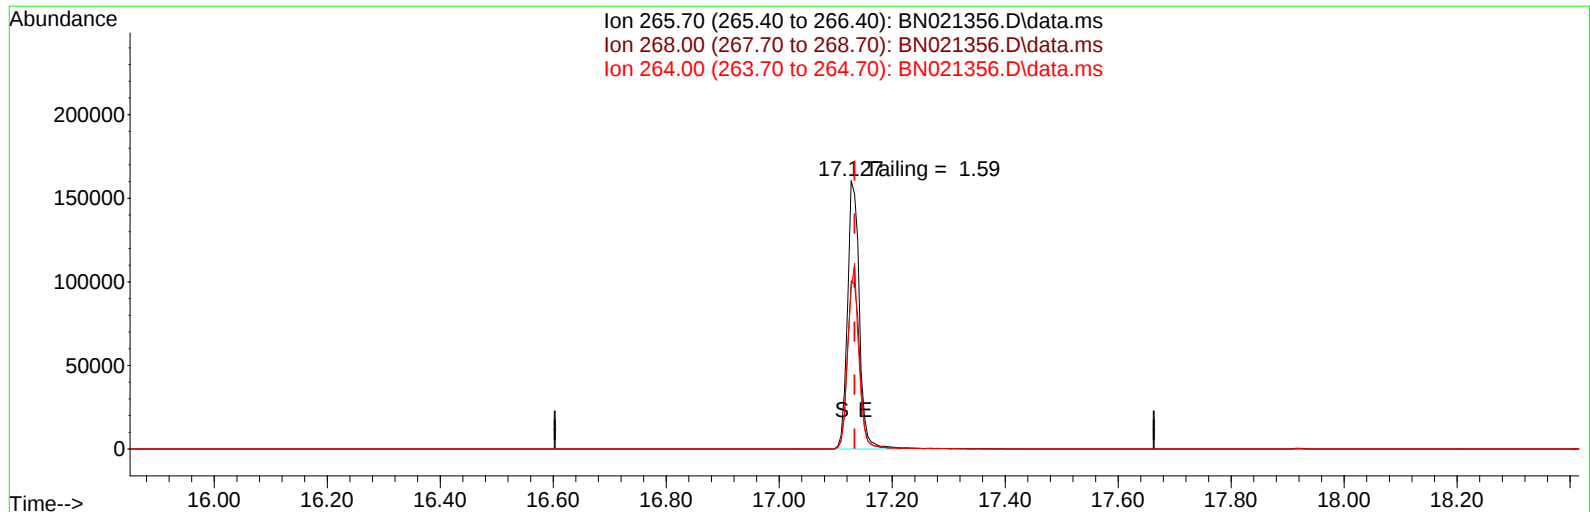

TIC: BN021356.D\data.ms

(70) Pentachlorophenol (C)

17.127min (-0.006) 20721.33 ng




response 235305

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.67
264.00	61.60	59.50
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082422\
Data File : BN021356.D
Acq On : 25 Aug 2022 04:41
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 25 08:23:30 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 25 08:21:54 2022
Response via : Initial Calibration

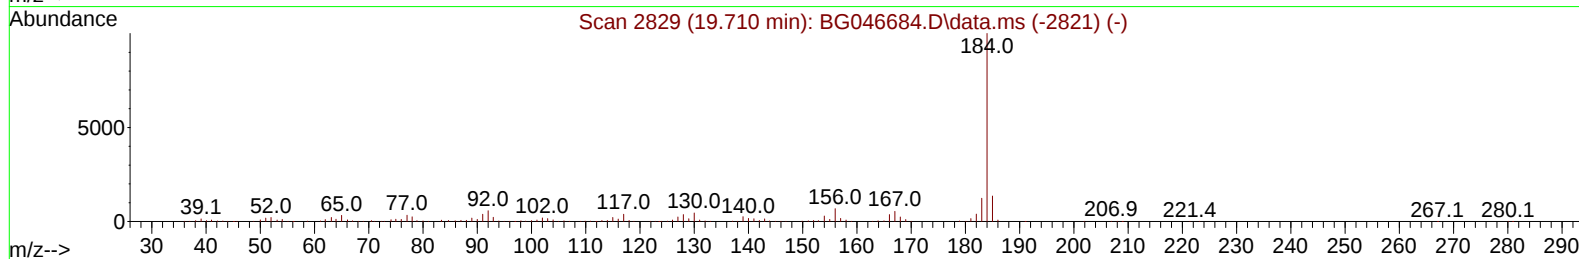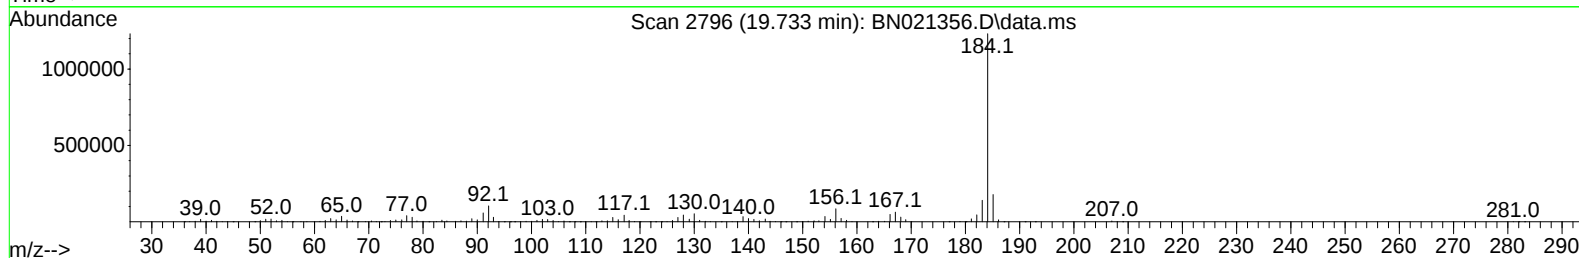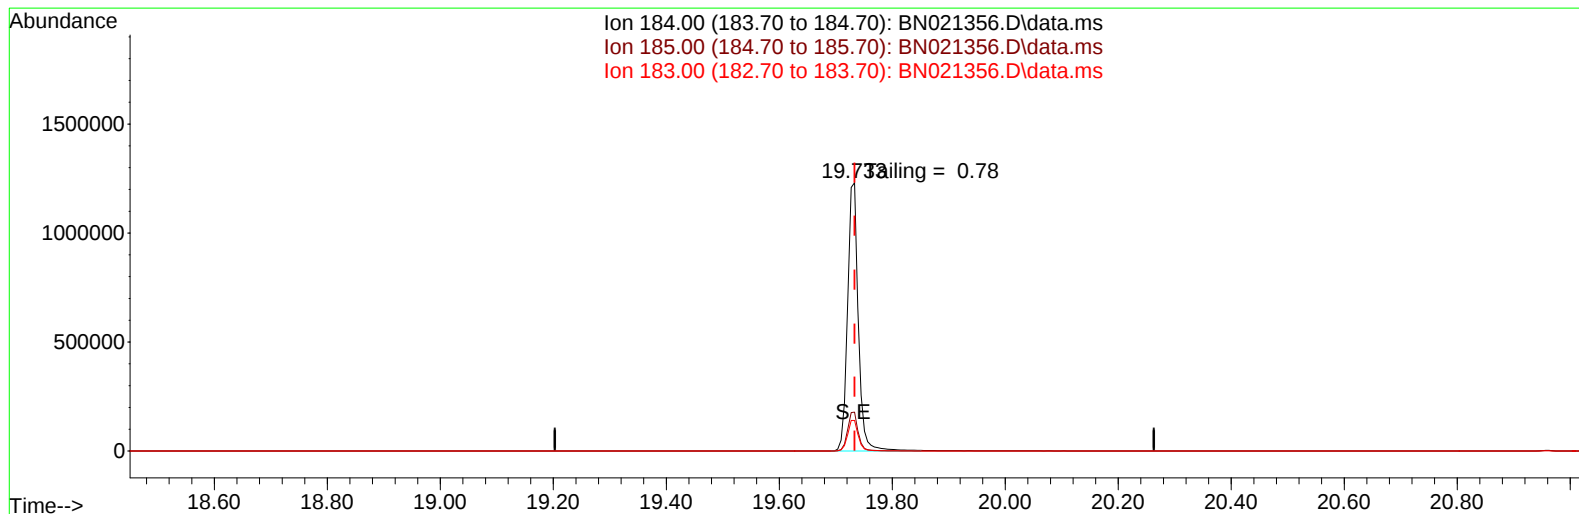

TIC: BN021356.D\data.ms

(77) Benzidine

19.733min (-0.000) 165579.00 ng

response 1633291

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.51
183.00	13.20	11.41
0.00	0.00	0.00