
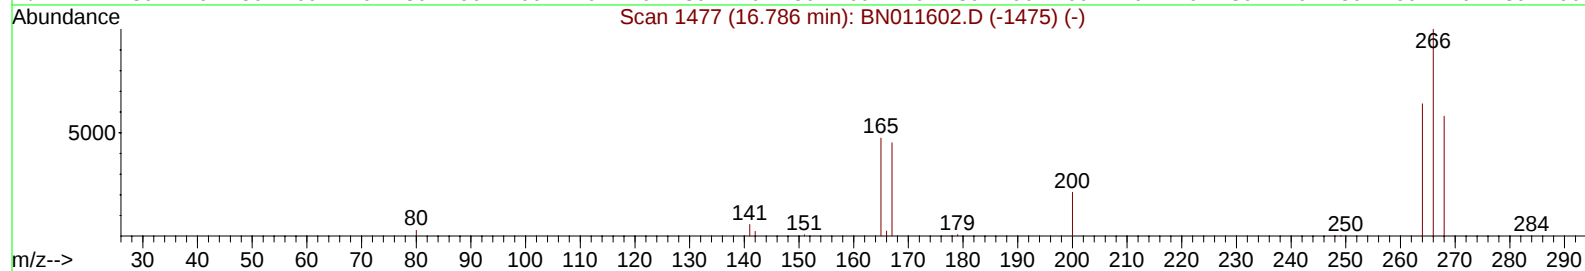
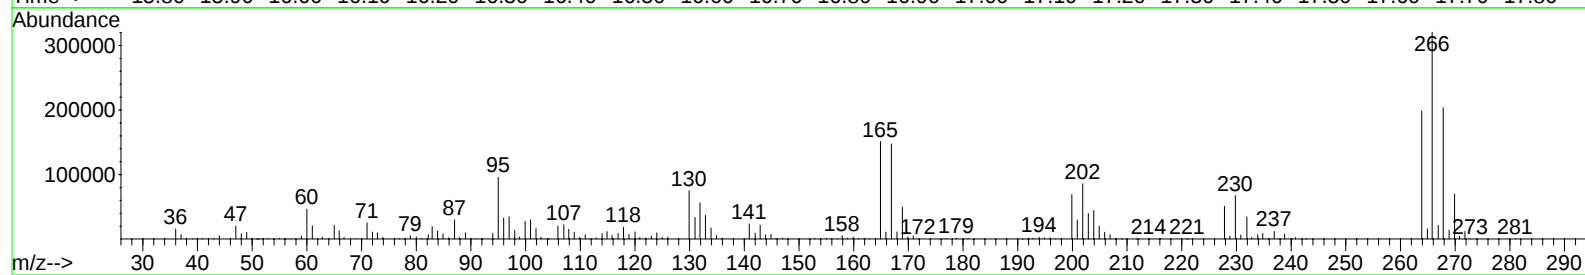


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN082520\
 Data File : BN011609.D
 Acq On : 25 Aug 2020 09:37
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 25 18:38:05 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN082420.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 25 03:31:11 2020
 Response via : Initial Calibration

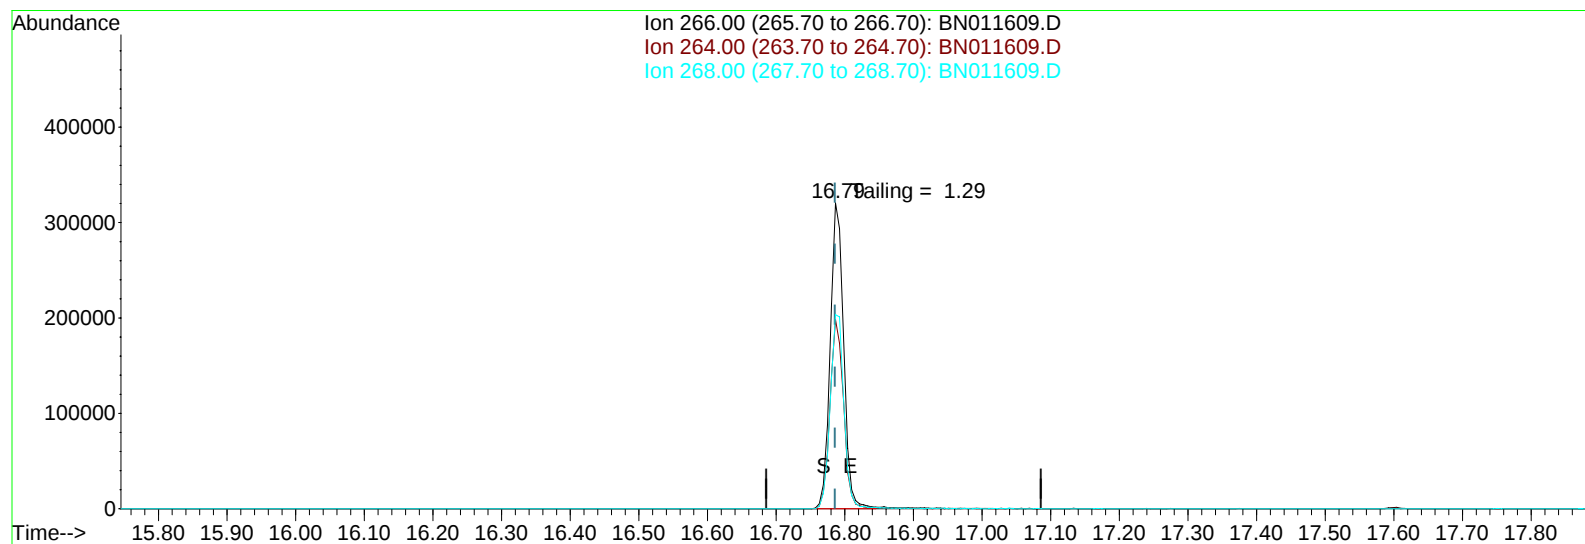

(24) Pentachlorophenol

16.786min (+0.001) 2309.01ng

response 439106

Ion	Exp%	Act%
266.00	100	100
264.00	60.10	62.15
268.00	60.50	65.22
0.00	0.00	0.00