


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082520\
 Data File : BN011609.D
 Acq On : 25 Aug 2020 09:37
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN082420.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Aug 25 03:31:11 2020

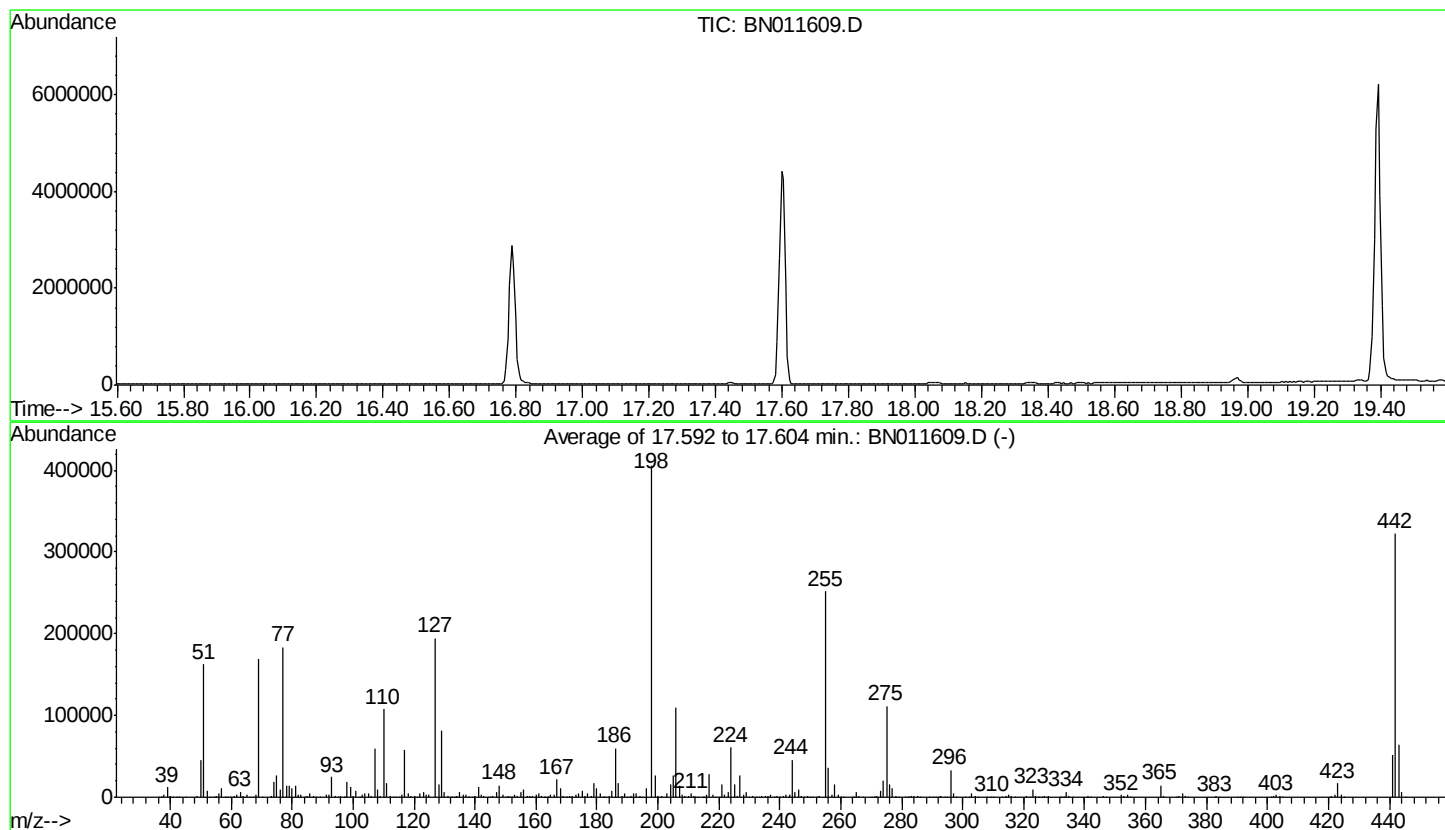

AutoFind: Scans 2483, 2484, 2485; Background Corrected with Scan 2477

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.1	162673	PASS
68	69	0.00	2	1.6	2762	PASS
69	198	0.00	100	41.7	169099	PASS
70	69	0.00	2	0.4	724	PASS
127	198	10	80	48.0	194666	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	405653	PASS
199	198	5	9	6.7	26981	PASS
275	198	10	60	27.5	111624	PASS
365	198	1	100	3.6	14506	PASS
441	198	0.01	100	12.6	51090	PASS
442	198	50	100	79.4	322218	PASS
443	442	15	24	20.1	64682	PASS