


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN082520\
 Data File : BN011625.D
 Acq On : 25 Aug 2020 21:24
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN082420.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Aug 25 03:31:11 2020

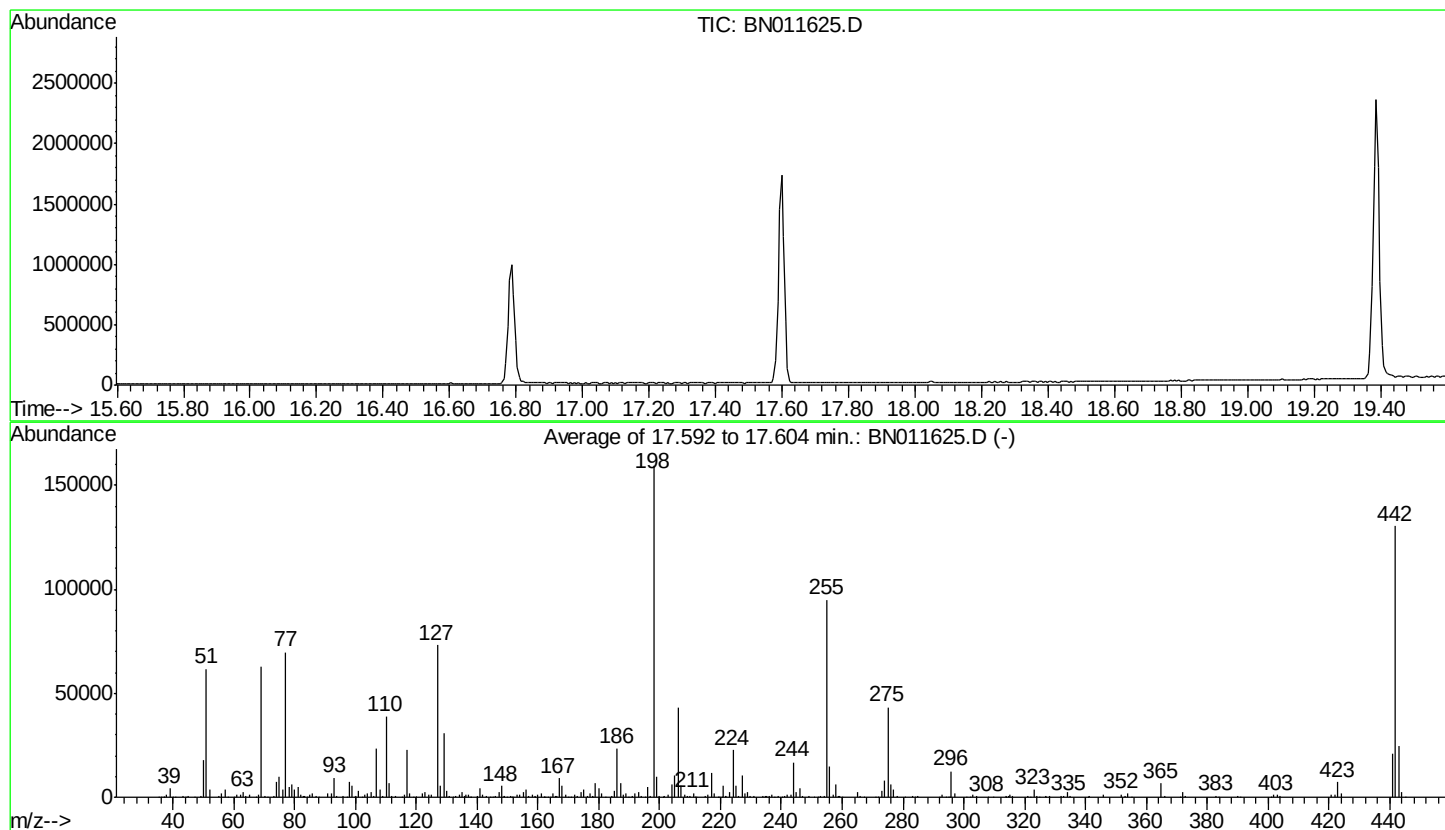

AutoFind: Scans 2483, 2484, 2485; Background Corrected with Scan 2477

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.6	61536	PASS
68	69	0.00	2	1.8	1115	PASS
69	198	0.00	100	39.4	62738	PASS
70	69	0.00	2	1.1	698	PASS
127	198	10	80	45.8	72941	PASS
197	198	0.00	2	0.3	404	PASS
198	198	100	100	100.0	159402	PASS
199	198	5	9	6.4	10156	PASS
275	198	10	60	27.1	43248	PASS
365	198	1	100	4.1	6612	PASS
441	198	0.01	100	13.0	20771	PASS
442	198	50	100	81.7	130280	PASS
443	442	15	24	19.1	24834	PASS