

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082521\
 Data File : BN016028.D
 Acq On : 24 Aug 2021 12:22
 Operator : CG/JU
 Sample : SSTDICC1.6
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC1.6

Quant Time: Aug 24 12:55:22 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN082521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 24 11:43:13 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.882	152	9064	0.400	ng	0.00
7) Naphthalene-d8	10.673	136	45891	0.400	ng	#-0.01
13) Acenaphthene-d10	14.510	164	24770	0.400	ng	0.00
19) Phenanthrene-d10	17.249	188	45221	0.400	ng	0.00
29) Chrysene-d12	21.450	240	48665	0.400	ng	# 0.01
35) Perylene-d12	23.844	264	44439	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.457	112	37122	1.575	ng	0.00
5) Phenol-d6	7.052	99	52179	1.577	ng	0.00
8) Nitrobenzene-d5	9.038	82	53165	1.171	ng	0.00
11) 2-Methylnaphthalene-d10	12.265	152	117317	1.734	ng	0.00
14) 2,4,6-Tribromophenol	15.994	330	14531	1.644	ng	0.00
15) 2-Fluorobiphenyl	13.140	172	150635	1.339	ng	0.00
27) Fluoranthene-d10	19.286	212	224406	1.709	ng	0.00
31) Terphenyl-d14	19.882	244	192394	1.711	ng	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.392	88	8455	2.196	ng	# 88
3) n-Nitrosodimethylamine	3.733	42	14298	2.255	ng	95
6) bis(2-Chloroethyl)ether	7.310	93	41859	1.515	ng	100
9) Naphthalene	10.724	128	195017	1.537	ng	99
10) Hexachlorobutadiene	11.015	225	43809	1.610	ng	# 100
12) 2-Methylnaphthalene	12.336	142	128308	1.611	ng	99
16) Acenaphthylene	14.231	152	166412	1.415	ng	100
17) Acenaphthene	14.573	154	112773	1.470	ng	99
18) Fluorene	15.550	166	137054	1.476	ng	99
20) 4,6-Dinitro-2-methylph...	15.626	198	6800	1.816	ng	# 80
21) 4-Bromophenyl-phenylether	16.446	248	38709	1.455	ng	99
22) Hexachlorobenzene	16.567	284	50806	1.459	ng	99
23) Atrazine	16.713	200	28619	2.089	ng	98
24) Pentachlorophenol	16.908	266	15012	1.834	ng	100
25) Phenanthrene	17.297	178	209022	1.467	ng	99
26) Anthracene	17.383	178	188684	1.556	ng	100
28) Fluoranthene	19.316	202	245858	1.519	ng	100
30) Pyrene	19.679	202	241756	1.637	ng	100
32) Benzo(a)anthracene	21.429	228	253730	1.637	ng	99
33) Chrysene	21.482	228	243945	1.502	ng	99
34) Bis(2-ethylhexyl)phtha...	21.355	149	70064	1.351	ng	100
36) Indeno(1,2,3-cd)pyrene	26.322	276	273061	1.418	ng	99
37) Benzo(b)fluoranthene	23.115	252	259980	1.541	ng	# 95
38) Benzo(k)fluoranthene	23.159	252	236376	1.481	ng	98
39) Benzo(a)pyrene	23.738	252	225735	1.501	ng	# 91
40) Dibenzo(a,h)anthracene	26.343	278	227366	1.422	ng	98
41) Benzo(g,h,i)perylene	27.082	276	232641	1.448	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082521\
Data File : BN016028.D
Acq On : 24 Aug 2021 12:22
Operator : CG/JU
Sample : SSTDICC1.6
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6

Quant Time: Aug 24 12:55:22 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN082521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 24 11:43:13 2021
Response via : Initial Calibration




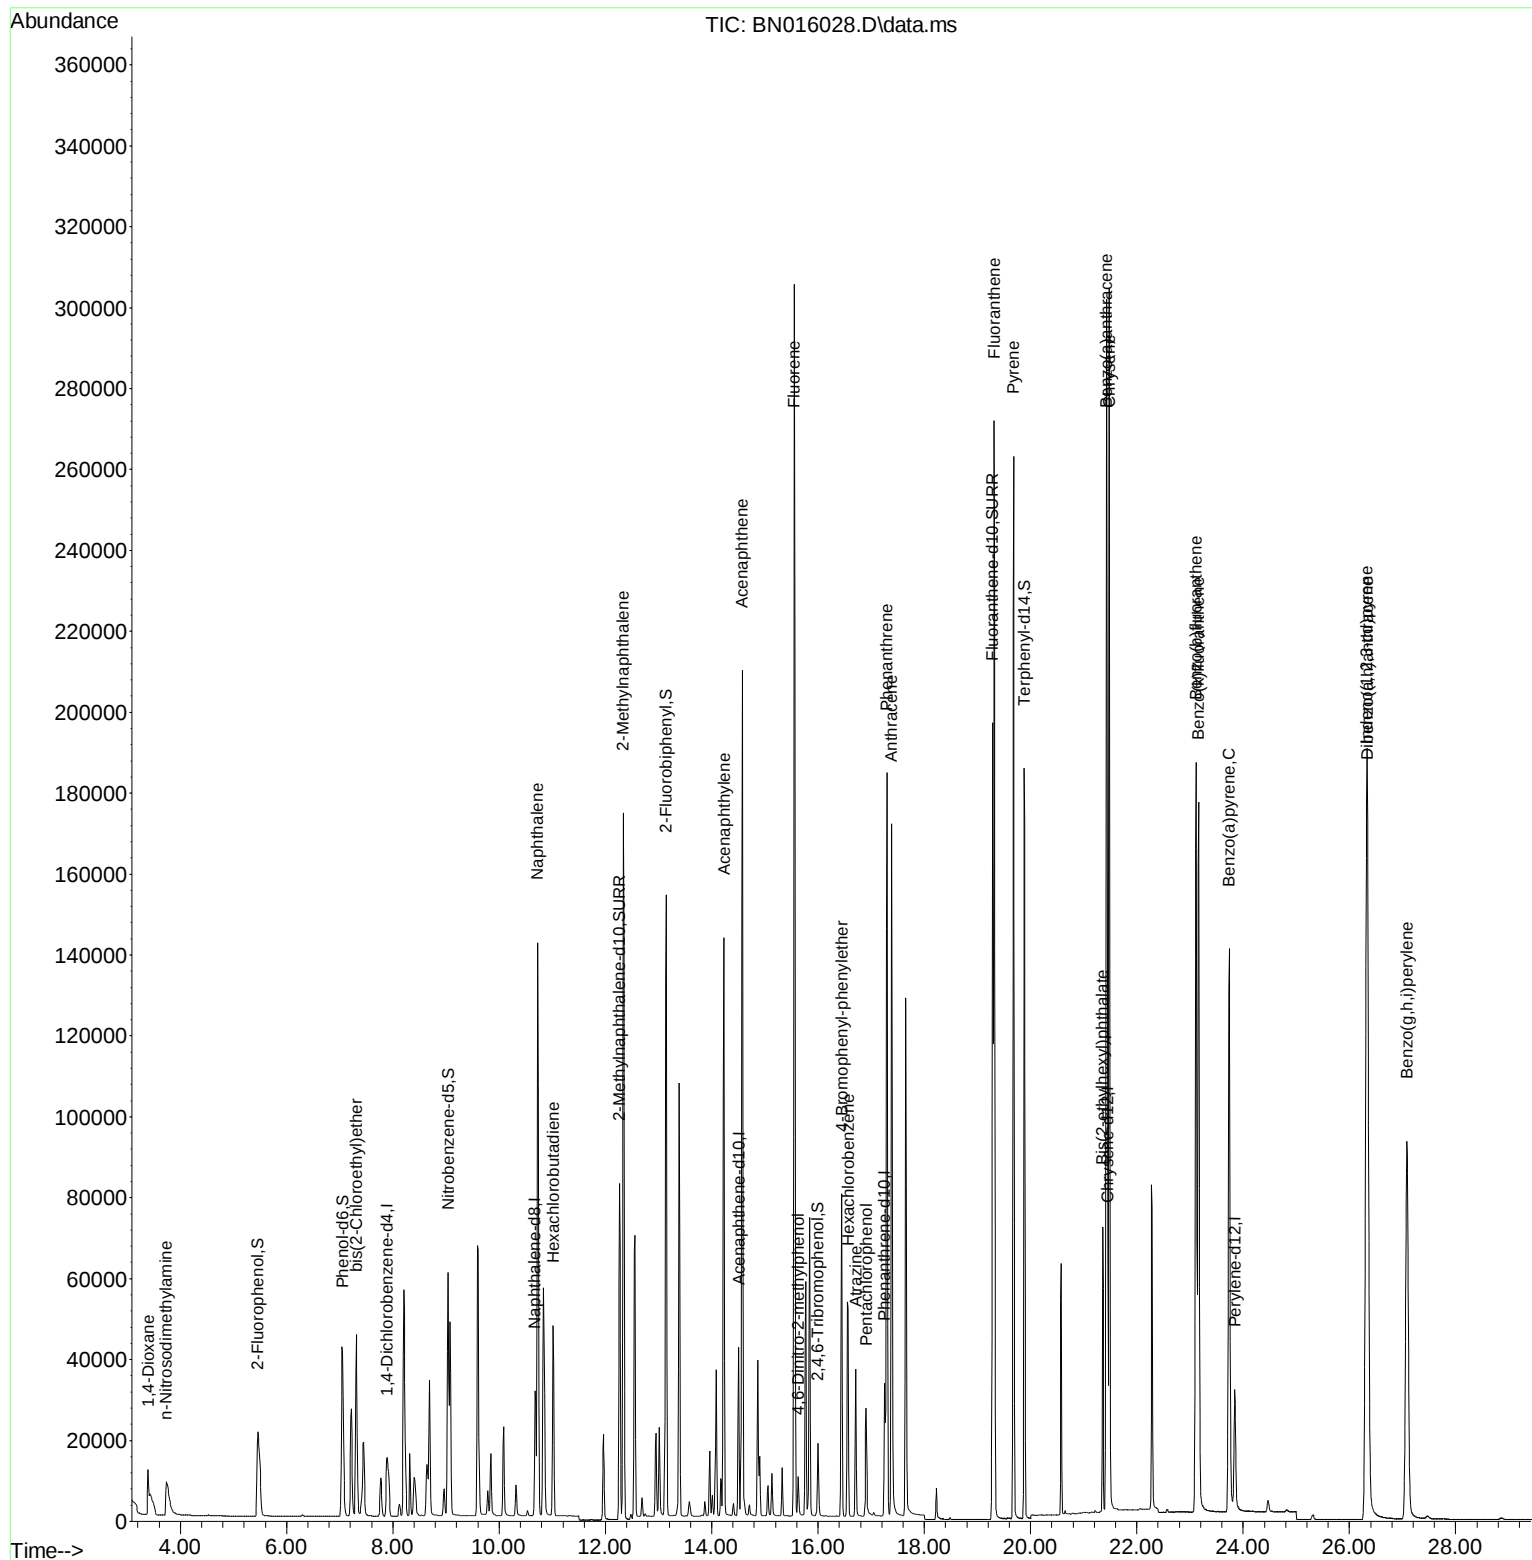


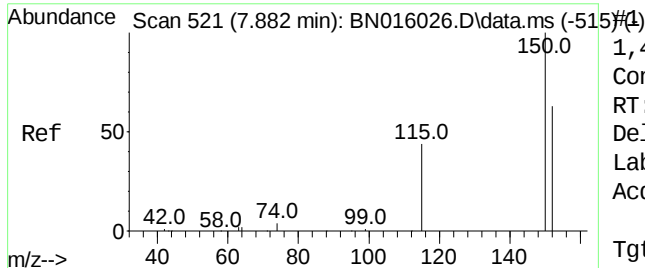

1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.882 min Scan# 521
 Delta R.T. 0.000 min
 Lab File: BN016028.D
 Acq: 24 Aug 2021 12:22




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC1.6


Tgt Ion:	152	Resp:	9064
Ion	Ratio	Lower	Upper
152	100		
150	158.1	126.5	189.7
115	69.5	56.5	84.7

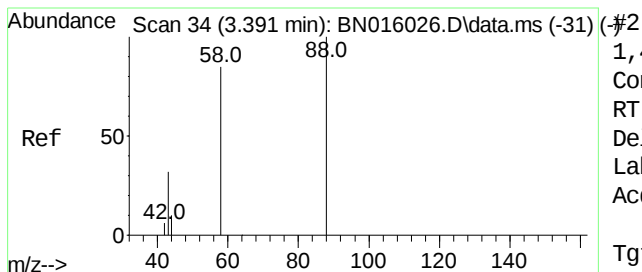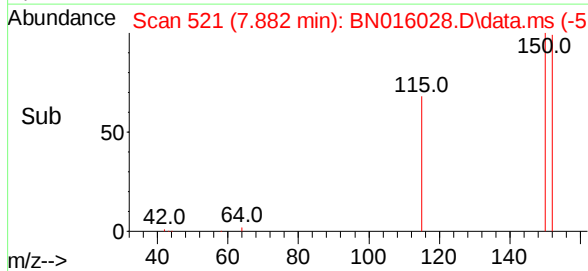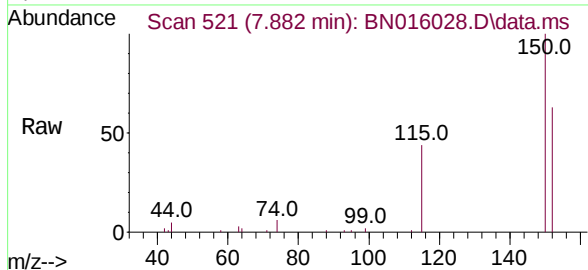

1,4-Dioxane
 Concen: 2.196 ng
 RT: 3.392 min Scan# 34
 Delta R.T. 0.001 min
 Lab File: BN016028.D
 Acq: 24 Aug 2021 12:22

Tgt Ion:	88	Resp:	8455
Ion	Ratio	Lower	Upper
88	100		
43	34.1	21.0	31.4#
58	77.7	54.8	82.2


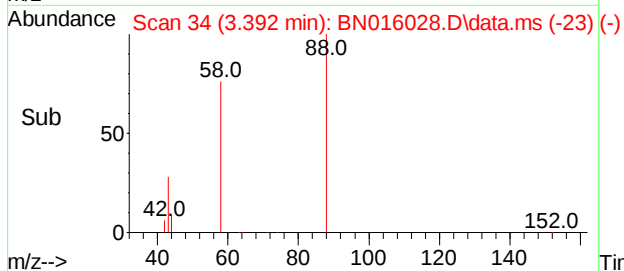

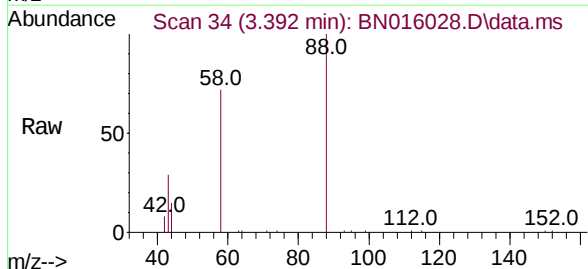


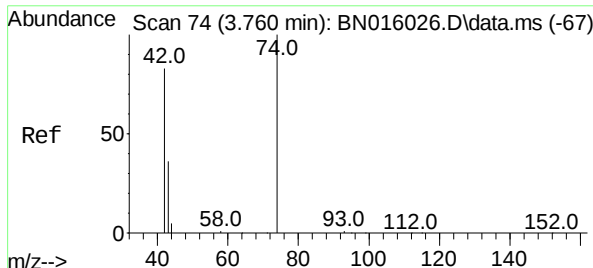

n-Nitrosodimethylamine
 Concen: 2.255 ng
 RT: 3.733 min Scan# 71
 Delta R.T. -0.027 min
 Lab File: BN016028.D
 Acq: 24 Aug 2021 12:22




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC1.6


Tgt Ion:	42	Resp:	14298
Ion	Ratio	Lower	Upper
42	100		
74	122.5	93.8	140.8
44	7.8	7.7	11.5

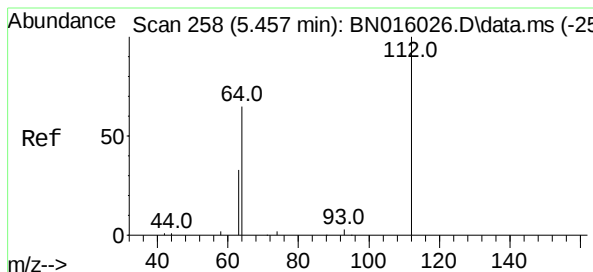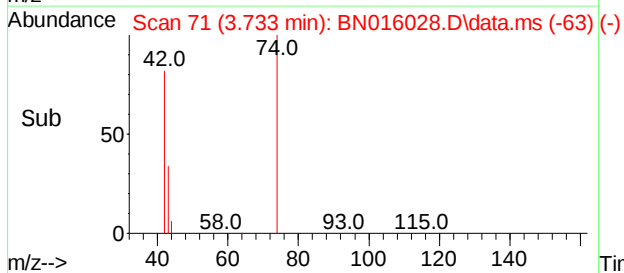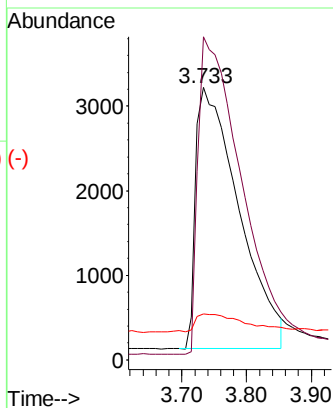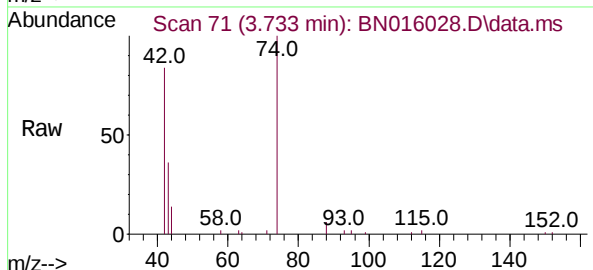

2-Fluorophenol
 Concen: 1.575 ng
 RT: 5.457 min Scan# 258
 Delta R.T. 0.000 min
 Lab File: BN016028.D
 Acq: 24 Aug 2021 12:22

Tgt Ion:	112	Resp:	37122
Ion	Ratio	Lower	Upper
112	100		
64	65.7	52.5	78.7
63	33.8	26.9	40.3


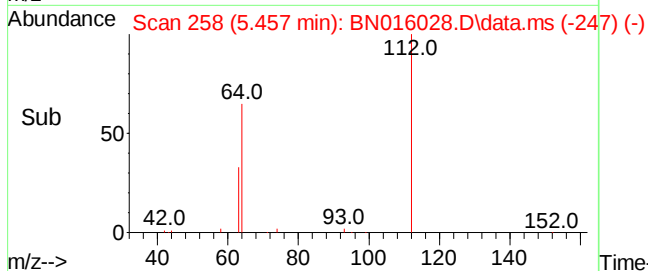

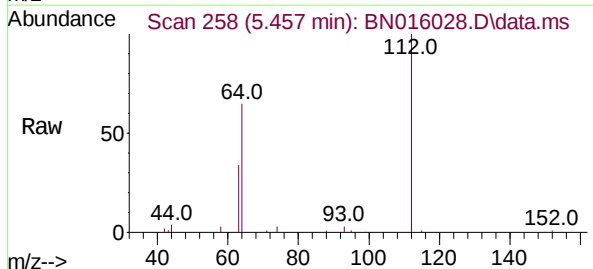


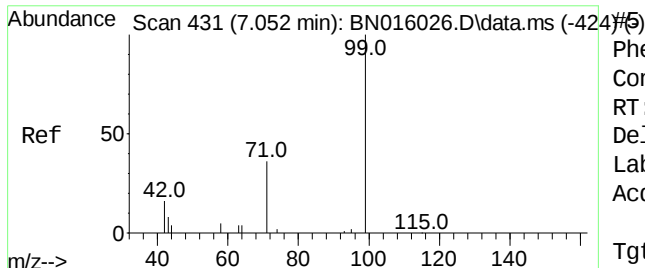

Phenol-d6
 Concen: 1.577 ng
 RT: 7.052 min Scan# 431
 Delta R.T. 0.000 min
 Lab File: BN016028.D
 Acq: 24 Aug 2021 12:22




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC1.6


Tgt Ion:	99	Resp:	52179
Ion	Ratio	Lower	Upper
99	100		
42	19.4	15.6	23.4
71	37.5	29.8	44.8

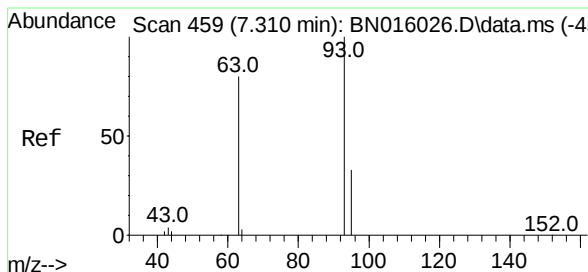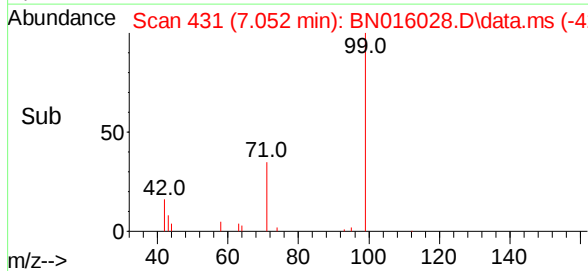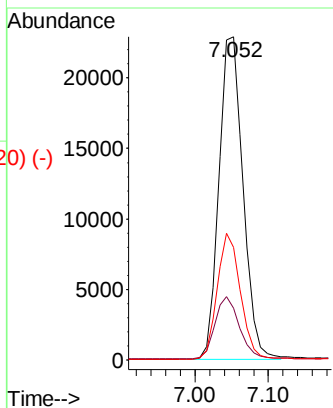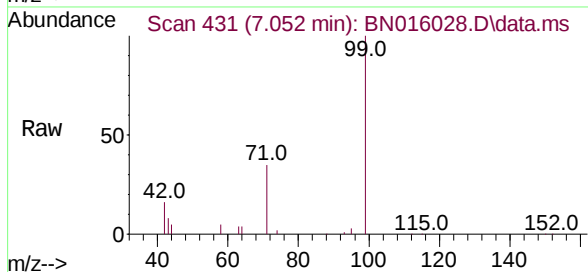

bis(2-Chloroethyl)ether
 Concen: 1.515 ng
 RT: 7.310 min Scan# 459
 Delta R.T. 0.000 min
 Lab File: BN016028.D
 Acq: 24 Aug 2021 12:22

Tgt Ion:	93	Resp:	41859
Ion	Ratio	Lower	Upper
93	100		
63	77.0	62.0	93.0
95	32.7	26.2	39.4


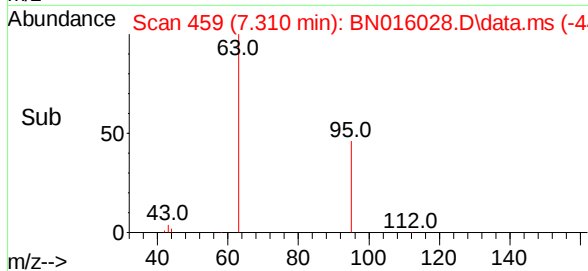

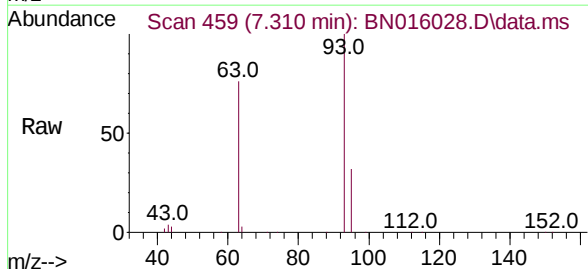


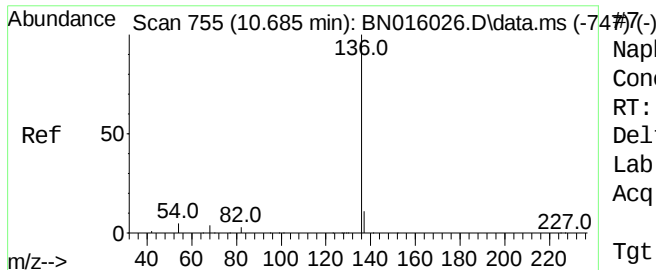

Naphthalene-d8
 Concen: 0.400 ng
 RT: 10.673 min Scan# 754
 Delta R.T. -0.012 min
 Lab File: BN016028.D
 Acq: 24 Aug 2021 12:22




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC1.6


Tgt Ion:	136	Resp:	45891
Ion	Ratio	Lower	Upper
136	100		
137	11.2	8.9	13.3
54	10.1	4.2	6.4#
68	7.8	3.4	5.2#

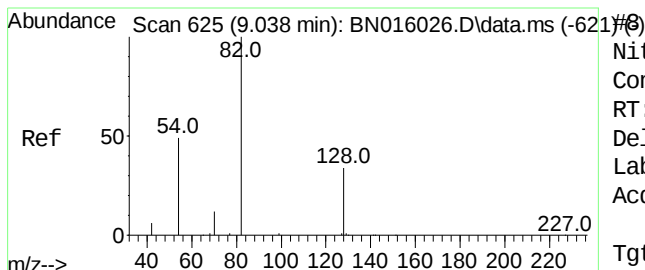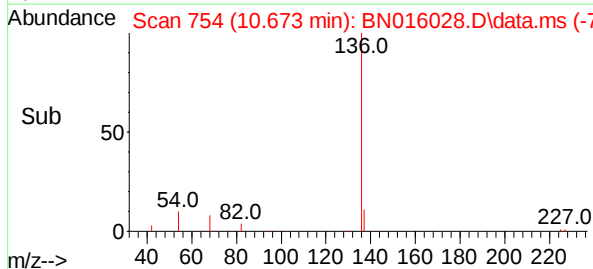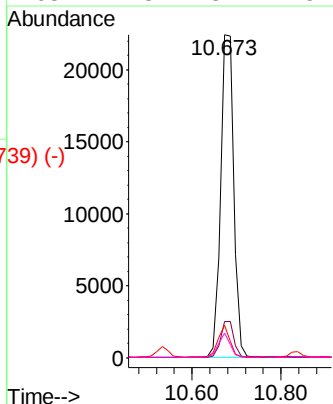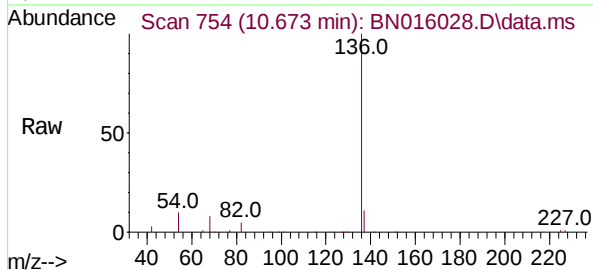

Nitrobenzene-d5
 Concen: 1.171 ng
 RT: 9.038 min Scan# 625
 Delta R.T. 0.000 min
 Lab File: BN016028.D
 Acq: 24 Aug 2021 12:22

Tgt Ion:	82	Resp:	53165
Ion	Ratio	Lower	Upper
82	100		
128	35.9	27.7	41.5
54	48.1	39.4	59.2


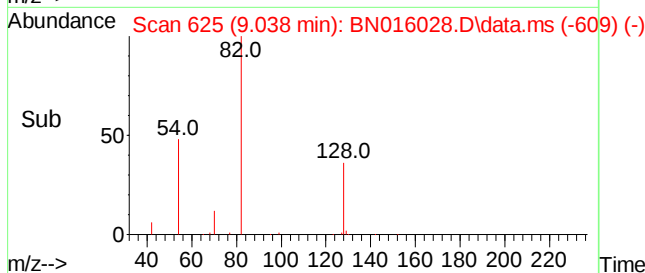

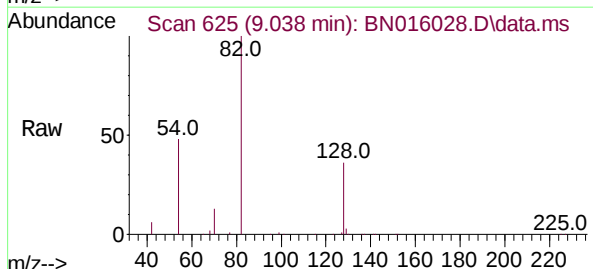


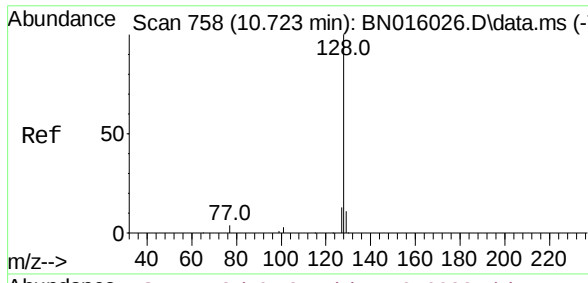

Naphthalene
 Concen: 1.537 ng
 RT: 10.724 min Scan# 758
 Delta R.T. 0.000 min
 Lab File: BN016028.D
 Acq: 24 Aug 2021 12:22




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC1.6

Tgt Ion:	128	Resp:	195017
Ion	Ratio	Lower	Upper
128	100		
129	10.9	8.9	13.3
127	13.2	10.7	16.1

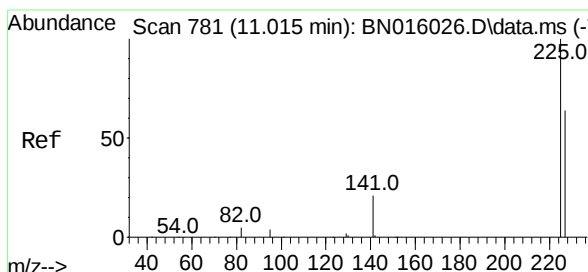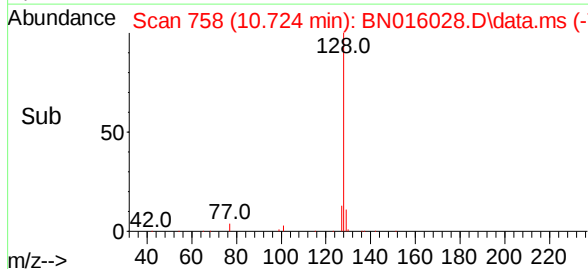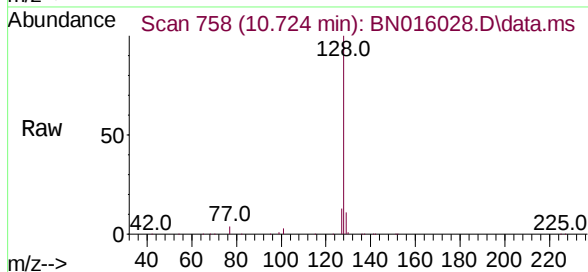


Hexachlorobutadiene
 Concen: 1.610 ng
 RT: 11.015 min Scan# 781
 Delta R.T. 0.000 min
 Lab File: BN016028.D
 Acq: 24 Aug 2021 12:22

Tgt Ion:	225	Resp:	43809
Ion	Ratio	Lower	Upper
225	100		
223	0.0	0.0	0.0
227	64.3	51.5	77.3

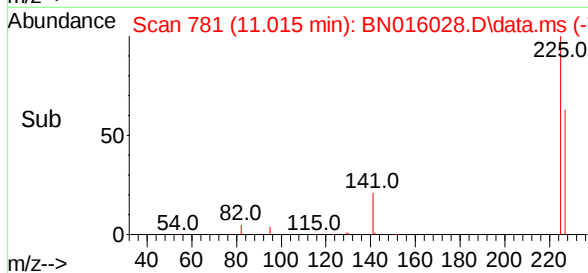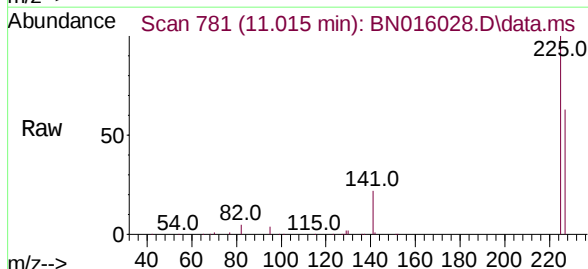




Abundance Scan 990 (12.265 min): BN016026.D\data.ms (-977) (-)

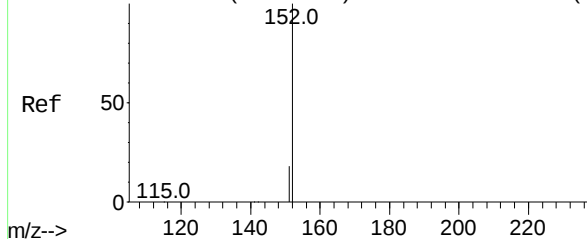


2-Methylnaphthalene-d10
Concen: 1.734 ng
RT: 12.265 min Scan# 990
Delta R.T. 0.000 min
Lab File: BN016028.D
Acq: 24 Aug 2021 12:22

Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6

Tgt Ion:152 Resp: 117317
Ion Ratio Lower Upper
152 100
151 20.4 16.6 24.8

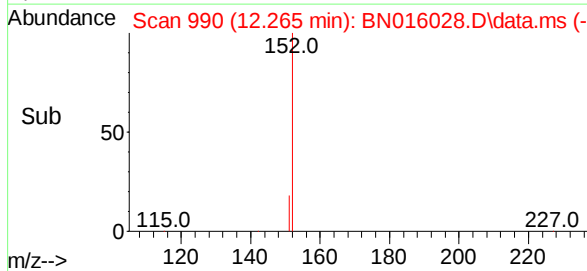
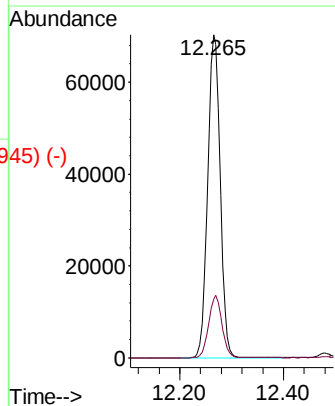
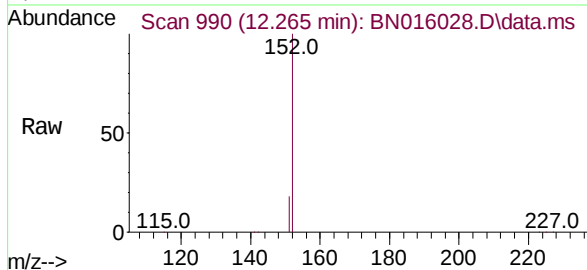


Abundance Scan 1007 (12.340 min): BN016026.D\data.ms (-990) (-)

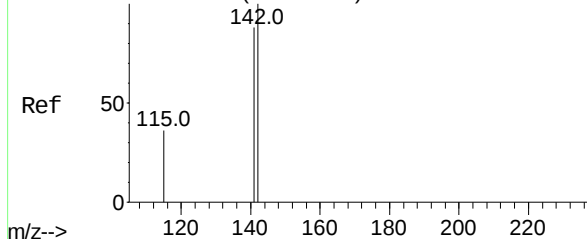

2-Methylnaphthalene
Concen: 1.611 ng
RT: 12.336 min Scan# 1006
Delta R.T. -0.004 min
Lab File: BN016028.D
Acq: 24 Aug 2021 12:22


Tgt Ion:142 Resp: 128308
Ion Ratio Lower Upper
142 100
141 88.4 70.3 105.5
115 36.9 28.7 43.1

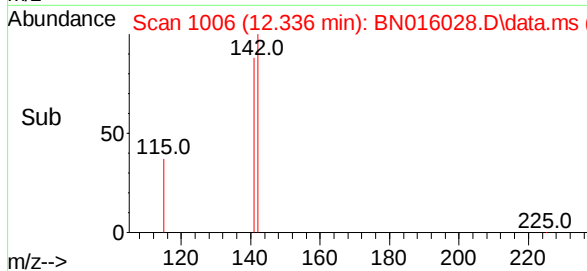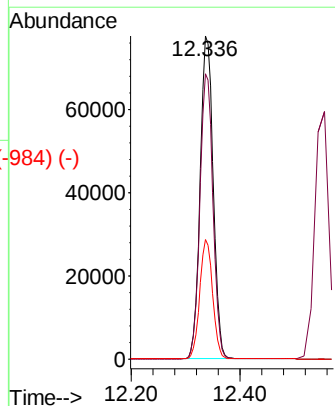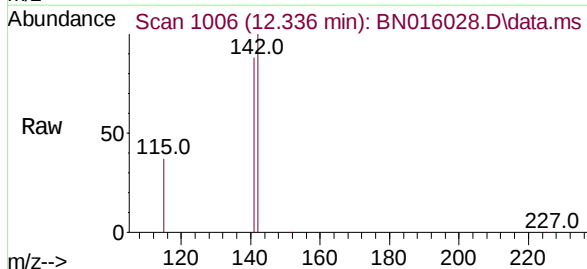




Abundance Scan 1202 (14.509 min): BN016026.D\data.ms (-1196) (-)

Acenaphthene-d10
Concen: 0.400 ng
RT: 14.510 min Scan# 1202
Delta R.T. 0.000 min
Lab File: BN016028.D
Acq: 24 Aug 2021 12:22

Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6

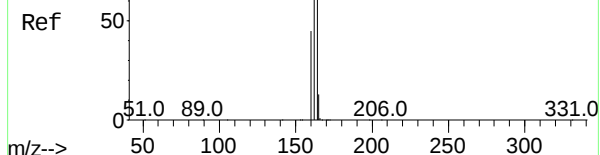





Tgt Ion	Ratio	Lower	Upper
164	100		
162	99.5	80.2	120.4
160	43.8	35.9	53.9

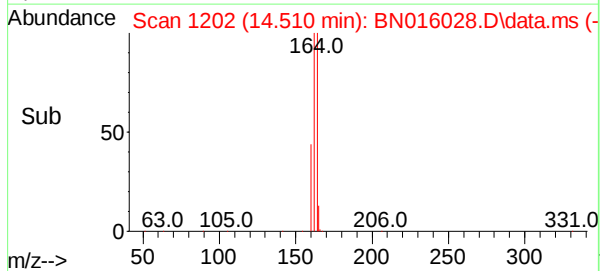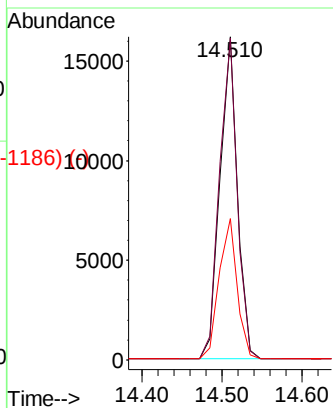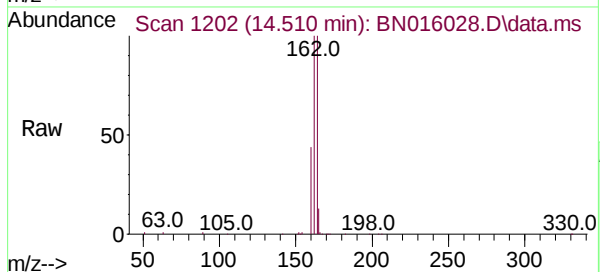


Abundance Scan 1319 (15.994 min): BN016026.D\data.ms (-1311) (-)

2,4,6-Tribromophenol
Concen: 1.644 ng
RT: 15.994 min Scan# 1319
Delta R.T. 0.000 min
Lab File: BN016028.D
Acq: 24 Aug 2021 12:22

Tgt Ion	Ratio	Lower	Upper
330	100		
332	0.0	0.0	0.0
141	31.4	24.6	36.8

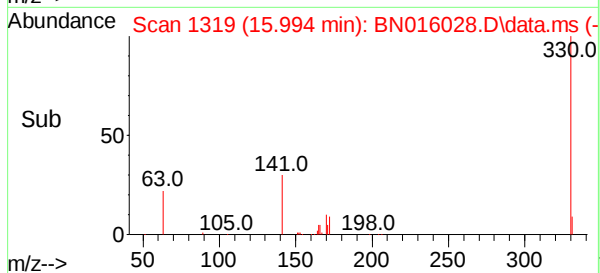

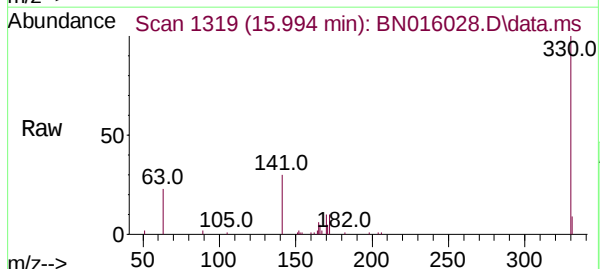
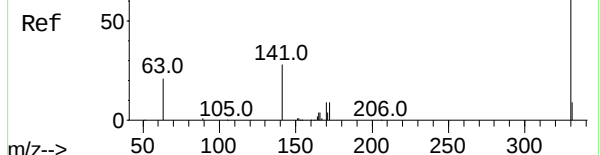


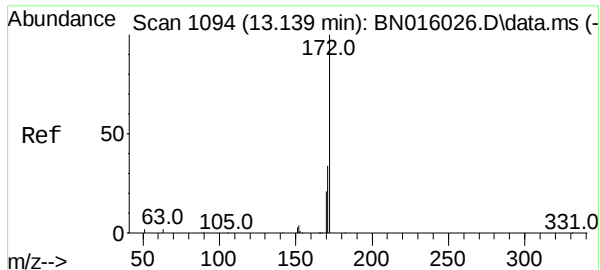

2-Fluorobiphenyl
Concen: 1.339 ng
RT: 13.140 min Scan# 1094
Delta R.T. 0.000 min
Lab File: BN016028.D
Acq: 24 Aug 2021 12:22




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6

Tgt Ion:	172	Resp:	150635
Ion	Ratio	Lower	Upper
172	100		
171	33.9	27.1	40.7
170	21.3	17.3	25.9

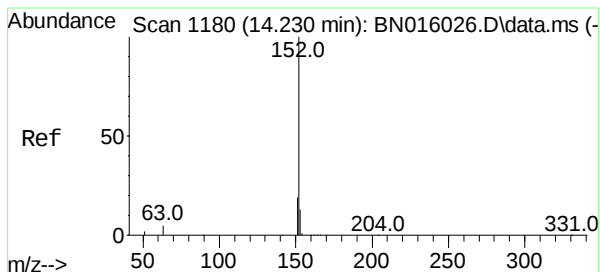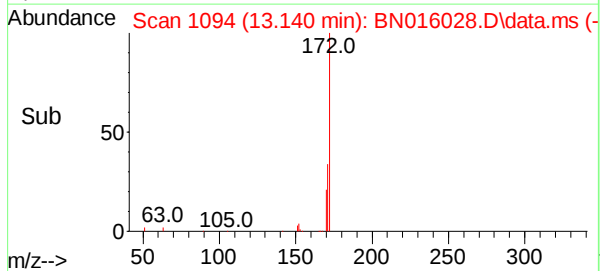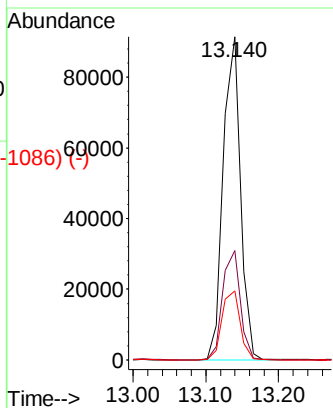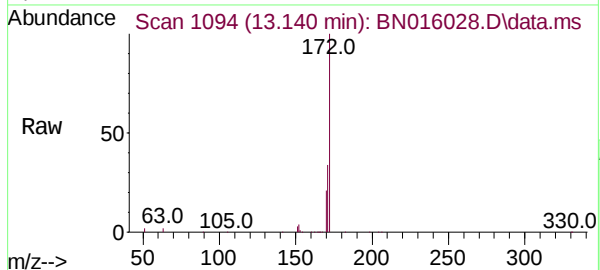

Acenaphthylene
Concen: 1.415 ng
RT: 14.231 min Scan# 1180
Delta R.T. 0.000 min
Lab File: BN016028.D
Acq: 24 Aug 2021 12:22


Tgt Ion:	152	Resp:	166412
Ion	Ratio	Lower	Upper
152	100		
151	19.4	15.3	22.9
153	13.1	10.5	15.7

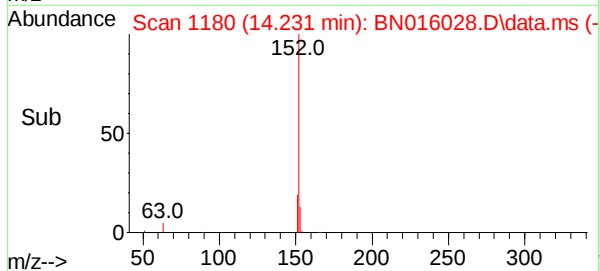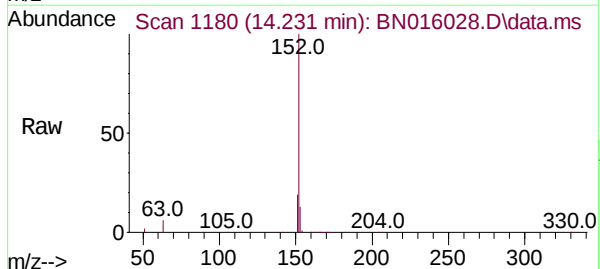



Abundance Scan 1207 (14.573 min): BN016026.D\data.ms (-1207) (-)

Acenaphthene
Concen: 1.470 ng
RT: 14.573 min Scan# 1207
Delta R.T. 0.000 min
Lab File: BN016028.D
Acq: 24 Aug 2021 12:22


Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6

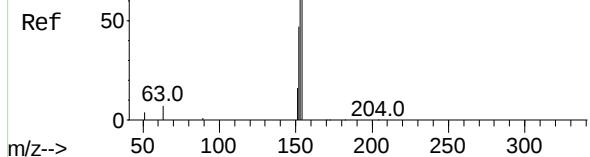

Tgt Ion	Ratio	Lower	Upper
154	100		
153	110.8	89.3	133.9
152	52.6	43.5	65.3

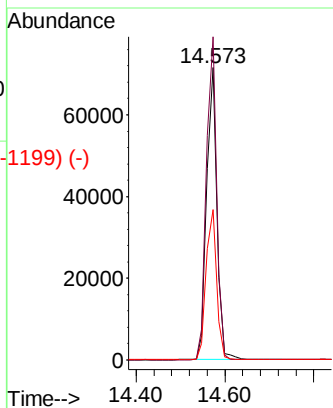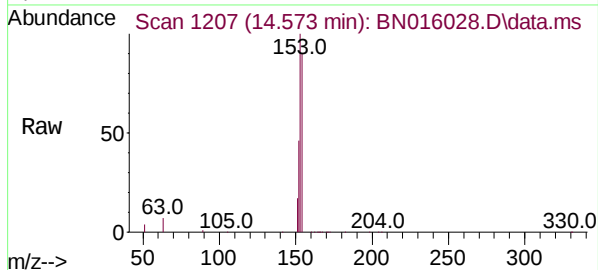


Abundance Scan 1207 (14.573 min): BN016028.D\data.ms (-1199) (-)


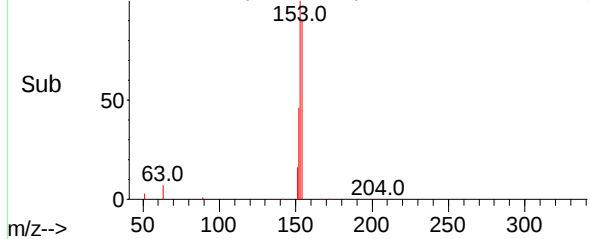


Abundance Scan 1284 (15.550 min): BN016026.D\data.ms (-1219) (-)


Fluorene
Concen: 1.476 ng
RT: 15.550 min Scan# 1284
Delta R.T. 0.000 min
Lab File: BN016028.D
Acq: 24 Aug 2021 12:22

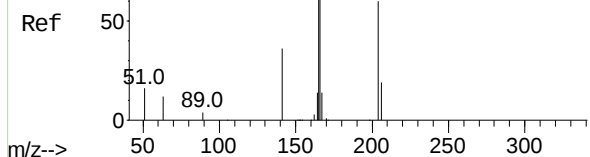

Tgt Ion	Ratio	Lower	Upper
166	100		
165	96.9	78.2	117.4
167	13.5	10.9	16.3

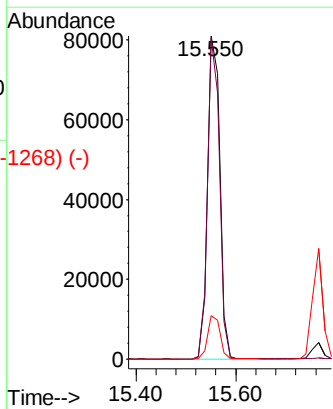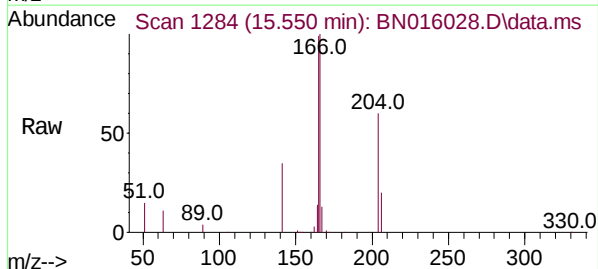


Abundance Scan 1284 (15.550 min): BN016028.D\data.ms (-1268) (-)

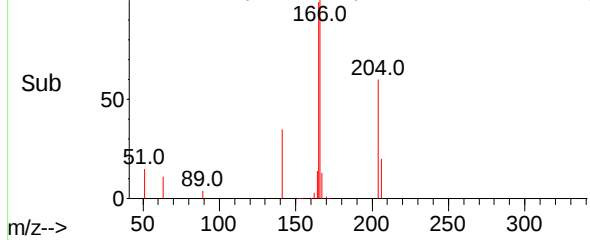



Abundance Scan 1422 (17.248 min): BN016026.D\data.ms (-1406) (-)

Phenanthrene-d10
Concen: 0.400 ng
RT: 17.249 min Scan# 1422
Delta R.T. 0.000 min
Lab File: BN016028.D
Acq: 24 Aug 2021 12:22


Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6

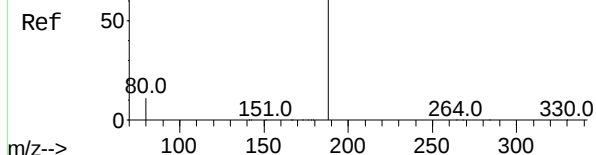

Tgt Ion:	188	Resp:	45221
Ion Ratio	Lower	Upper	
188	100		
94	0.0	0.0	0.0
80	11.7	9.0	13.6

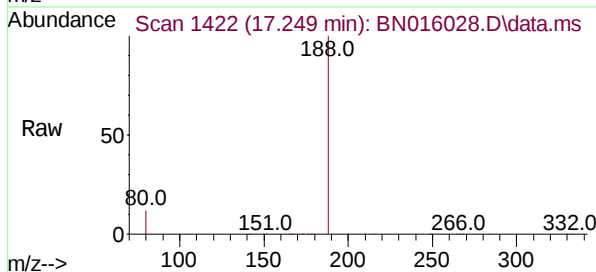


Abundance Scan 1422 (17.249 min): BN016028.D\data.ms (-1406) (-)





Abundance Scan 1291 (15.639 min): BN016026.D\data.ms (-1283) (-)

4,6-Dinitro-2-methylphenol
Concen: 1.816 ng
RT: 15.626 min Scan# 1290
Delta R.T. -0.012 min
Lab File: BN016028.D
Acq: 24 Aug 2021 12:22


Tgt Ion:	198	Resp:	6800
Ion Ratio	Lower	Upper	
198	100		
182	11.4	16.8	25.2#
77	0.0	0.0	0.0

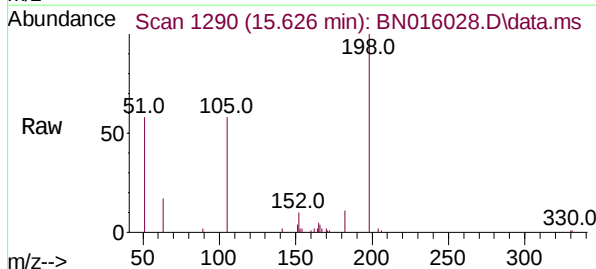

Abundance Scan 1290 (15.626 min): BN016028.D\data.ms (-1283) (-)





Abundance Scan 1356 (16.445 min): BN016026.D\data.ms (-1350) (-)

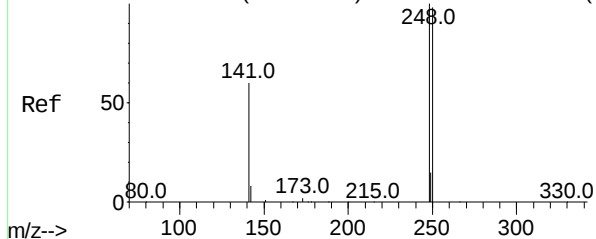


4-Bromophenyl-phenylether
Concen: 1.455 ng
RT: 16.446 min Scan# 1356
Delta R.T. 0.000 min
Lab File: BN016028.D
Acq: 24 Aug 2021 12:22

Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:	248	Resp:	38709
Ion Ratio	Lower	Upper	
248	100		
250	97.8	78.3	117.5
141	61.9	48.0	72.0

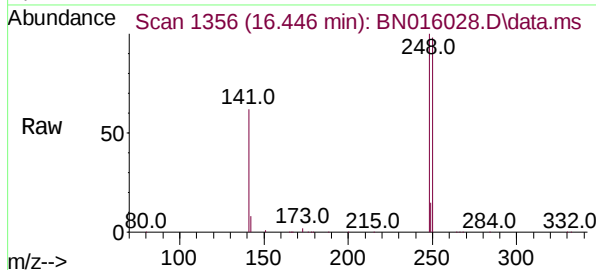

Abundance Scan 1356 (16.446 min): BN016028.D\data.ms (-1348) (-)


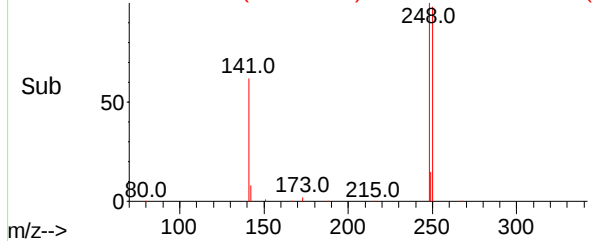


Abundance Scan 1366 (16.567 min): BN016026.D\data.ms (-1342) (-)

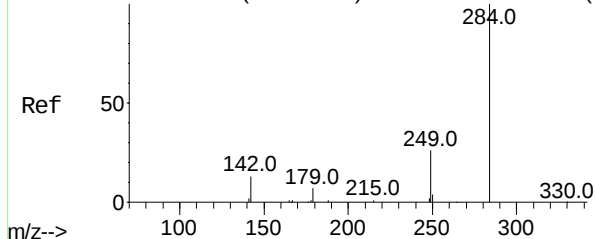


Hexachlorobenzene
Concen: 1.459 ng
RT: 16.567 min Scan# 1366
Delta R.T. 0.000 min
Lab File: BN016028.D
Acq: 24 Aug 2021 12:22

Tgt Ion:	284	Resp:	50806
Ion Ratio	Lower	Upper	
284	100		
142	29.5	23.4	35.2
249	31.2	24.4	36.6

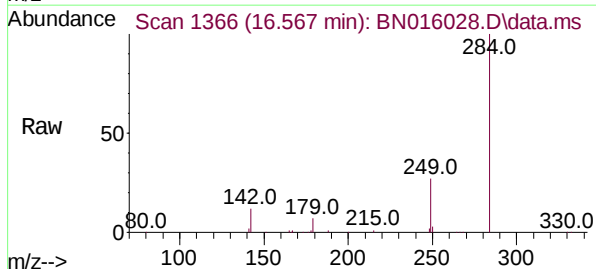


Abundance Scan 1366 (16.567 min): BN016028.D\data.ms (-1358) (-)

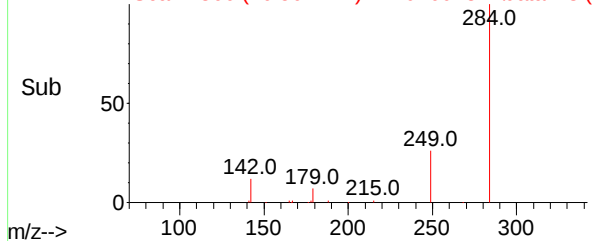



Abundance Scan 1378 (16.713 min): BN016026.D\data.ms (-1378) (-)

Atrazine
Concen: 2.089 ng
RT: 16.713 min Scan# 1378
Delta R.T. 0.000 min
Lab File: BN016028.D
Acq: 24 Aug 2021 12:22


Instrument :
BNA_N
ClientSampleId :
SSTDIC1.6

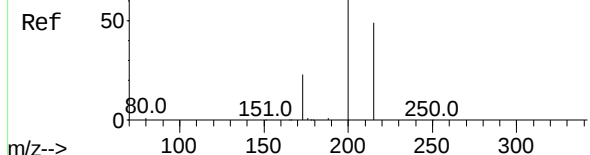

Tgt Ion	Ratio	Lower	Upper
200	100		
173	23.8	19.7	29.5
215	50.4	39.5	59.3

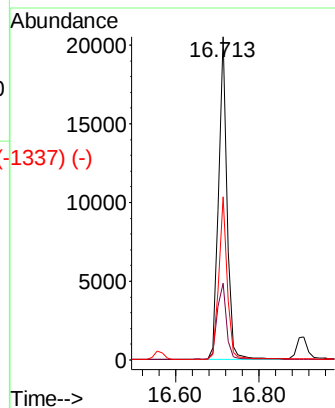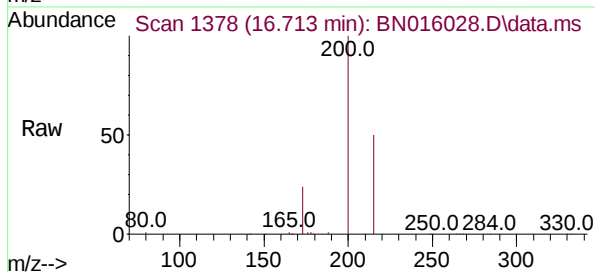



Abundance Scan 1378 (16.713 min): BN016028.D\data.ms (-1337) (-)

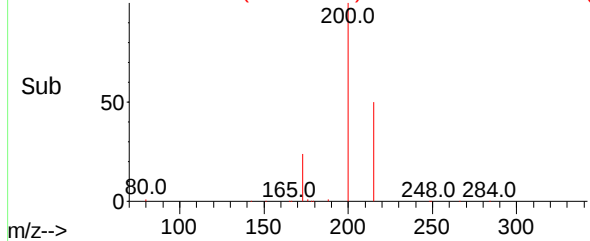


Abundance Scan 1394 (16.908 min): BN016026.D\data.ms (-1394) (-)

Pentachlorophenol
Concen: 1.834 ng
RT: 16.908 min Scan# 1394
Delta R.T. 0.000 min
Lab File: BN016028.D
Acq: 24 Aug 2021 12:22


Tgt Ion	Ratio	Lower	Upper
266	100		
264	62.7	50.2	75.4
268	63.9	51.1	76.7

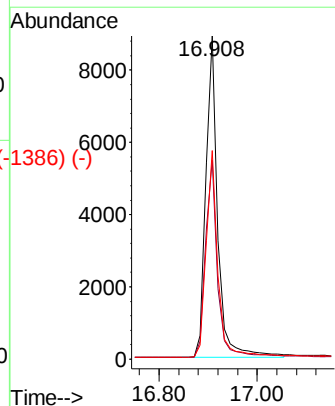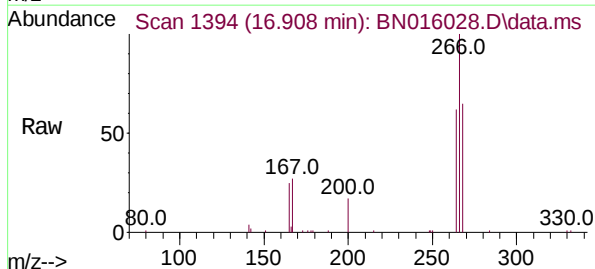

Abundance Scan 1394 (16.908 min): BN016028.D\data.ms (-1386) (-)

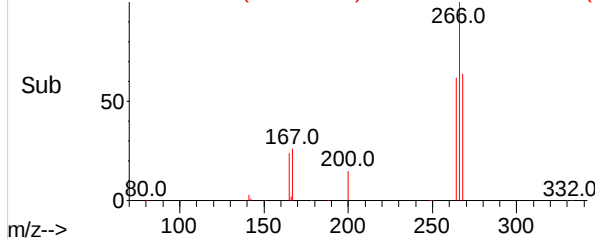



Abundance Scan 1426 (17.297 min): BN016026.D\data.ms (-1425) (-)

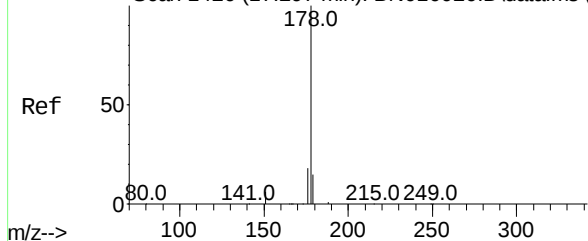


Phenanthrene
Concen: 1.467 ng
RT: 17.297 min Scan# 1426
Delta R.T. 0.000 min
Lab File: BN016028.D
Acq: 24 Aug 2021 12:22

Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:	178	Resp:	209022
Ion	Ratio	Lower	Upper
178	100		
176	18.2	14.7	22.1
179	15.4	12.6	19.0

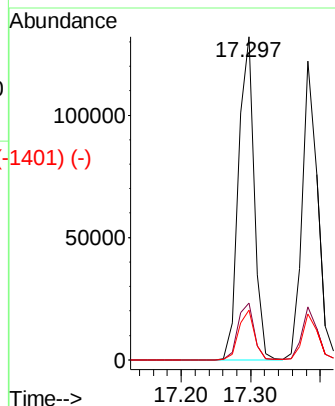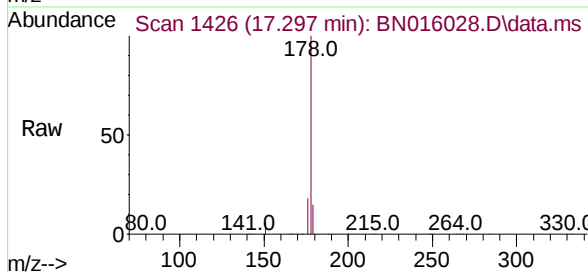

Abundance Scan 1426 (17.297 min): BN016028.D\data.ms (-1401) (-)





Abundance Scan 1433 (17.382 min): BN016026.D\data.ms (-1426) (-)

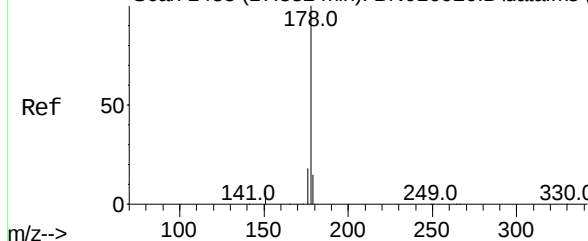


Anthracene
Concen: 1.556 ng
RT: 17.383 min Scan# 1433
Delta R.T. 0.000 min
Lab File: BN016028.D
Acq: 24 Aug 2021 12:22


Tgt Ion:	178	Resp:	188684
Ion	Ratio	Lower	Upper
178	100		
176	17.7	14.2	21.2
179	15.5	12.2	18.2

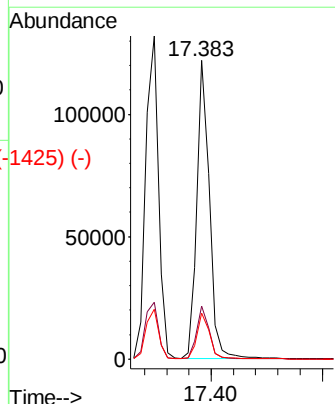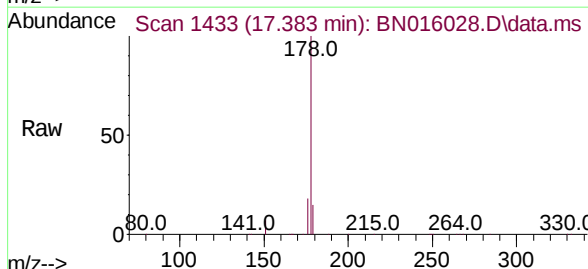

Abundance Scan 1433 (17.383 min): BN016028.D\data.ms (-1425) (-)

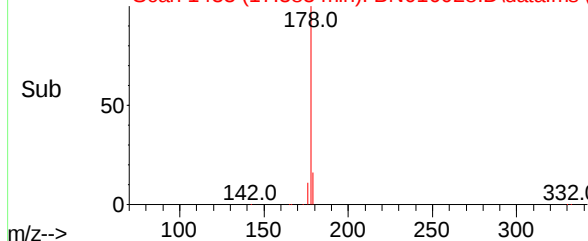




Abundance Scan 1741 (19.286 min): BN016026.D\data.ms (-1721) (-)

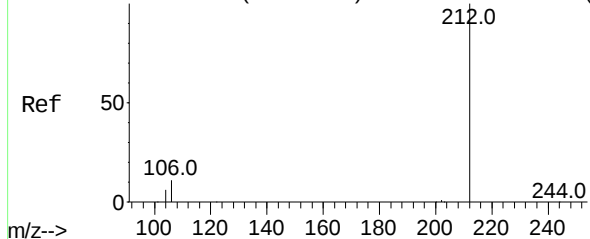


Fluoranthene-d10
Concen: 1.709 ng
RT: 19.286 min Scan# 1741
Delta R.T. 0.000 min
Lab File: BN016028.D
Acq: 24 Aug 2021 12:22

Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6

Tgt Ion:	212	Resp:	224406
Ion Ratio	Lower	Upper	
212	100		
106	11.5	9.4	14.2
104	6.5	5.4	8.0

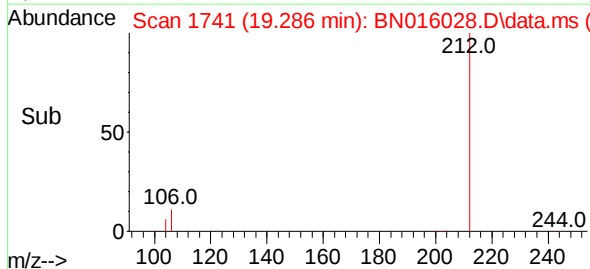
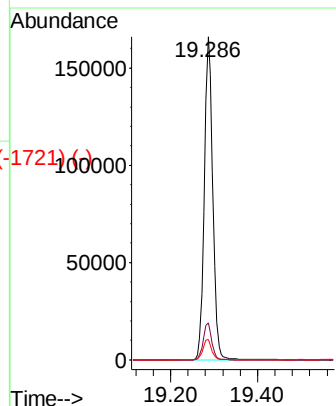
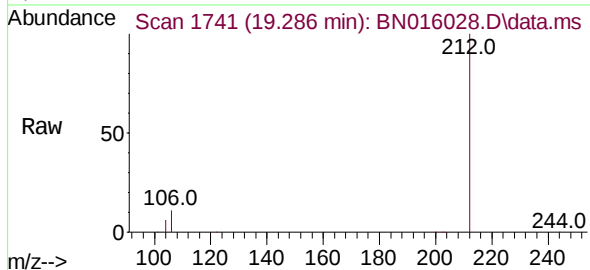


Abundance Scan 1747 (19.316 min): BN016026.D\data.ms (-1723) (-)

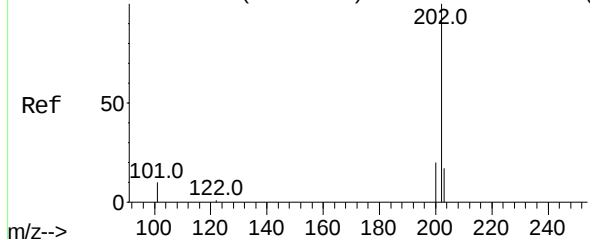


Fluoranthene
Concen: 1.519 ng
RT: 19.316 min Scan# 1747
Delta R.T. 0.000 min
Lab File: BN016028.D
Acq: 24 Aug 2021 12:22

Tgt Ion:	202	Resp:	245858
Ion Ratio	Lower	Upper	
202	100		
101	10.5	8.4	12.6
203	17.4	14.0	21.0

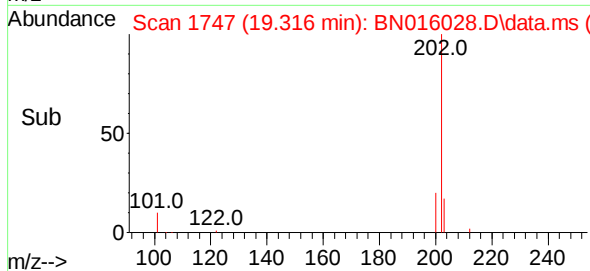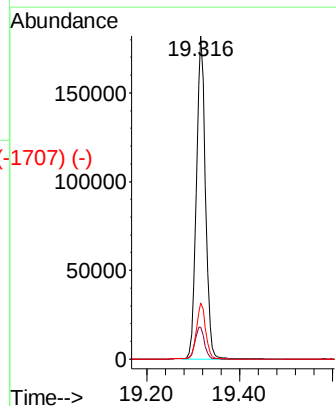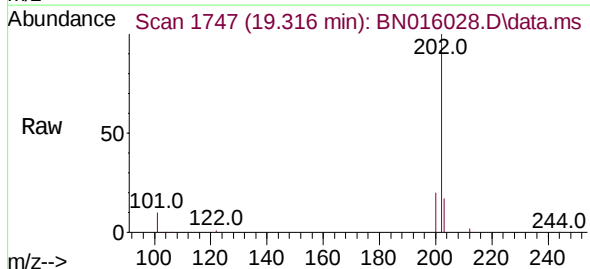




Abundance Scan 2021 (21.440 min): BN016026.D\data.ms (-2021) (-)

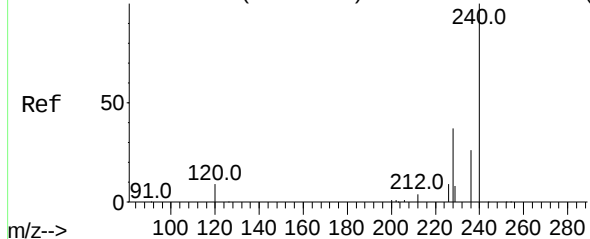


Chrysene-d12
Concen: 0.400 ng
RT: 21.450 min Scan# 2022
Delta R.T. 0.011 min
Lab File: BN016028.D
Acq: 24 Aug 2021 12:22

Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6

Tgt Ion:	240	Resp:	48665
Ion	Ratio	Lower	Upper
240	100		
120	5.0	7.8	11.6#
236	24.8	21.0	31.6

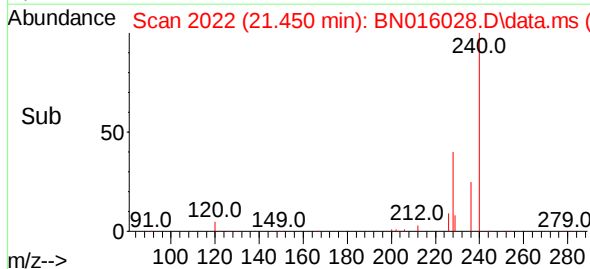
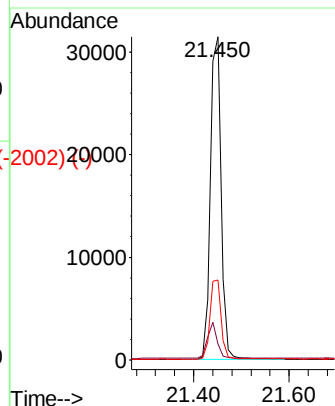
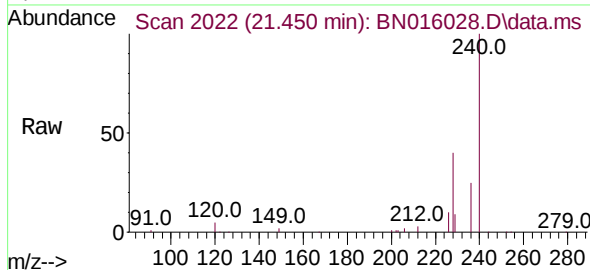


Abundance Scan 1820 (19.678 min): BN016026.D\data.ms (-1820) (-)

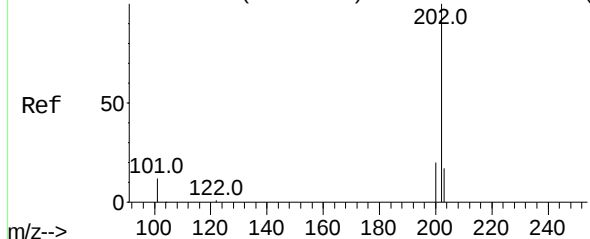

Pyrene
Concen: 1.637 ng
RT: 19.679 min Scan# 1820
Delta R.T. 0.000 min
Lab File: BN016028.D
Acq: 24 Aug 2021 12:22


Tgt Ion:	202	Resp:	241756
Ion	Ratio	Lower	Upper
202	100		
200	20.0	16.1	24.1
203	17.6	14.1	21.1

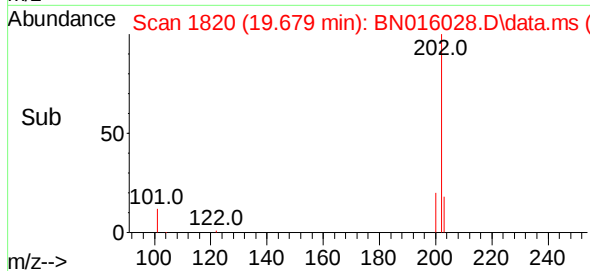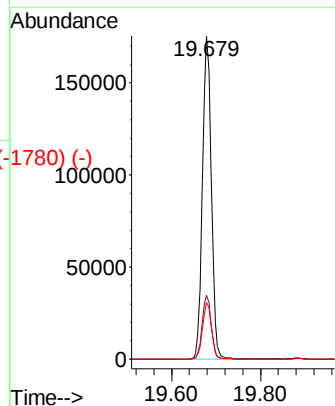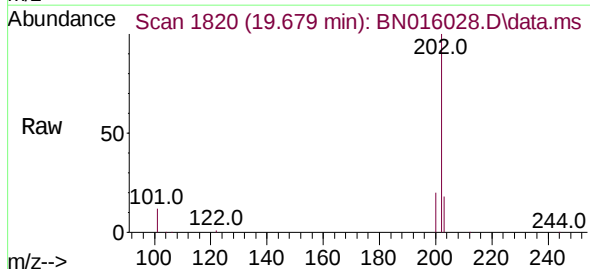



Abundance Scan 1861 (19.882 min): BN016026.D\data.ms (-1831) (-)

Terphenyl-d14
Concen: 1.711 ng
RT: 19.882 min Scan# 1861
Delta R.T. 0.000 min
Lab File: BN016028.D
Acq: 24 Aug 2021 12:22


Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6

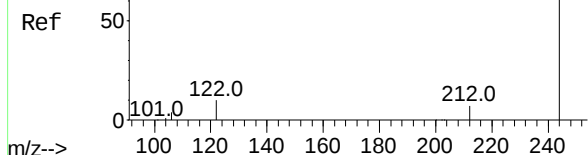

Tgt Ion:	244	Resp:	192394
Ion	Ratio	Lower	Upper
244	100		
212	7.3	6.0	9.0
122	10.3	8.5	12.7

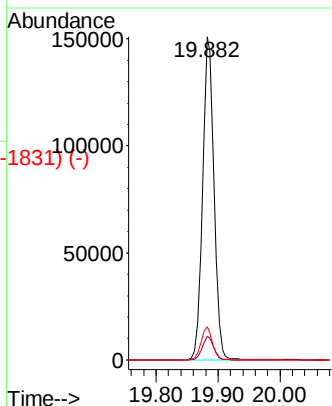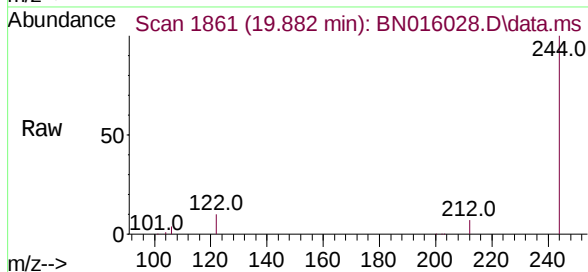



Abundance Scan 1861 (19.882 min): BN016028.D\data.ms (-1831) (-)




Abundance Scan 2020 (21.429 min): BN016026.D\data.ms (-2001) (-)

Benzo(a)anthracene
Concen: 1.637 ng
RT: 21.429 min Scan# 2020
Delta R.T. 0.000 min
Lab File: BN016028.D
Acq: 24 Aug 2021 12:22


Tgt Ion:	228	Resp:	253730
Ion	Ratio	Lower	Upper
228	100		
226	25.9	20.6	30.8
229	19.6	16.0	24.0

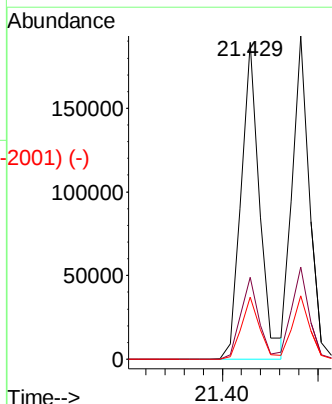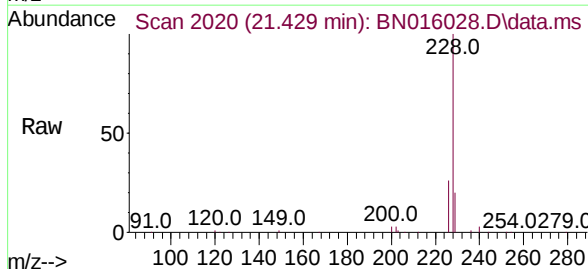

Abundance Scan 2020 (21.429 min): BN016028.D\data.ms (-2001) (-)




Abundance Scan 2025 (21.482 min): BN016026.D\data.ms (-2023) (-)

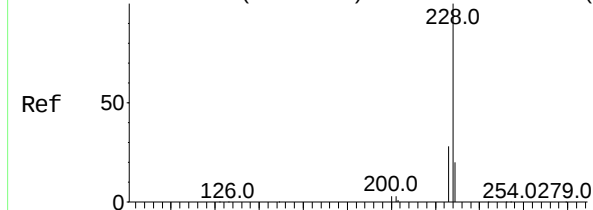


Chrysene
Concen: 1.502 ng
RT: 21.482 min Scan# 2025
Delta R.T. 0.000 min
Lab File: BN016028.D
Acq: 24 Aug 2021 12:22

Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Abundance Scan 2025 (21.482 min): BN016028.D\data.ms

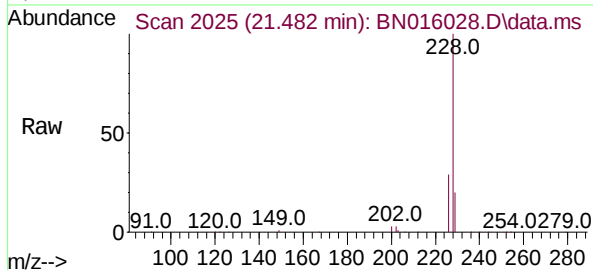


Tgt Ion	Ratio	Lower	Upper
228	100		
226	28.5	22.2	33.2
229	19.5	16.1	24.1



Abundance Scan 2025 (21.482 min): BN016028.D\data.ms (-2016) (-)

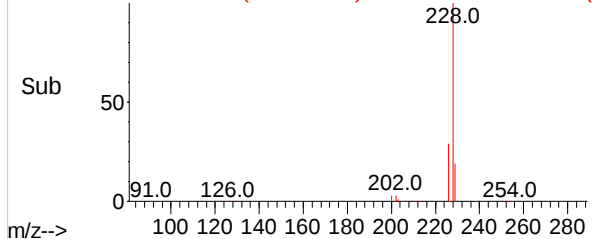



Abundance Scan 2013 (21.355 min): BN016026.D\data.ms (-2037) (-)

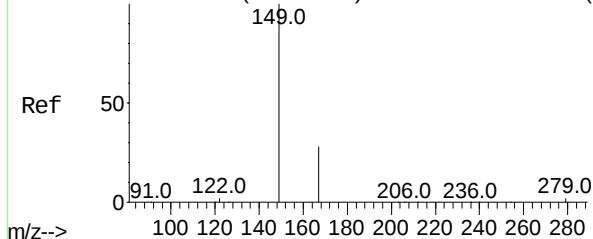


Bis(2-ethylhexyl)phthalate
Concen: 1.351 ng
RT: 21.355 min Scan# 2013
Delta R.T. 0.000 min
Lab File: BN016028.D
Acq: 24 Aug 2021 12:22

Tgt Ion	Ratio	Lower	Upper
149	100		
167	28.7	22.8	34.2
279	5.1	4.1	6.1

Abundance Scan 2013 (21.355 min): BN016028.D\data.ms

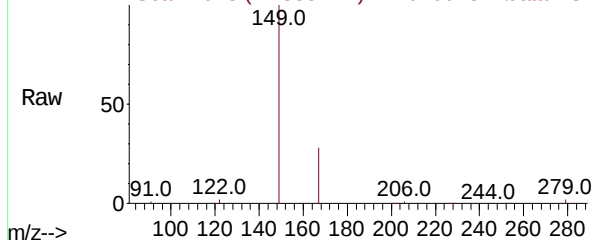



Abundance Scan 2013 (21.355 min): BN016028.D\data.ms (-2004) (-)

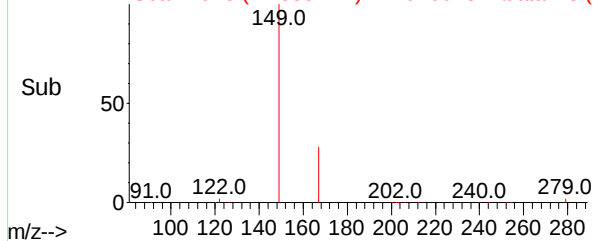


Abundance Scan 2531 (23.840 min): BN016026.D\data.ms (-2531) (-)

Perylene-d12
Concen: 0.400 ng
RT: 23.844 min Scan# 2532
Delta R.T. 0.004 min
Lab File: BN016028.D
Acq: 24 Aug 2021 12:22


Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6

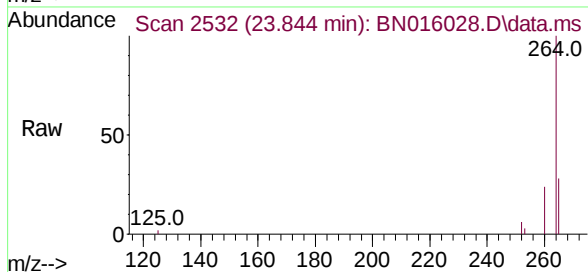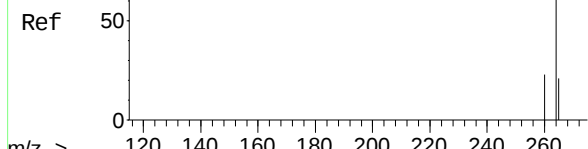

Tgt Ion	Ratio	Lower	Upper
264	100		
260	24.2	19.0	28.4
265	27.8	22.7	34.1


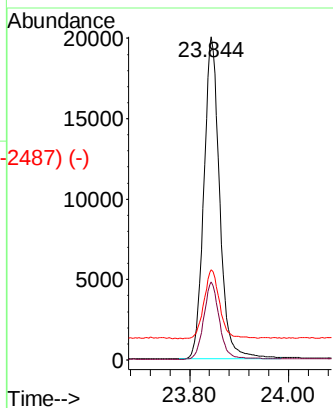


Abundance Scan 2532 (23.844 min): BN016028.D\data.ms (-2487) (-)




Abundance Scan 3255 (26.318 min): BN016026.D\data.ms (-3226) (-)


Indeno(1,2,3-cd)pyrene
Concen: 1.418 ng
RT: 26.322 min Scan# 3256
Delta R.T. 0.004 min
Lab File: BN016028.D
Acq: 24 Aug 2021 12:22

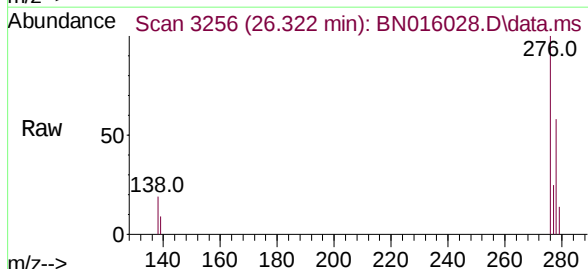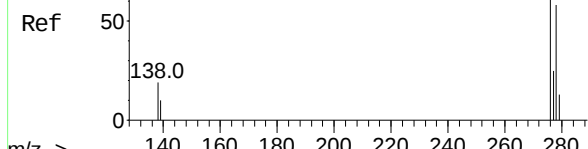


Tgt Ion	Ratio	Lower	Upper
276	100		
138	19.9	16.9	25.3
277	25.2	20.2	30.4

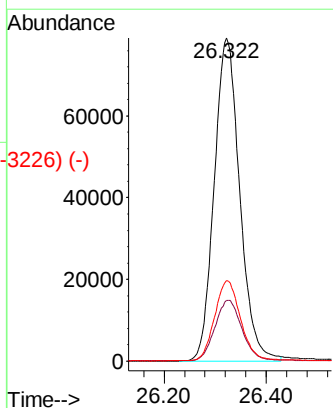

Abundance Scan 3256 (26.322 min): BN016028.D\data.ms (-3226) (-)





Abundance Scan 2318 (23.111 min): BN016026.D\data.ms (-2318) (-)

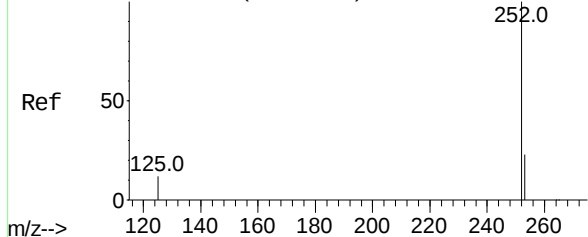


Benzo(b)fluoranthene
Concen: 1.541 ng
RT: 23.115 min Scan# 2319
Delta R.T. 0.004 min
Lab File: BN016028.D
Acq: 24 Aug 2021 12:22

Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:252 Resp: 259980
Ion Ratio Lower Upper
252 100
253 22.2 18.6 28.0
125 9.0 10.4 15.6#

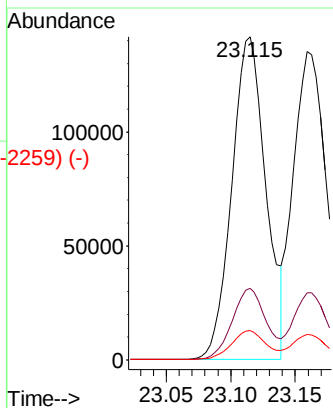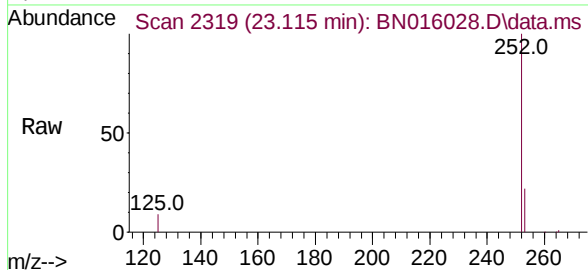

Abundance Scan 2319 (23.115 min): BN016028.D\data.ms (-2259) (-)





Abundance Scan 2331 (23.156 min): BN016026.D\data.ms (-2331) (-)




Benzo(k)fluoranthene
Concen: 1.481 ng
RT: 23.159 min Scan# 2332
Delta R.T. 0.004 min
Lab File: BN016028.D
Acq: 24 Aug 2021 12:22

Tgt Ion:252 Resp: 236376
Ion Ratio Lower Upper
252 100
253 21.9 17.9 26.9
125 8.4 7.5 11.3

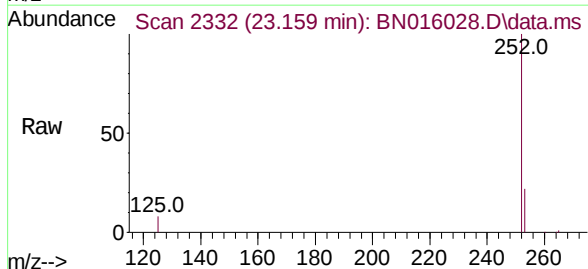


Abundance Scan 2332 (23.159 min): BN016028.D\data.ms (-2316) (-)






Abundance Scan 2500 (23.734 min): BN016026.D\data.ms (-2439) (-)

Benzo(a)pyrene
Concen: 1.501 ng
RT: 23.738 min Scan# 2501
Delta R.T. 0.004 min
Lab File: BN016028.D
Acq: 24 Aug 2021 12:22

Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6

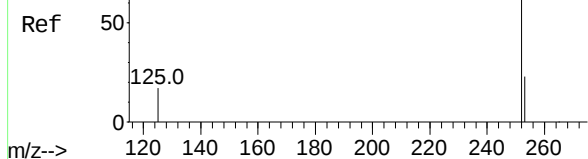


Tgt Ion	Ratio	Lower	Upper
252	100		
253	22.3	19.2	28.8
125	10.4	14.2	21.2#

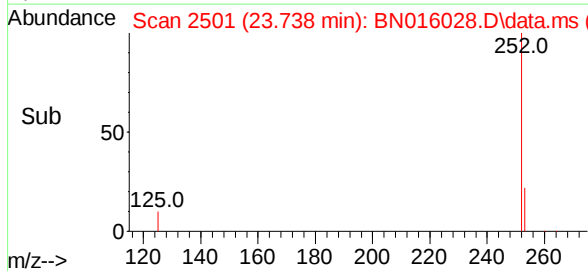
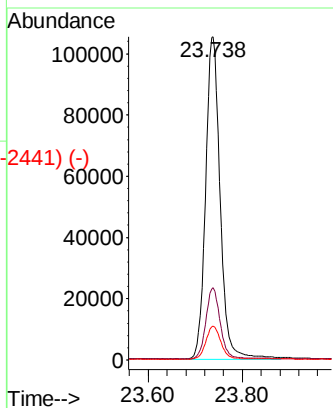
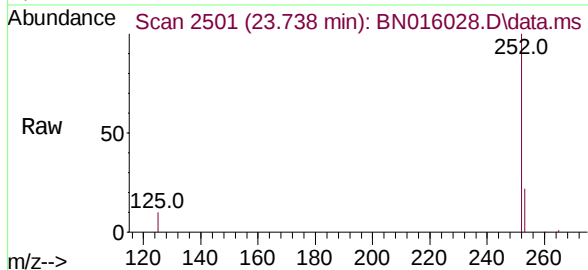


Abundance Scan 3261 (26.339 min): BN016026.D\data.ms (-3240) (-)


Dibenzo(a,h)anthracene
Concen: 1.422 ng
RT: 26.343 min Scan# 3262
Delta R.T. 0.004 min
Lab File: BN016028.D
Acq: 24 Aug 2021 12:22

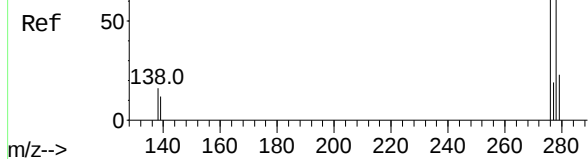

Tgt Ion	Ratio	Lower	Upper
278	100		
139	12.7	10.7	16.1
279	23.7	19.7	29.5

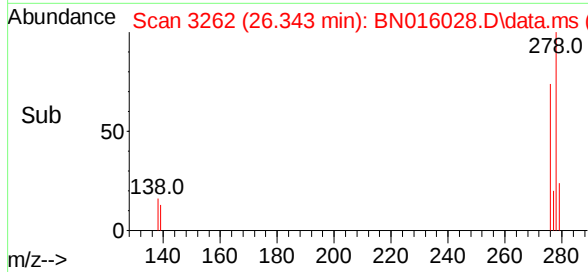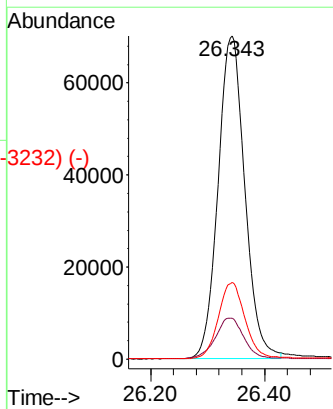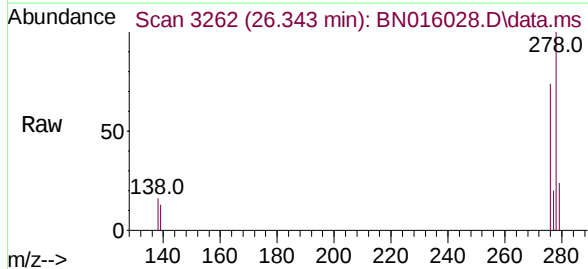


Abundance Scan 3477 (27.078 min): BN016026.D\data.ms (-3418)

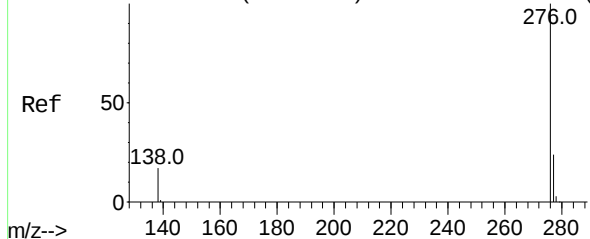


Benzo(g,h,i)perylene
Concen: 1.448 ng
RT: 27.082 min Scan# 3478
Delta R.T. 0.004 min
Lab File: BN016028.D
Acq: 24 Aug 2021 12:22

Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6

Abundance Scan 3478 (27.082 min): BN016028.D\data.ms

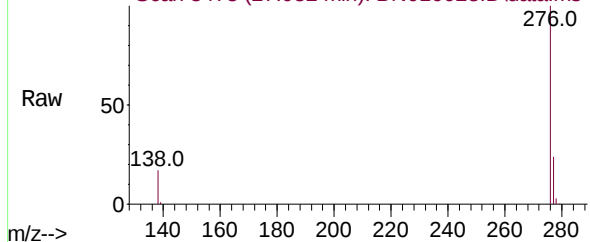

Tgt Ion:	276	Resp:	232641
Ion Ratio	Lower	Upper	
276	100		
277	23.7	19.3	28.9
138	17.3	14.0	21.0

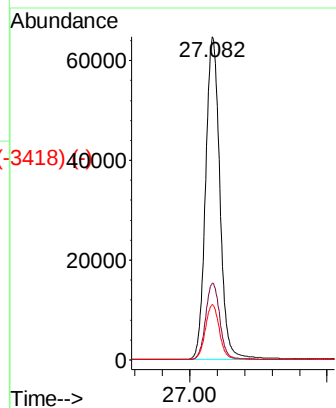

Abundance Scan 3478 (27.082 min): BN016028.D\data.ms (-3418)

