
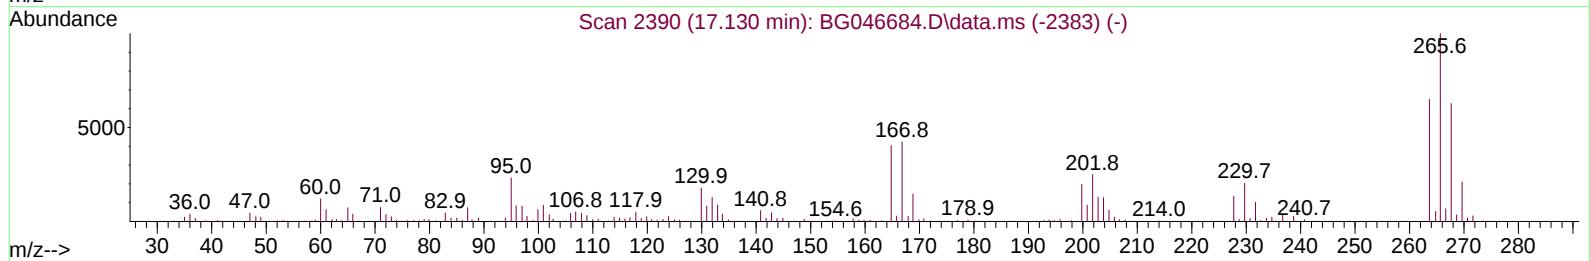
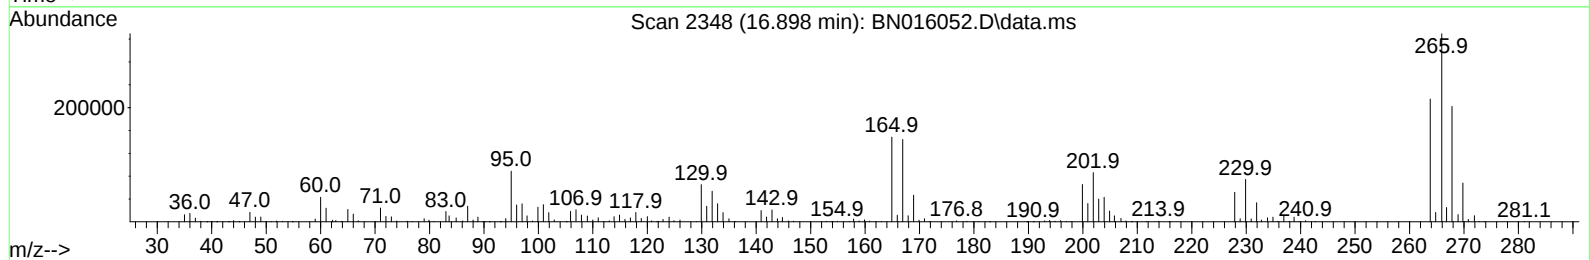


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082521\
Data File : BN016052.D
Acq On : 25 Aug 2021 05:24
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 25 07:30:10 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 24 17:12:56 2021
Response via : Initial Calibration

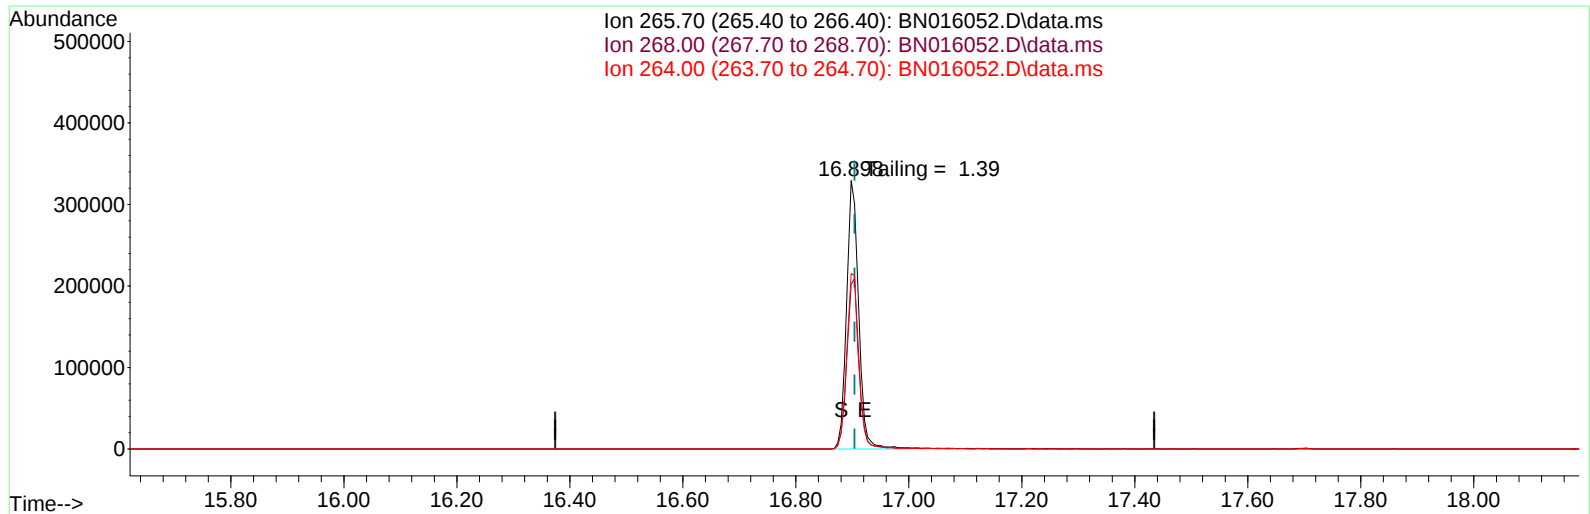

TIC: BN016052.D\data.ms

(70) Pentachlorophenol (C)




16.898min (-0.006) 20646.01 ng

response 492069

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.38
264.00	61.60	65.34
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082521\
Data File : BN016052.D
Acq On : 25 Aug 2021 05:24
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 25 07:30:10 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 24 17:12:56 2021
Response via : Initial Calibration

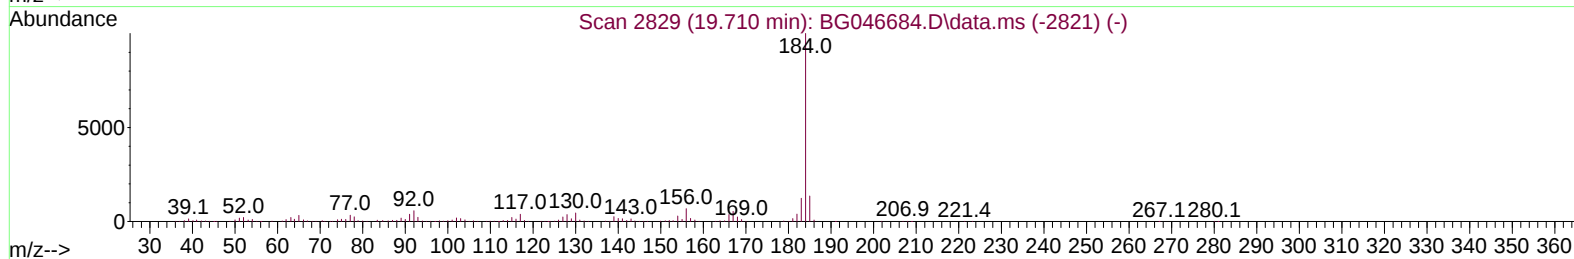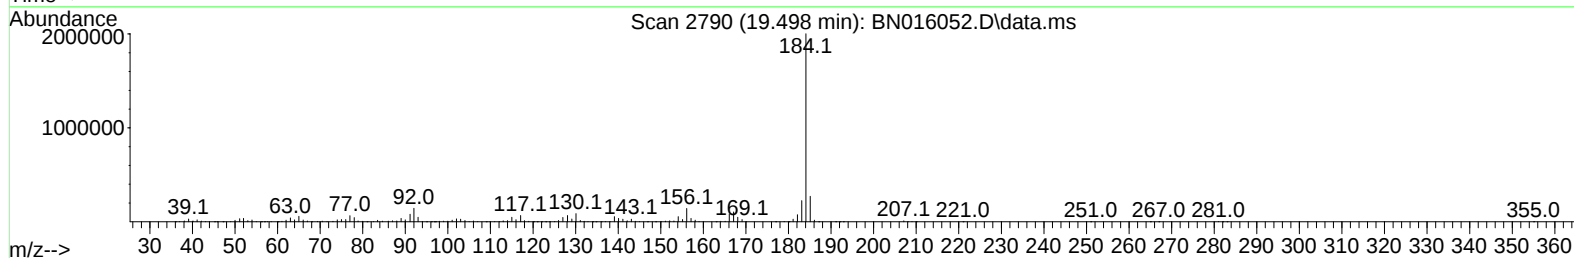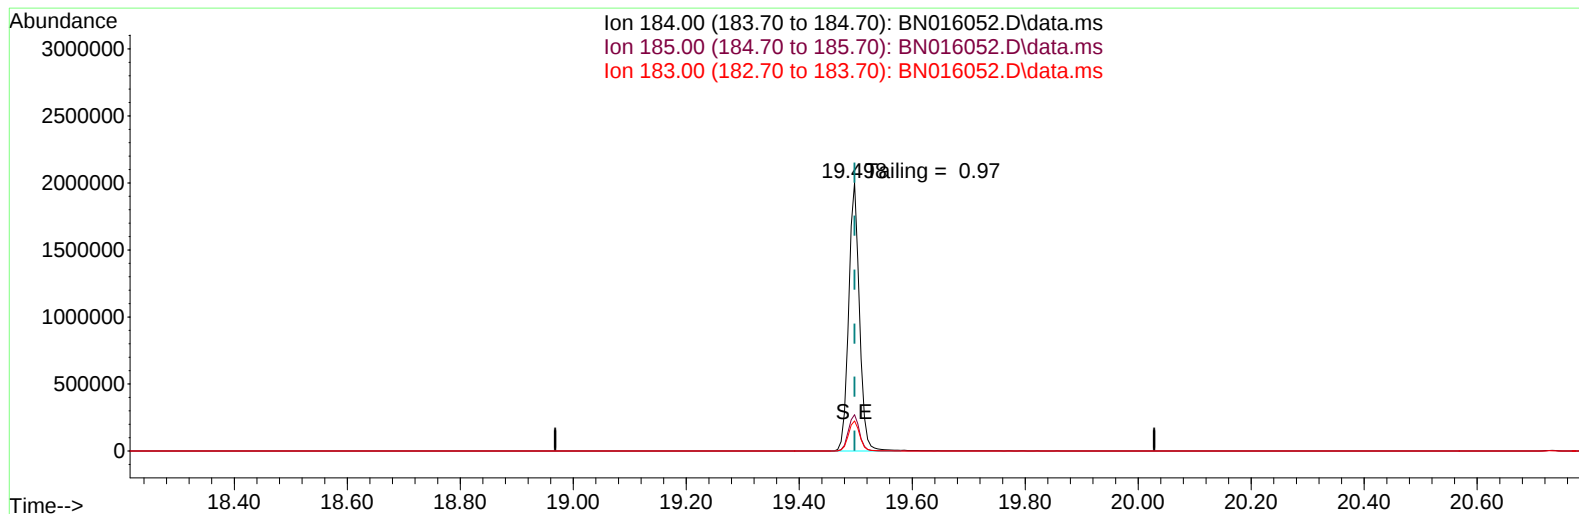

TIC: BN016052.D\data.ms

(77) Benzidine**19.498min (-0.001) 0.00 ng****response 2663350**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.54
183.00	13.20	11.21
0.00	0.00	0.00