

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082521\
 Data File : BN016031.D
 Acq On : 24 Aug 2021 14:38
 Operator : CG/JU
 Sample : SSTDICV0.4
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 ICVBN082521

Quant Time: Aug 24 15:09:43 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN082521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 24 14:26:02 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.882	152	8586	0.400	ng	0.00
7) Naphthalene-d8	10.673	136	46024	0.400	ng	#-0.01
13) Acenaphthene-d10	14.510	164	24966	0.400	ng	0.00
19) Phenanthrene-d10	17.249	188	46291	0.400	ng	0.00
29) Chrysene-d12	21.450	240	48420	0.400	ng	# 0.01
35) Perylene-d12	23.850	264	44642	0.400	ng	0.01
System Monitoring Compounds						
4) 2-Fluorophenol	5.457	112	8747	0.426	ng	0.00
5) Phenol-d6	7.043	99	12173	0.425	ng	0.00
8) Nitrobenzene-d5	9.038	82	12499	0.413	ng	0.00
11) 2-Methylnaphthalene-d10	12.265	152	27983	0.403	ng	0.00
14) 2,4,6-Tribromophenol	15.994	330	2864	0.404	ng	0.00
15) 2-Fluorobiphenyl	13.139	172	36147	0.360	ng	0.00
27) Fluoranthene-d10	19.286	212	50926	0.390	ng	0.00
31) Terphenyl-d14	19.887	244	45605	0.384	ng	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.391	88	1972	0.418	ng	99
3) n-Nitrosodimethylamine	3.742	42	3144	0.425	ng	# 93
6) bis(2-Chloroethyl)ether	7.310	93	9803	0.409	ng	99
9) Naphthalene	10.723	128	46550	0.385	ng	100
10) Hexachlorobutadiene	11.015	225	10675	0.397	ng	# 100
12) 2-Methylnaphthalene	12.340	142	30640	0.397	ng	100
16) Acenaphthylene	14.230	152	35152	0.383	ng	99
17) Acenaphthene	14.573	154	26294	0.374	ng	99
18) Fluorene	15.550	166	31424	0.374	ng	99
20) 4,6-Dinitro-2-methylph...	15.639	198	1188	0.452	ng	92
21) 4-Bromophenyl-phenylether	16.445	248	8205	0.353	ng	96
22) Hexachlorobenzene	16.567	284	12142	0.372	ng	99
23) Atrazine	16.713	200	6135	0.438	ng	98
24) Pentachlorophenol	16.908	266	3141	0.367	ng	98
25) Phenanthrene	17.297	178	49105	0.373	ng	100
26) Anthracene	17.382	178	40903	0.379	ng	100
28) Fluoranthene	19.321	202	55750	0.382	ng	100
30) Pyrene	19.683	202	56384	0.392	ng	100
32) Benzo(a)anthracene	21.429	228	56477	0.384	ng	99
33) Chrysene	21.482	228	57828	0.372	ng	98
34) Bis(2-ethylhexyl)phtha...	21.365	149	16704	0.426	ng	100
36) Indeno(1,2,3-cd)pyrene	26.329	276	62019	0.367	ng	100
37) Benzo(b)fluoranthene	23.118	252	59615	0.373	ng	100
38) Benzo(k)fluoranthene	23.166	252	56004	0.376	ng	99
39) Benzo(a)pyrene	23.744	252	52415	0.380	ng	100
40) Dibenzo(a,h)anthracene	26.349	278	51530	0.369	ng	99
41) Benzo(g,h,i)perylene	27.092	276	53025	0.367	ng	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082521\
Data File : BN016031.D
Acq On : 24 Aug 2021 14:38
Operator : CG/JU
Sample : SSTDICV0.4
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
ICVBN082521

Quant Time: Aug 24 15:09:43 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN082521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 24 14:26:02 2021
Response via : Initial Calibration

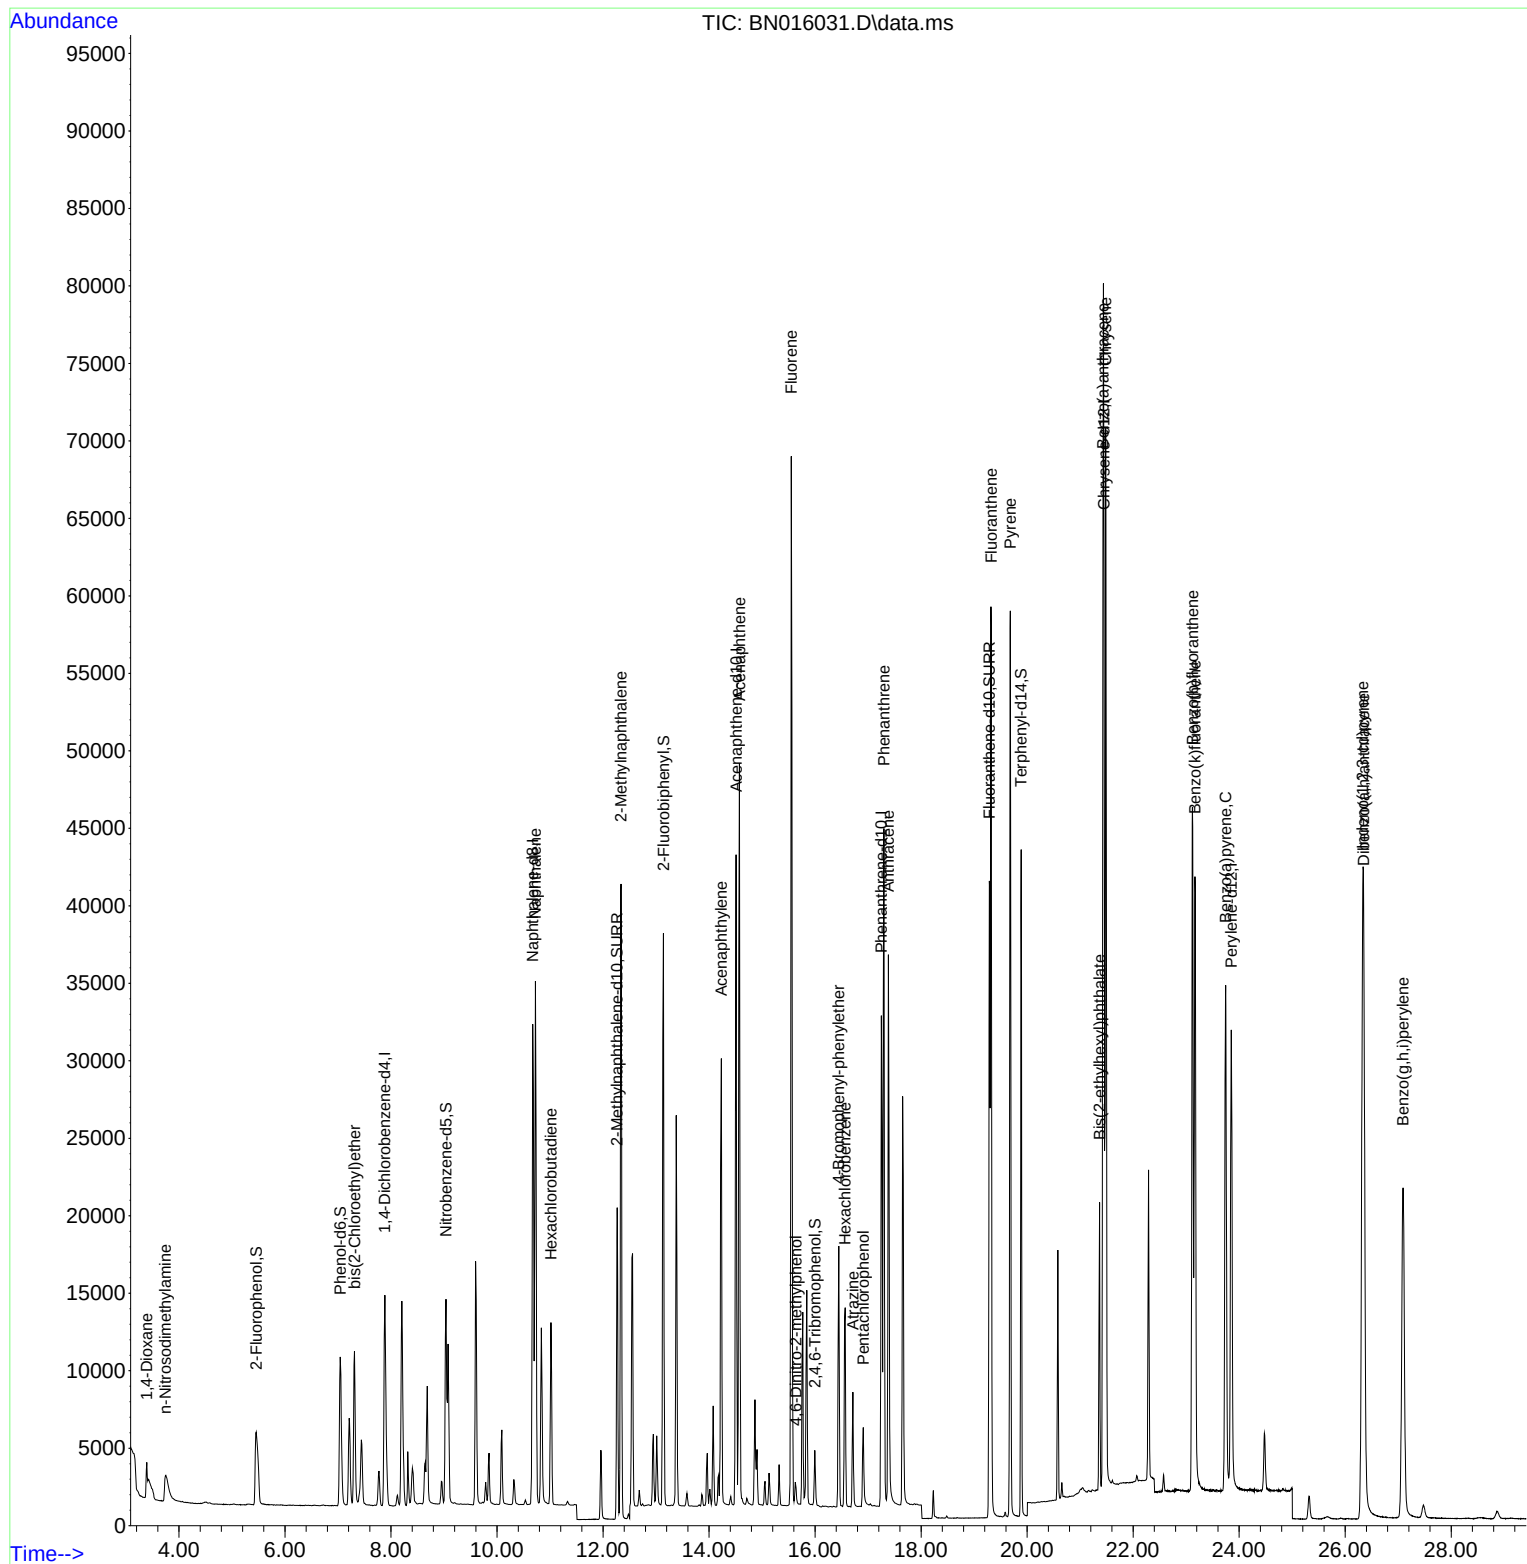







#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.882 min Scan# 521
 Delta R.T. -0.000 min
 Lab File: BN016031.D
 Acq: 24 Aug 2021 14:38

Instrument :
 BNA_N
 ClientSampleId :
 ICVBN082521

Tgt Ion: 152 Resp: 8586




Ion	Ratio	Lower	Upper
152	100		
150	154.5	126.5	189.7
115	67.3	56.5	84.7

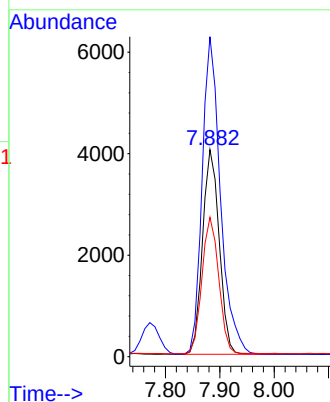


#2
 1,4-Dioxane
 Concen: 0.418 ng
 RT: 3.391 min Scan# 34
 Delta R.T. 0.000 min
 Lab File: BN016031.D
 Acq: 24 Aug 2021 14:38

Tgt Ion: 88 Resp: 1972

Ion	Ratio	Lower	Upper
88	100		
43	25.5	21.0	31.4
58	67.5	54.8	82.2







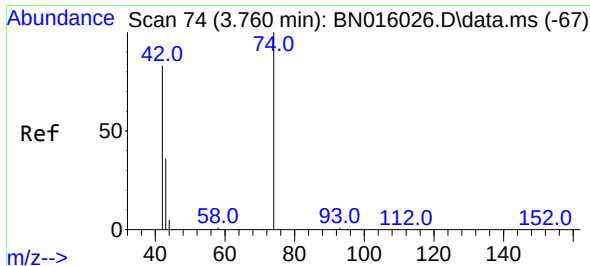

#3
n-Nitrosodimethylamine
Concen: 0.425 ng
RT: 3.742 min Scan# 72
Delta R.T. -0.018 min
Lab File: BN016031.D
Acq: 24 Aug 2021 14:38




Instrument :
BNA_N
ClientSampleId :
ICVBN082521


Tgt Ion: 42 Resp: 3144
Ion Ratio Lower Upper
42 100
74 123.8 93.8 140.8
44 3.5 7.7 11.5#

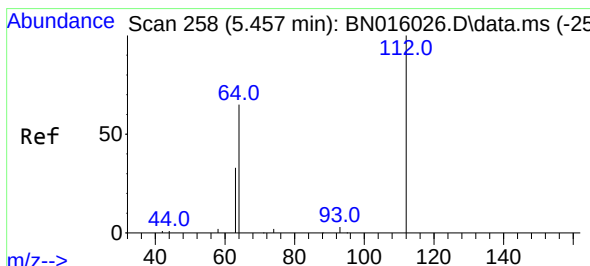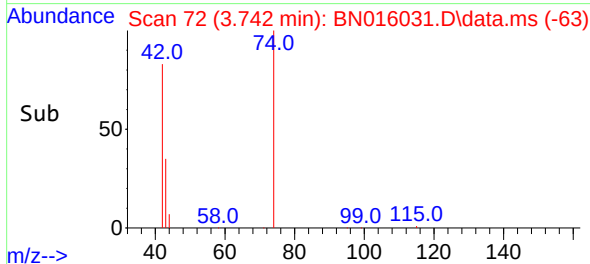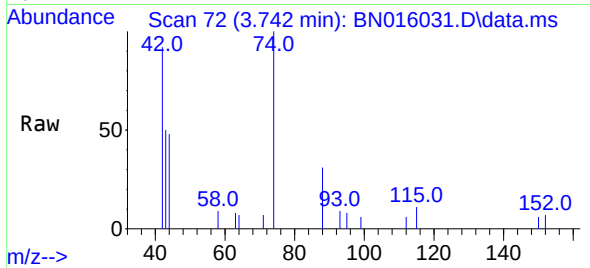

#4
2-Fluorophenol
Concen: 0.426 ng
RT: 5.457 min Scan# 258
Delta R.T. 0.000 min
Lab File: BN016031.D
Acq: 24 Aug 2021 14:38

Tgt Ion: 112 Resp: 8747
Ion Ratio Lower Upper
112 100
64 66.2 52.5 78.7
63 33.8 26.9 40.3


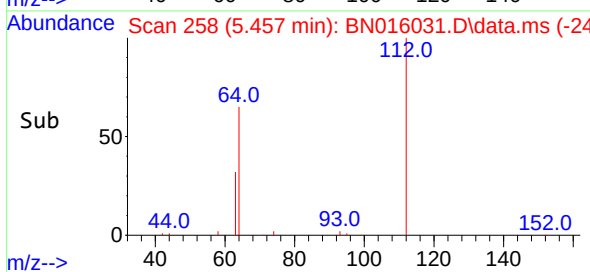

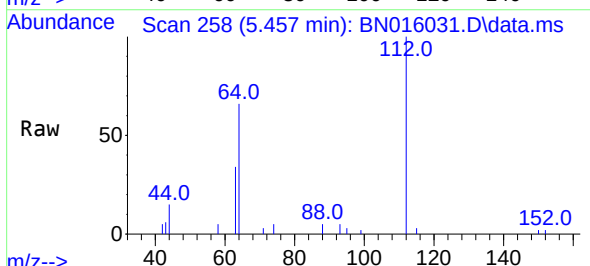




#5
Phenol-d6
Concen: 0.425 ng
RT: 7.043 min Scan# 430
Delta R.T. -0.009 min
Lab File: BN016031.D
Acq: 24 Aug 2021 14:38




Instrument :
BNA_N
ClientSampleId :
ICVBN082521


Tgt Ion: 99 Resp: 12173
Ion Ratio Lower Upper
99 100
42 19.1 15.6 23.4
71 37.9 29.8 44.8



#6
bis(2-Chloroethyl)ether
Concen: 0.409 ng
RT: 7.310 min Scan# 459
Delta R.T. 0.000 min
Lab File: BN016031.D
Acq: 24 Aug 2021 14:38

Tgt Ion: 93 Resp: 9803
Ion Ratio Lower Upper
93 100
63 76.9 62.0 93.0
95 33.3 26.2 39.4



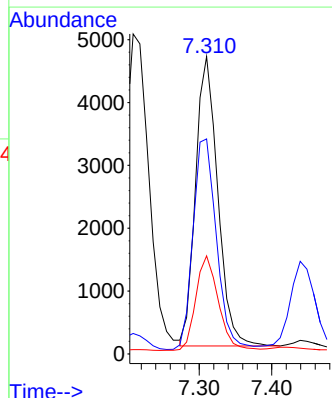





#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.673 min Scan# 754
Delta R.T. -0.013 min
Lab File: BN016031.D
Acq: 24 Aug 2021 14:38




Instrument :
BNA_N
ClientSampleId :
ICVBN082521


Tgt Ion:	136	Resp:	46024
Ion Ratio	Lower	Upper	
136	100		
137	11.1	8.9	13.3
54	9.5	4.2	6.4#
68	7.3	3.4	5.2#



#8
Nitrobenzene-d5
Concen: 0.413 ng
RT: 9.038 min Scan# 625
Delta R.T. 0.000 min
Lab File: BN016031.D
Acq: 24 Aug 2021 14:38

Tgt Ion:	82	Resp:	12499
Ion Ratio	Lower	Upper	
82	100		
128	37.0	27.7	41.5
54	47.2	39.4	59.2


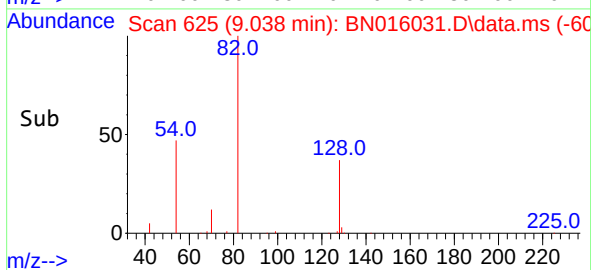




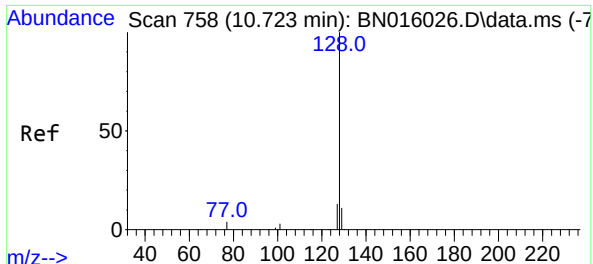

#9
Naphthalene
Concen: 0.385 ng
RT: 10.723 min Scan# 758
Delta R.T. 0.000 min
Lab File: BN016031.D
Acq: 24 Aug 2021 14:38




Instrument :
BNA_N
ClientSampleId :
ICVBN082521


Tgt Ion:	128	Resp:	46550
Ion	Ratio	Lower	Upper
128	100		
129	11.1	8.9	13.3
127	13.5	10.7	16.1

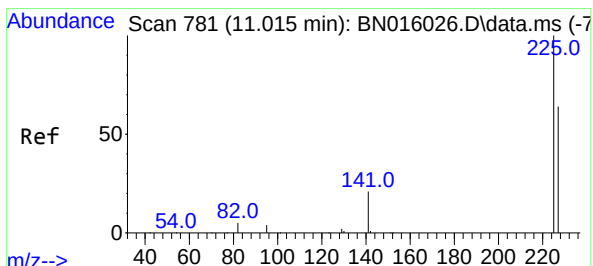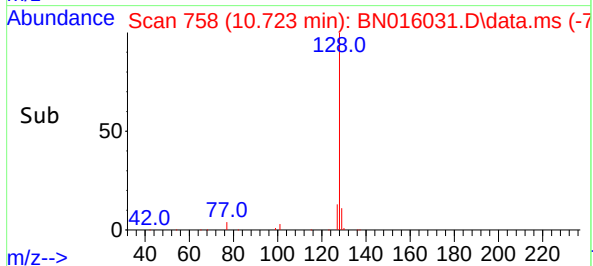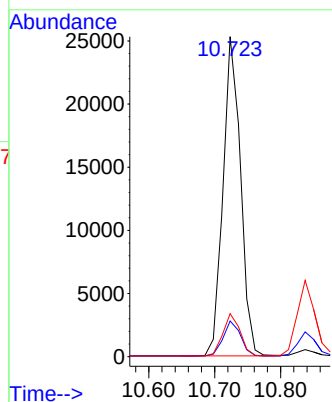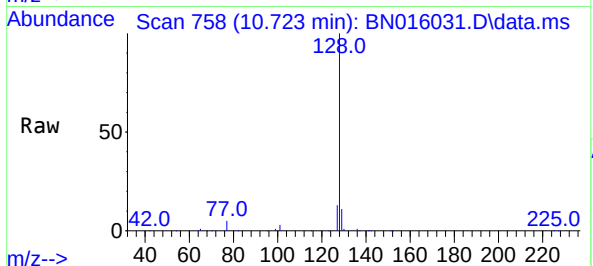

#10
Hexachlorobutadiene
Concen: 0.397 ng
RT: 11.015 min Scan# 781
Delta R.T. 0.000 min
Lab File: BN016031.D
Acq: 24 Aug 2021 14:38

Tgt Ion:	225	Resp:	10675
Ion	Ratio	Lower	Upper
225	100		
223	0.0	0.0	0.0
227	64.1	51.5	77.3


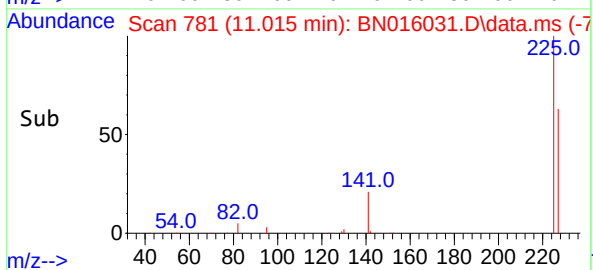
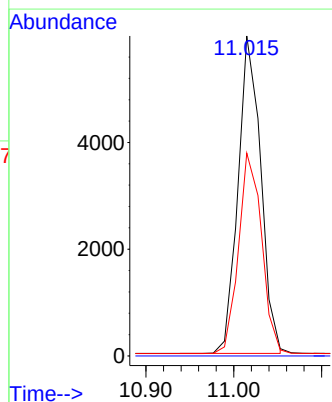
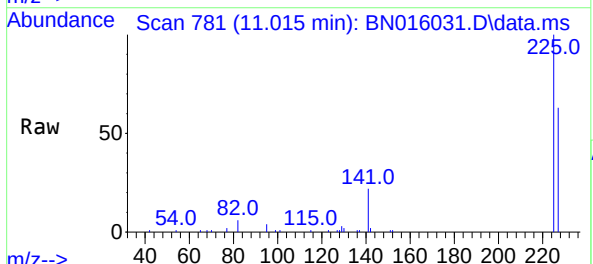


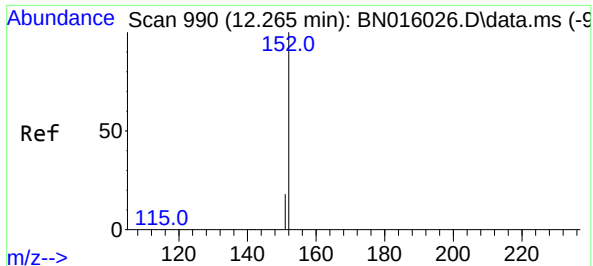

#11
2-Methylnaphthalene-d10
Concen: 0.403 ng
RT: 12.265 min Scan# 990
Delta R.T. 0.000 min
Lab File: BN016031.D
Acq: 24 Aug 2021 14:38




Instrument :
BNA_N
ClientSampleId :
ICVBN082521


Tgt Ion:152 Resp: 27983
Ion Ratio Lower Upper
152 100
151 20.4 16.6 24.8

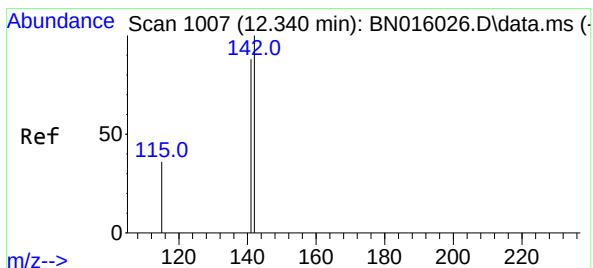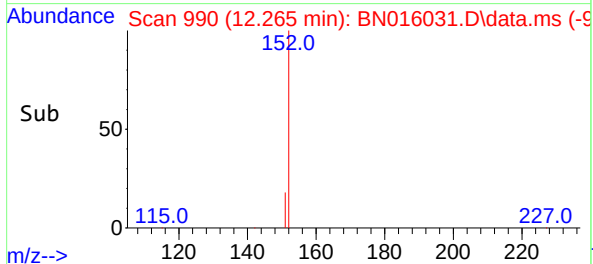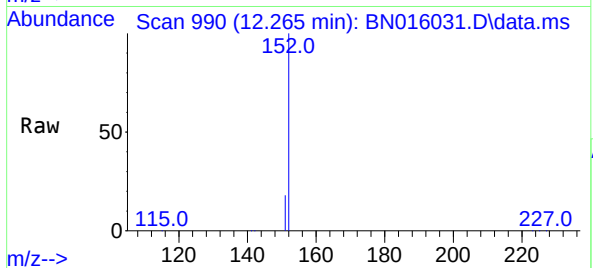

#12
2-Methylnaphthalene
Concen: 0.397 ng
RT: 12.340 min Scan# 1007
Delta R.T. 0.000 min
Lab File: BN016031.D
Acq: 24 Aug 2021 14:38

Tgt Ion:142 Resp: 30640
Ion Ratio Lower Upper
142 100
141 88.0 70.3 105.5
115 35.9 28.7 43.1


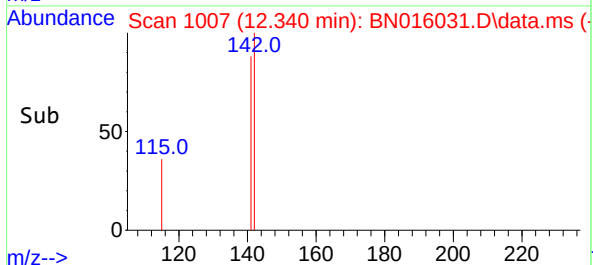

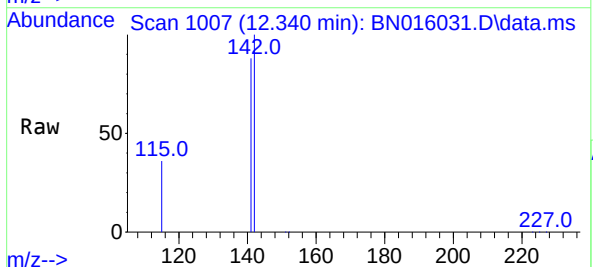




#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.510 min Scan# 1202
Delta R.T. 0.000 min
Lab File: BN016031.D
Acq: 24 Aug 2021 14:38




Instrument :
BNA_N
ClientSampleId :
ICVBN082521


Tgt Ion:164 Resp: 24966
Ion Ratio Lower Upper
164 100
162 99.3 80.2 120.4
160 43.9 35.9 53.9

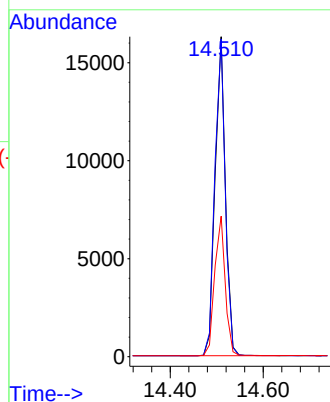

#14
2,4,6-Tribromophenol
Concen: 0.404 ng
RT: 15.994 min Scan# 1319
Delta R.T. -0.000 min
Lab File: BN016031.D
Acq: 24 Aug 2021 14:38

Tgt Ion:330 Resp: 2864
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 32.0 24.6 36.8









#15
2-Fluorobiphenyl
Concen: 0.360 ng
RT: 13.139 min Scan# 1094
Delta R.T. 0.000 min
Lab File: BN016031.D
Acq: 24 Aug 2021 14:38




Instrument :
BNA_N
ClientSampleId :
ICVBN082521


Tgt Ion:172 Resp: 36147
Ion Ratio Lower Upper
172 100
171 34.3 27.1 40.7
170 21.4 17.3 25.9



#16
Acenaphthylene
Concen: 0.383 ng
RT: 14.230 min Scan# 1180
Delta R.T. 0.000 min
Lab File: BN016031.D
Acq: 24 Aug 2021 14:38

Tgt Ion:152 Resp: 35152
Ion Ratio Lower Upper
152 100
151 19.5 15.3 22.9
153 13.1 10.5 15.7



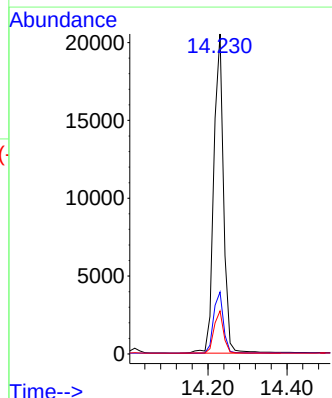





#17
Acenaphthene
Concen: 0.374 ng
RT: 14.573 min Scan# 1207
Delta R.T. 0.000 min
Lab File: BN016031.D
Acq: 24 Aug 2021 14:38




Instrument :
BNA_N
ClientSampleId :
ICVBN082521


Tgt Ion:	154	Resp:	26294
Ion	Ratio	Lower	Upper
154	100		
153	111.8	89.3	133.9
152	53.1	43.5	65.3

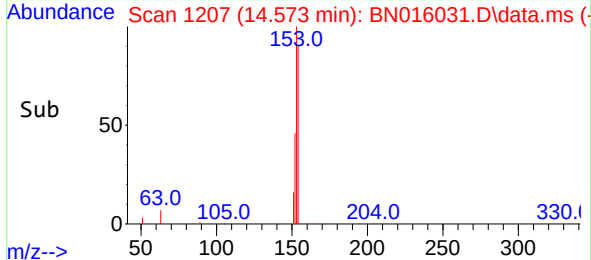

#18
Fluorene
Concen: 0.374 ng
RT: 15.550 min Scan# 1284
Delta R.T. 0.000 min
Lab File: BN016031.D
Acq: 24 Aug 2021 14:38

Tgt Ion:	166	Resp:	31424
Ion	Ratio	Lower	Upper
166	100		
165	96.9	78.2	117.4
167	13.5	10.9	16.3


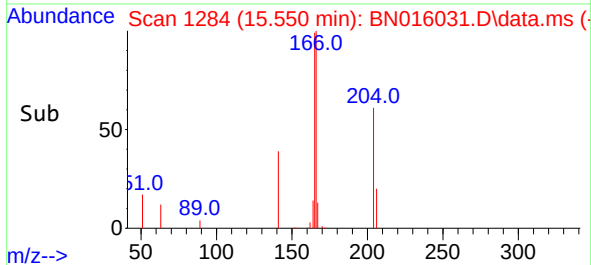

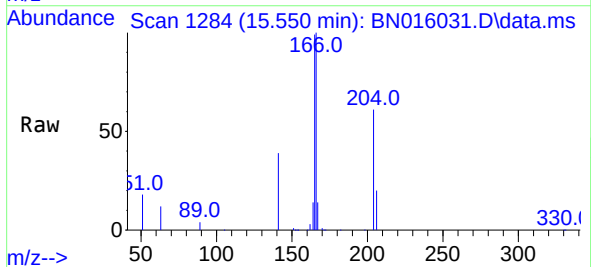


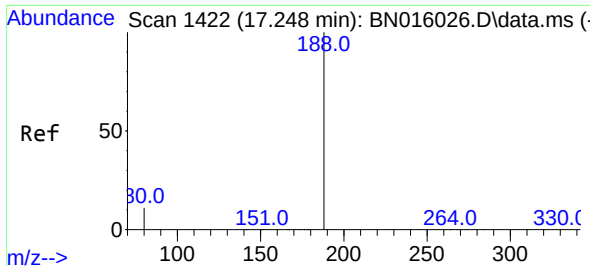

#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.249 min Scan# 1422
Delta R.T. 0.000 min
Lab File: BN016031.D
Acq: 24 Aug 2021 14:38




Instrument :
BNA_N
ClientSampleId :
ICVBN082521


Tgt Ion:188	Resp:	46291
Ion Ratio	Lower	Upper
188	100	
94	0.0	0.0
80	12.1	9.0 13.6

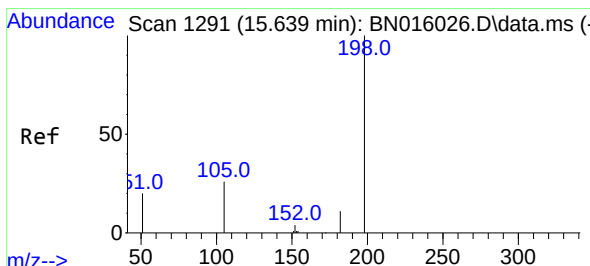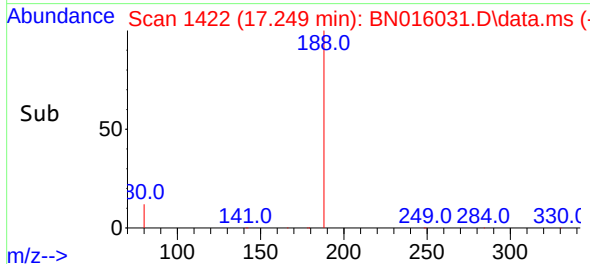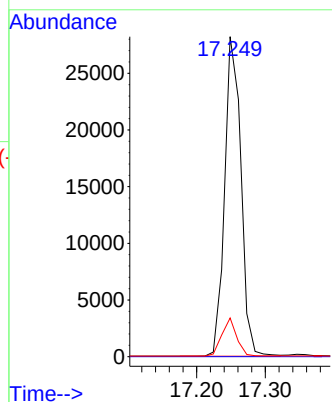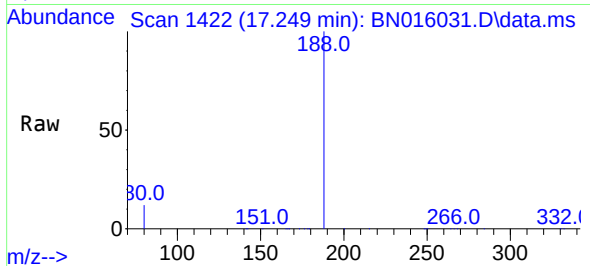

#20
4,6-Dinitro-2-methylphenol
Concen: 0.452 ng
RT: 15.639 min Scan# 1291
Delta R.T. -0.000 min
Lab File: BN016031.D
Acq: 24 Aug 2021 14:38

Tgt Ion:198	Resp:	1188
Ion Ratio	Lower	Upper
198	100	
182	17.4	16.8 25.2
77	0.0	0.0 0.0


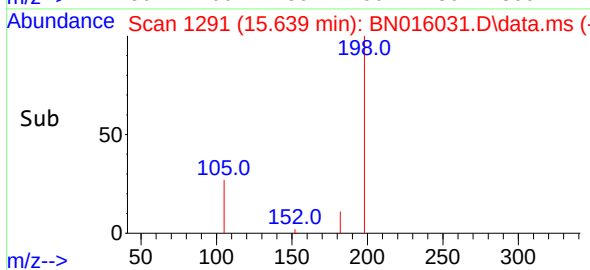

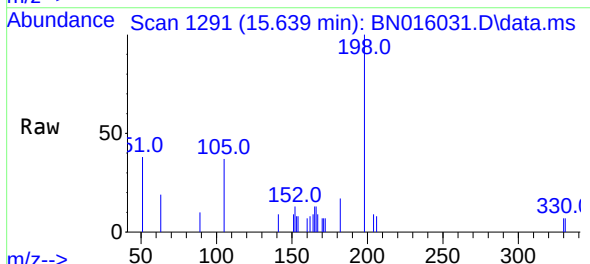


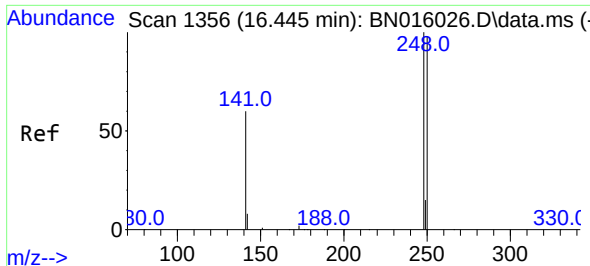

#21
4-Bromophenyl-phenylether
Concen: 0.353 ng
RT: 16.445 min Scan# 1356
Delta R.T. 0.000 min
Lab File: BN016031.D
Acq: 24 Aug 2021 14:38




Instrument :
BNA_N
ClientSampleId :
ICVBN082521


Tgt Ion:	248	Resp:	8205
Ion	Ratio	Lower	Upper
248	100		
250	96.6	78.3	117.5
141	66.1	48.0	72.0

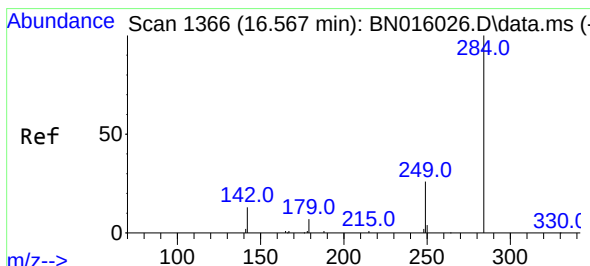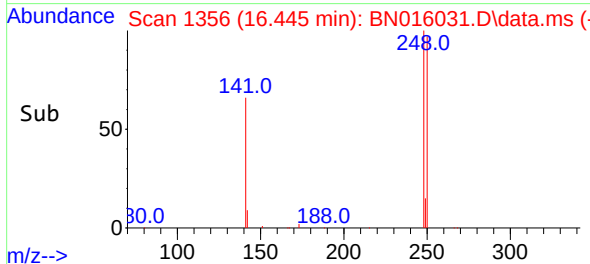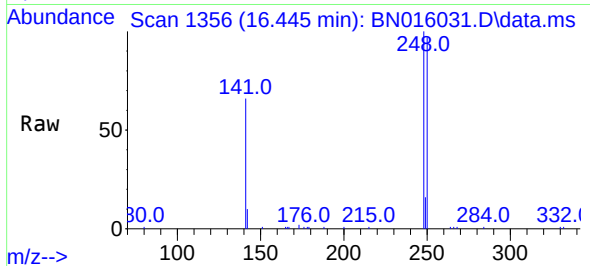

#22
Hexachlorobenzene
Concen: 0.372 ng
RT: 16.567 min Scan# 1366
Delta R.T. 0.000 min
Lab File: BN016031.D
Acq: 24 Aug 2021 14:38

Tgt Ion:	284	Resp:	12142
Ion	Ratio	Lower	Upper
284	100		
142	29.3	23.4	35.2
249	31.2	24.4	36.6


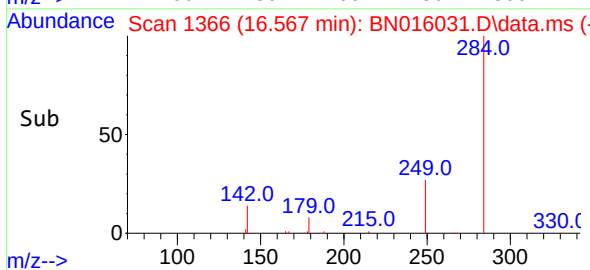

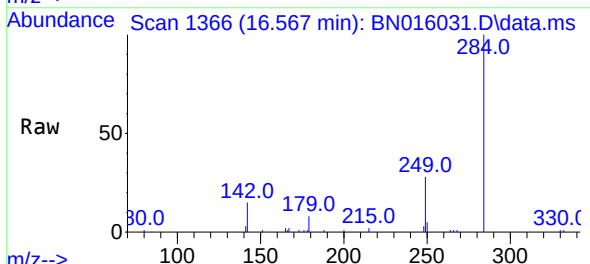




#23
Atrazine
Concen: 0.438 ng
RT: 16.713 min Scan# 1378
Delta R.T. 0.000 min
Lab File: BN016031.D
Acq: 24 Aug 2021 14:38




Instrument :
BNA_N
ClientSampleId :
ICVBN082521


Tgt Ion:200 Resp: 6135
Ion Ratio Lower Upper
200 100
173 24.0 19.7 29.5
215 51.1 39.5 59.3

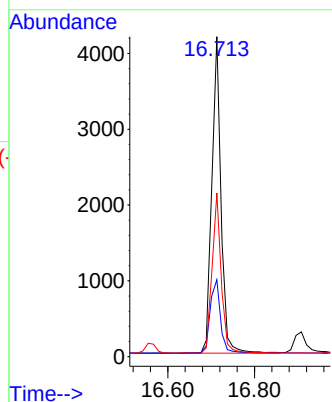

#24
Pentachlorophenol
Concen: 0.367 ng
RT: 16.908 min Scan# 1394
Delta R.T. -0.000 min
Lab File: BN016031.D
Acq: 24 Aug 2021 14:38

Tgt Ion:266 Resp: 3141
Ion Ratio Lower Upper
266 100
264 61.3 50.2 75.4
268 62.7 51.1 76.7









#25
Phenanthrene
Concen: 0.373 ng
RT: 17.297 min Scan# 1426
Delta R.T. 0.000 min
Lab File: BN016031.D
Acq: 24 Aug 2021 14:38




Instrument :
BNA_N
ClientSampleId :
ICVBN082521


Tgt Ion:178 Resp: 49105
Ion Ratio Lower Upper
178 100
176 18.3 14.7 22.1
179 15.5 12.6 19.0

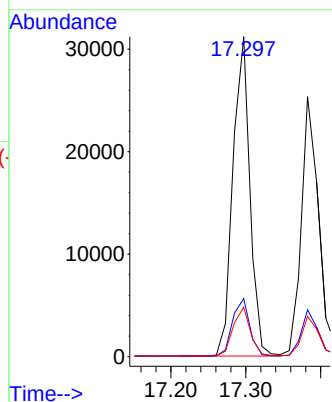

#26
Anthracene
Concen: 0.379 ng
RT: 17.382 min Scan# 1433
Delta R.T. 0.000 min
Lab File: BN016031.D
Acq: 24 Aug 2021 14:38

Tgt Ion:178 Resp: 40903
Ion Ratio Lower Upper
178 100
176 17.5 14.2 21.2
179 15.3 12.2 18.2


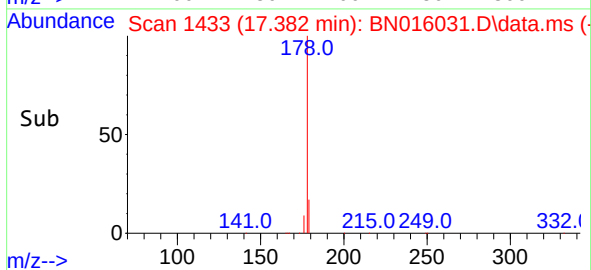






#27
Fluoranthene-d10
Concen: 0.390 ng
RT: 19.286 min Scan# 1741
Delta R.T. 0.000 min
Lab File: BN016031.D
Acq: 24 Aug 2021 14:38




Instrument :
BNA_N
ClientSampleId :
ICVBN082521


Tgt Ion:212 Resp: 50926
Ion Ratio Lower Upper
212 100
106 11.5 9.4 14.2
104 6.5 5.4 8.0



#28
Fluoranthene
Concen: 0.382 ng
RT: 19.321 min Scan# 1748
Delta R.T. 0.005 min
Lab File: BN016031.D
Acq: 24 Aug 2021 14:38

Tgt Ion:202 Resp: 55750
Ion Ratio Lower Upper
202 100
101 10.6 8.4 12.6
203 17.5 14.0 21.0



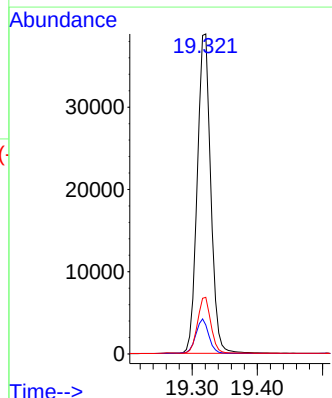





#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.450 min Scan# 2022
Delta R.T. 0.010 min
Lab File: BN016031.D
Acq: 24 Aug 2021 14:38




Instrument :
BNA_N
ClientSampleId :
ICVBN082521


Tgt Ion:240 Resp: 48420
Ion Ratio Lower Upper
240 100
120 6.5 7.8 11.6#
236 25.4 21.0 31.6



#30
Pyrene
Concen: 0.392 ng
RT: 19.683 min Scan# 1821
Delta R.T. 0.005 min
Lab File: BN016031.D
Acq: 24 Aug 2021 14:38

Tgt Ion:202 Resp: 56384
Ion Ratio Lower Upper
202 100
200 19.9 16.1 24.1
203 17.4 14.1 21.1


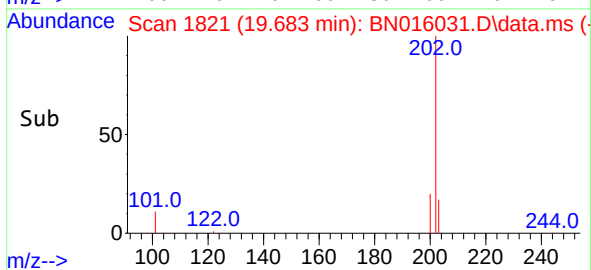






#31
 Terphenyl-d14
 Concen: 0.384 ng
 RT: 19.887 min Scan# 1862
 Delta R.T. 0.005 min
 Lab File: BN016031.D
 Acq: 24 Aug 2021 14:38




Instrument :
 BNA_N
 ClientSampleId :
 ICVBN082521


Tgt Ion:244	Resp:	45605
Ion Ratio	Lower	Upper
244	100	
212	7.3	6.0 9.0
122	9.5	8.5 12.7



#32
 Benzo(a)anthracene
 Concen: 0.384 ng
 RT: 21.429 min Scan# 2020
 Delta R.T. 0.000 min
 Lab File: BN016031.D
 Acq: 24 Aug 2021 14:38

Tgt Ion:228	Resp:	56477
Ion Ratio	Lower	Upper
228	100	
226	26.4	20.6 30.8
229	19.6	16.0 24.0



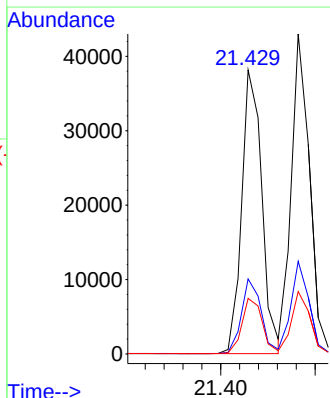



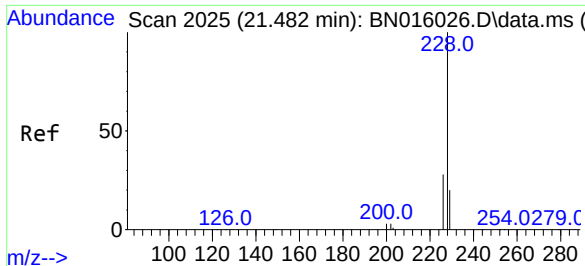

#33
Chrysene
Concen: 0.372 ng
RT: 21.482 min Scan# 2025
Delta R.T. 0.000 min
Lab File: BN016031.D
Acq: 24 Aug 2021 14:38




Instrument :
BNA_N
ClientSampleId :
ICVBN082521


Tgt Ion:	228	Resp:	57828
Ion	Ratio	Lower	Upper
228	100		
226	29.0	22.2	33.2
229	19.5	16.1	24.1

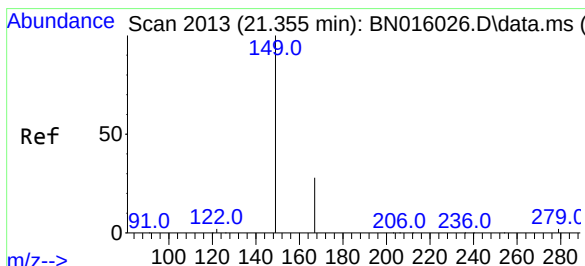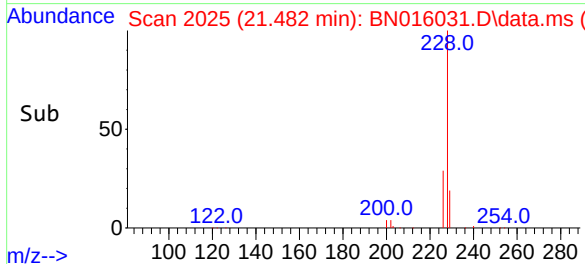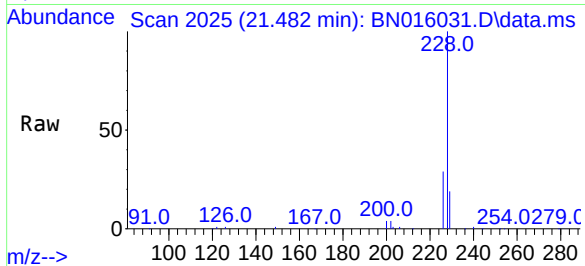

#34
Bis(2-ethylhexyl)phthalate
Concen: 0.426 ng
RT: 21.365 min Scan# 2014
Delta R.T. 0.011 min
Lab File: BN016031.D
Acq: 24 Aug 2021 14:38


Tgt Ion:	149	Resp:	16704
Ion	Ratio	Lower	Upper
149	100		
167	28.6	22.8	34.2
279	5.4	4.1	6.1

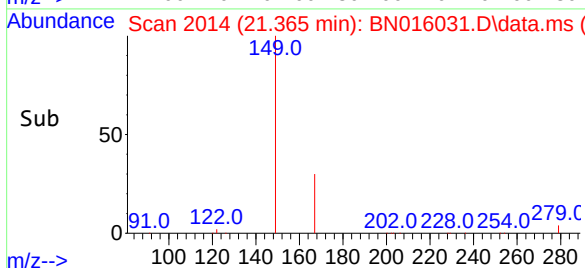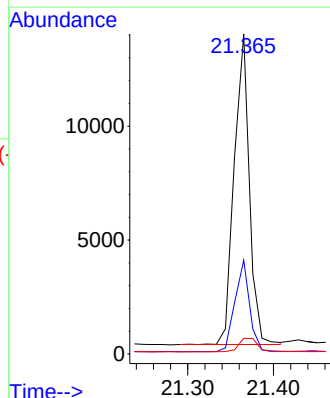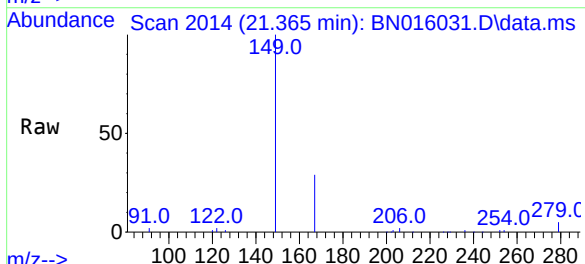






#35
 Perylene-d12
 Concen: 0.400 ng
 RT: 23.850 min Scan# 2534
 Delta R.T. 0.010 min
 Lab File: BN016031.D
 Acq: 24 Aug 2021 14:38

Instrument :
 BNA_N
 ClientSampleId :
 ICVBN082521



Tgt Ion: 264 Resp: 44642




Ion	Ratio	Lower	Upper
264	100		
260	23.7	19.0	28.4
265	27.6	22.7	34.1

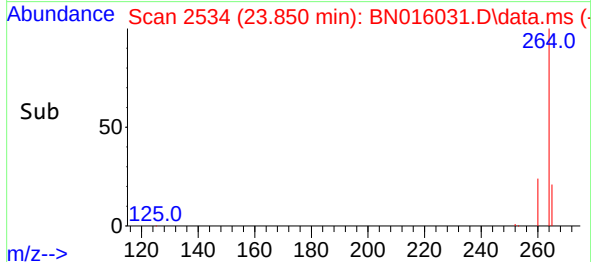


#36
 Indeno(1,2,3-cd)pyrene
 Concen: 0.367 ng
 RT: 26.329 min Scan# 3258
 Delta R.T. 0.010 min
 Lab File: BN016031.D
 Acq: 24 Aug 2021 14:38

Tgt Ion: 276 Resp: 62019

Ion	Ratio	Lower	Upper
276	100		
138	20.7	16.9	25.3
277	25.3	20.2	30.4


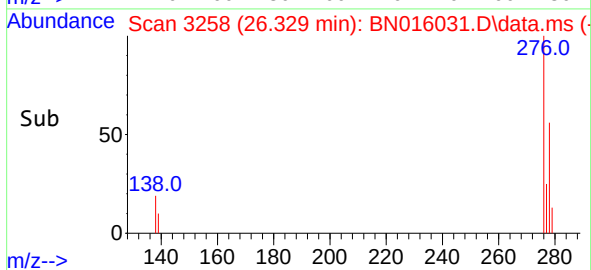






#37
Benzo(b)fluoranthene
Concen: 0.373 ng
RT: 23.118 min Scan# 2320
Delta R.T. 0.007 min
Lab File: BN016031.D
Acq: 24 Aug 2021 14:38




Instrument :
BNA_N
ClientSampleId :
ICVBN082521


Tgt Ion:252 Resp: 59615
Ion Ratio Lower Upper
252 100
253 23.4 18.6 28.0
125 12.6 10.4 15.6

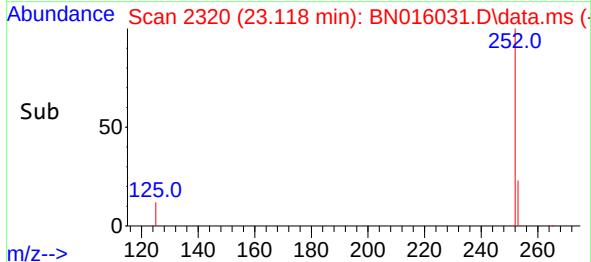

#38
Benzo(k)fluoranthene
Concen: 0.376 ng
RT: 23.166 min Scan# 2334
Delta R.T. 0.010 min
Lab File: BN016031.D
Acq: 24 Aug 2021 14:38

Tgt Ion:252 Resp: 56004
Ion Ratio Lower Upper
252 100
253 22.7 17.9 26.9
125 9.6 7.5 11.3


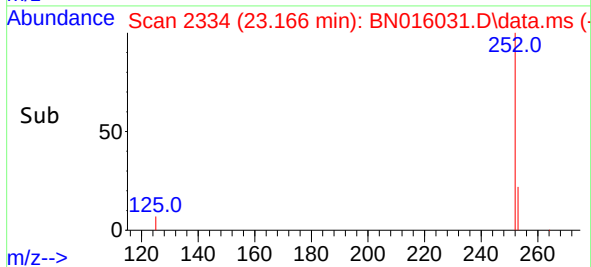

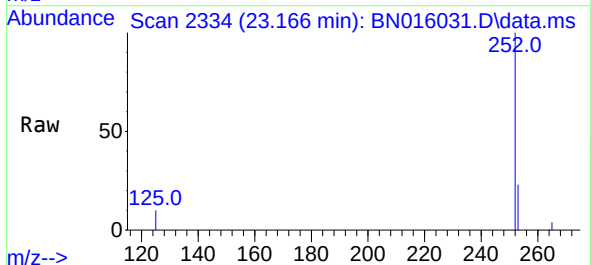




#39
Benzo(a)pyrene
Concen: 0.380 ng
RT: 23.744 min Scan# 2503
Delta R.T. 0.010 min
Lab File: BN016031.D
Acq: 24 Aug 2021 14:38




Instrument :
BNA_N
ClientSampleId :
ICVBN082521


Tgt Ion:	252	Resp:	52415
Ion	Ratio	Lower	Upper
252	100		
253	24.3	19.2	28.8
125	17.5	14.2	21.2

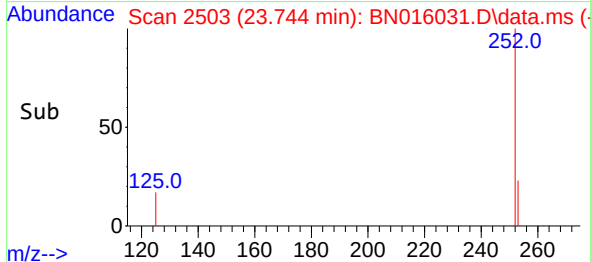

#40
Dibenzo(a,h)anthracene
Concen: 0.369 ng
RT: 26.349 min Scan# 3264
Delta R.T. 0.010 min
Lab File: BN016031.D
Acq: 24 Aug 2021 14:38

Tgt Ion:	278	Resp:	51530
Ion	Ratio	Lower	Upper
278	100		
139	13.4	10.7	16.1
279	24.0	19.7	29.5

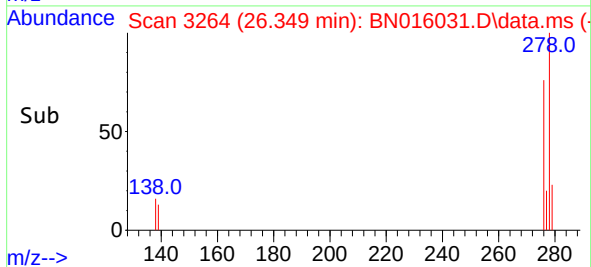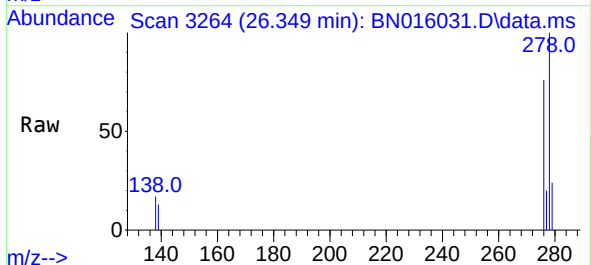

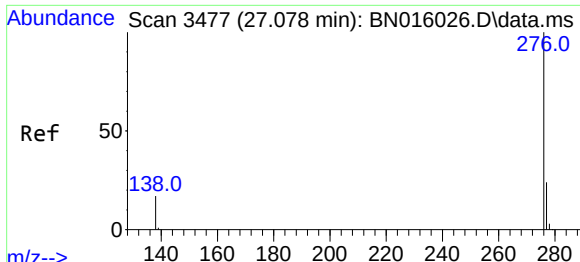

#41
Benzo(g,h,i)perylene
Concen: 0.367 ng
RT: 27.092 min Scan# 3481
Delta R.T. 0.014 min
Lab File: BN016031.D
Acq: 24 Aug 2021 14:38

Instrument :
BNA_N
ClientSampleId :
ICVBN082521

Tgt Ion:	276	Resp:	53025
Ion Ratio	Lower	Upper	
276	100		
277	24.2	19.3	28.9
138	17.3	14.0	21.0

