
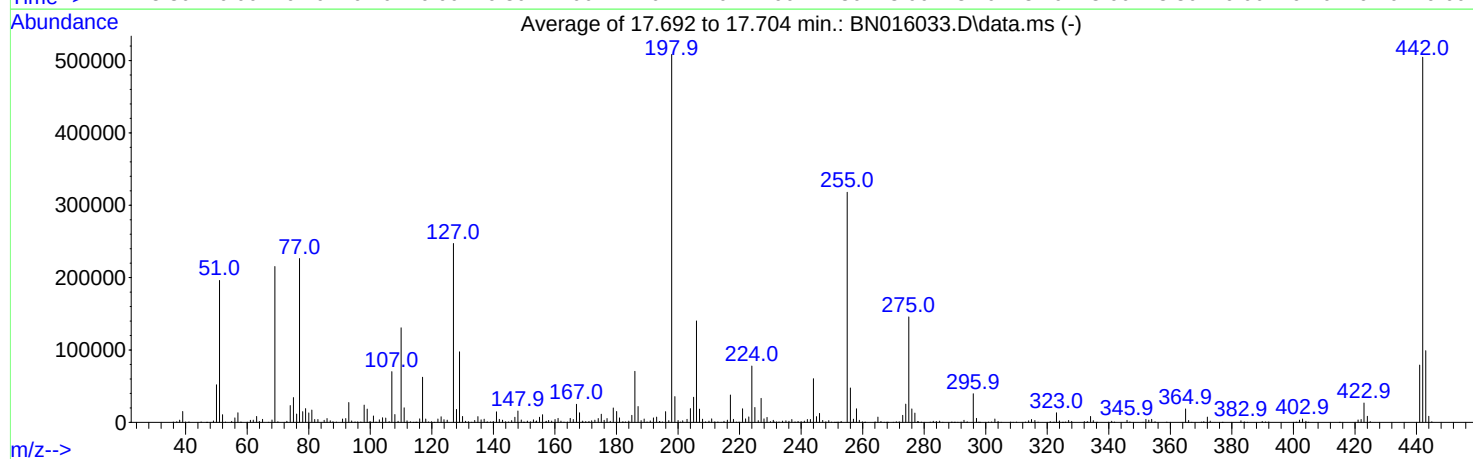


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082521\
 Data File : BN016033.D
 Acq On : 24 Aug 2021 16:32
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN082521.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Aug 24 14:26:02 2021

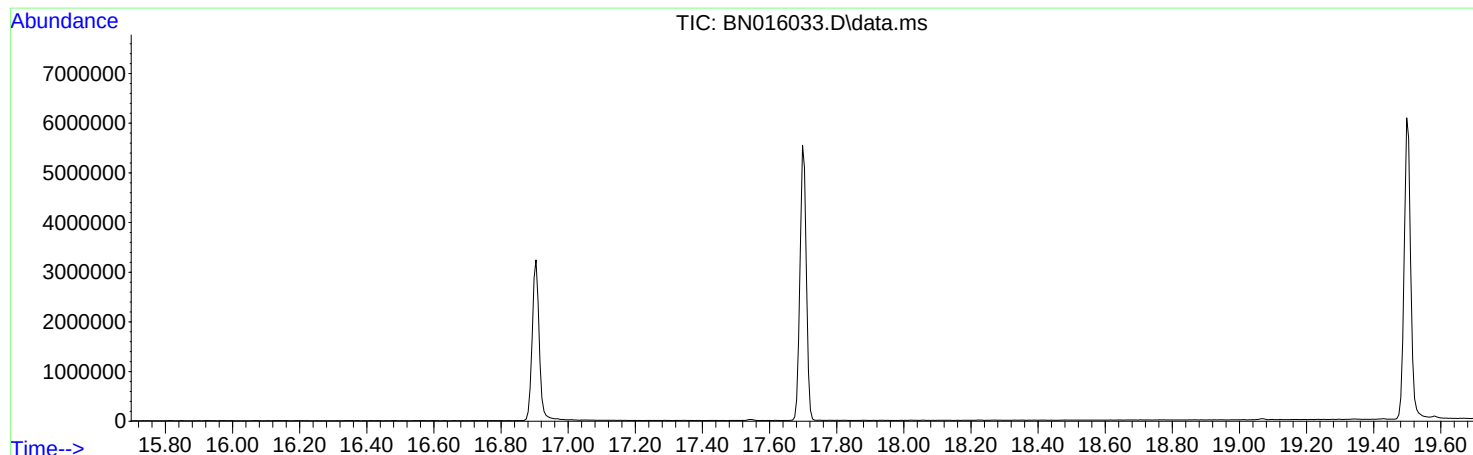




AutoFind: Scans 2483, 2484, 2485; Background Corrected with Scan 2476

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.6	196160	PASS
68	69	0.00	2	1.5	3305	PASS
69	198	0.00	100	42.3	215275	PASS
70	69	0.00	2	0.4	944	PASS
127	198	10	80	48.6	247168	PASS
197	198	0.00	2	0.5	2385	PASS
198	198	100	100	100.0	508331	PASS
199	198	5	9	7.0	35629	PASS
275	198	10	60	28.7	145744	PASS
365	198	1	100	3.6	18518	PASS
441	198	0.01	100	15.6	79259	PASS
442	442	50	100	100.0	504555	PASS
443	442	15	24	19.6	99021	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082521\
Data File : BN016033.D
Acq On : 24 Aug 2021 16:32
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 24 17:13:04 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 24 17:12:56 2021
Response via : Initial Calibration

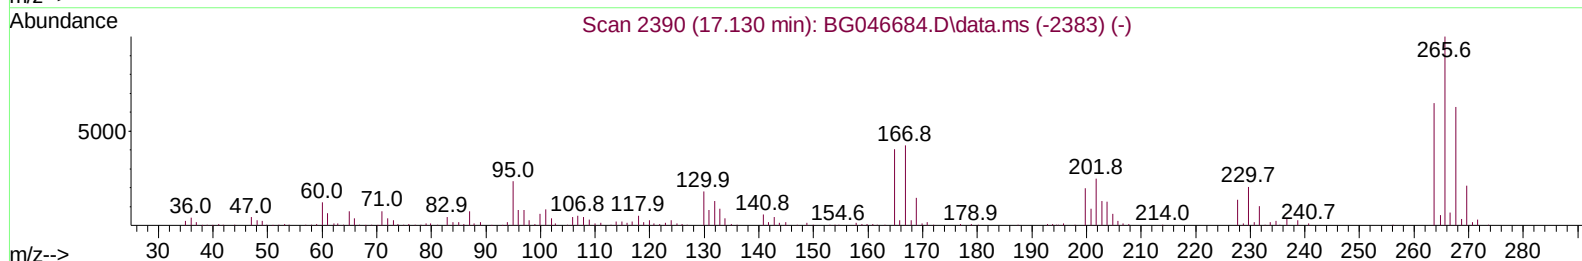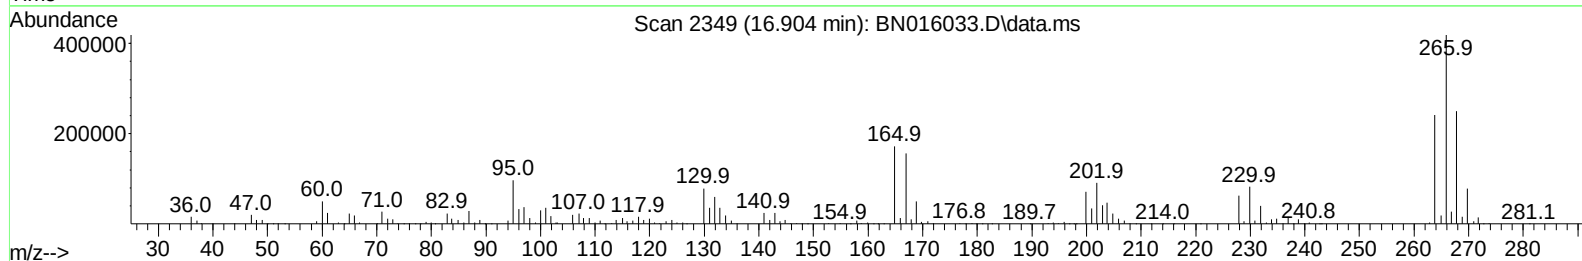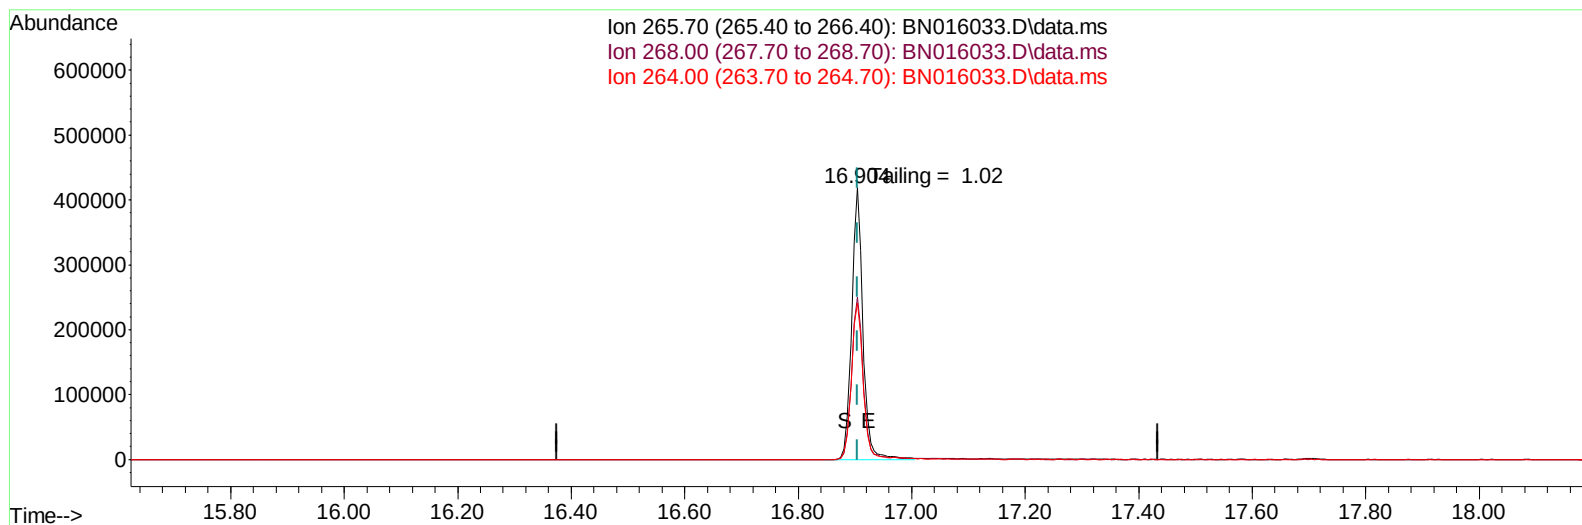

TIC: BN016033.D\data.ms

(70) Pentachlorophenol (C)

16.904min (0.000) 21272.59 ng




response 583295

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	59.73
264.00	61.60	57.64
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082521\
Data File : BN016033.D
Acq On : 24 Aug 2021 16:32
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 24 17:13:04 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 24 17:12:56 2021
Response via : Initial Calibration

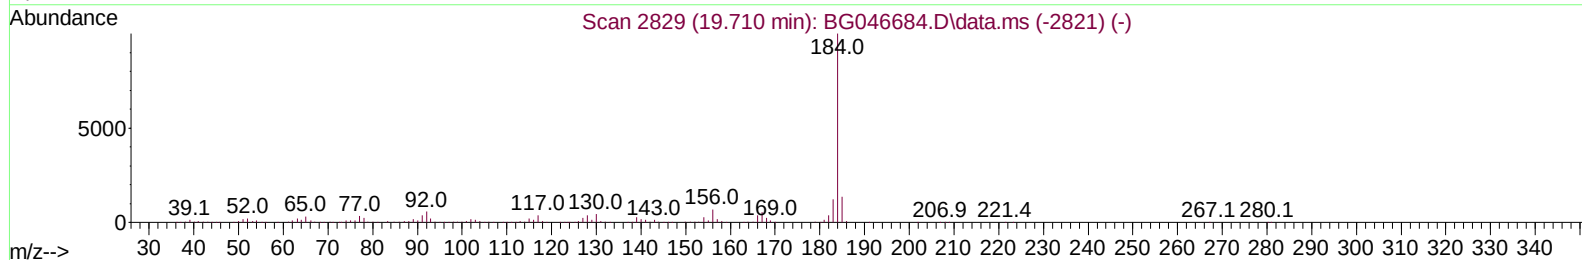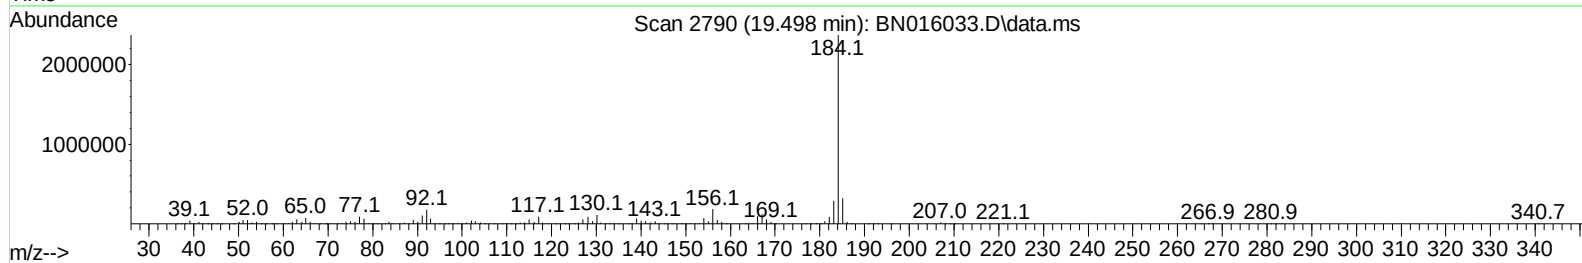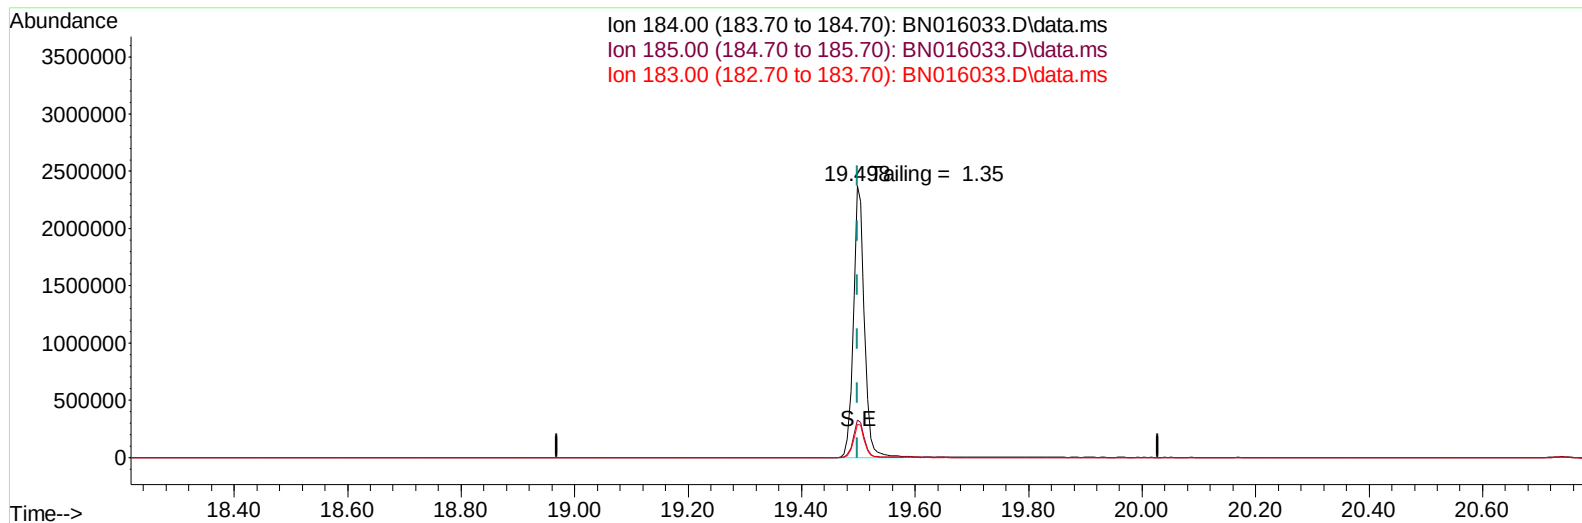

TIC: BN016033.D\data.ms

(77) Benzidine

19.498min (0.000) 0.00 ng

response 3204533

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.75
183.00	13.20	12.15
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/25/2021	BNA_N	<u>BN016033.D</u>
Compound Name	Response	Retention Time
DDT	1619389	20.739
DDD	8050	20.298
DDE	2396	19.786
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10446	1629835	0.64

Instrument :
BNA_N
ClientSampleId :
DFTPP