
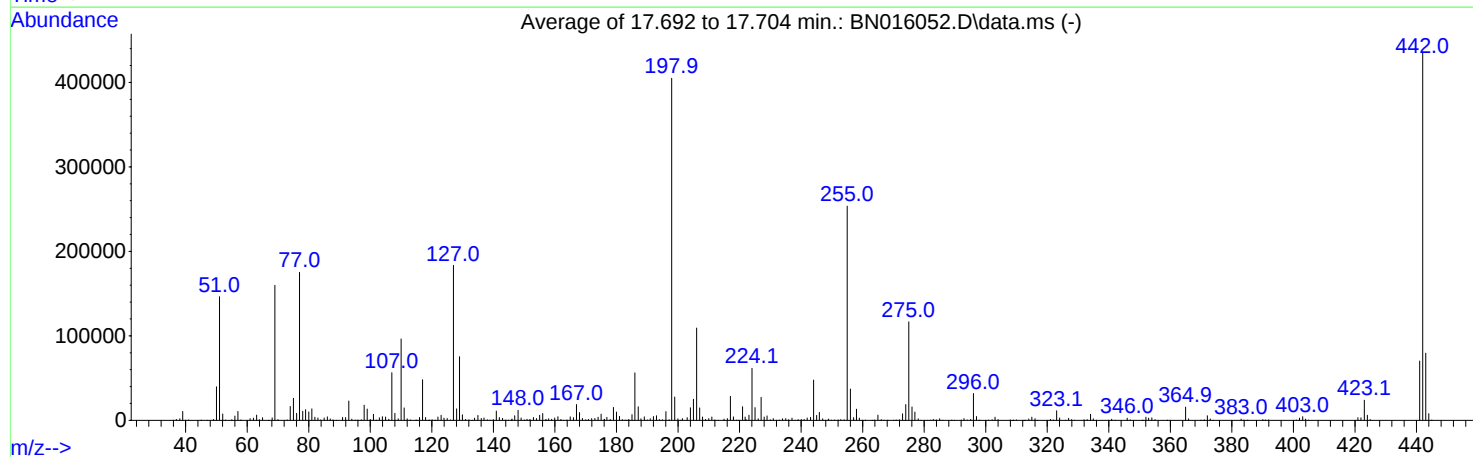


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082521\
 Data File : BN016052.D
 Acq On : 25 Aug 2021 05:24
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN082521.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Aug 24 14:26:02 2021

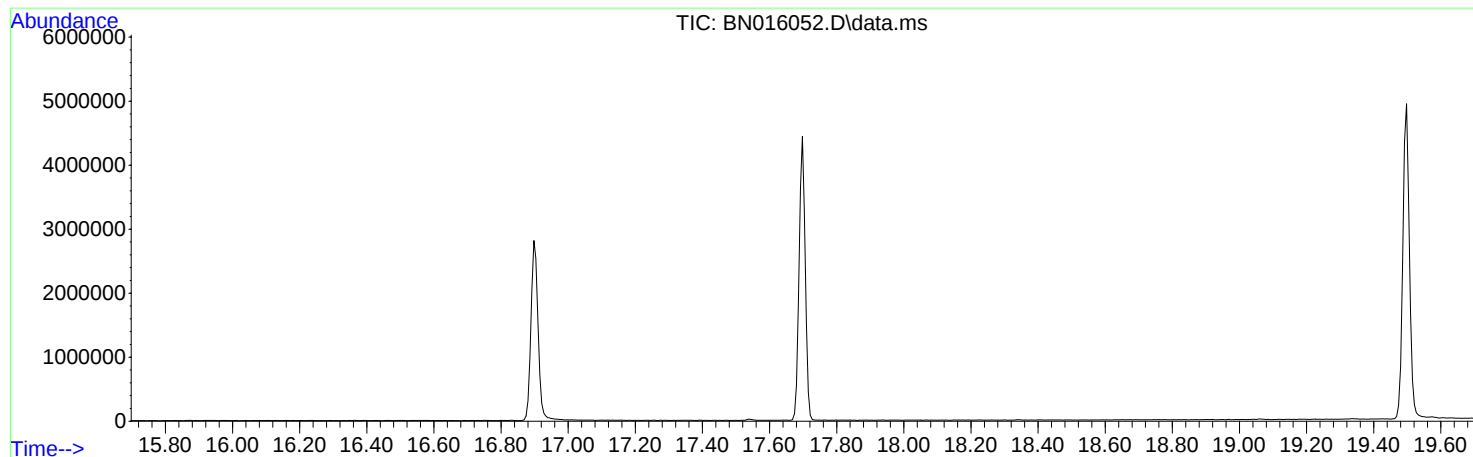




AutoFind: Scans 2483, 2484, 2485; Background Corrected with Scan 2476

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.2	146485	PASS
68	69	0.00	2	1.9	3092	PASS
69	198	0.00	100	39.5	159928	PASS
70	69	0.00	2	0.5	735	PASS
127	198	10	80	45.3	183531	PASS
197	198	0.00	2	0.2	760	PASS
198	198	100	100	100.0	404885	PASS
199	198	5	9	6.8	27653	PASS
275	198	10	60	28.8	116773	PASS
365	198	1	100	3.9	15800	PASS
441	198	0.01	100	17.4	70275	PASS
442	442	50	100	100.0	435435	PASS
443	442	15	24	18.3	79645	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082521\
 Data File : BN016052.D
 Acq On : 25 Aug 2021 05:24
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Aug 25 07:30:10 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 24 17:12:56 2021
 Response via : Initial Calibration

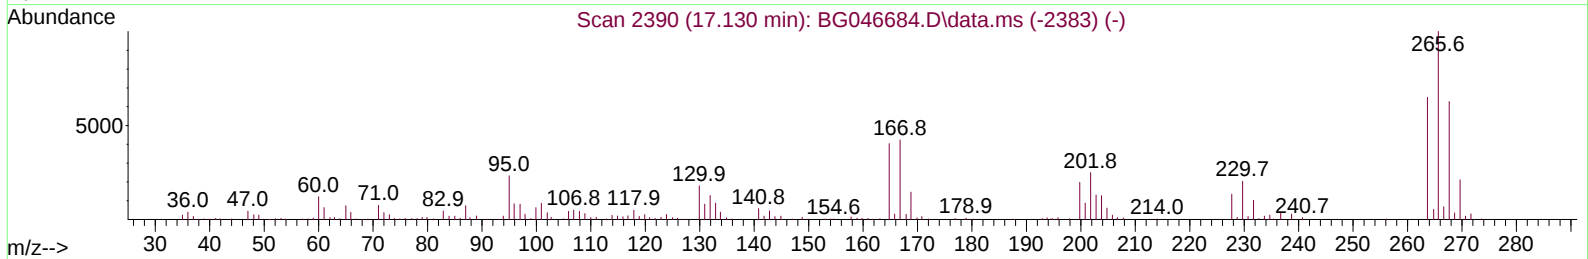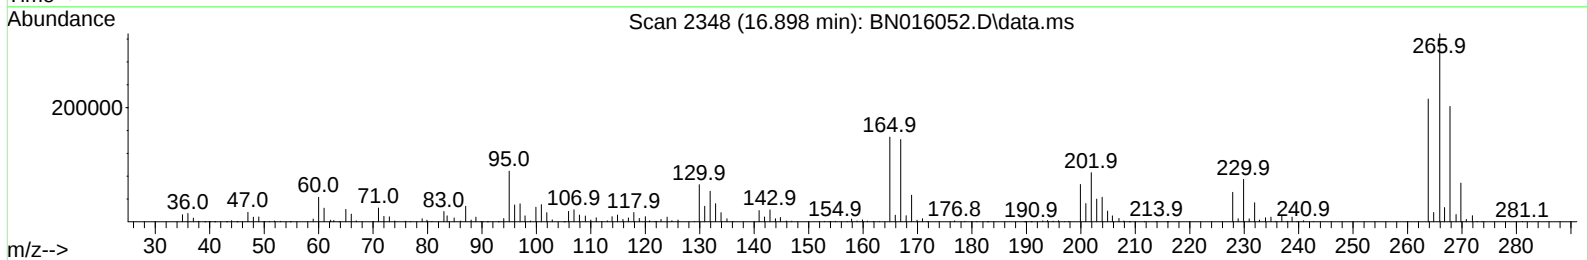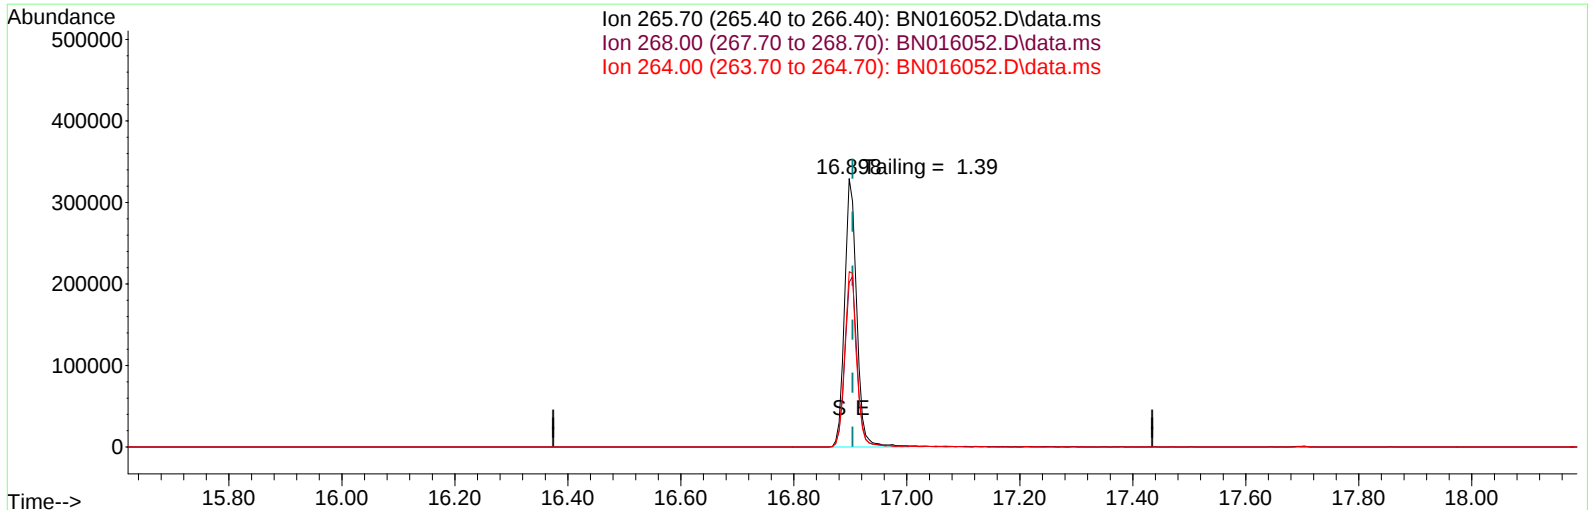

TIC: BN016052.D\data.ms

(70) Pentachlorophenol (C)

16.898min (-0.006) 20646.01 ng




response 492069

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.38
264.00	61.60	65.34
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082521\
Data File : BN016052.D
Acq On : 25 Aug 2021 05:24
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 25 07:30:10 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 24 17:12:56 2021
Response via : Initial Calibration

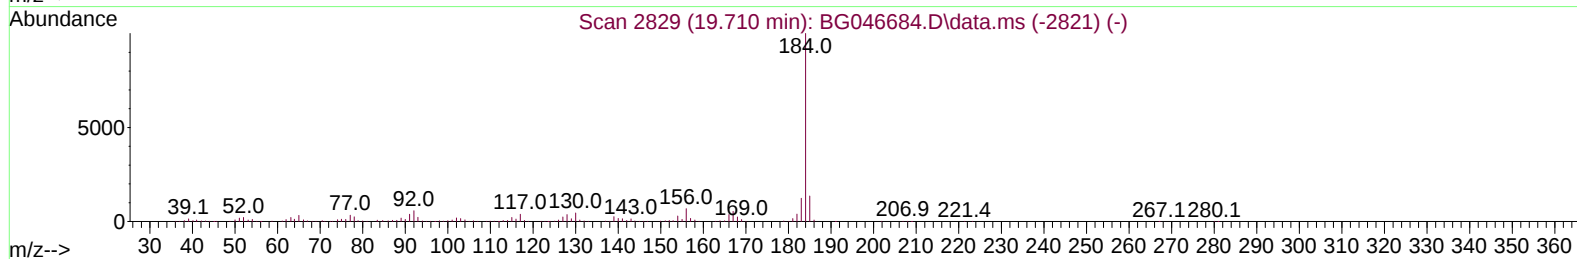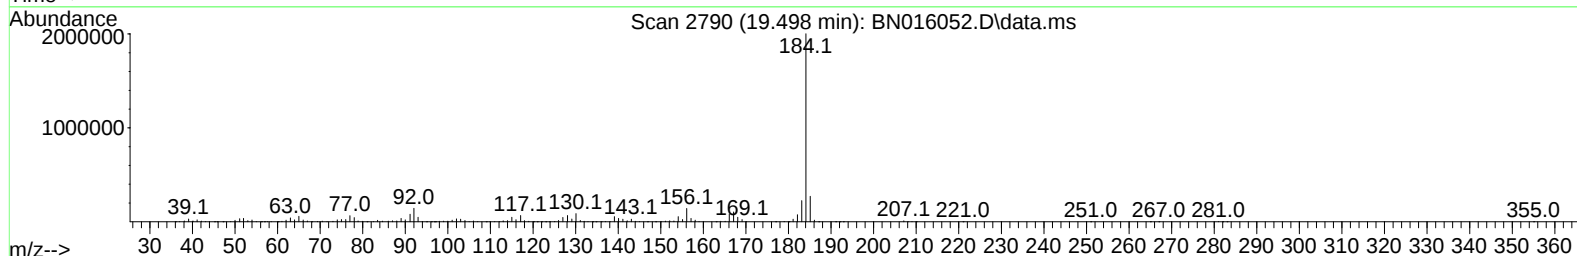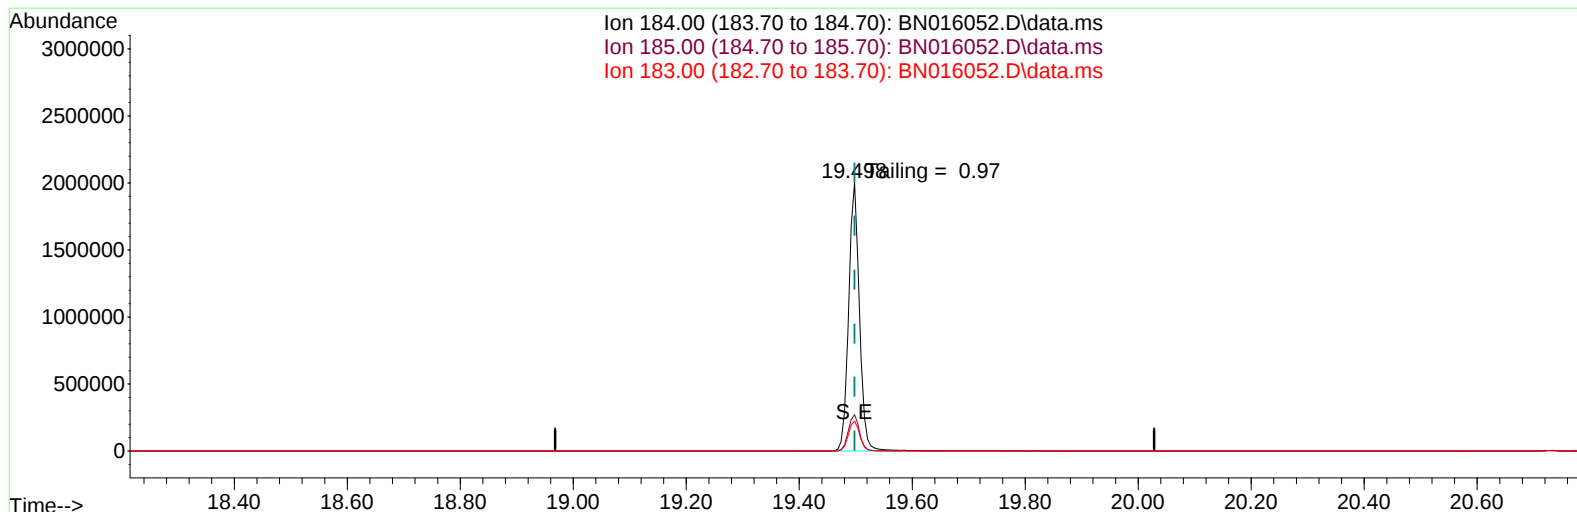

TIC: BN016052.D\data.ms

(77) Benzidine

19.498min (-0.001) 0.00 ng

response 2663350

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.54
183.00	13.20	11.21
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/25/2021	BNA_N	<u>BN016052.D</u>
Compound Name	Response	Retention Time
DDT	1369966	20.733
DDD	24755	20.292
DDE	2480	19.786
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
27235	1397201	1.95

Instrument :
BNA_N
ClientSampleId :
DFTPP