
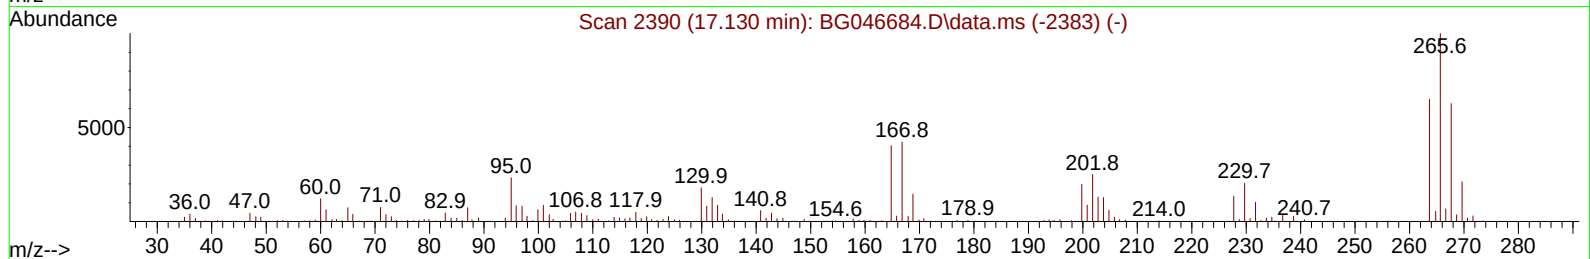
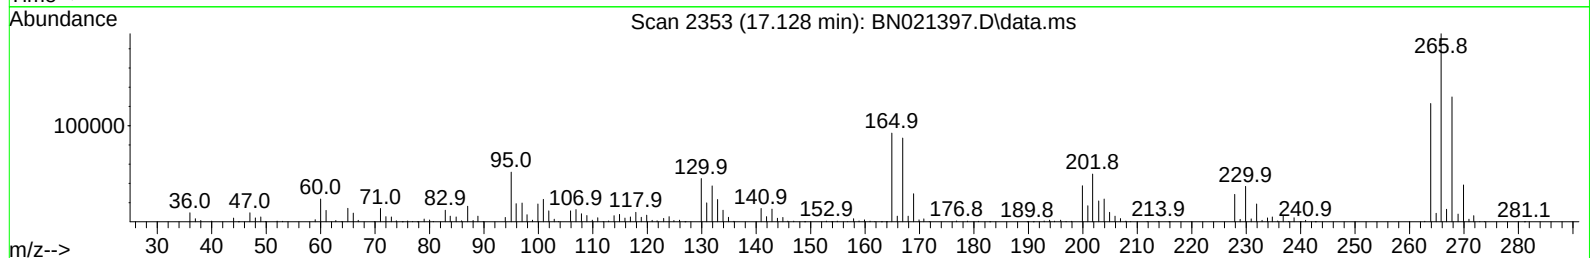


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082622\
Data File : BN021397.D
Acq On : 27 Aug 2022 00:01
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 27 04:56:41 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Aug 27 04:55:17 2022
Response via : Initial Calibration

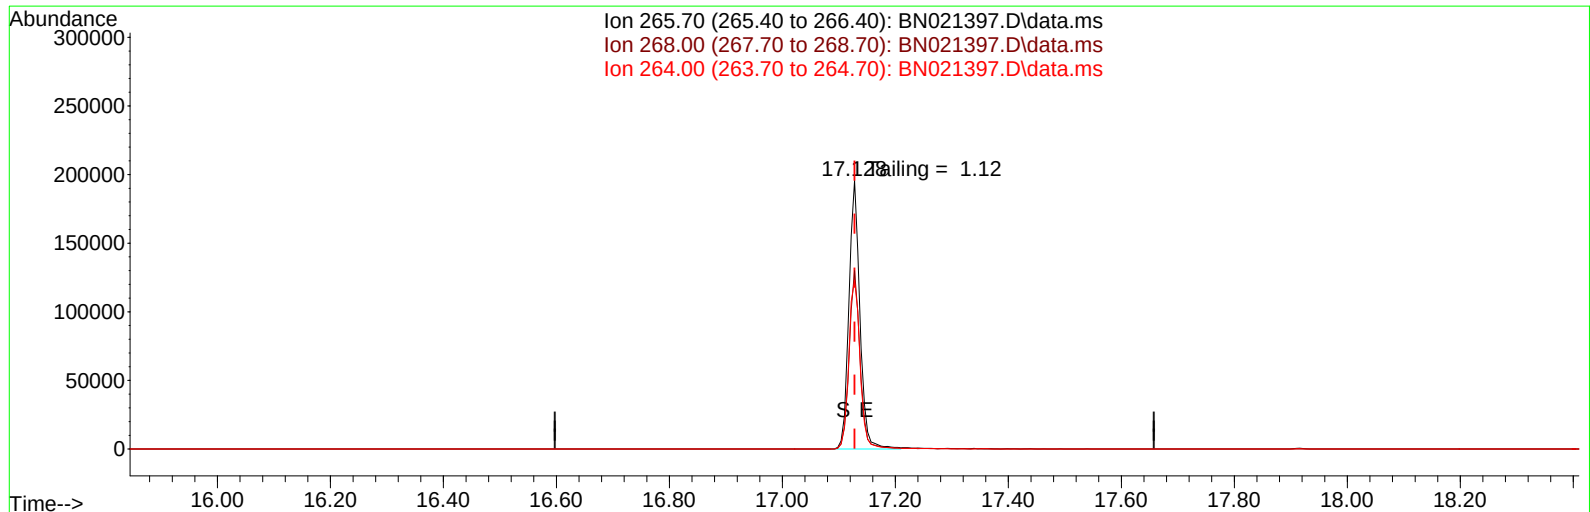

TIC: BN021397.D\data.ms

(70) Pentachlorophenol (C)




17.128min (-0.000) 19650.68 ng

response 267869

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	66.40
264.00	61.60	62.88
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082622\
Data File : BN021397.D
Acq On : 27 Aug 2022 00:01
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 27 04:56:41 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Aug 27 04:55:17 2022
Response via : Initial Calibration

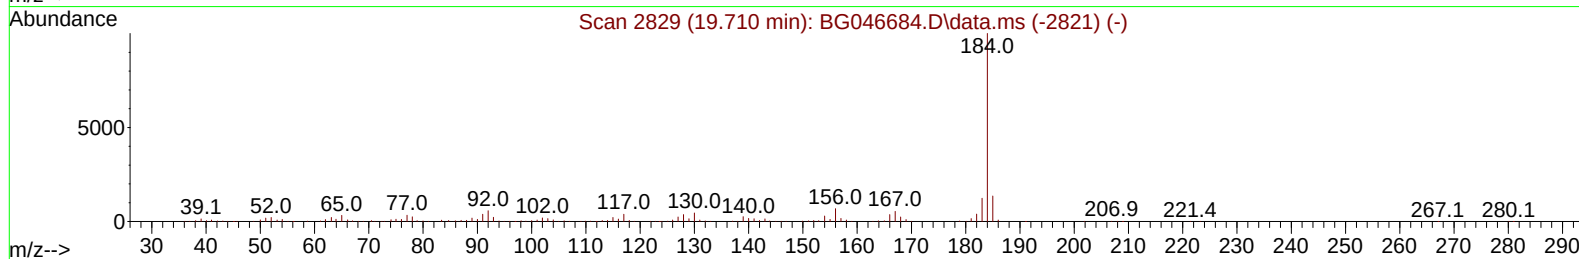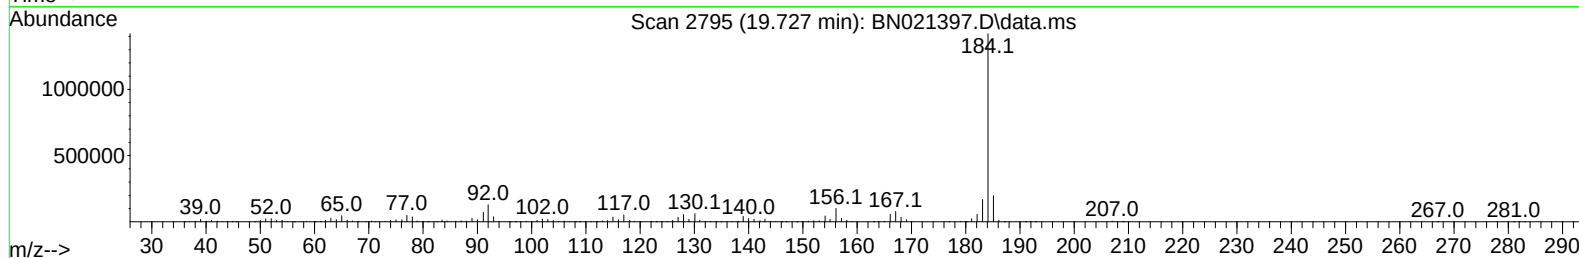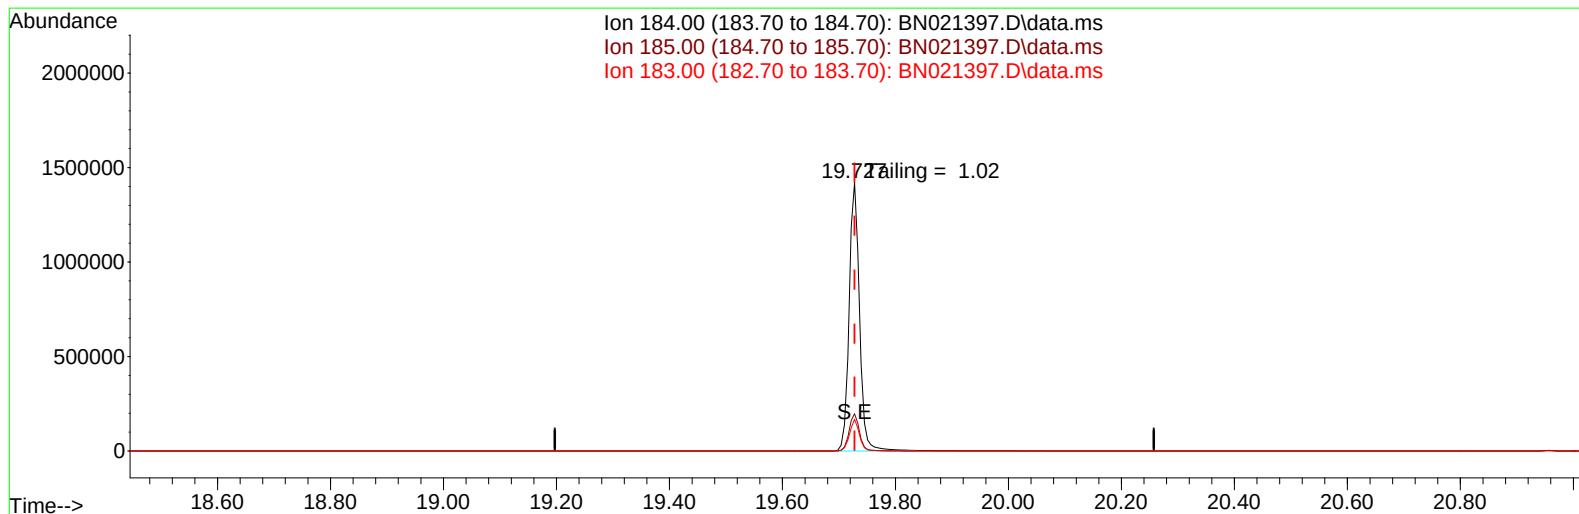

TIC: BN021397.D\data.ms

(77) Benzidine

19.727min (-0.000) 0.00 ng

response 1826036

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.89
183.00	13.20	11.84
0.00	0.00	0.00