
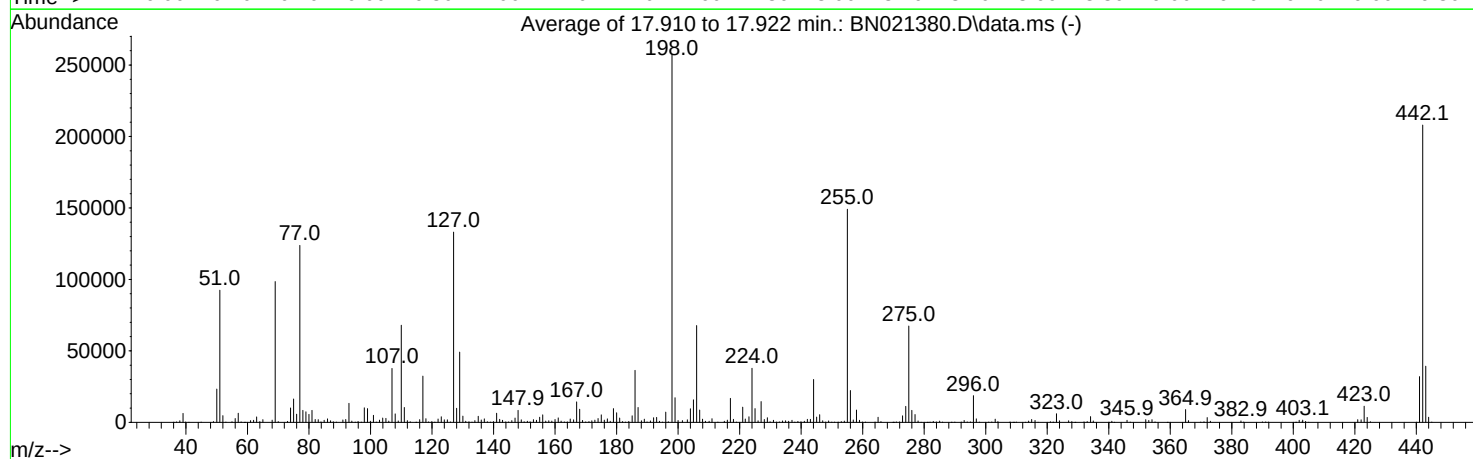


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082622\
 Data File : BN021380.D
 Acq On : 26 Aug 2022 11:12
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN082422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Aug 26 23:37:03 2022

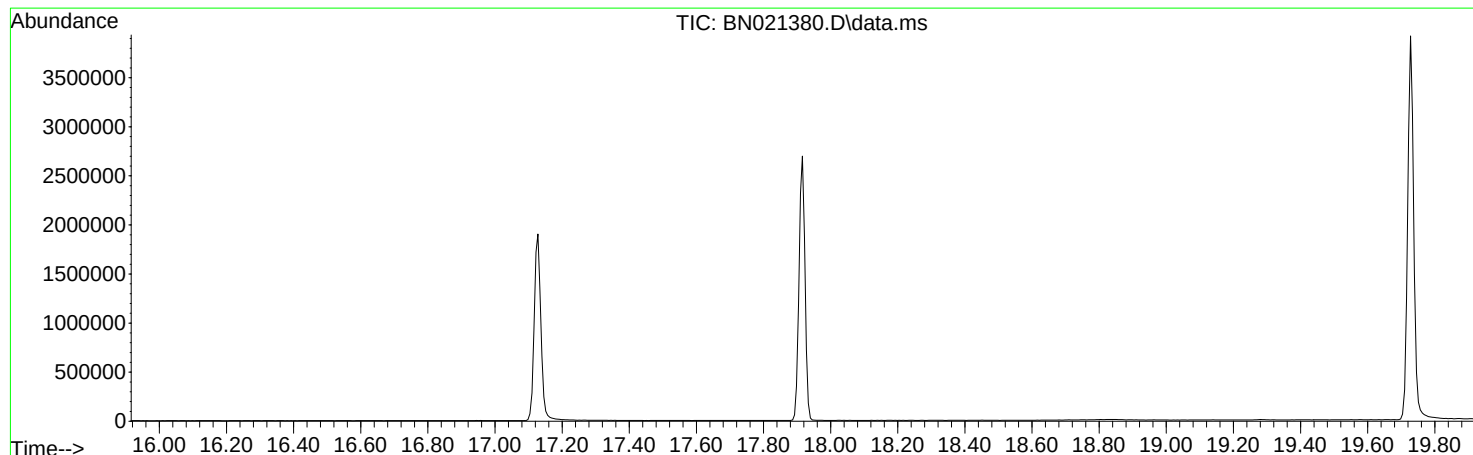

AutoFind: Scans 2486, 2487, 2488; Background Corrected with Scan 2479

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.9	92467	PASS
68	69	0.00	2	1.6	1537	PASS
69	198	0.00	100	38.3	98565	PASS
70	69	0.00	2	0.6	561	PASS
127	198	10	80	51.7	133059	PASS
197	198	0.00	2	0.2	429	PASS
198	198	100	100	100.0	257365	PASS
199	198	5	9	6.7	17309	PASS
275	198	10	60	26.2	67432	PASS
365	198	1	100	3.5	9004	PASS
441	198	0.01	100	12.5	32064	PASS
442	442	50	100	100.0	208043	PASS
443	442	15	24	18.9	39296	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/26/2022	BNA_N	<u>BN021380.D</u>
Compound Name	Response	Retention Time
DDT	855876	20.963
DDD	16309	20.516
DDE	514	20.01
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
16823	872699	1.93

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082622\
Data File : BN021380.D
Acq On : 26 Aug 2022 11:12
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 27 04:55:22 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Aug 27 04:55:17 2022
Response via : Initial Calibration

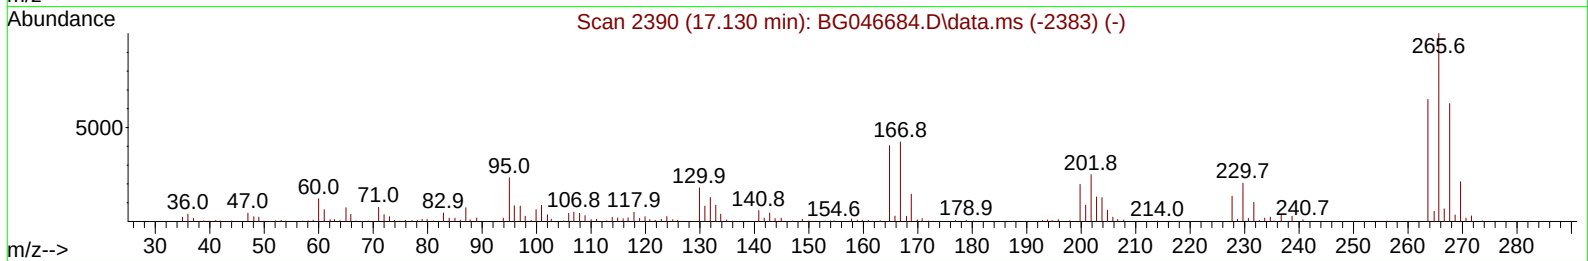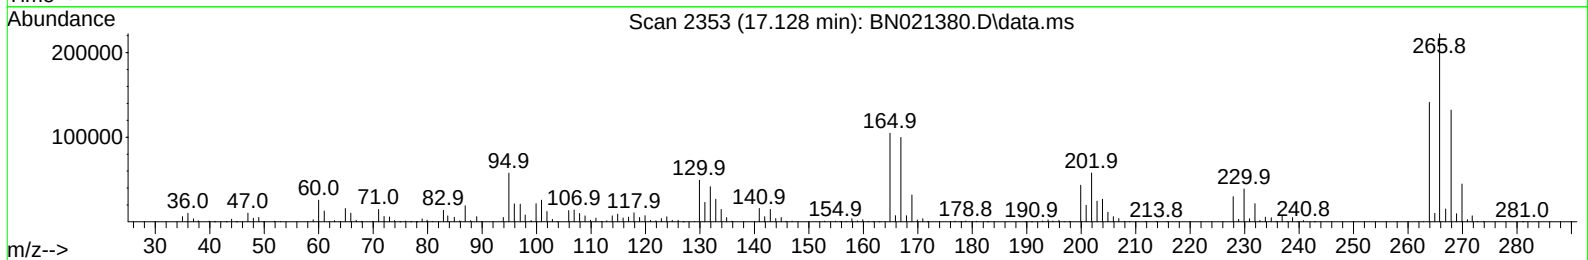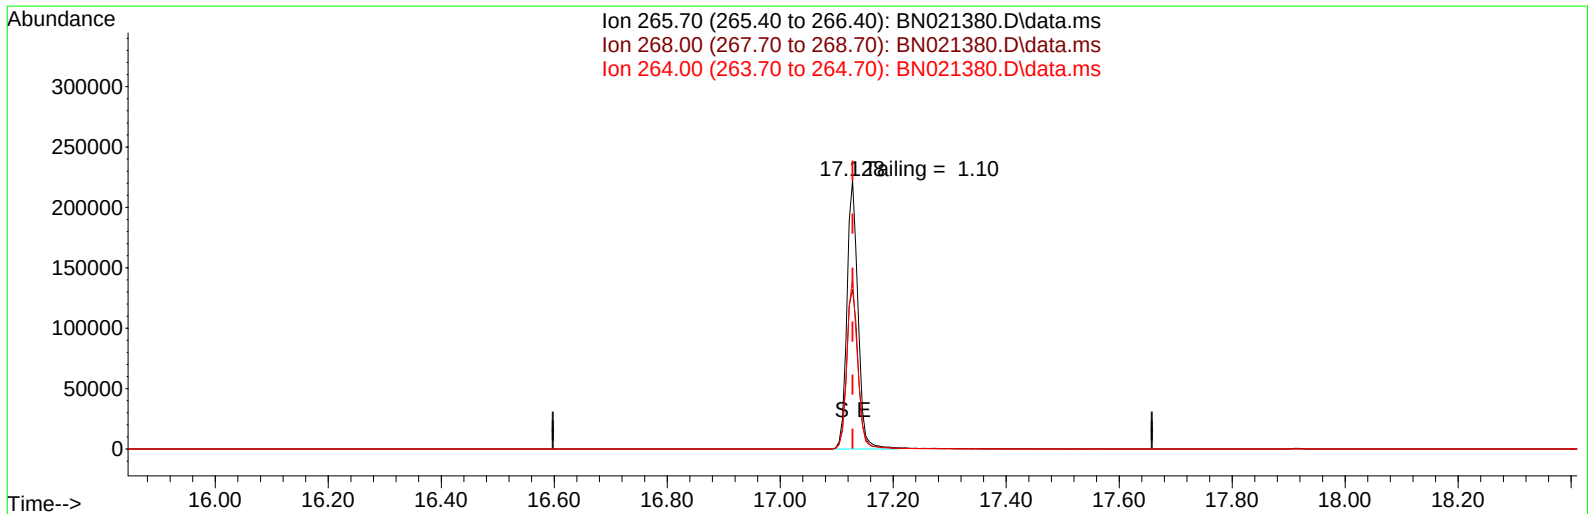

TIC: BN021380.D\data.ms

(70) Pentachlorophenol (C)

17.128min (0.000) 554464.78 ng




response 304591

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	59.45
264.00	61.60	63.51
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082622\
 Data File : BN021380.D
 Acq On : 26 Aug 2022 11:12
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Aug 27 04:55:22 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Aug 27 04:55:17 2022
 Response via : Initial Calibration

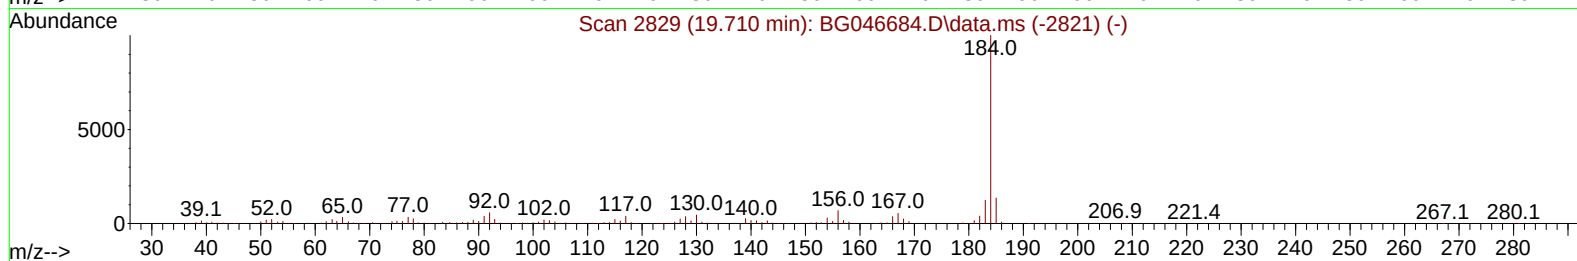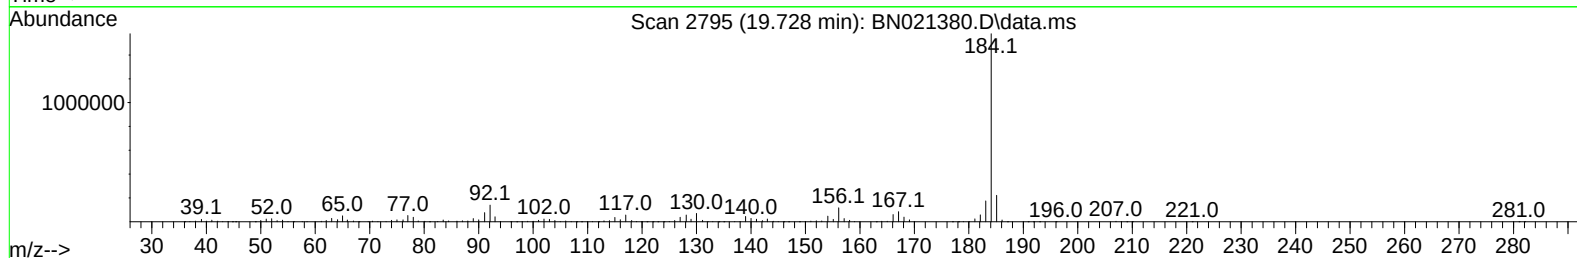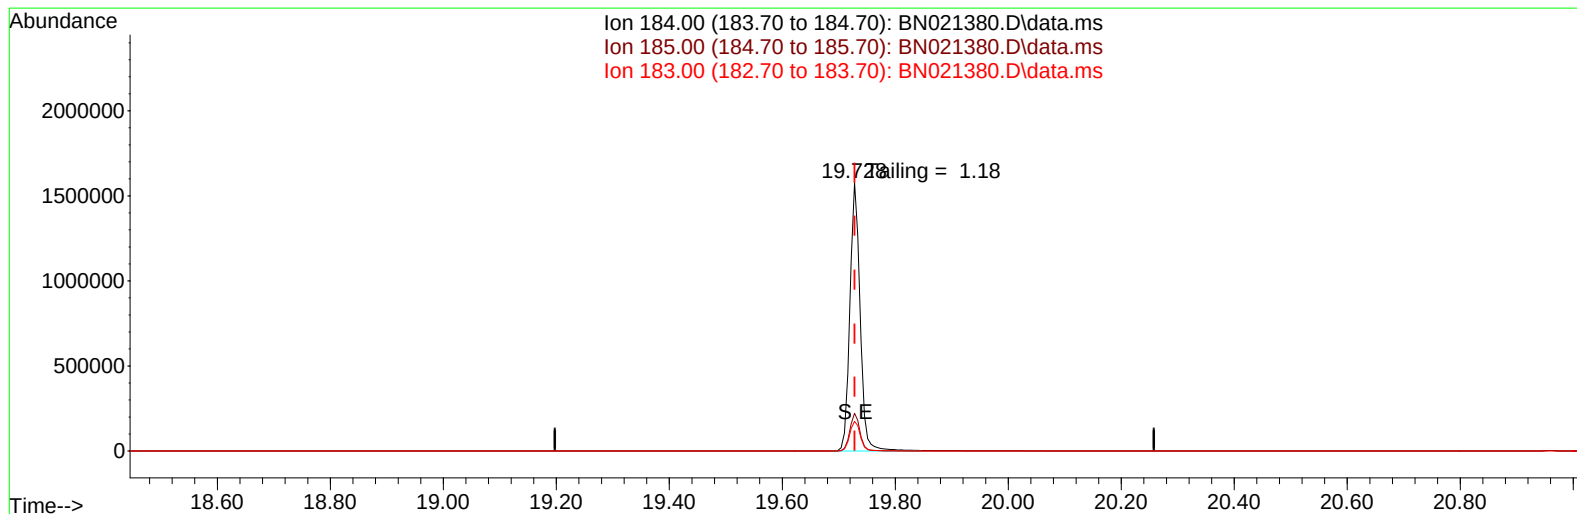

TIC: BN021380.D\data.ms

(77) Benzidine

19.728min (0.000) 207006.15 ng

response 2003647

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.07
183.00	13.20	11.05
0.00	0.00	0.00