
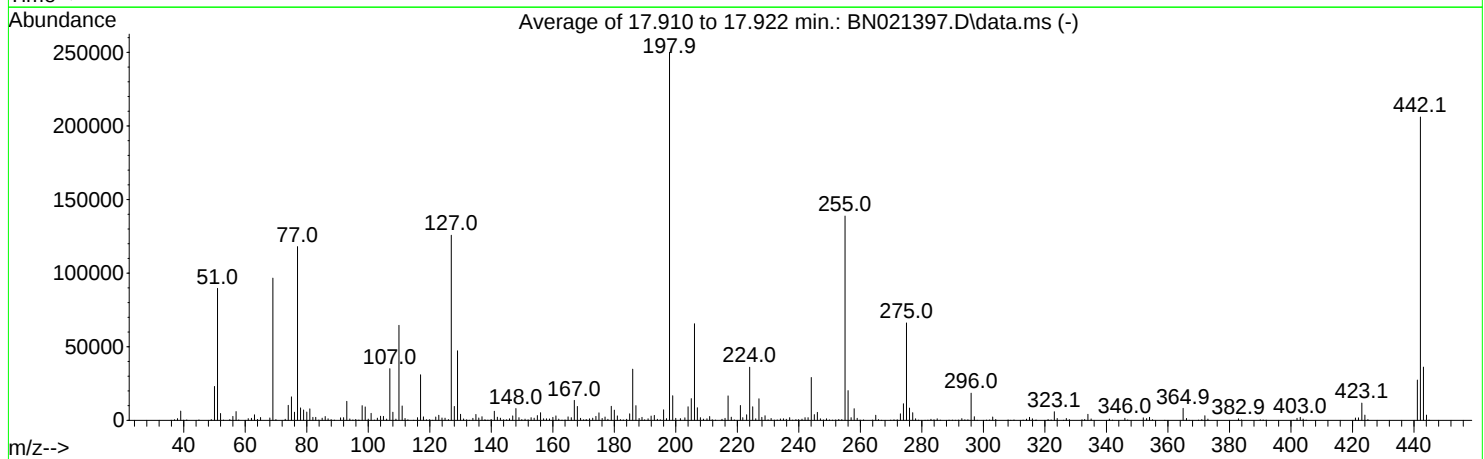


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082622\
 Data File : BN021397.D
 Acq On : 27 Aug 2022 00:01
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN082422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 29 04:26:29 2022

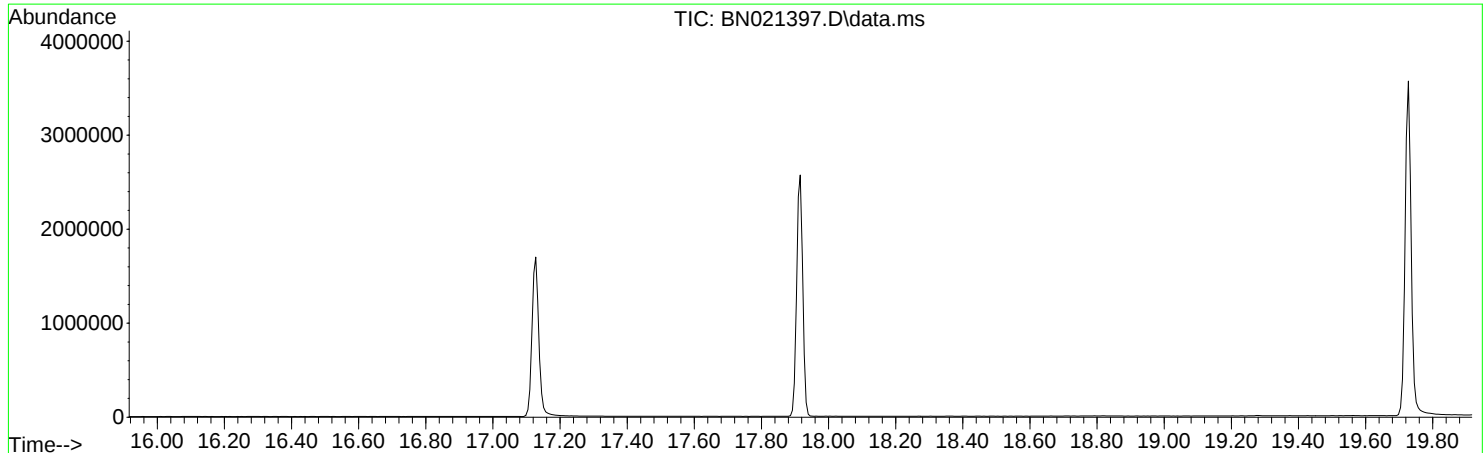




AutoFind: Scans 2486, 2487, 2488; Background Corrected with Scan 2479

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.9	89709	PASS
68	69	0.00	2	1.6	1536	PASS
69	198	0.00	100	38.7	96683	PASS
70	69	0.00	2	0.5	509	PASS
127	198	10	80	50.3	125739	PASS
197	198	0.00	2	0.4	1121	PASS
198	198	100	100	100.0	250005	PASS
199	198	5	9	6.7	16744	PASS
275	198	10	60	26.5	66176	PASS
365	198	1	100	3.2	8115	PASS
441	198	0.01	100	10.9	27323	PASS
442	442	50	100	100.0	206144	PASS
443	442	15	24	17.6	36216	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082622\
 Data File : BN021397.D
 Acq On : 27 Aug 2022 00:01
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Aug 27 04:56:41 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Aug 27 04:55:17 2022
 Response via : Initial Calibration

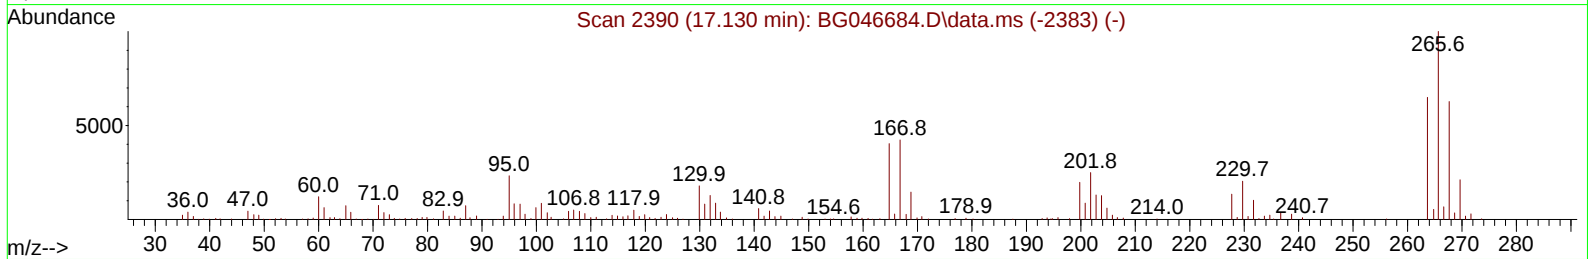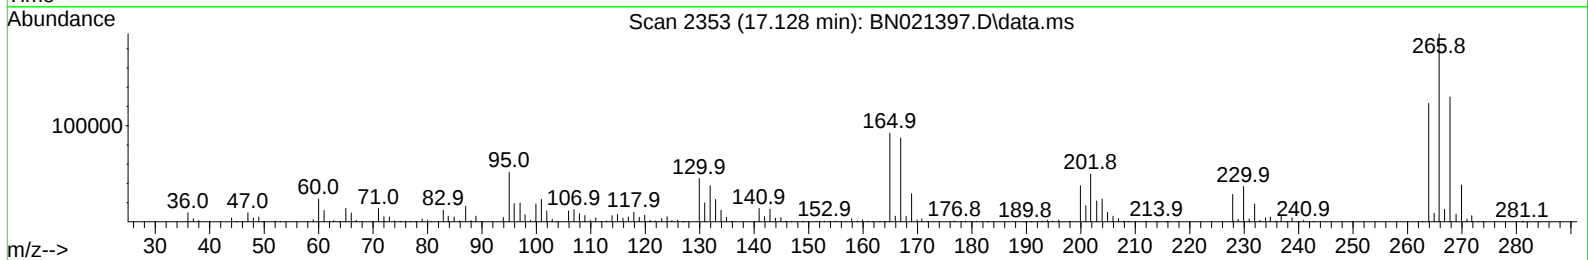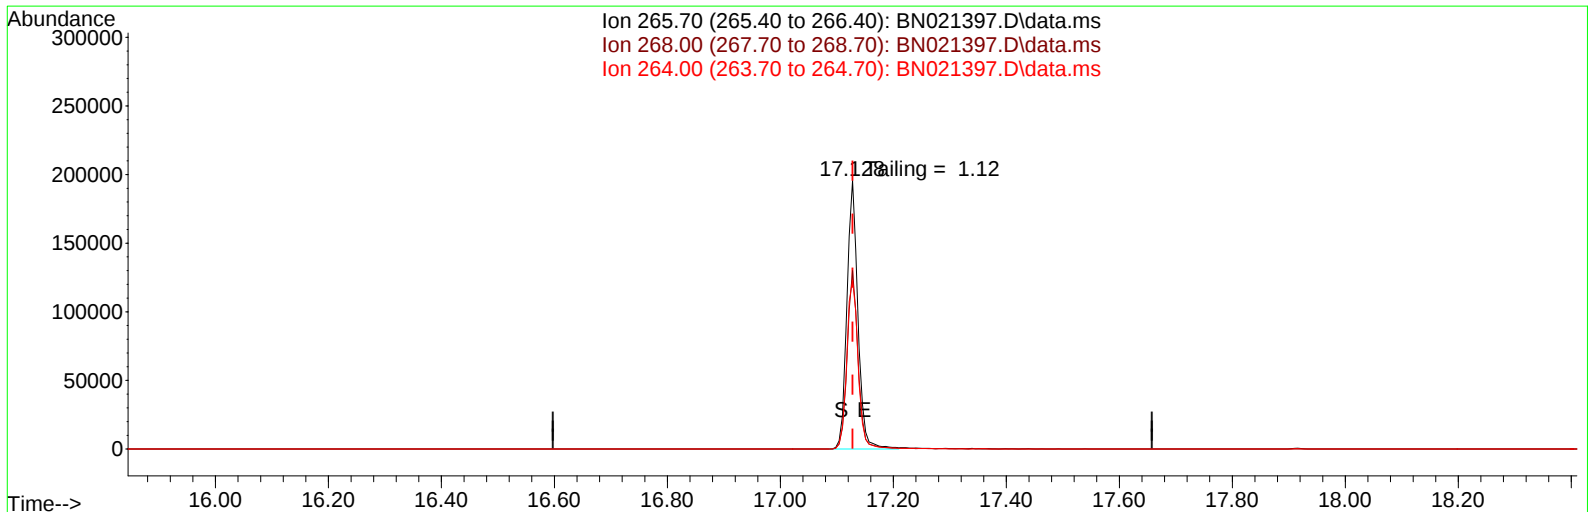

TIC: BN021397.D\data.ms

(70) Pentachlorophenol (C)

17.128min (-0.000) 19650.68 ng


response 267869

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	66.40
264.00	61.60	62.88
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082622\
Data File : BN021397.D
Acq On : 27 Aug 2022 00:01
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 27 04:56:41 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Aug 27 04:55:17 2022
Response via : Initial Calibration

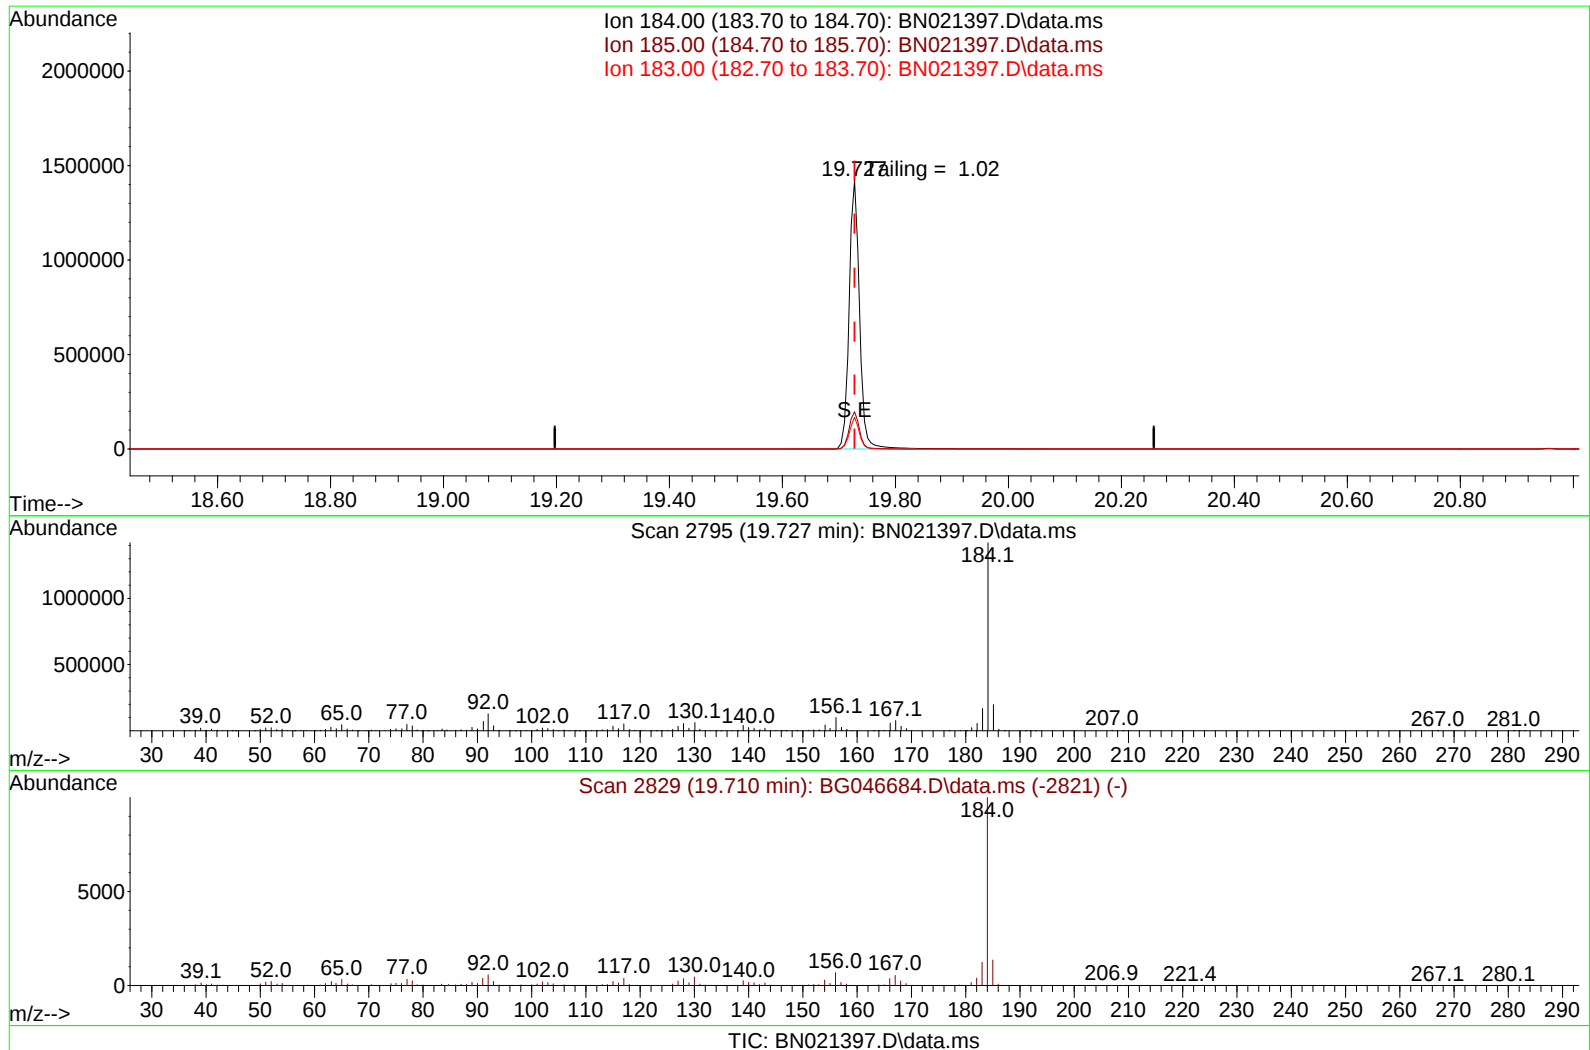

(77) Benzidine

19.727min (-0.000) 0.00 ng

response 1826036

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.89
183.00	13.20	11.84
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/26/2022	BNA_N	<u>BN021397.D</u>
Compound Name	Response	Retention Time
DDT	776336	20.957
DDD	11326	20.516
DDE	431	20.01
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11757	788093	1.49

Instrument :
BNA_N
ClientSampleId :
DFTPP