
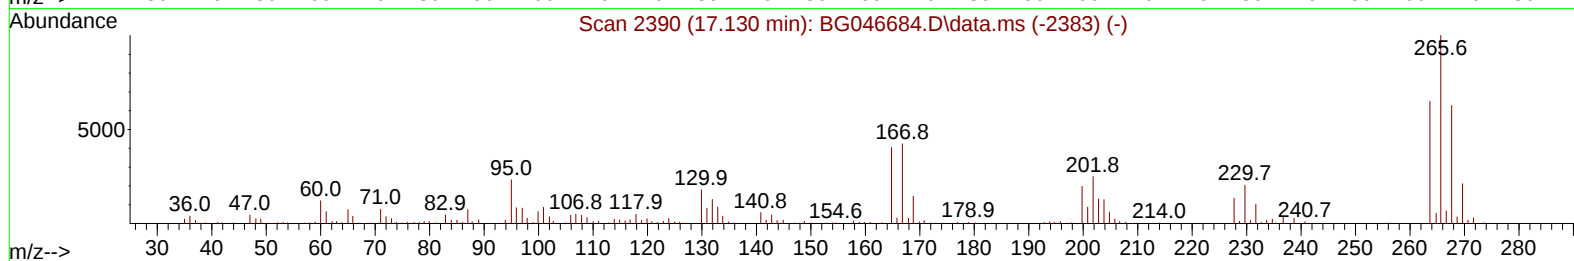
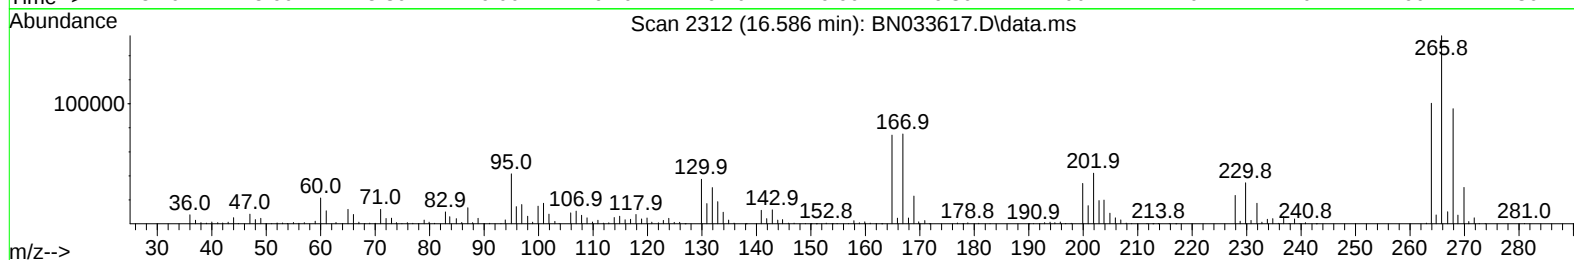


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082624\
Data File : BN033617.D
Acq On : 26 Aug 2024 10:03
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 26 14:34:33 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Aug 24 06:44:36 2024
Response via : Initial Calibration

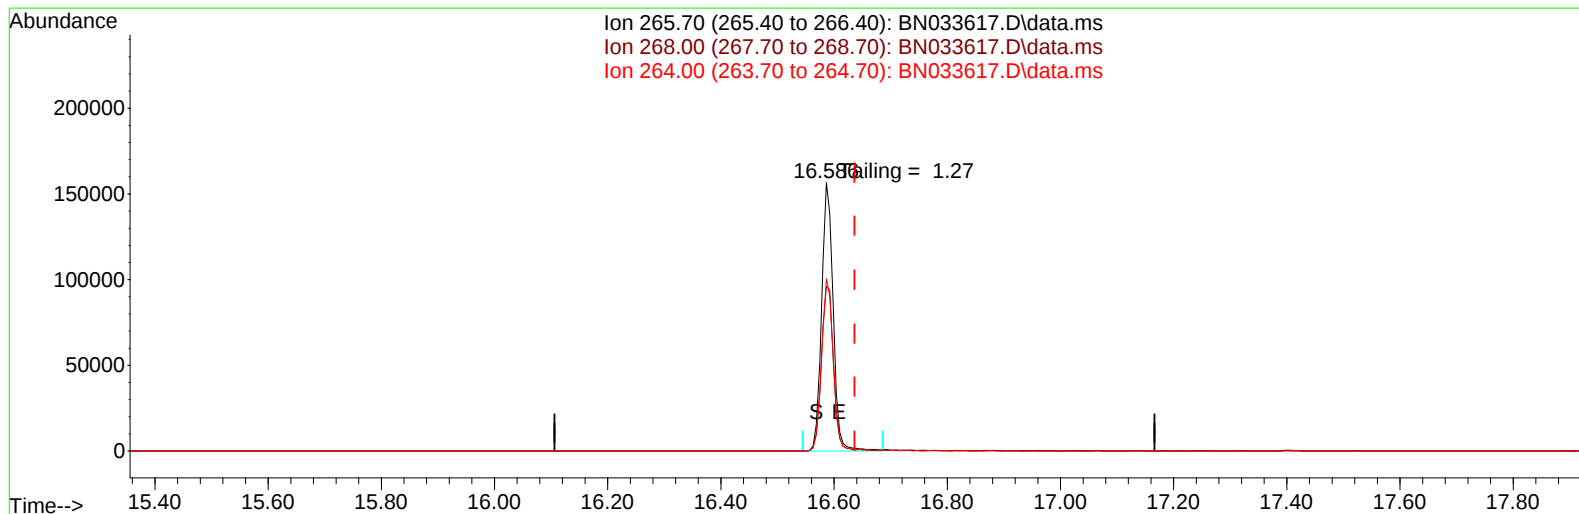

TIC: BN033617.D\data.ms

(70) Pentachlorophenol (C)




16.586min (-0.050) 23086.22 ng

response 221758

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.27
264.00	61.60	64.15
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082624\
Data File : BN033617.D
Acq On : 26 Aug 2024 10:03
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 26 14:34:33 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Aug 24 06:44:36 2024
Response via : Initial Calibration

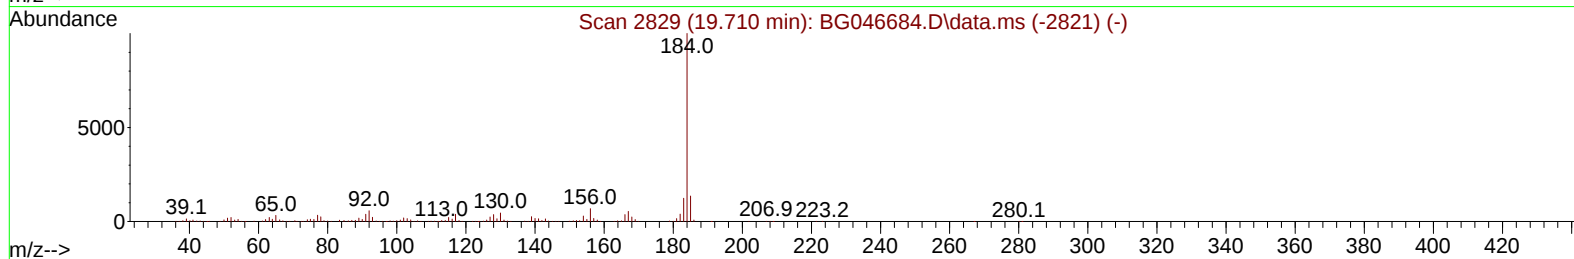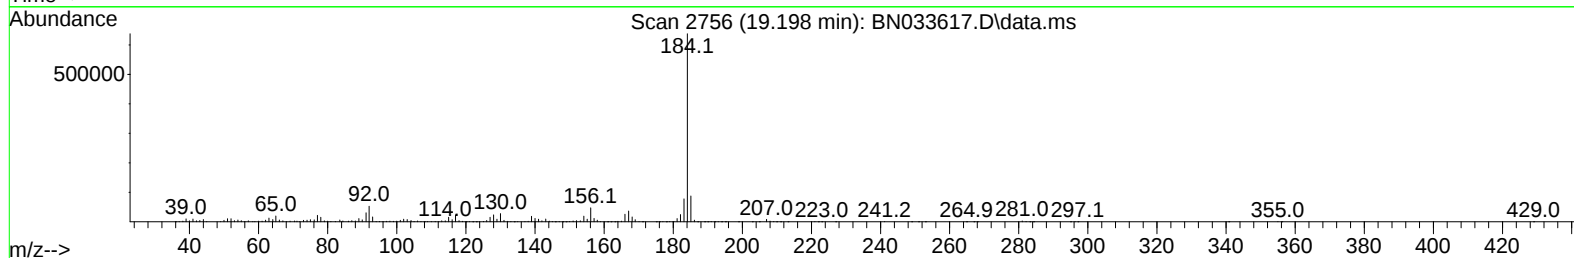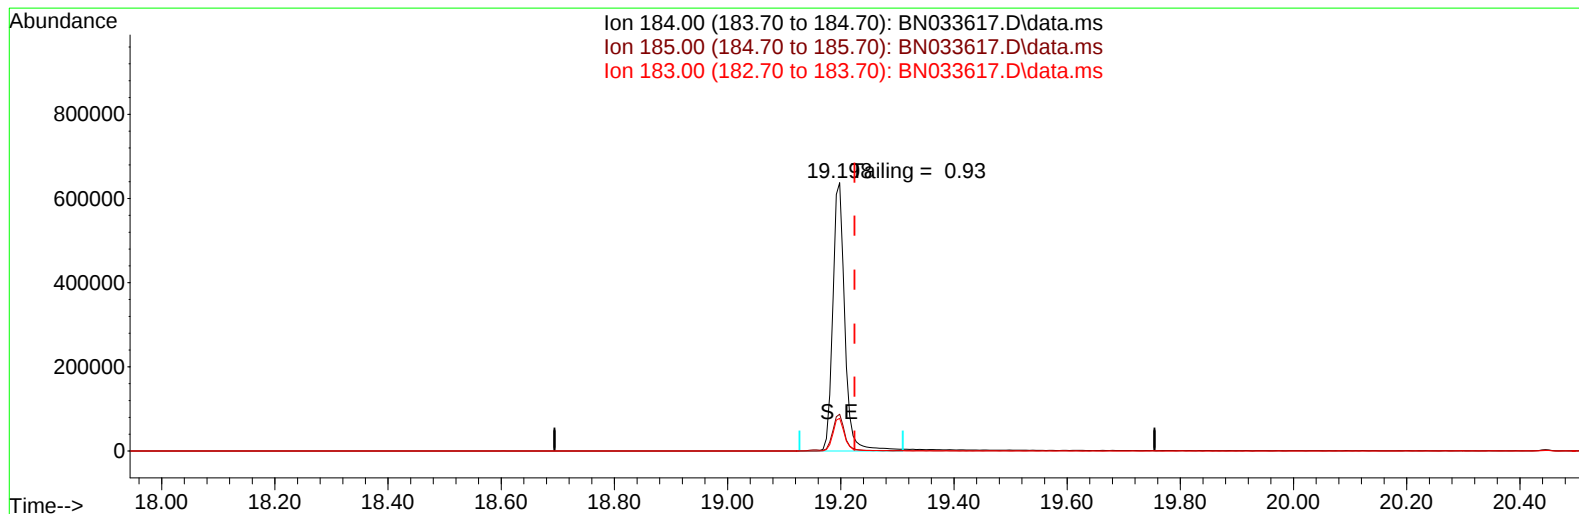

TIC: BN033617.D\data.ms

(77) Benzidine**19.198min (-0.026) 149307.71 ng****response 938903**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.75
183.00	13.20	12.20
0.00	0.00	0.00